

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082322\
 Data File : VY010180.D
 Acq On : 23 Aug 2022 21:06
 Operator : KP/MD
 Sample : N4188-16
 Misc : 10.77g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 S10

Quant Time: Aug 24 04:35:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081922S.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 22 02:37:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	167207	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	312536	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	312976	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	144034	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.130	65	97886	71.471	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	142.940%
35) Dibromofluoromethane	7.710	113	88948	50.508	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	101.020%
50) Toluene-d8	10.179	98	324649	49.197	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	98.400%
62) 4-Bromofluorobenzene	12.477	95	103685	43.976	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	87.960%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082322\
Data File : VY010180.D
Acq On : 23 Aug 2022 21:06
Operator : KP/MD
Sample : N4188-16
Misc : 10.77g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
S10

Quant Time: Aug 24 04:35:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081922S.M
Quant Title : SW846 8260
QLast Update : Mon Aug 22 02:37:07 2022
Response via : Initial Calibration




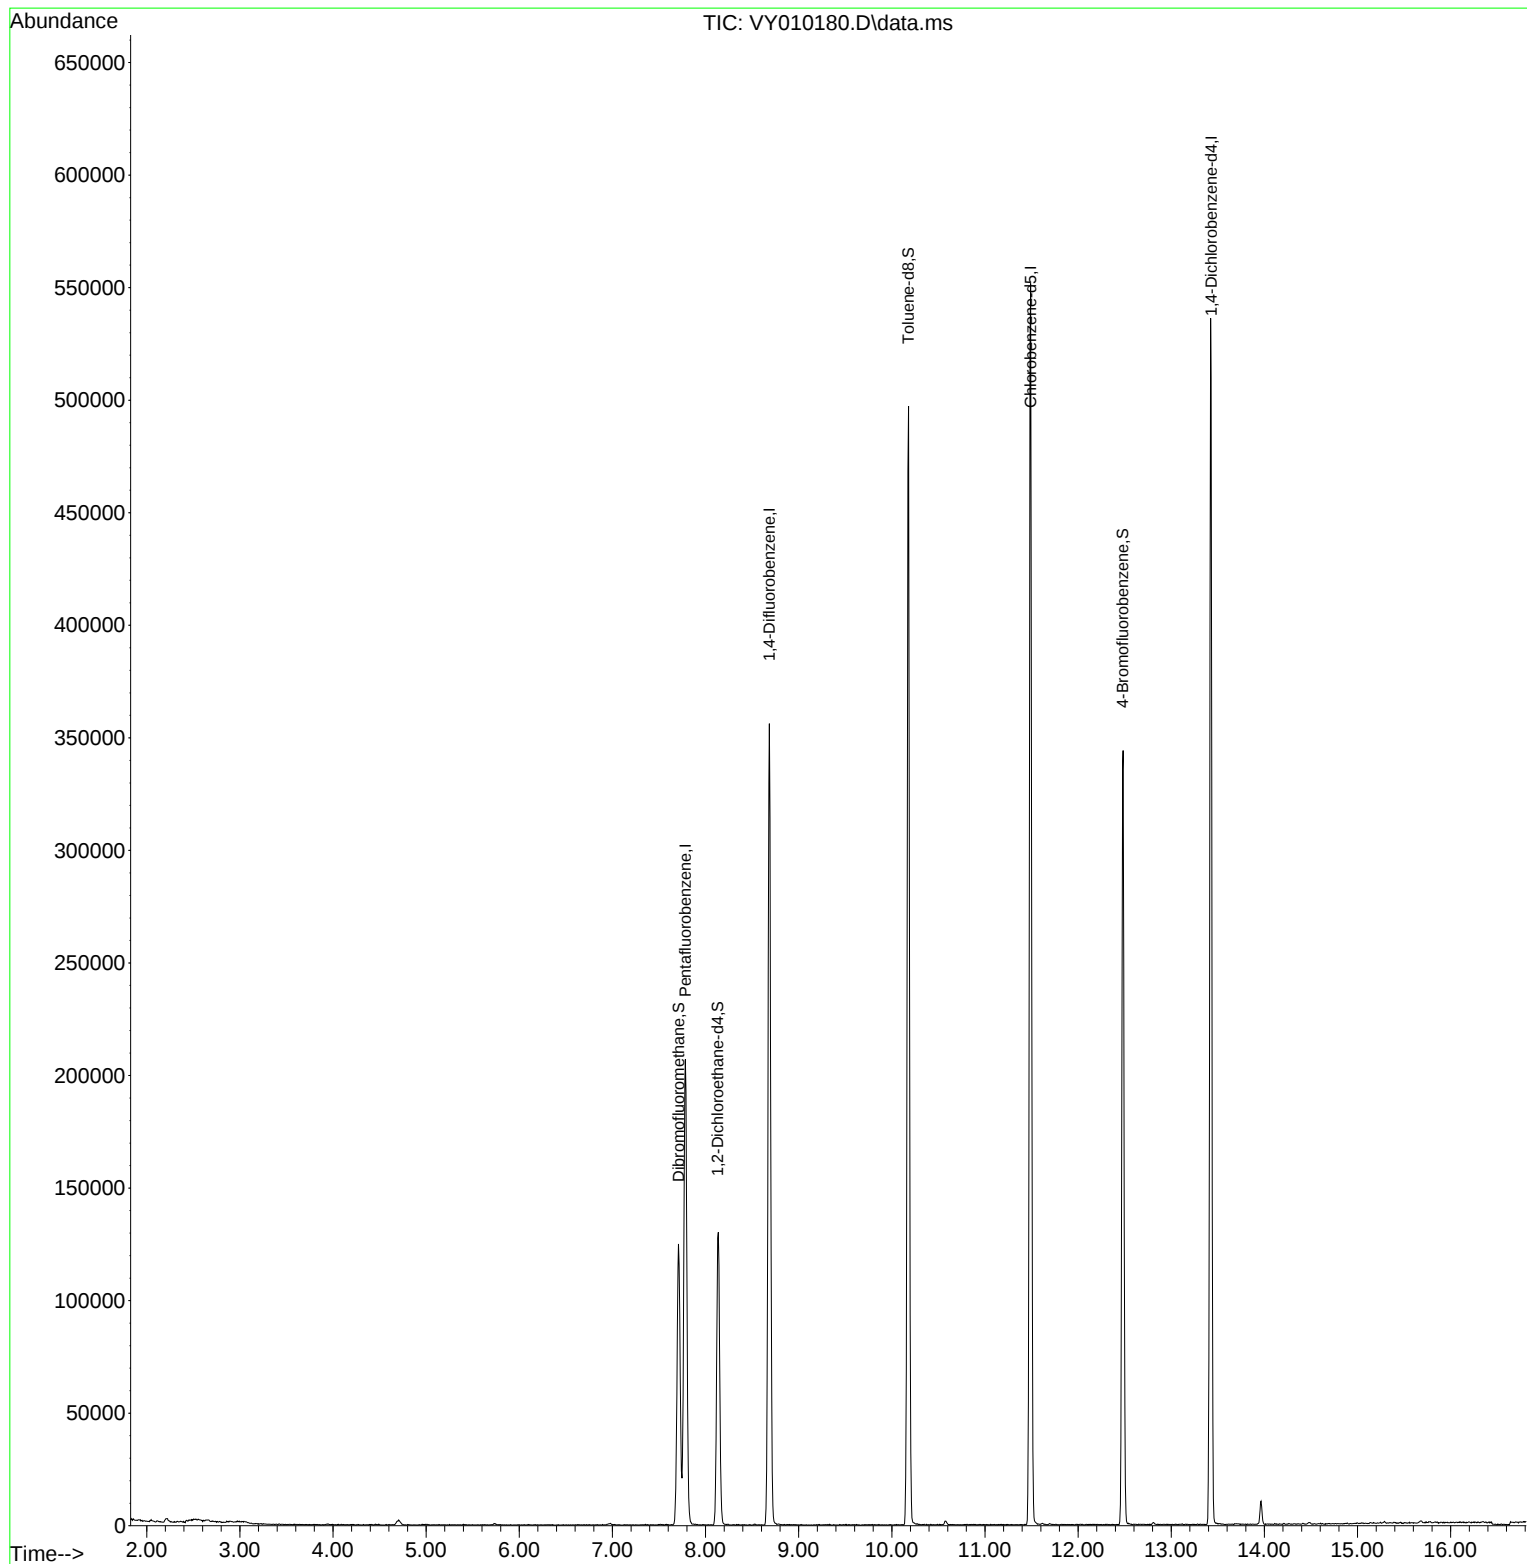


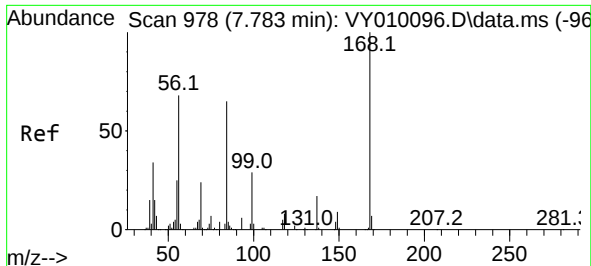

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY010180.D
Acq: 23 Aug 2022 21:06




Instrument :
MSVOA_Y
ClientSampleId :
S10


Tgt Ion:168 Resp: 167207
Ion Ratio Lower Upper
168 100
99 49.8 40.7 61.1

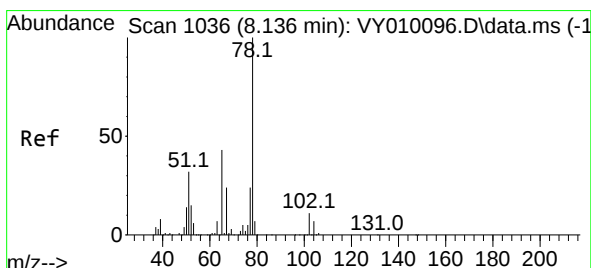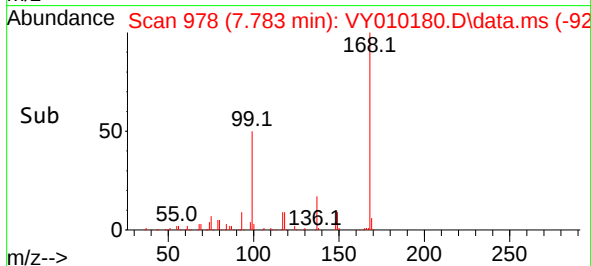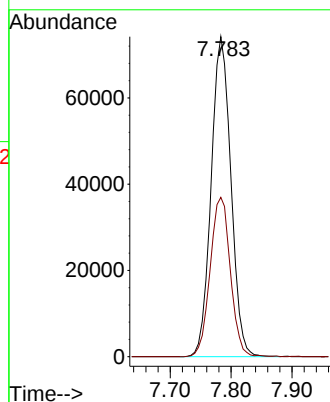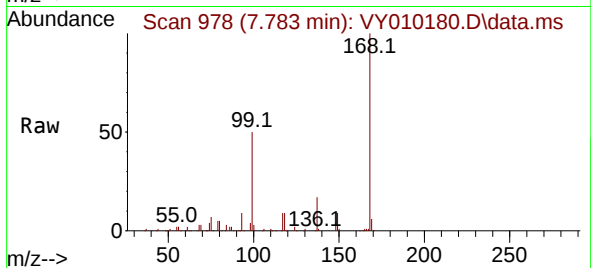

#33
1,2-Dichloroethane-d4
Concen: 71.471 ug/l
RT: 8.130 min Scan# 1035
Delta R.T. -0.006 min
Lab File: VY010180.D
Acq: 23 Aug 2022 21:06

Tgt Ion: 65 Resp: 97886
Ion Ratio Lower Upper
65 100
67 55.4 0.0 110.6


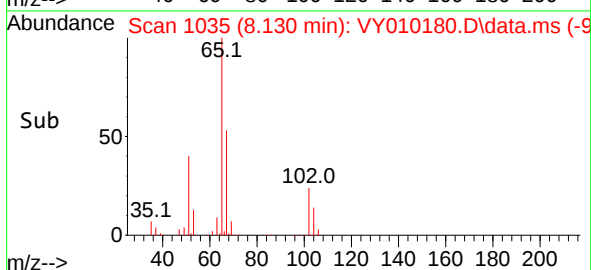
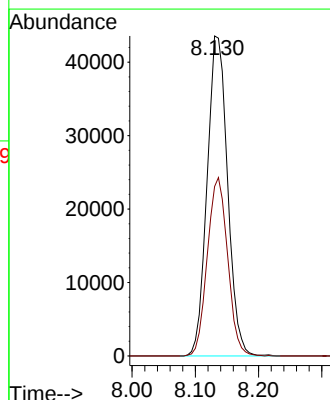
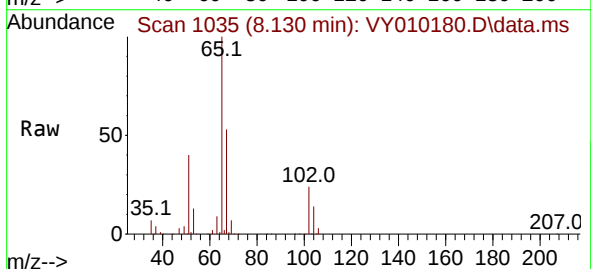


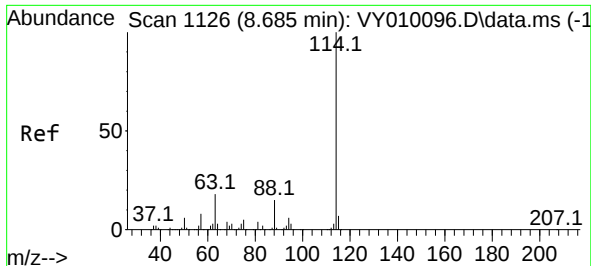

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.685 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VY010180.D
Acq: 23 Aug 2022 21:06




Instrument :
MSVOA_Y
ClientSampleId :
S10


Tgt Ion:114 Resp: 312536
Ion Ratio Lower Upper
114 100
63 18.4 0.0 35.6
88 14.8 0.0 29.6

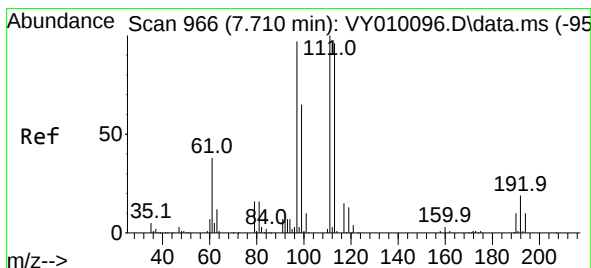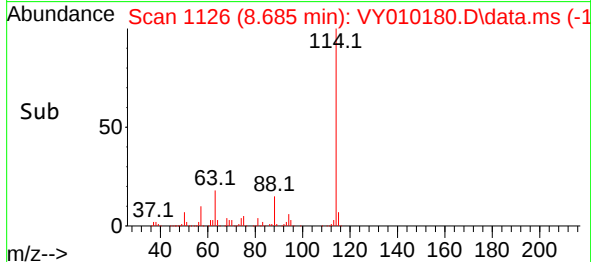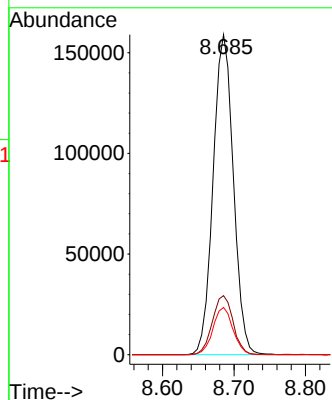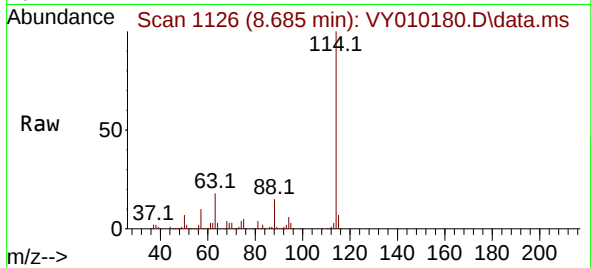

#35
Dibromofluoromethane
Concen: 50.508 ug/l
RT: 7.710 min Scan# 966
Delta R.T. -0.000 min
Lab File: VY010180.D
Acq: 23 Aug 2022 21:06

Tgt Ion:113 Resp: 88948
Ion Ratio Lower Upper
113 100
111 102.5 82.8 124.2
192 19.8 16.3 24.5

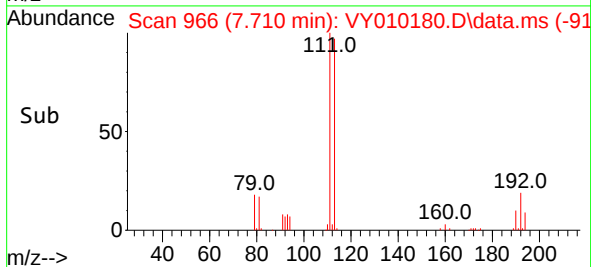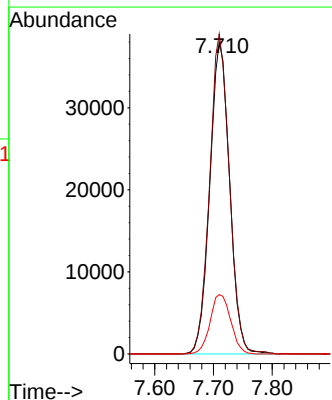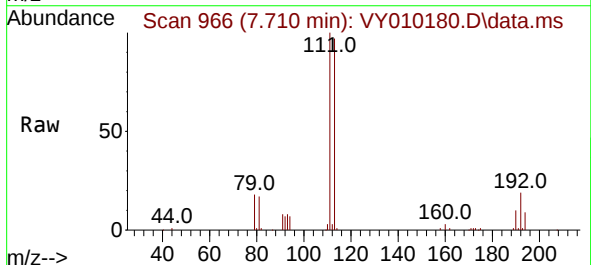

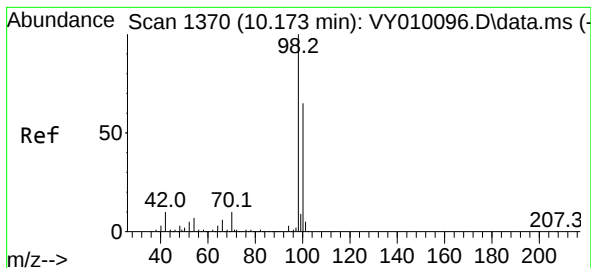

#50

Toluene-d8

Concen: 49.197 ug/l

RT: 10.179 min Scan# 1370

Delta R.T. 0.006 min

Lab File: VY010180.D

Acq: 23 Aug 2022 21:06

Instrument :

MSVOA_Y

ClientSampleId :





S10

Tgt Ion: 98 Resp: 324649

Ion Ratio Lower Upper

98 100

100 64.0 51.9 77.9

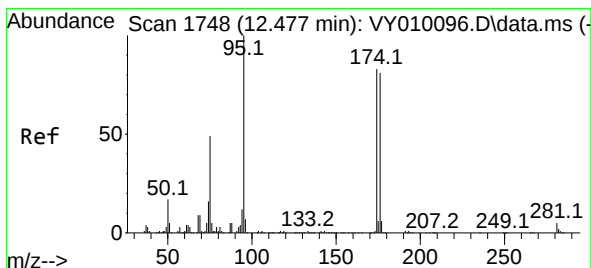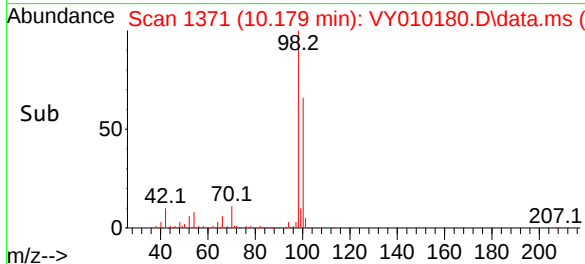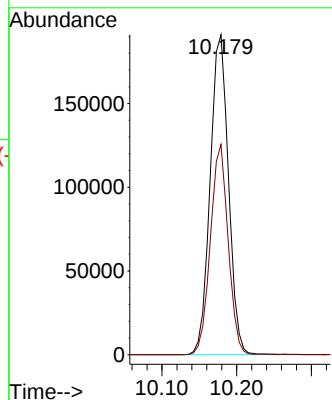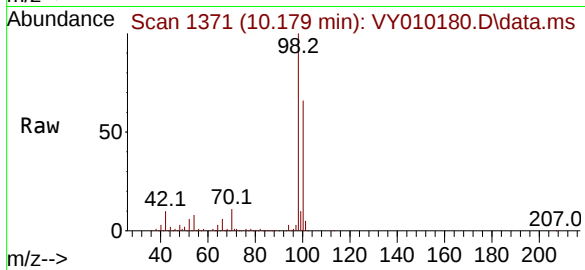

#62

4-Bromofluorobenzene

Concen: 43.976 ug/l

RT: 12.477 min Scan# 1748

Delta R.T. 0.000 min

Lab File: VY010180.D

Acq: 23 Aug 2022 21:06




Tgt Ion: 95 Resp: 103685


Ion Ratio Lower Upper

95 100

174 88.5 0.0 173.8

176 85.0 0.0 167.2

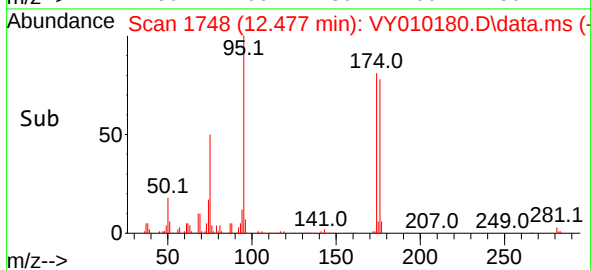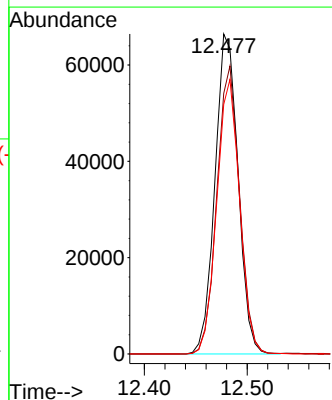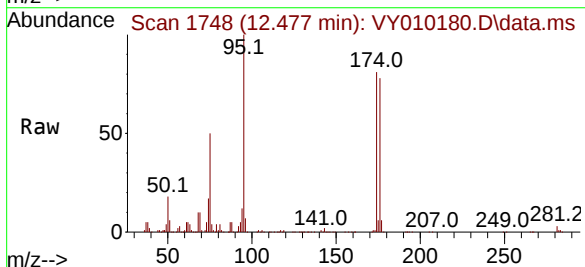

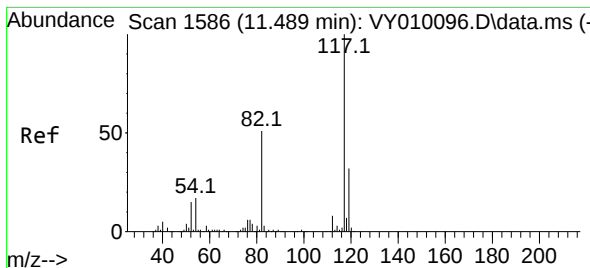

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.490 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY010180.D

Acq: 23 Aug 2022 21:06

Instrument :

MSVOA_Y

ClientSampleId :

S10





Tgt Ion:117 Resp: 312976

Ion Ratio Lower Upper

117 100

82 51.0 40.6 61.0

119 31.7 25.8 38.8

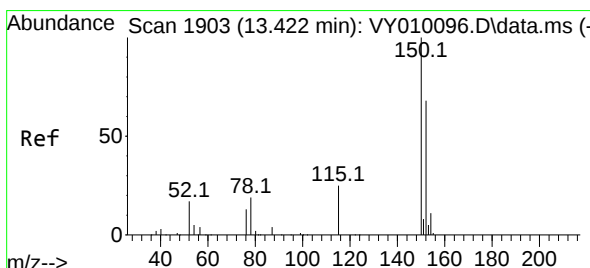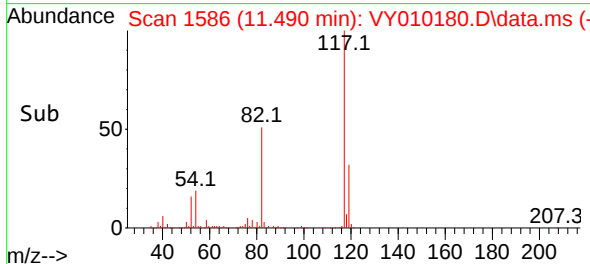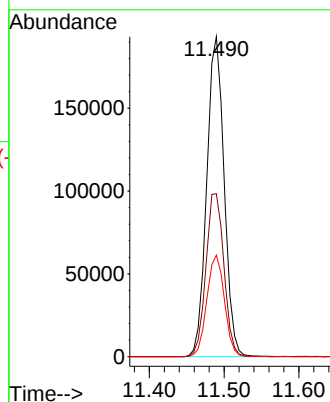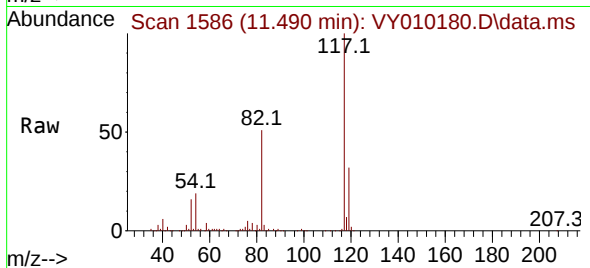

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.006 min

Lab File: VY010180.D

Acq: 23 Aug 2022 21:06

Tgt Ion:152 Resp: 144034

Ion Ratio Lower Upper

152 100

115 55.4 28.1 84.2

150 157.5 0.0 346.2

