
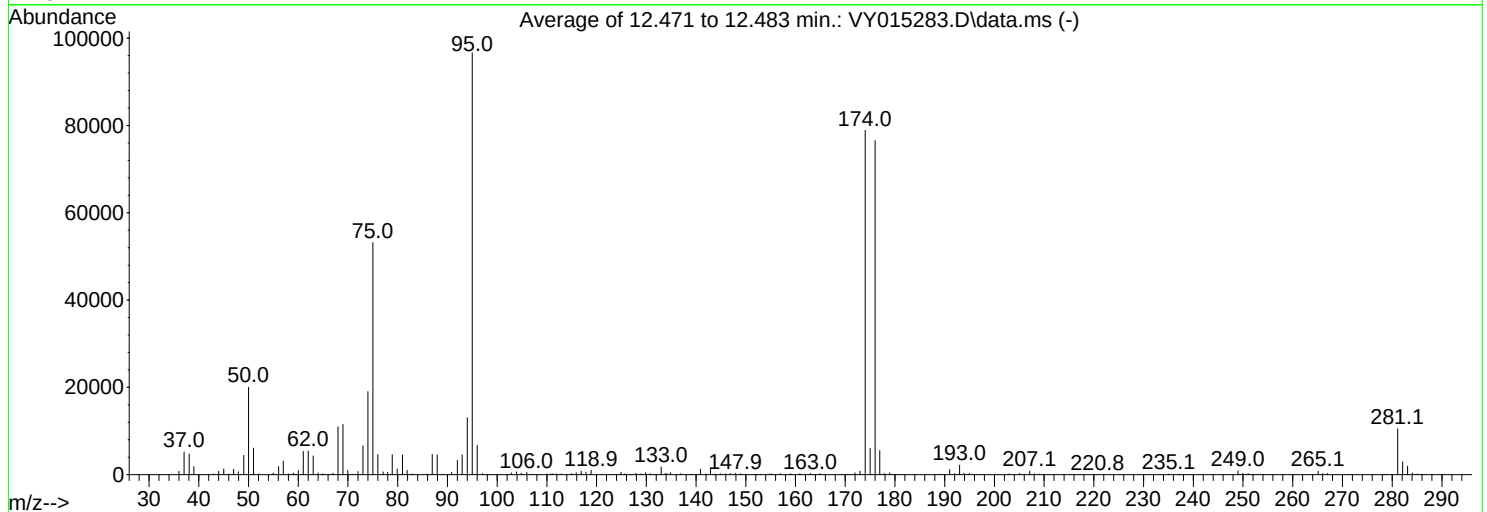


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082323\
Data File : VY015283.D
Acq On : 23 Aug 2023 14:33
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081423S.M
Title : SW846 8260
Last Update : Mon Aug 14 12:43:26 2023

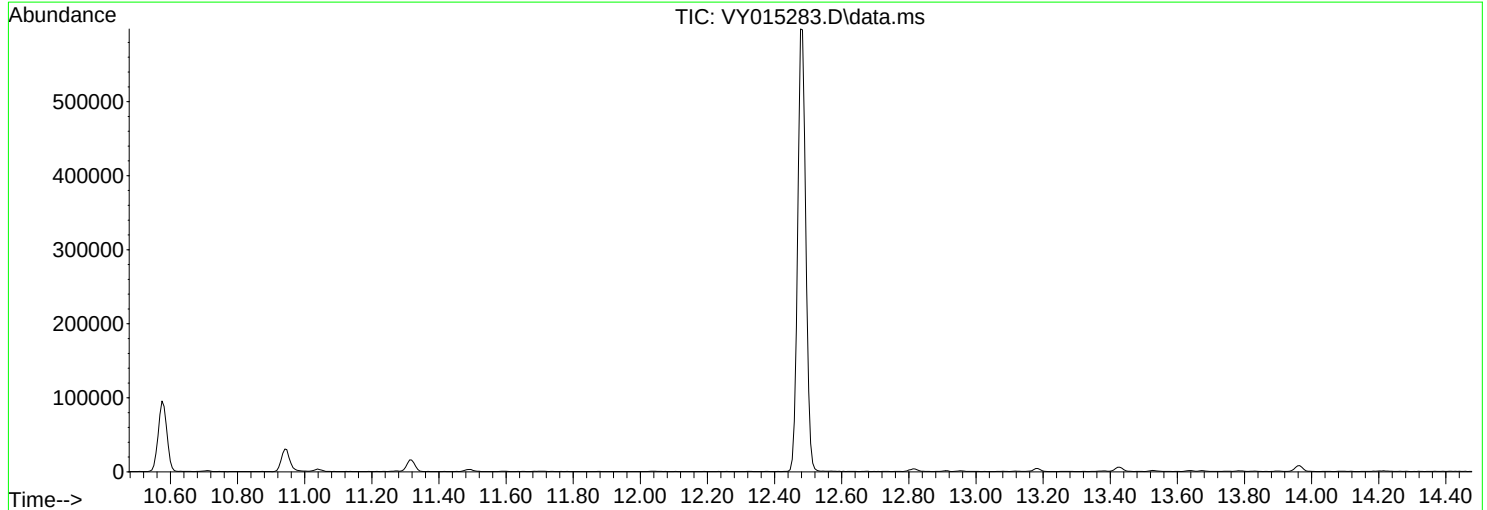

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	20032	PASS
75	95	30	60	55.0	53165	PASS
95	95	100	100	100.0	96640	PASS
96	95	5	9	6.9	6694	PASS
173	174	0.00	2	1.0	820	PASS
174	95	50	100	81.6	78888	PASS
175	174	5	9	7.6	6032	PASS
176	174	95	101	97.0	76531	PASS
177	176	5	9	7.2	5511	PASS