
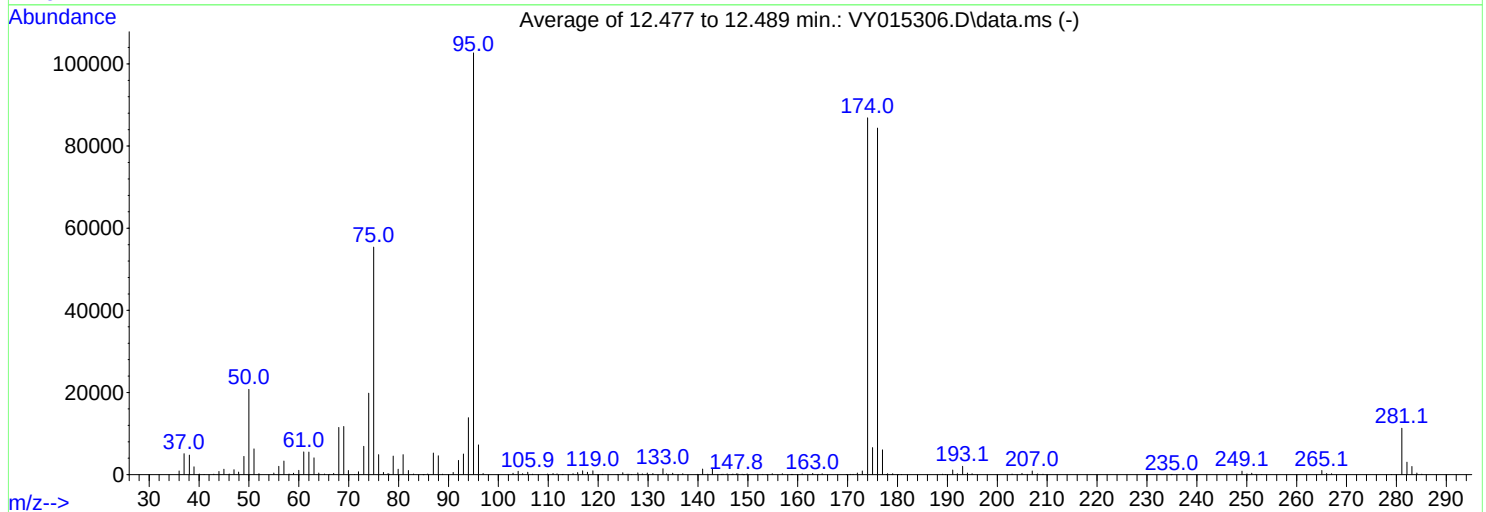


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY082423\  
Data File : VY015306.D  
Acq On : 24 Aug 2023 11:36  
Operator : SY/MD  
Sample : BFB  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y081423S.M  
Title : SW846 8260  
Last Update : Mon Aug 14 12:43:26 2023

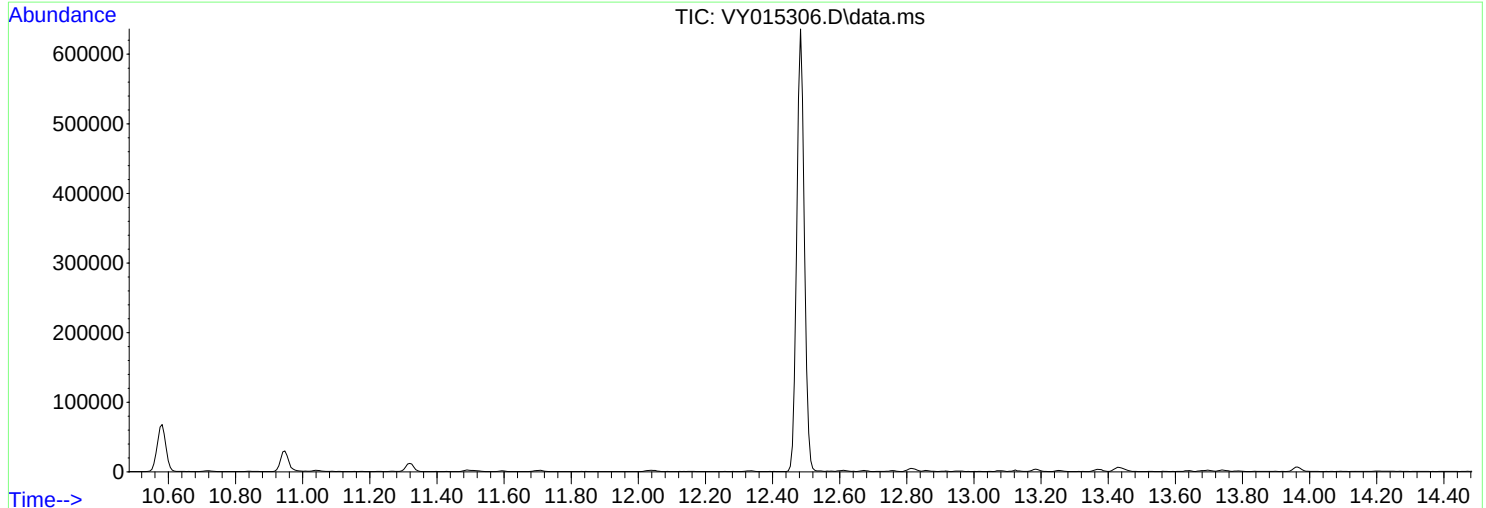

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 50     | 95      | 15     | 40     | 20.2  | 20787  | PASS      |
| 75     | 95      | 30     | 60     | 53.9  | 55392  | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 102699 | PASS      |
| 96     | 95      | 5      | 9      | 7.1   | 7265   | PASS      |
| 173    | 174     | 0.00   | 2      | 1.0   | 908    | PASS      |
| 174    | 95      | 50     | 100    | 84.6  | 86877  | PASS      |
| 175    | 174     | 5      | 9      | 7.6   | 6584   | PASS      |
| 176    | 174     | 95     | 101    | 97.1  | 84381  | PASS      |
| 177    | 176     | 5      | 9      | 7.1   | 6028   | PASS      |