
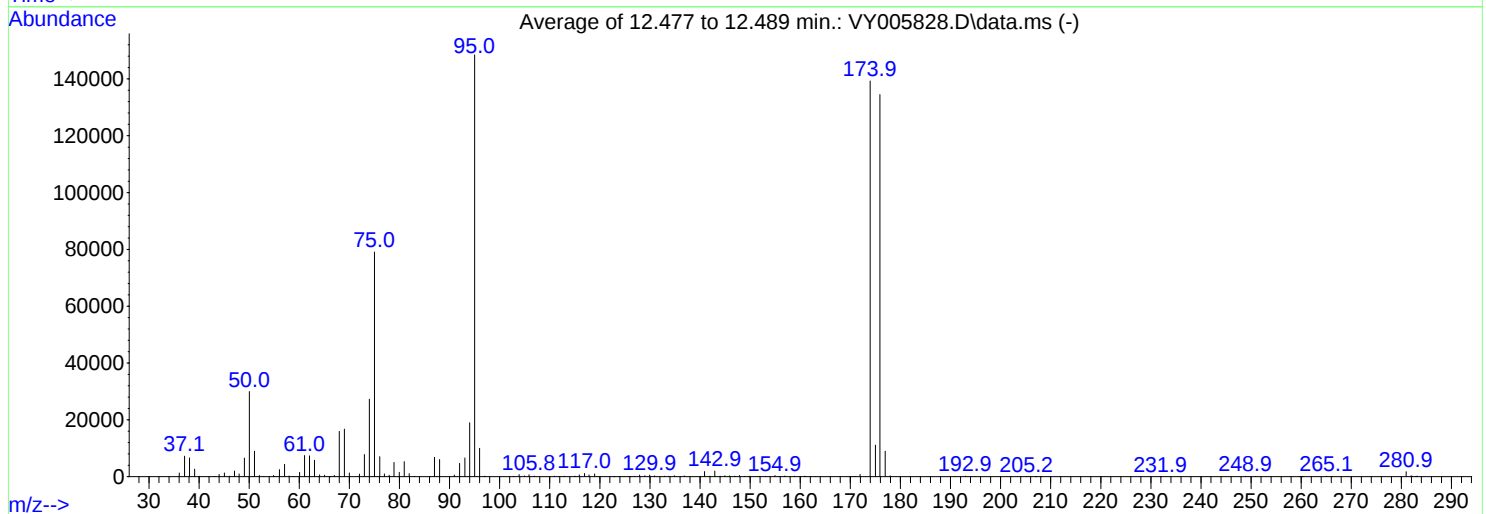


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY082521\  
Data File : VY005828.D  
Acq On : 25 Aug 2021 09:28  
Operator : SY/MD  
Sample : BFB  
Misc : 5.00G/5ML/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y080221S.M  
Title : SW846 8260  
Last Update : Tue Aug 03 04:52:05 2021

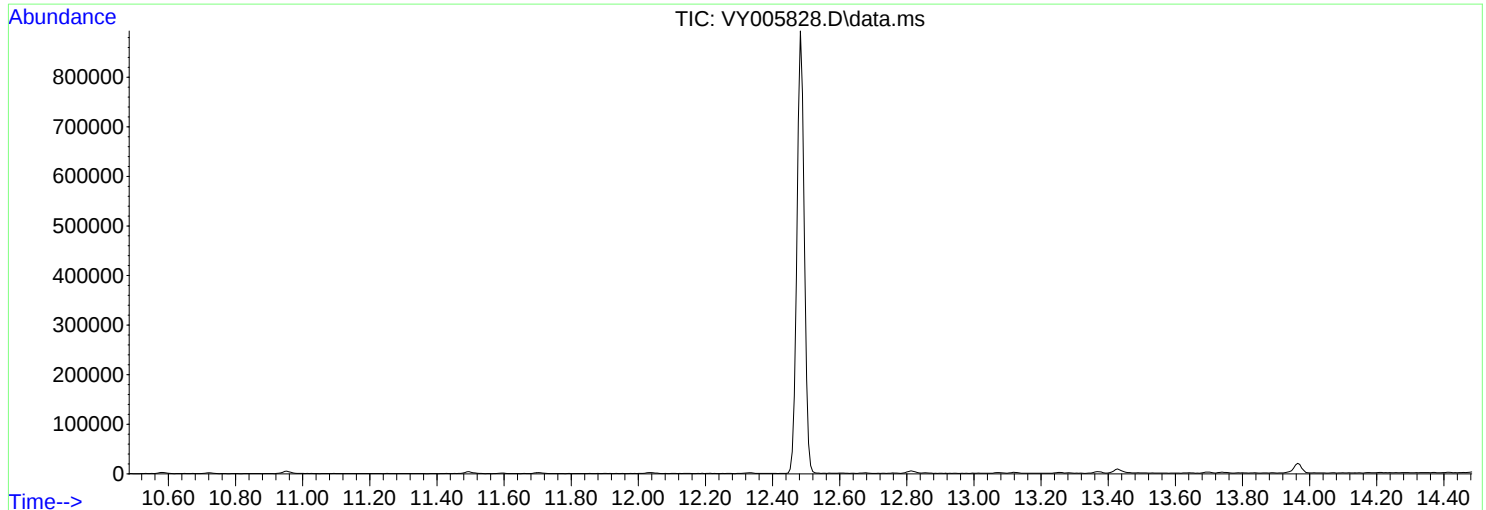

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 20.2         | 29987      | PASS                |
| 75             | 95              | 30              | 60              | 53.3         | 79088      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 148480     | PASS                |
| 96             | 95              | 5               | 9               | 6.7          | 9950       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 174            | 95              | 50              | 100             | 93.8         | 139307     | PASS                |
| 175            | 174             | 5               | 9               | 8.0          | 11078      | PASS                |
| 176            | 174             | 95              | 101             | 96.6         | 134517     | PASS                |
| 177            | 176             | 5               | 9               | 6.7          | 8981       | PASS                |