

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082523\
 Data File : VY015340.D
 Acq On : 25 Aug 2023 14:17
 Operator : SY/MD
 Sample : 04165-01
 Misc : 5.02g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VNJ-208

Quant Time: Aug 25 23:41:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081423S.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 14 12:43:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	5059	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	8288	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	7623	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	2972	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	3396	55.921	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	111.840%
35) Dibromofluoromethane	7.716	113	1486	27.870	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	55.740%
50) Toluene-d8	10.179	98	9515	47.938	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	95.880%
62) 4-Bromofluorobenzene	12.483	95	3223	44.457	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	88.920%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082523\
Data File : VY015340.D
Acq On : 25 Aug 2023 14:17
Operator : SY/MD
Sample : 04165-01
Misc : 5.02g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VNJ-208

Quant Time: Aug 25 23:41:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081423S.M
Quant Title : SW846 8260
QLast Update : Mon Aug 14 12:43:26 2023
Response via : Initial Calibration




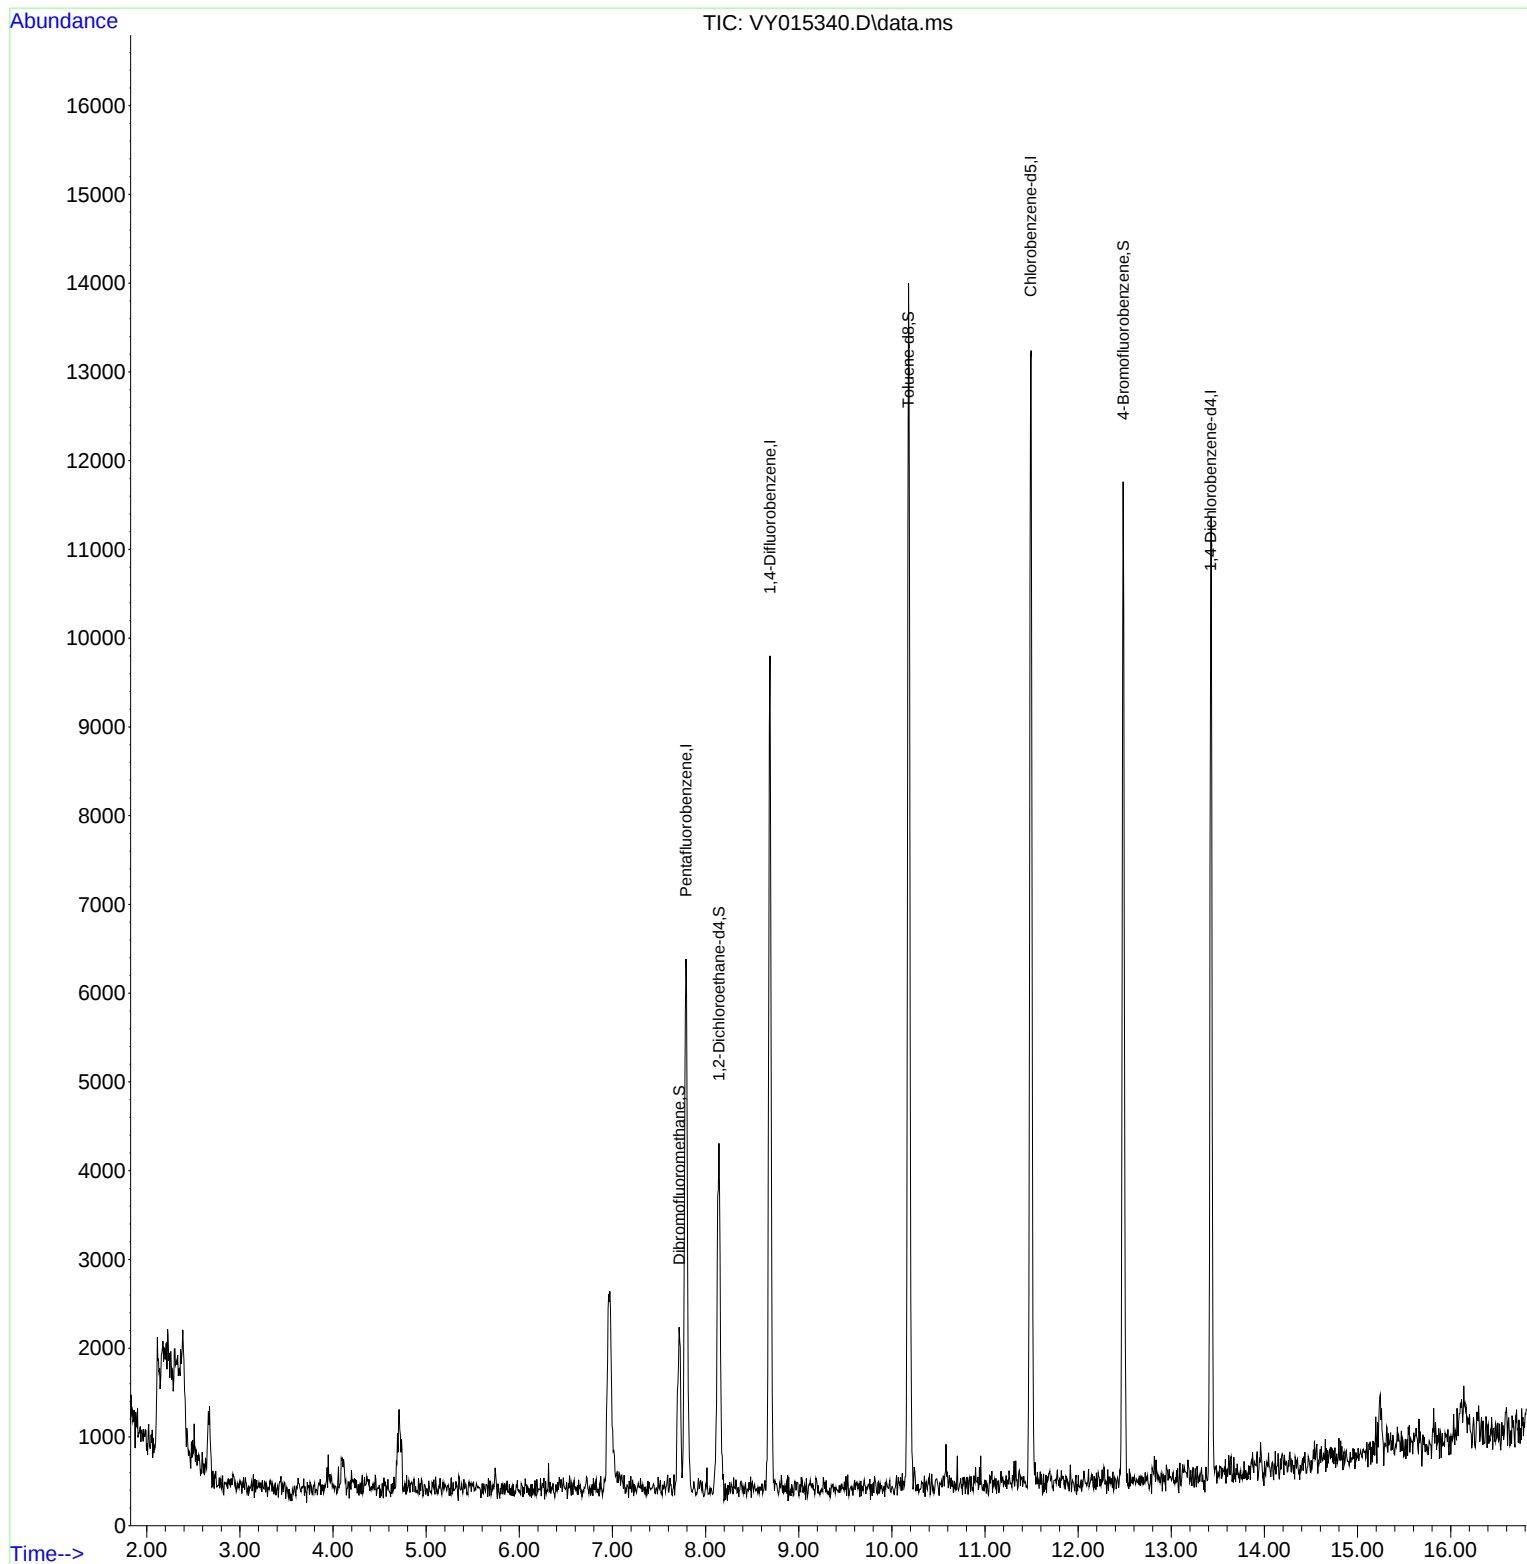


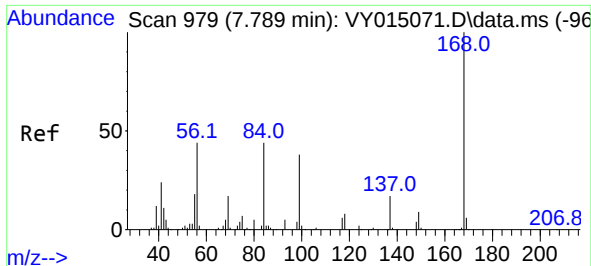

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY015340.D
Acq: 25 Aug 2023 14:17




Instrument :
MSVOA_Y
ClientSampleId :
VNJ-208


Tgt Ion:168 Resp: 5059
Ion Ratio Lower Upper
168 100
99 52.6 43.4 65.0

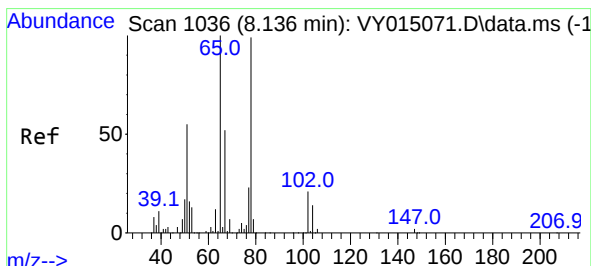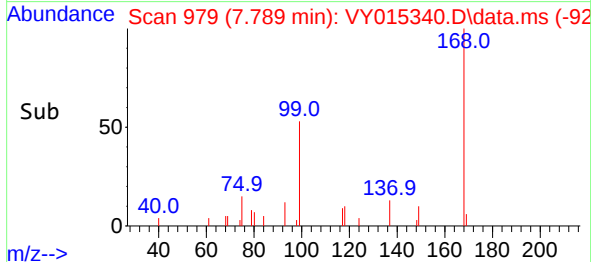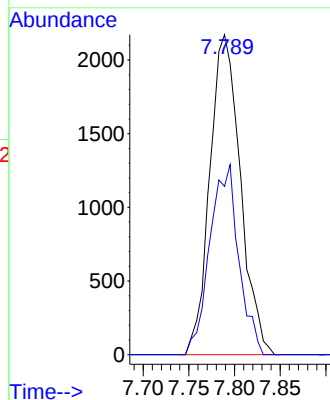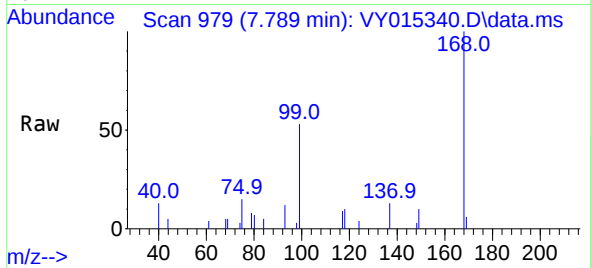

#33
1,2-Dichloroethane-d4
Concen: 55.921 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. 0.006 min
Lab File: VY015340.D
Acq: 25 Aug 2023 14:17

Tgt Ion: 65 Resp: 3396
Ion Ratio Lower Upper
65 100
67 53.7 0.0 101.8

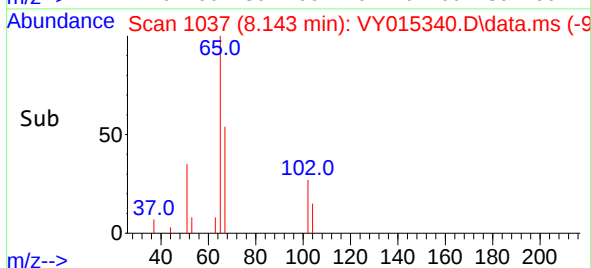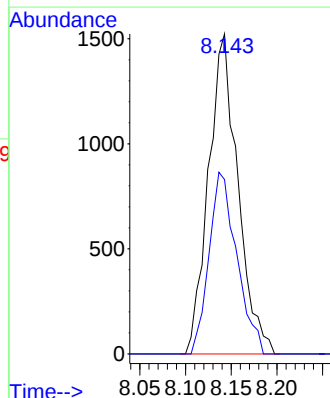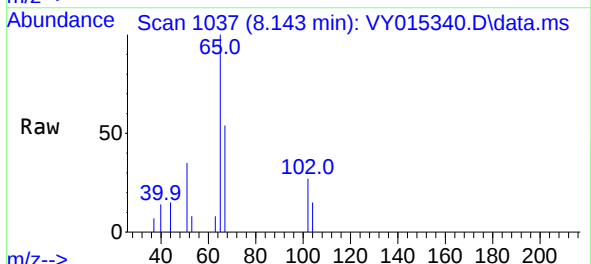

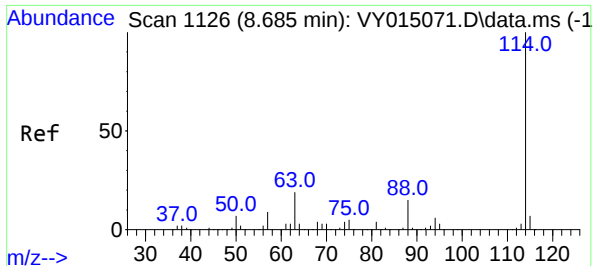

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VY015340.D

Acq: 25 Aug 2023 14:17

Instrument :

MSVOA_Y

ClientSampleId :

VNJ-208





Tgt Ion:114 Resp: 8288

Ion Ratio Lower Upper

114 100

63 20.0 0.0 42.4

88 13.9 0.0 30.6

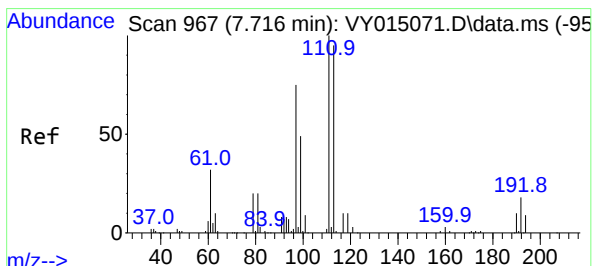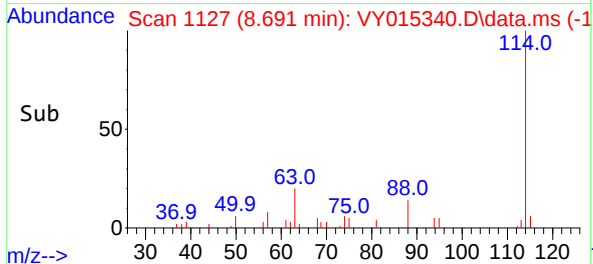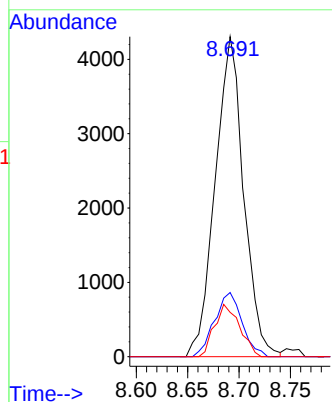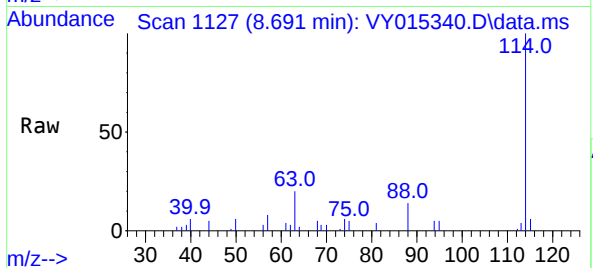

#35

Dibromofluoromethane

Concen: 27.870 ug/l

RT: 7.716 min Scan# 967

Delta R.T. 0.000 min

Lab File: VY015340.D

Acq: 25 Aug 2023 14:17




Tgt Ion:113 Resp: 1486


Ion Ratio Lower Upper

113 100

111 101.9 81.3 121.9

192 11.8 16.9 25.3#


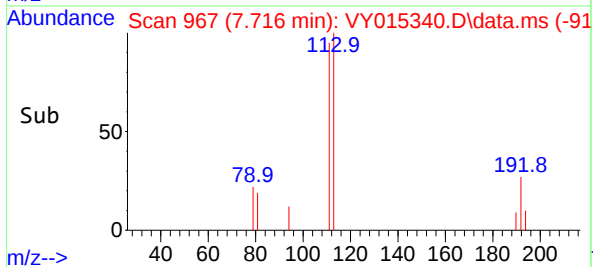
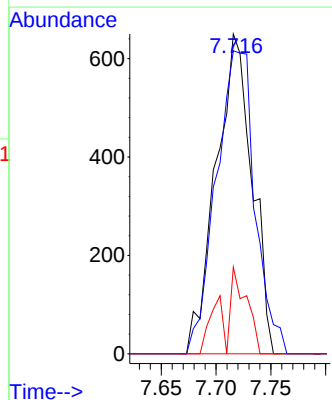
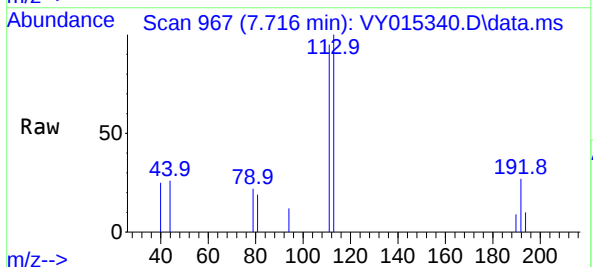


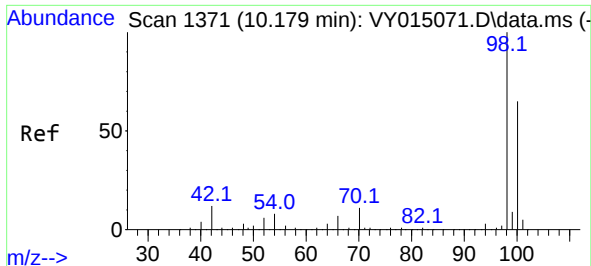

#50
Toluene-d8
Concen: 47.938 ug/l
RT: 10.179 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY015340.D
Acq: 25 Aug 2023 14:17




Instrument :
MSVOA_Y
ClientSampleId :
VNJ-208


Tgt Ion: 98 Resp: 9515
Ion Ratio Lower Upper
98 100
100 65.1 50.1 75.1

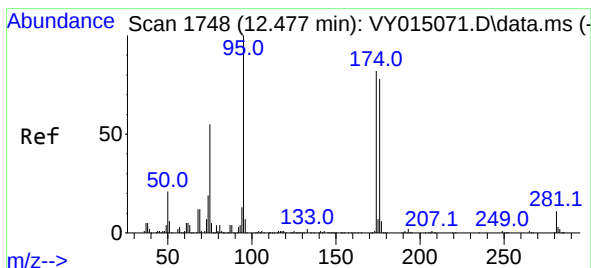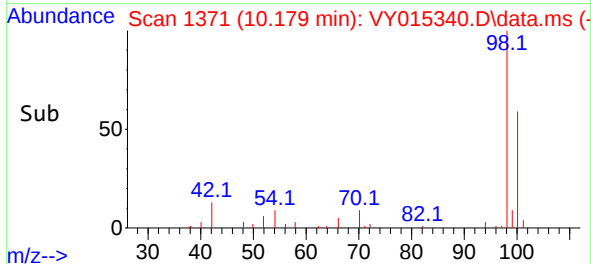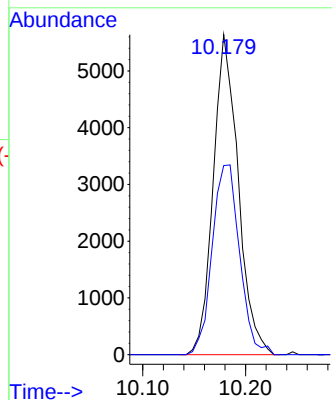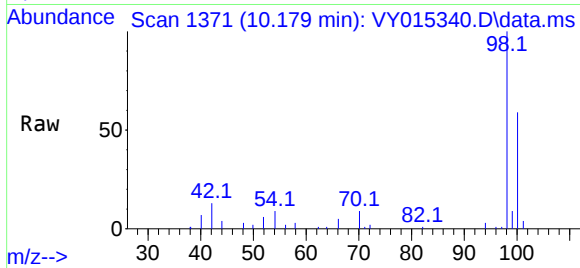

#62
4-Bromofluorobenzene
Concen: 44.457 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.006 min
Lab File: VY015340.D
Acq: 25 Aug 2023 14:17

Tgt Ion: 95 Resp: 3223
Ion Ratio Lower Upper
95 100
174 81.8 0.0 178.2
176 85.2 0.0 173.8


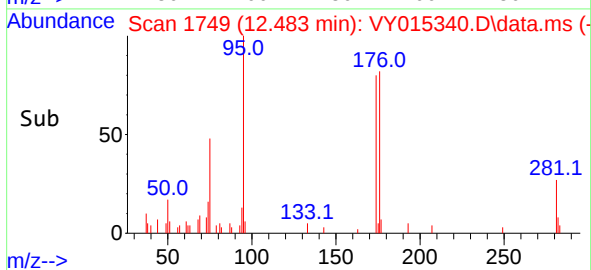
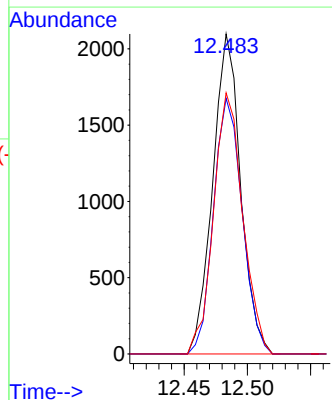
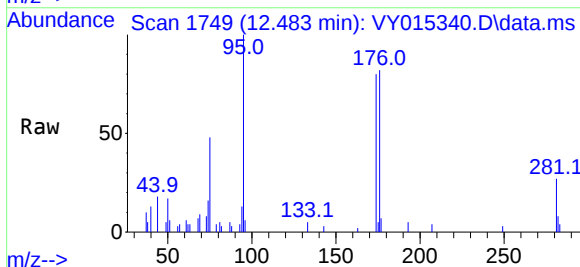


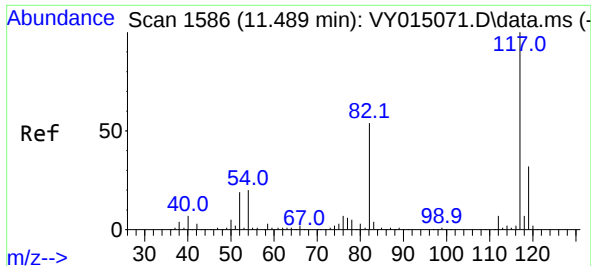

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY015340.D
Acq: 25 Aug 2023 14:17

Instrument :
MSVOA_Y
ClientSampleId :
VNJ-208

Tgt Ion:	117	Resp:	7623
Ion	Ratio	Lower	Upper
117	100		
82	54.4	43.4	65.0
119	32.4	26.3	39.5

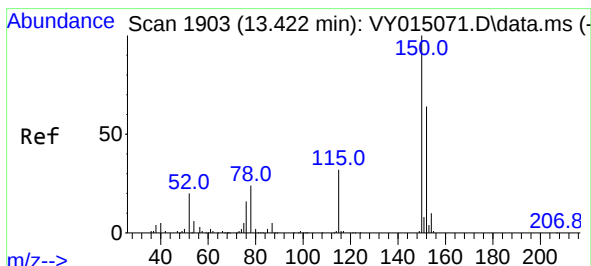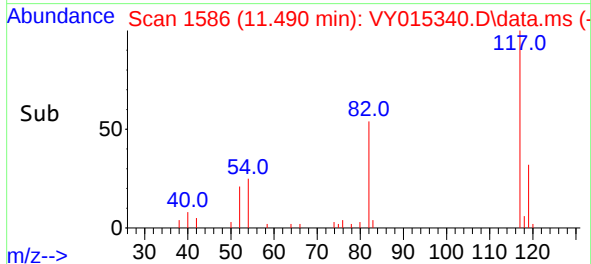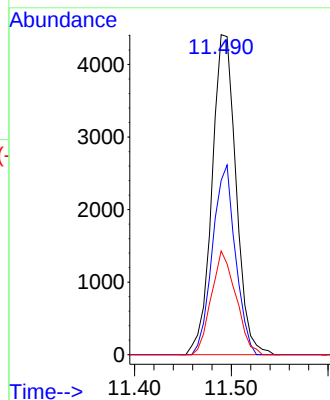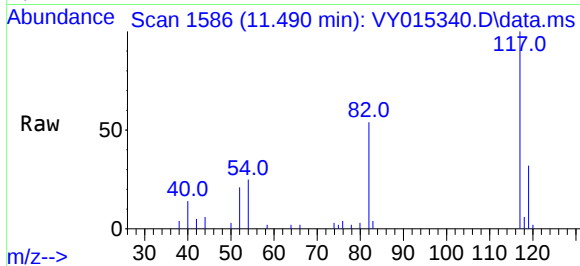

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. 0.000 min
Lab File: VY015340.D
Acq: 25 Aug 2023 14:17

Tgt Ion:	152	Resp:	2972
Ion	Ratio	Lower	Upper
152	100		
115	55.7	28.8	86.5
150	161.3	0.0	348.8

