

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082724\
 Data File : VY019283.D
 Acq On : 27 Aug 2024 13:57
 Operator : SY/MD
 Sample : P3714-01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 EO-01-08222024

Quant Time: Aug 27 15:43:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081524S.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 16 05:10:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.701	168	71543	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.609	114	126336	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	115524	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	44275	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.055	65	36710	51.188	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	102.380%
35) Dibromofluoromethane	7.628	113	40467	48.988	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	97.980%
50) Toluene-d8	10.103	98	142211	47.839	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	95.680%
62) 4-Bromofluorobenzene	12.408	95	43486	42.911	ug/l	0.00
Spiked Amount	50.000	Range	29 - 146	Recovery	=	85.820%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082724\
Data File : VY019283.D
Acq On : 27 Aug 2024 13:57
Operator : SY/MD
Sample : P3714-01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
EO-01-08222024

Quant Time: Aug 27 15:43:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081524S.M
Quant Title : SW846 8260
QLast Update : Fri Aug 16 05:10:30 2024
Response via : Initial Calibration




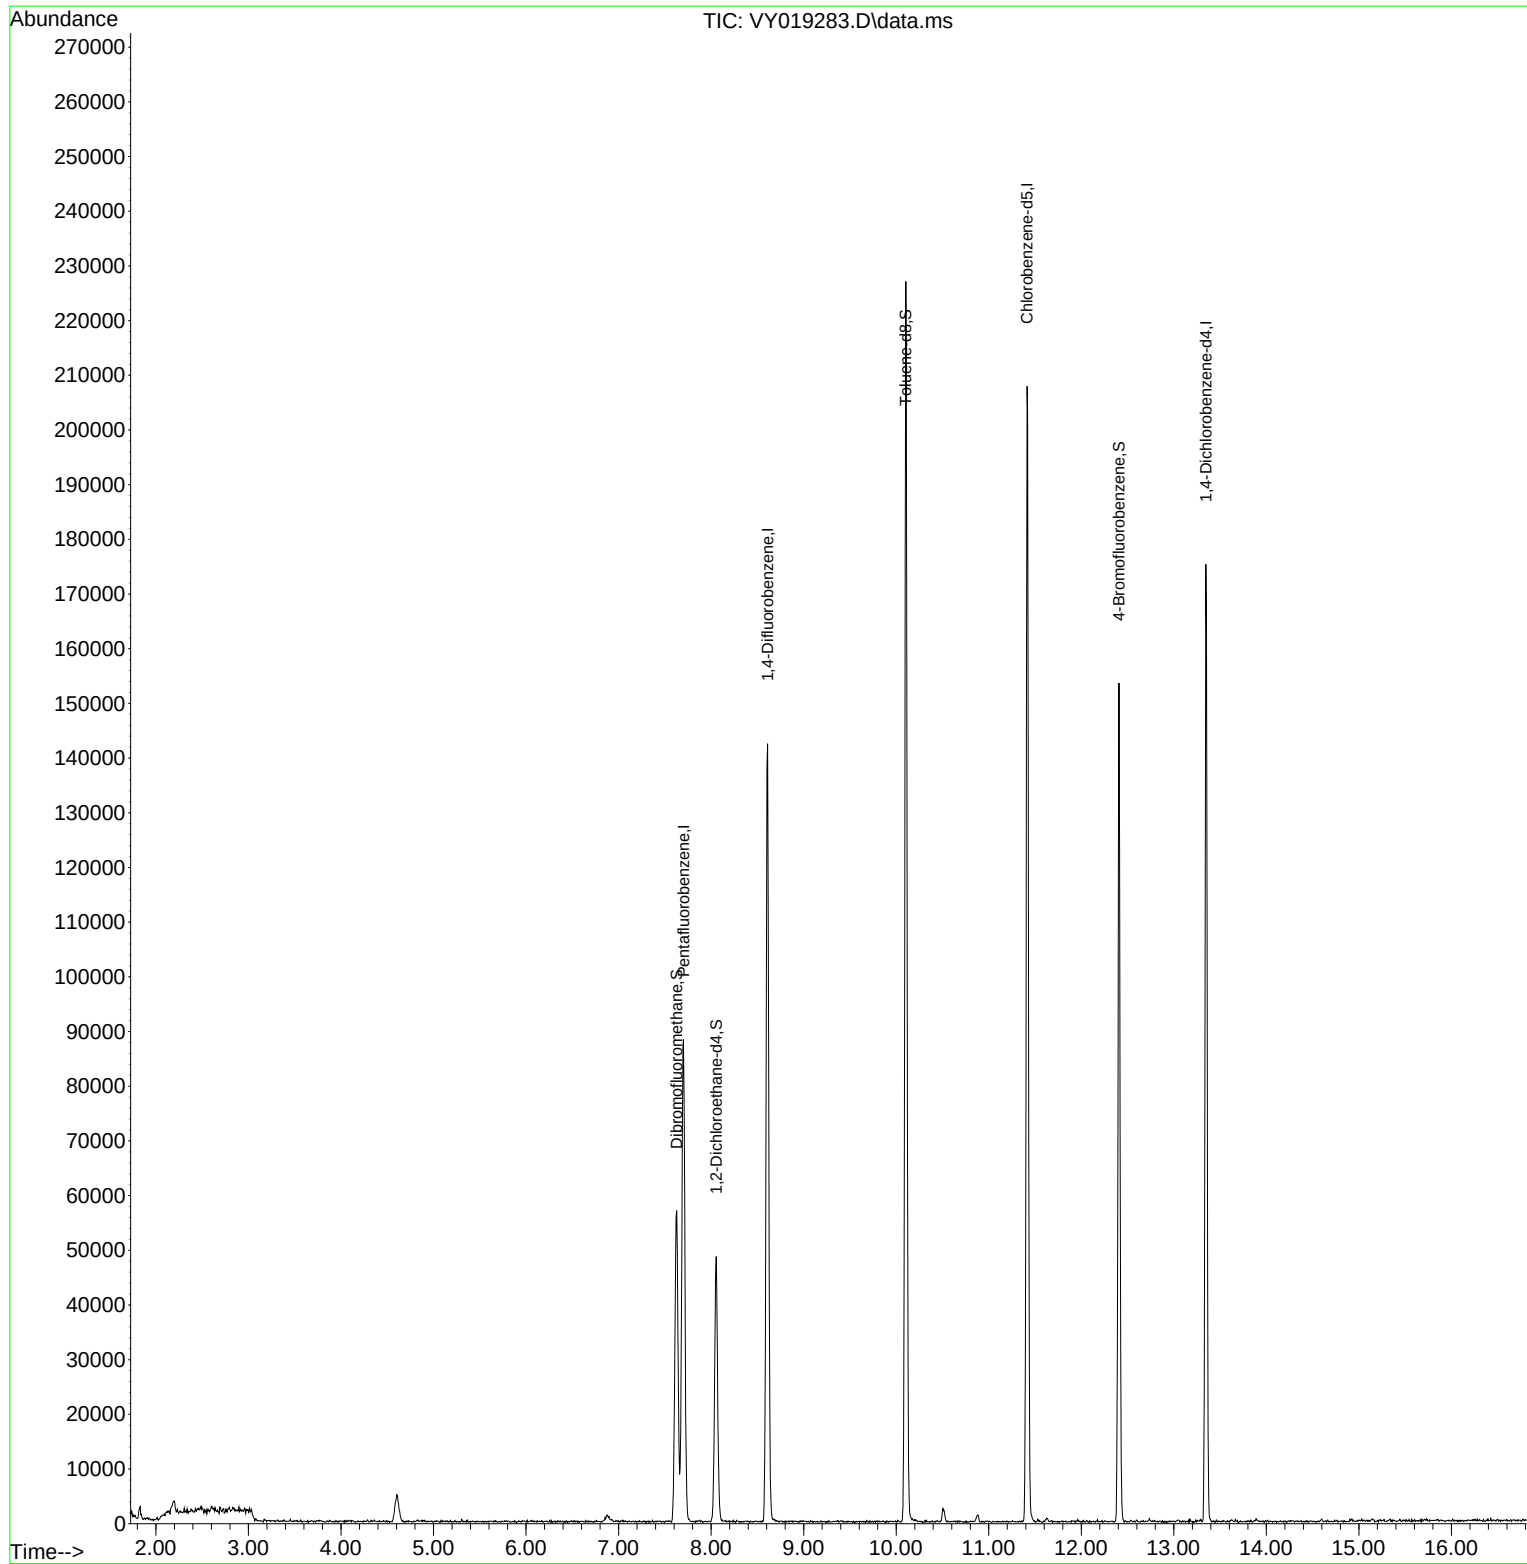


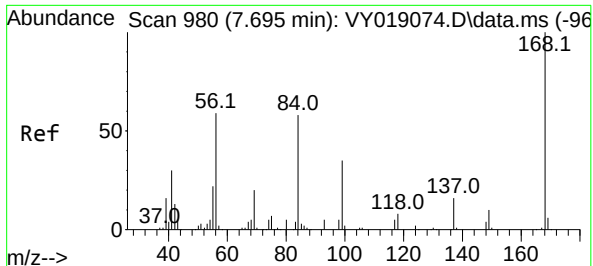

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.701 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY019283.D
Acq: 27 Aug 2024 13:57




Instrument :
MSVOA_Y
ClientSampleId :
EO-01-08222024


Tgt Ion:168 Resp: 71543
Ion Ratio Lower Upper
168 100
99 55.0 39.1 58.7

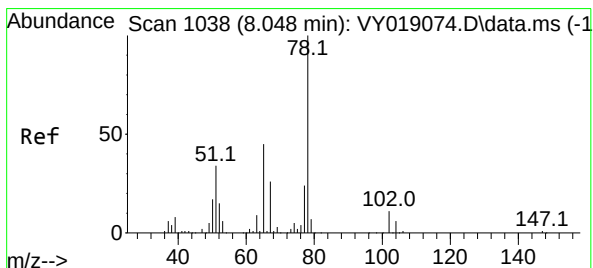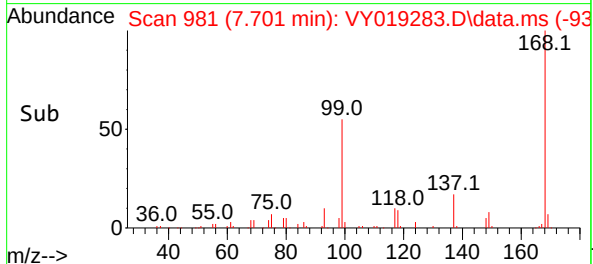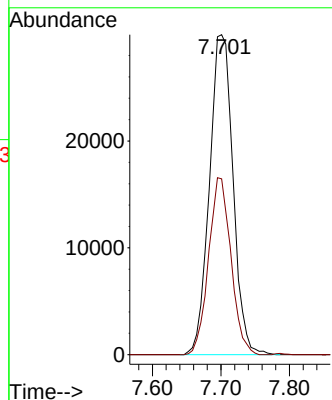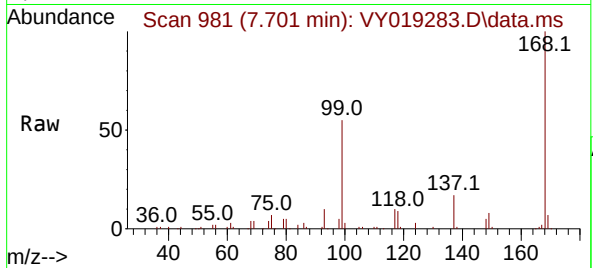

#33
1,2-Dichloroethane-d4
Concen: 51.188 ug/l
RT: 8.055 min Scan# 1039
Delta R.T. 0.006 min
Lab File: VY019283.D
Acq: 27 Aug 2024 13:57

Tgt Ion: 65 Resp: 36710
Ion Ratio Lower Upper
65 100
67 52.3 0.0 109.6


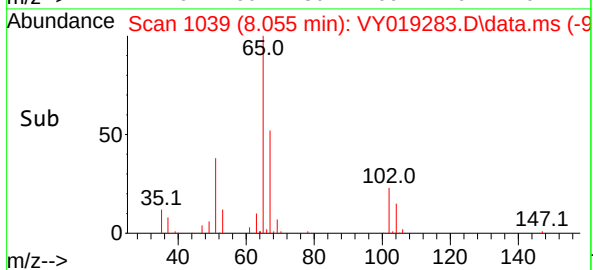
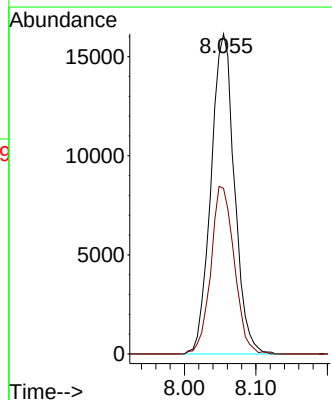
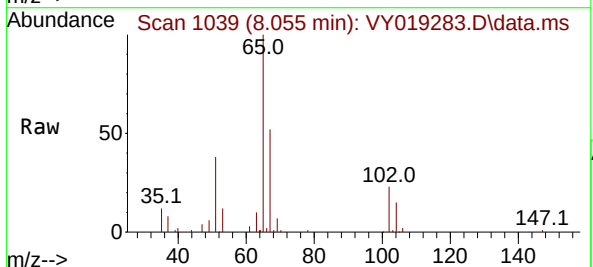


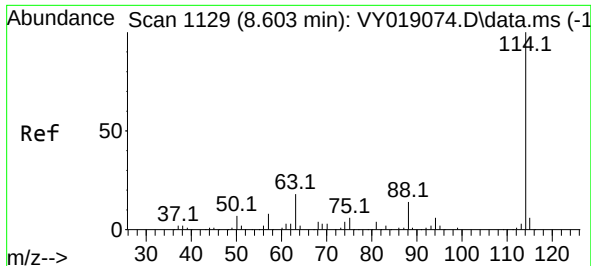

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.609 min Scan# 1129
Delta R.T. 0.006 min
Lab File: VY019283.D
Acq: 27 Aug 2024 13:57




Instrument :
MSVOA_Y
ClientSampleId :
EO-01-08222024


Tgt Ion:114 Resp: 126336
Ion Ratio Lower Upper
114 100
63 19.9 0.0 35.0
88 13.6 0.0 27.2

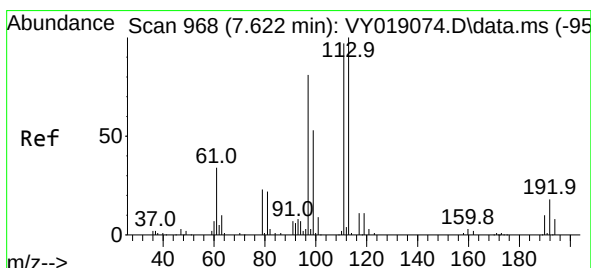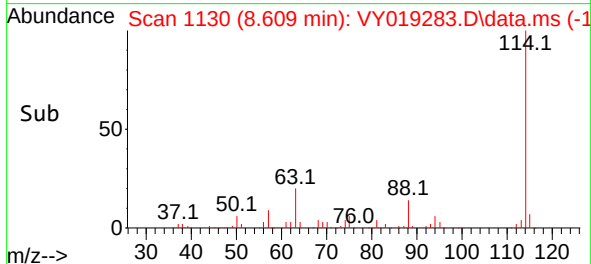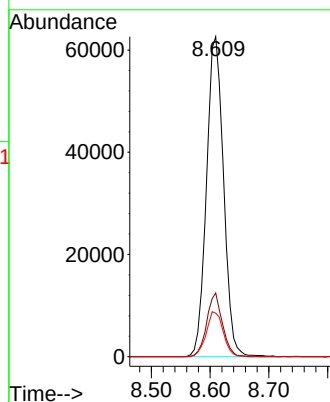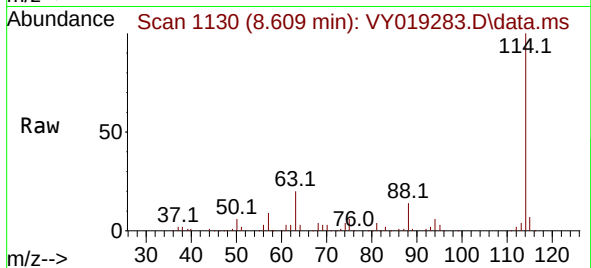

#35
Dibromofluoromethane
Concen: 48.988 ug/l
RT: 7.628 min Scan# 969
Delta R.T. 0.006 min
Lab File: VY019283.D
Acq: 27 Aug 2024 13:57

Tgt Ion:113 Resp: 40467
Ion Ratio Lower Upper
113 100
111 102.7 82.2 123.4
192 20.1 15.9 23.9


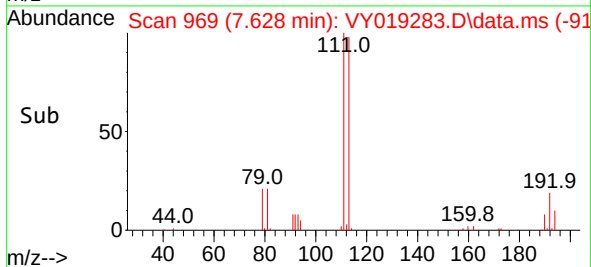
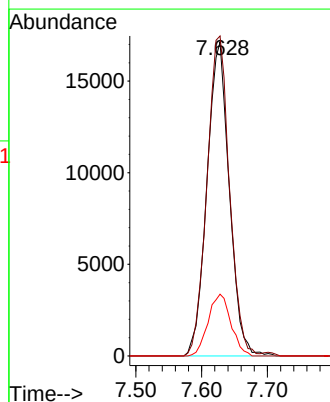
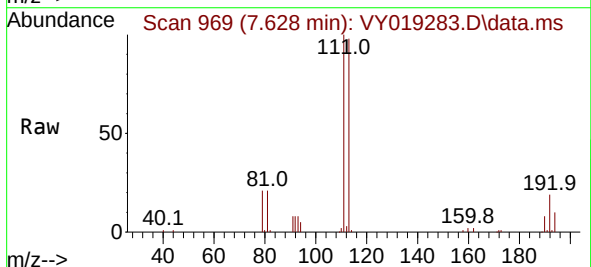


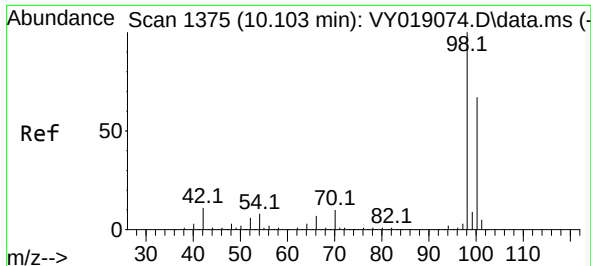

#50
Toluene-d8
Concen: 47.839 ug/l
RT: 10.103 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY019283.D
Acq: 27 Aug 2024 13:57




Instrument :
MSVOA_Y
ClientSampleId :
EO-01-08222024


Tgt Ion: 98 Resp: 142211
Ion Ratio Lower Upper
98 100
100 67.9 52.0 78.0

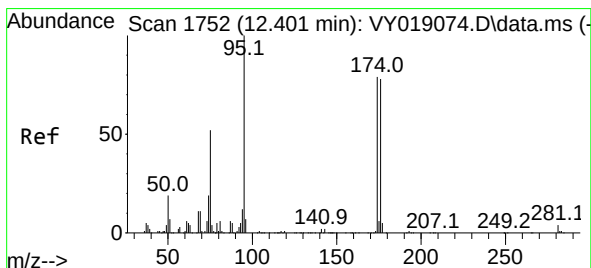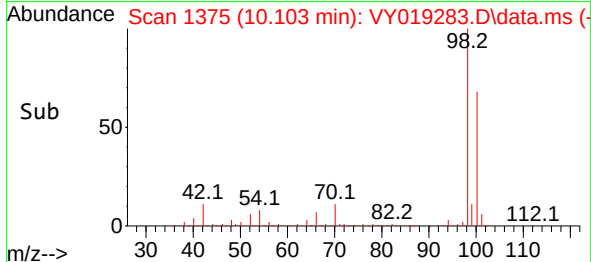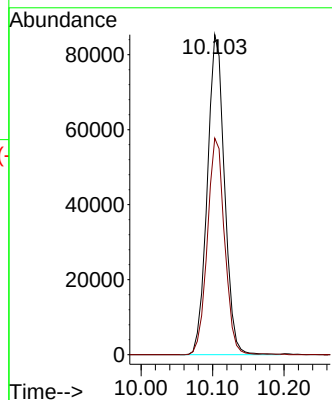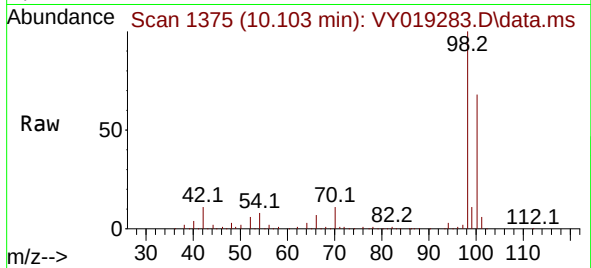

#62
4-Bromofluorobenzene
Concen: 42.911 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.006 min
Lab File: VY019283.D
Acq: 27 Aug 2024 13:57

Tgt Ion: 95 Resp: 43486
Ion Ratio Lower Upper
95 100
174 87.4 0.0 175.6
176 87.1 0.0 171.4


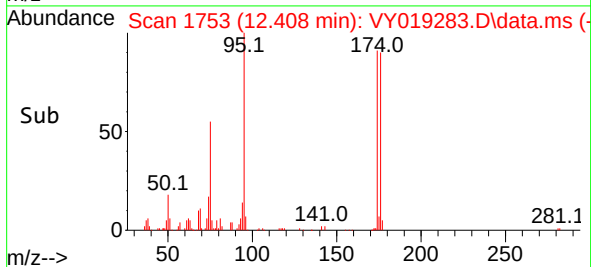
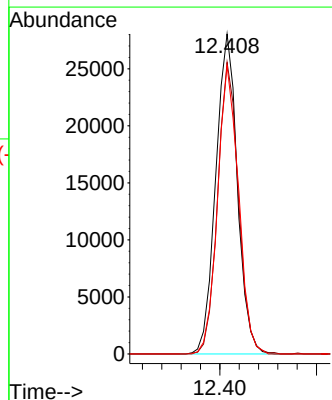
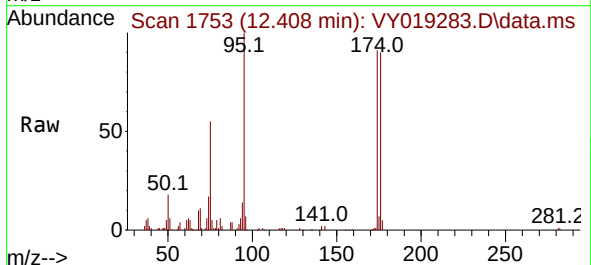


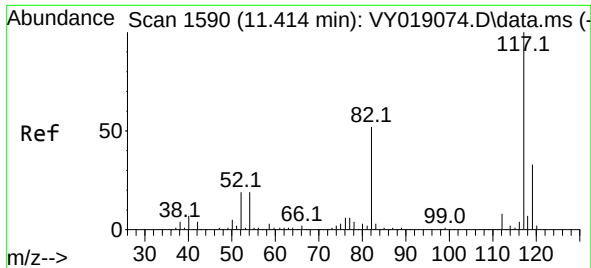

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY019283.D
Acq: 27 Aug 2024 13:57

Instrument :
MSVOA_Y
ClientSampleId :
EO-01-08222024

Tgt Ion:117 Resp: 115524
Ion Ratio Lower Upper
117 100
82 51.6 42.4 63.6
119 32.1 25.9 38.9

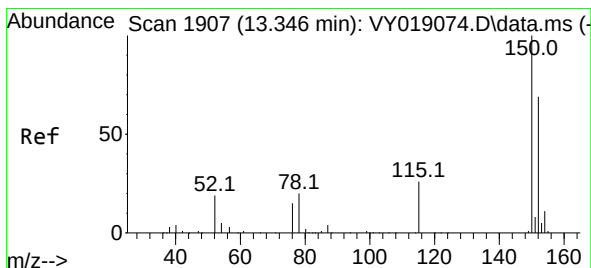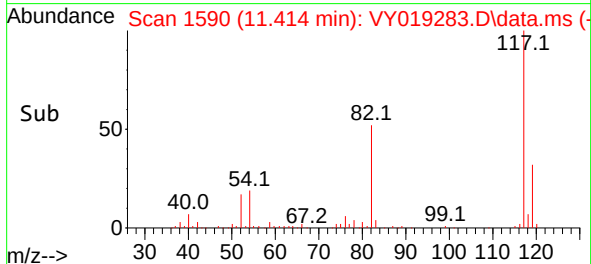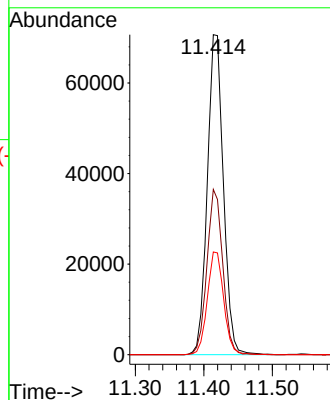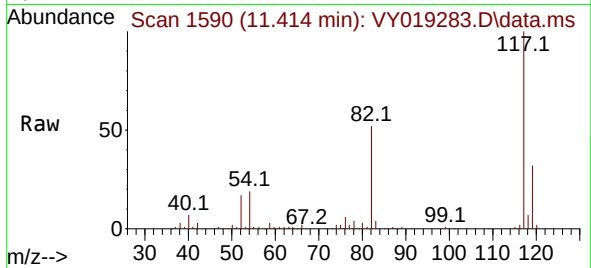

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.346 min Scan# 1907
Delta R.T. 0.000 min
Lab File: VY019283.D
Acq: 27 Aug 2024 13:57

Tgt Ion:152 Resp: 44275
Ion Ratio Lower Upper
152 100
115 56.1 28.2 84.7
150 158.3 0.0 345.6

