

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082724\
 Data File : VY019304.D
 Acq On : 28 Aug 2024 00:56
 Operator : SY/MD
 Sample : P3717-01
 Misc : 5.08g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-1

Quant Time: Aug 28 03:34:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081524S.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 16 05:10:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.701	168	107692	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.609	114	186582	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	167074	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	61189	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.055	65	57126	52.918	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	105.840%
35) Dibromofluoromethane	7.628	113	59287	48.597	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	97.200%
50) Toluene-d8	10.103	98	211720	48.224	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	96.440%
62) 4-Bromofluorobenzene	12.408	95	61970	41.406	ug/l	0.00
Spiked Amount	50.000	Range	29 - 146	Recovery	=	82.820%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082724\
Data File : VY019304.D
Acq On : 28 Aug 2024 00:56
Operator : SY/MD
Sample : P3717-01
Misc : 5.08g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TP-1

Quant Time: Aug 28 03:34:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081524S.M
Quant Title : SW846 8260
QLast Update : Fri Aug 16 05:10:30 2024
Response via : Initial Calibration




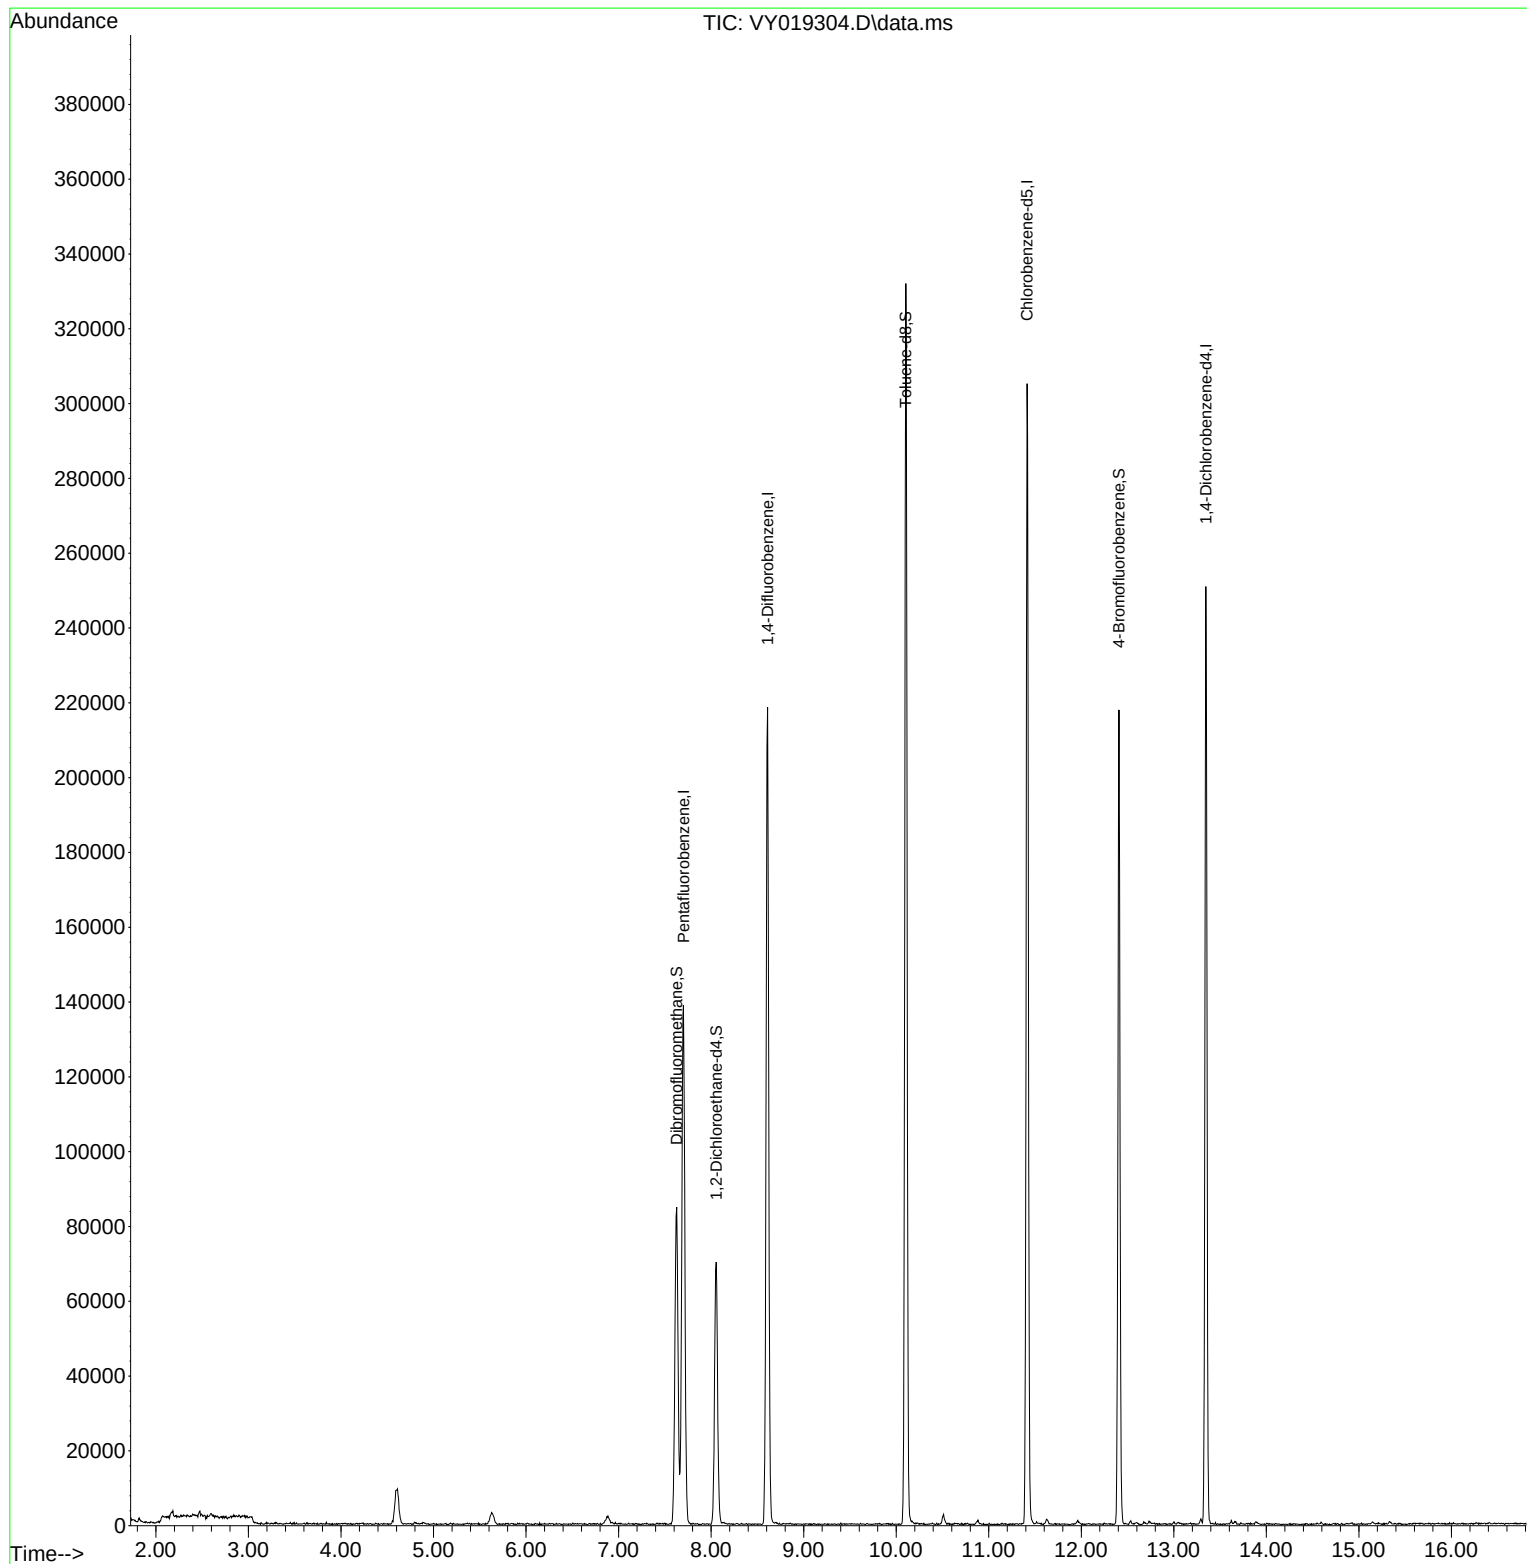


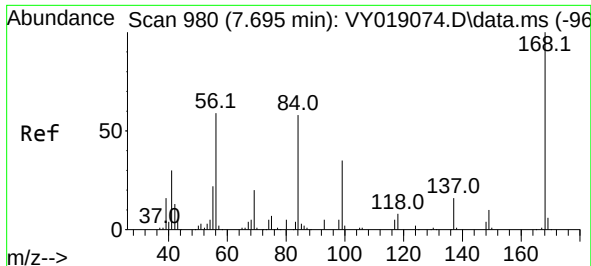

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.701 min Scan# 981
Delta R.T. 0.006 min
Lab File: VY019304.D
Acq: 28 Aug 2024 00:56




Instrument :
MSVOA_Y
ClientSampleId :
TP-1


Tgt Ion:168 Resp: 107692
Ion Ratio Lower Upper
168 100
99 54.6 39.1 58.7

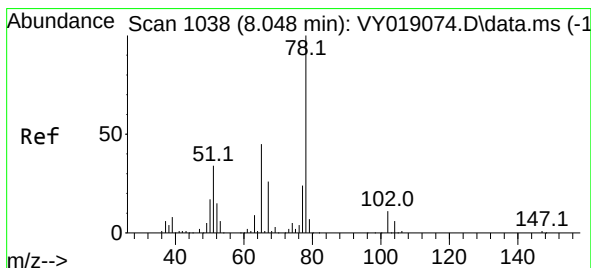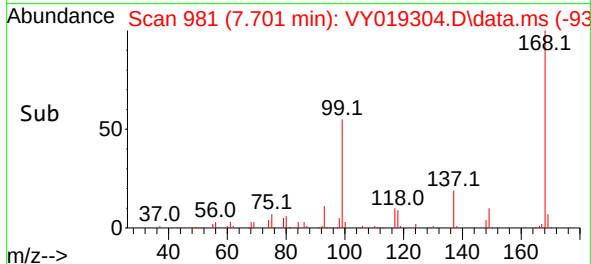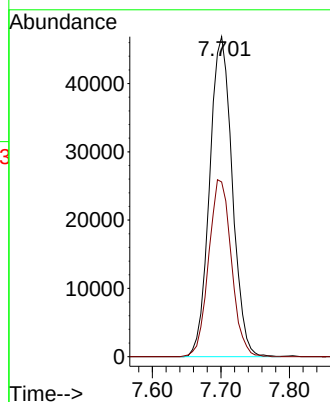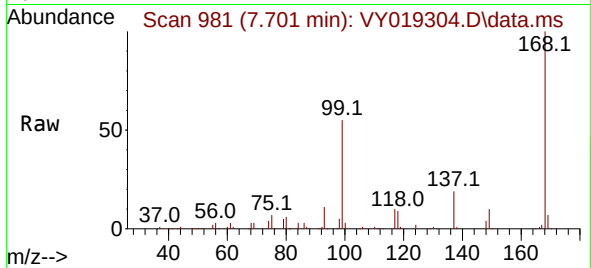

#33
1,2-Dichloroethane-d4
Concen: 52.918 ug/l
RT: 8.055 min Scan# 1039
Delta R.T. 0.006 min
Lab File: VY019304.D
Acq: 28 Aug 2024 00:56

Tgt Ion: 65 Resp: 57126
Ion Ratio Lower Upper
65 100
67 50.0 0.0 109.6

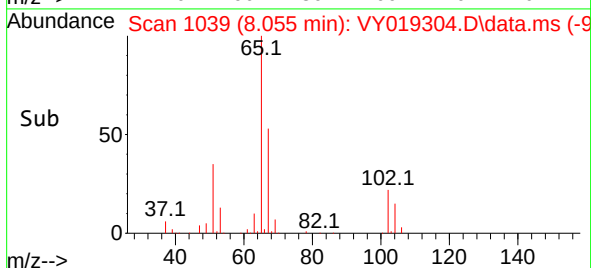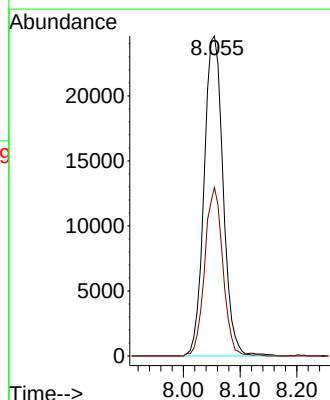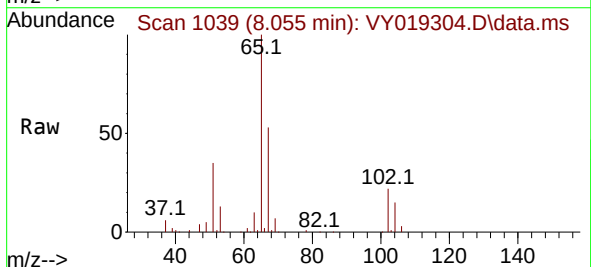

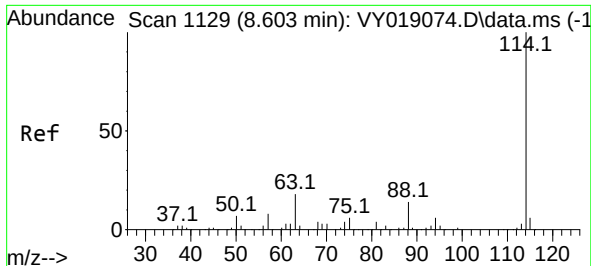

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.609 min Scan# 1129

Delta R.T. 0.006 min

Lab File: VY019304.D

Acq: 28 Aug 2024 00:56

Instrument :

MSVOA_Y

ClientSampleId :

TP-1





Tgt Ion:114 Resp: 186582

Ion Ratio Lower Upper

114 100

63 19.3 0.0 35.0

88 14.9 0.0 27.2

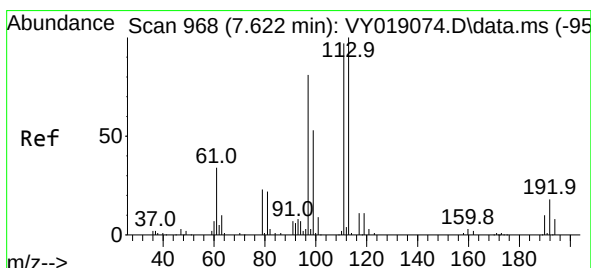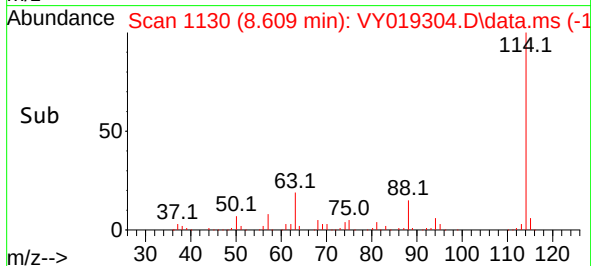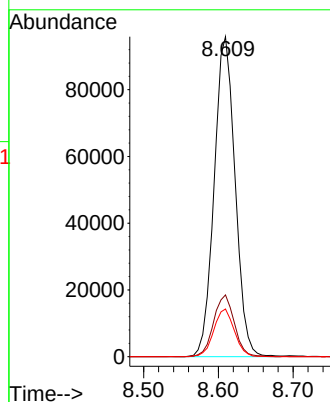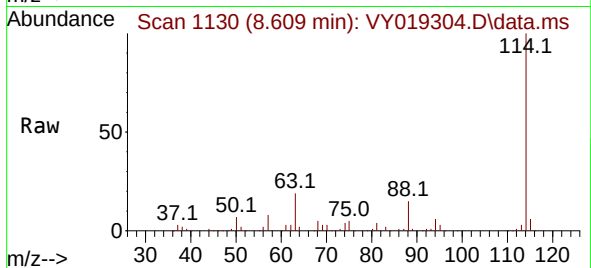

#35

Dibromofluoromethane

Concen: 48.597 ug/l

RT: 7.628 min Scan# 969

Delta R.T. 0.006 min

Lab File: VY019304.D

Acq: 28 Aug 2024 00:56




Tgt Ion:113 Resp: 59287


Ion Ratio Lower Upper

113 100

111 102.8 82.2 123.4

192 19.1 15.9 23.9


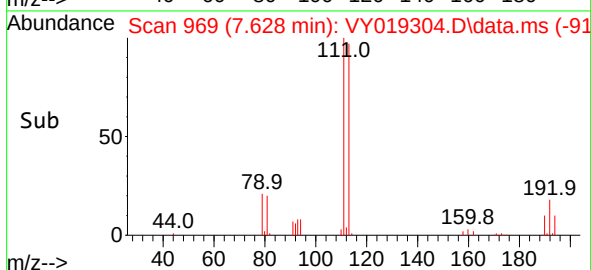
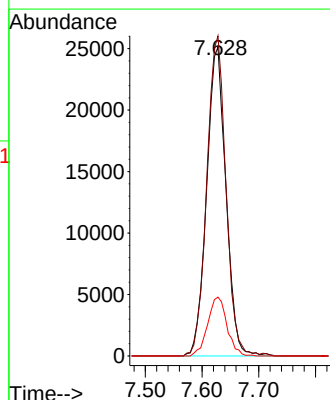
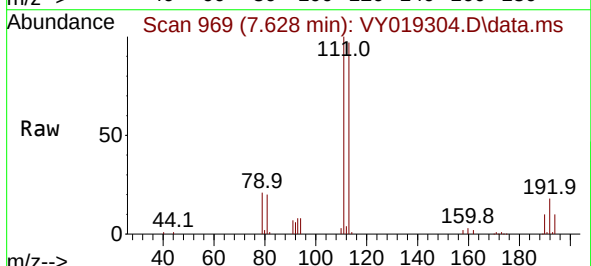


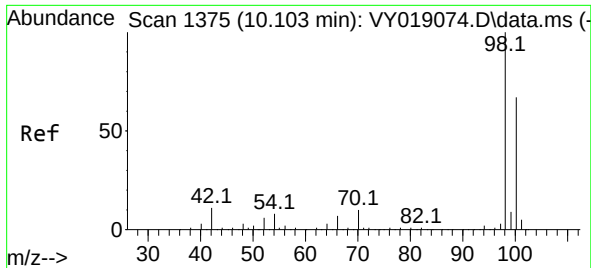

#50
Toluene-d8
Concen: 48.224 ug/l
RT: 10.103 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY019304.D
Acq: 28 Aug 2024 00:56




Instrument :
MSVOA_Y
ClientSampleId :
TP-1


Tgt Ion: 98 Resp: 211720
Ion Ratio Lower Upper
98 100
100 67.6 52.0 78.0

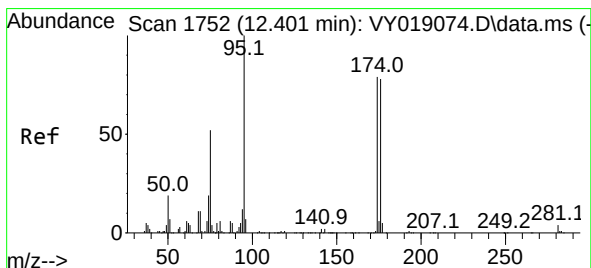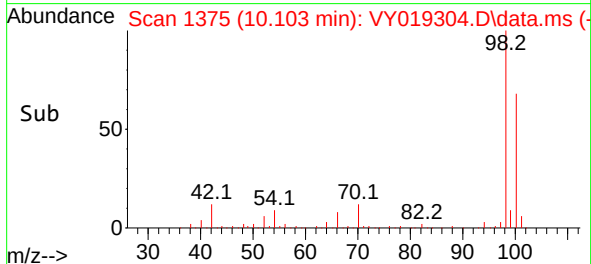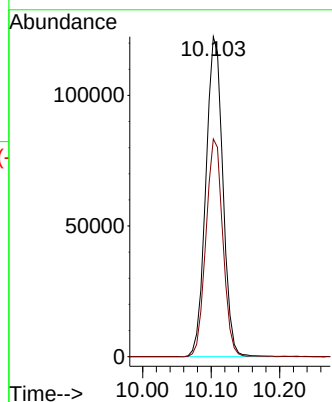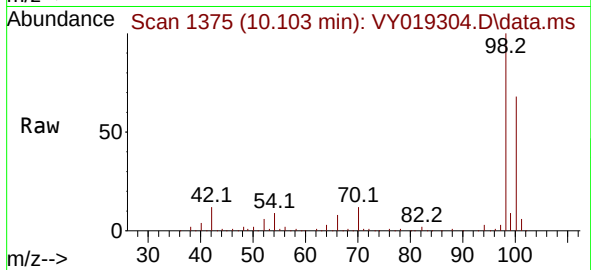

#62
4-Bromofluorobenzene
Concen: 41.406 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.006 min
Lab File: VY019304.D
Acq: 28 Aug 2024 00:56

Tgt Ion: 95 Resp: 61970
Ion Ratio Lower Upper
95 100
174 89.1 0.0 175.6
176 85.2 0.0 171.4


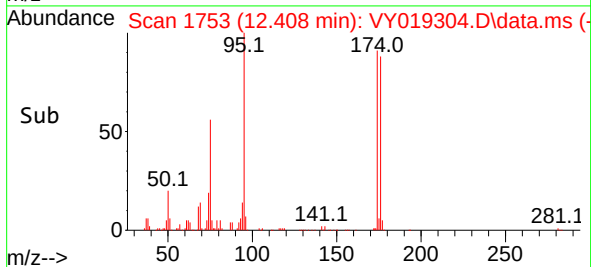
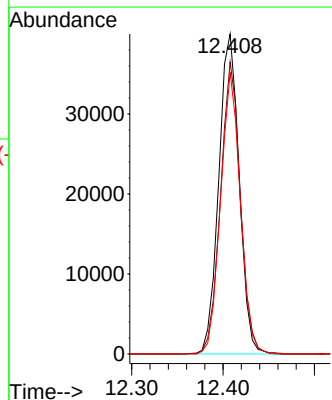
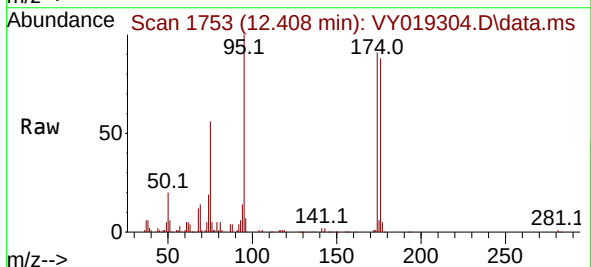


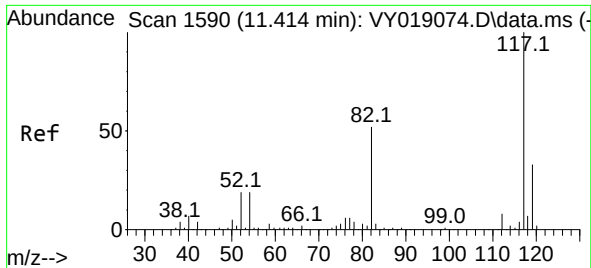

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY019304.D
Acq: 28 Aug 2024 00:56

Instrument :
MSVOA_Y
ClientSampleId :
TP-1

Tgt Ion:117 Resp: 167074
Ion Ratio Lower Upper
117 100
82 54.4 42.4 63.6
119 32.6 25.9 38.9

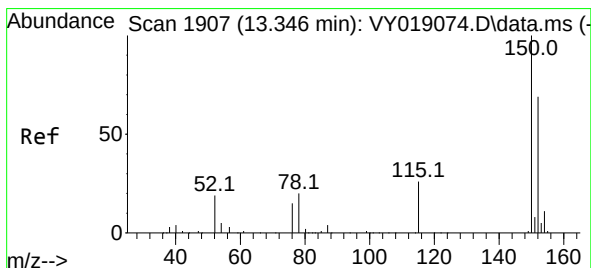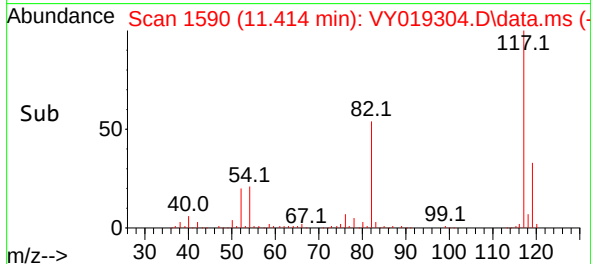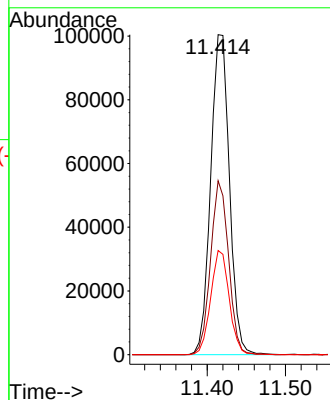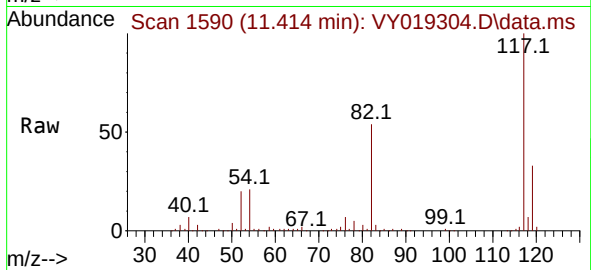

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.346 min Scan# 1907
Delta R.T. 0.000 min
Lab File: VY019304.D
Acq: 28 Aug 2024 00:56

Tgt Ion:152 Resp: 61189
Ion Ratio Lower Upper
152 100
115 57.4 28.2 84.7
150 157.3 0.0 345.6

