

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY083023\
 Data File : VY015386.D
 Acq On : 30 Aug 2023 18:36
 Operator : SY/MD
 Sample : 04202-02
 Misc : 4.16g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 C-2

Quant Time: Aug 31 01:03:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y082923S.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 29 22:47:33 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	206315	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	356111	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	309565	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	120740	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	132937	60.107	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	120.220%
35) Dibromofluoromethane	7.710	113	111957	54.583	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	109.160%
50) Toluene-d8	10.179	98	415871	55.988	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	111.980%
62) 4-Bromofluorobenzene	12.477	95	124960	45.316	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	90.640%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY083023\
Data File : VY015386.D
Acq On : 30 Aug 2023 18:36
Operator : SY/MD
Sample : 04202-02
Misc : 4.16g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
C-2


Quant Time: Aug 31 01:03:44 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y082923S.M
Quant Title : SW846 8260
QLast Update : Tue Aug 29 22:47:33 2023
Response via : Initial Calibration

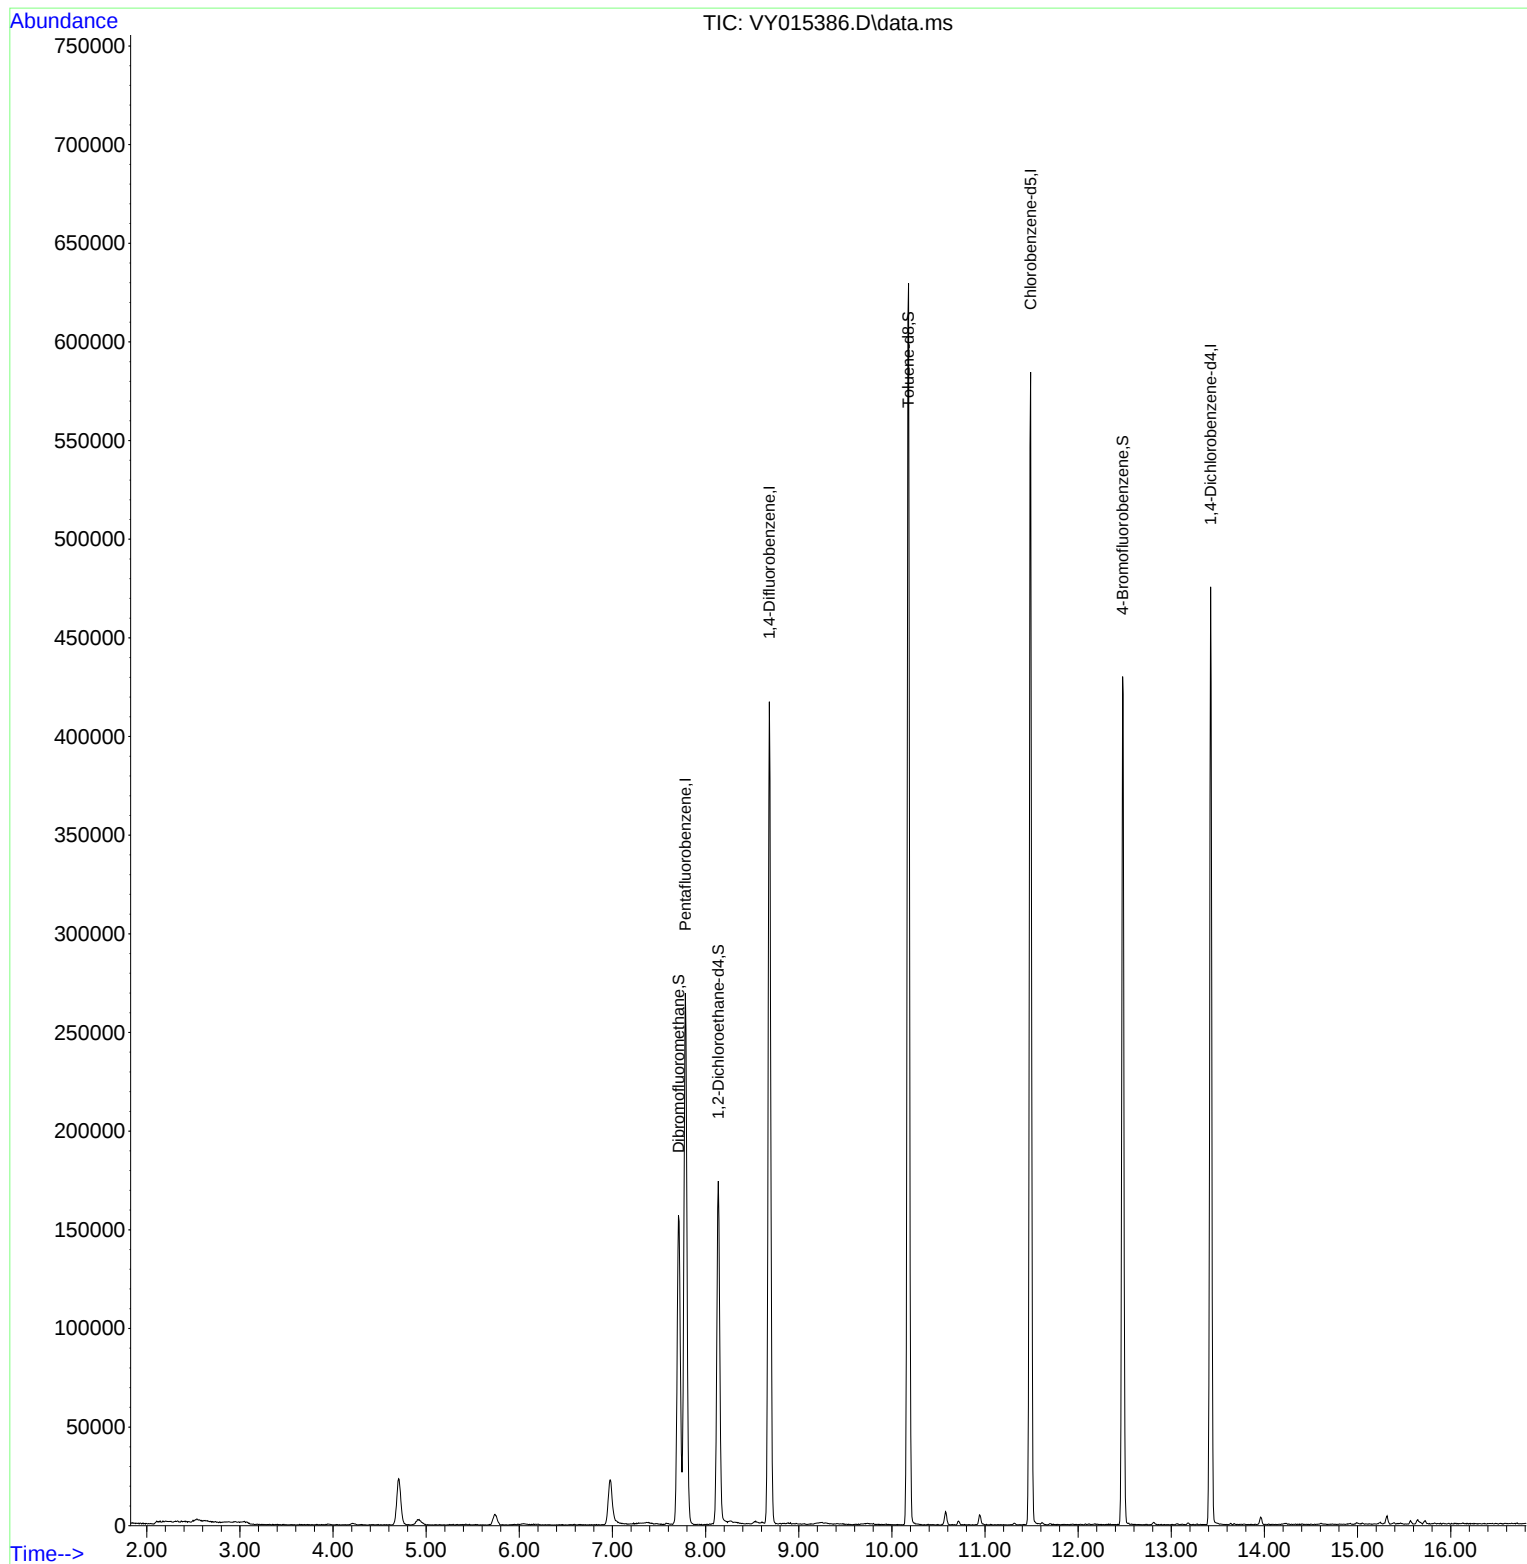



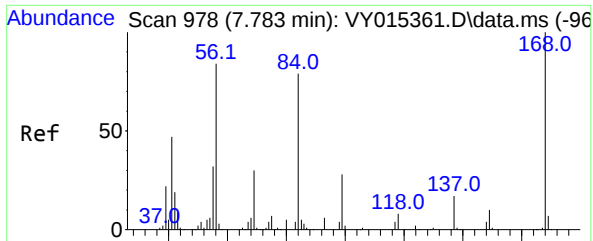


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY015386.D
Acq: 30 Aug 2023 18:36

Instrument :
MSVOA_Y
ClientSampleId :
C-2



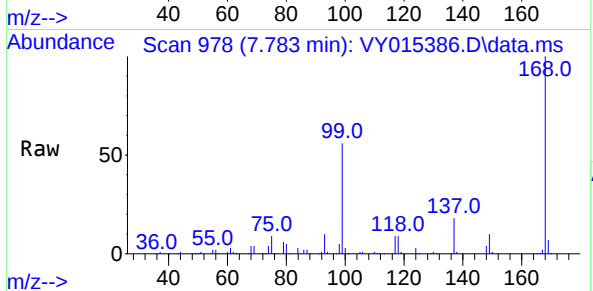



Tgt Ion:168 Resp: 206315
Ion Ratio Lower Upper
168 100
99 56.1 43.4 65.0

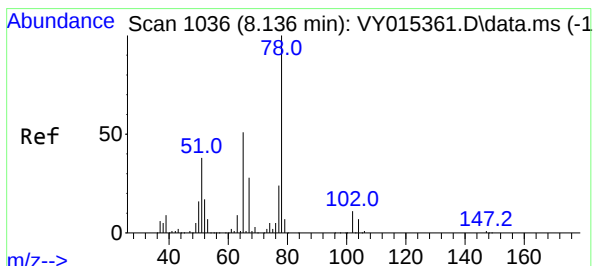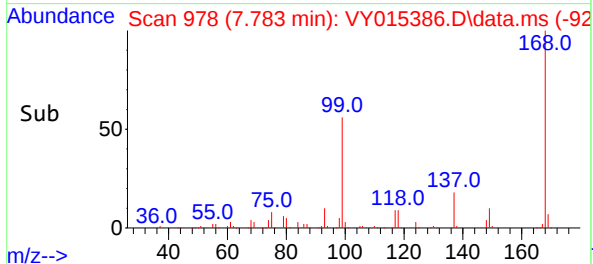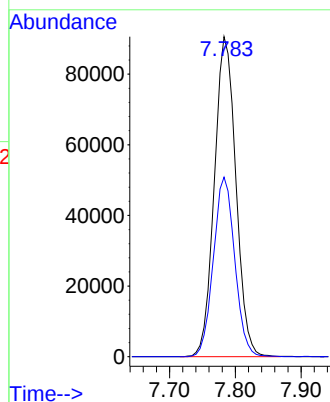

#33
1,2-Dichloroethane-d4
Concen: 60.107 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. -0.000 min
Lab File: VY015386.D
Acq: 30 Aug 2023 18:36

Tgt Ion: 65 Resp: 132937
Ion Ratio Lower Upper
65 100
67 52.9 0.0 101.8

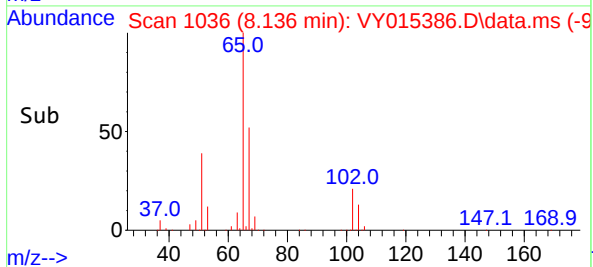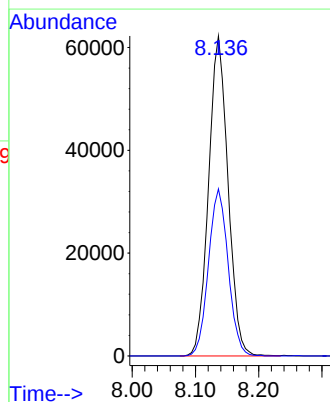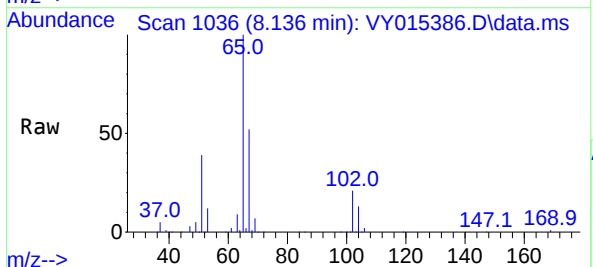




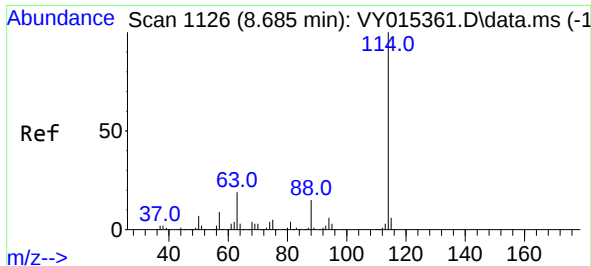


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.685 min Scan# 1126
Delta R.T. -0.000 min
Lab File: VY015386.D
Acq: 30 Aug 2023 18:36

Instrument :
MSVOA_Y
ClientSampleId :
C-2

Tgt Ion:114 Resp: 356111




Ion	Ratio	Lower	Upper
114	100		
63	19.3	0.0	42.4
88	14.3	0.0	30.6

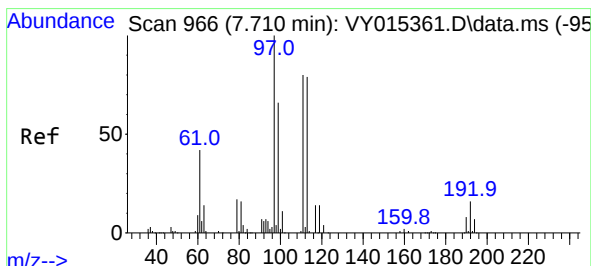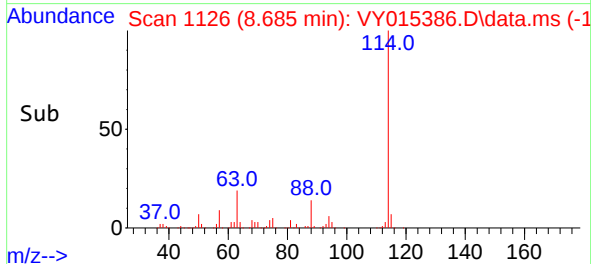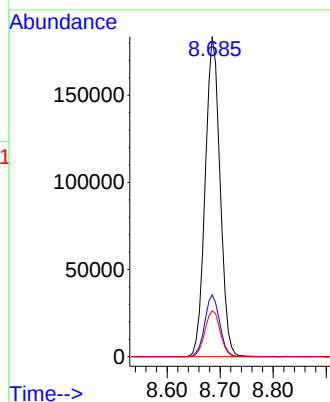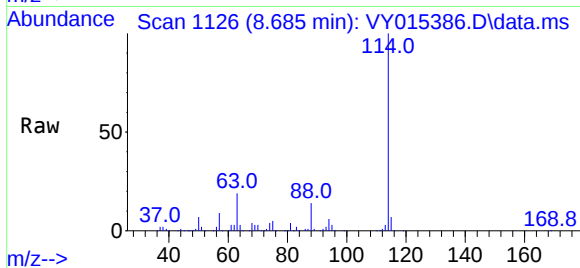


#35
Dibromofluoromethane
Concen: 54.583 ug/l
RT: 7.710 min Scan# 966
Delta R.T. -0.006 min
Lab File: VY015386.D
Acq: 30 Aug 2023 18:36

Tgt Ion:113 Resp: 111957

Ion	Ratio	Lower	Upper
113	100		
111	101.2	81.3	121.9
192	19.5	16.9	25.3


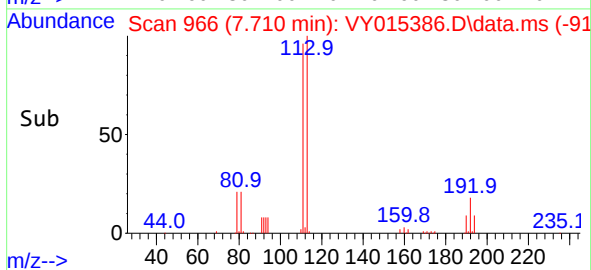
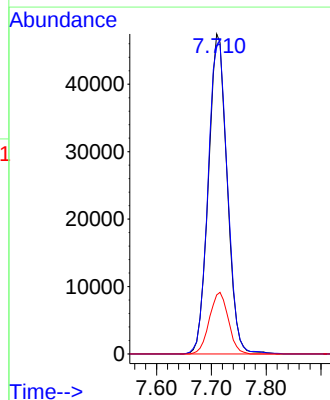
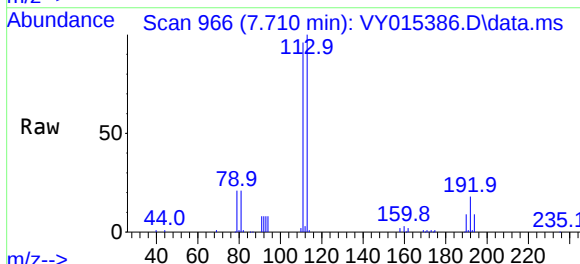


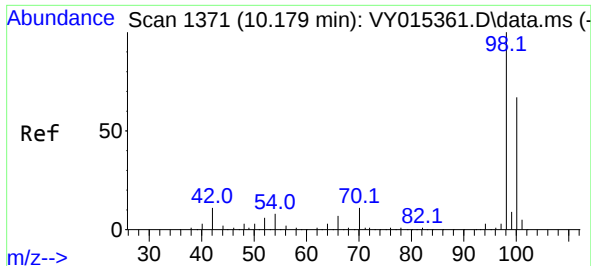

#50
Toluene-d8
Concen: 55.988 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY015386.D
Acq: 30 Aug 2023 18:36




Instrument :
MSVOA_Y
ClientSampleId :
C-2


Tgt Ion: 98 Resp: 415871
Ion Ratio Lower Upper
98 100
100 65.2 50.1 75.1

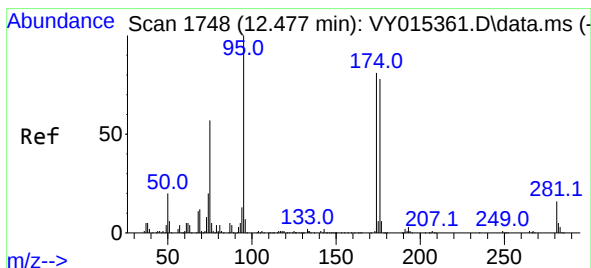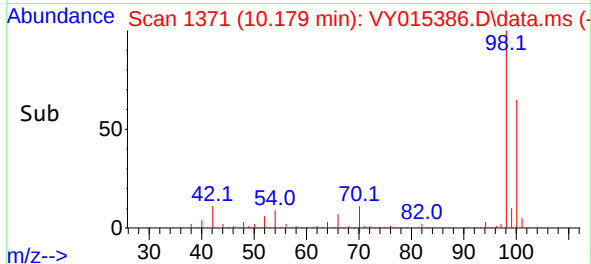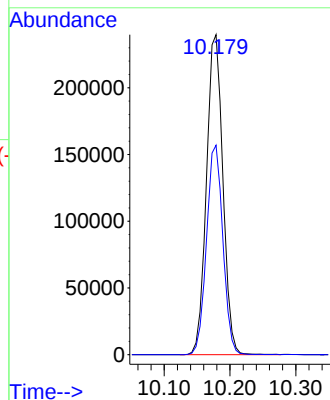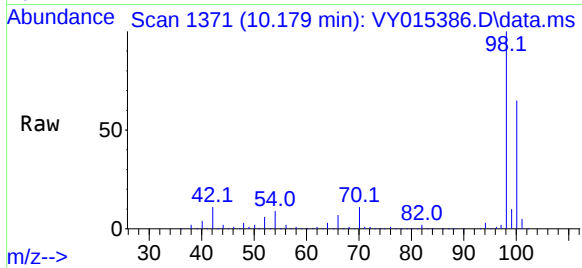

#62
4-Bromofluorobenzene
Concen: 45.316 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.000 min
Lab File: VY015386.D
Acq: 30 Aug 2023 18:36

Tgt Ion: 95 Resp: 124960
Ion Ratio Lower Upper
95 100
174 85.9 0.0 178.2
176 82.5 0.0 173.8


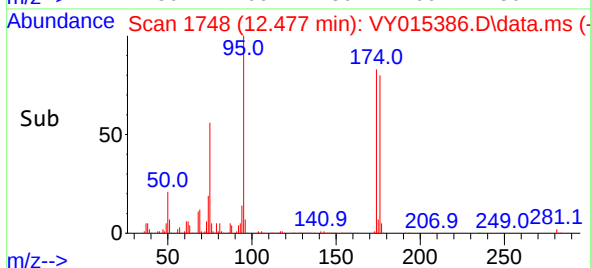
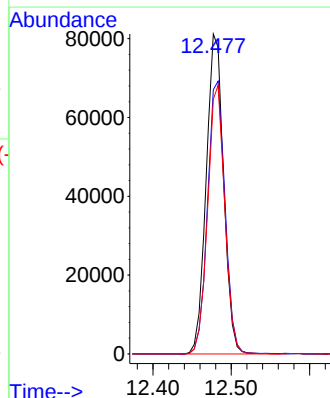
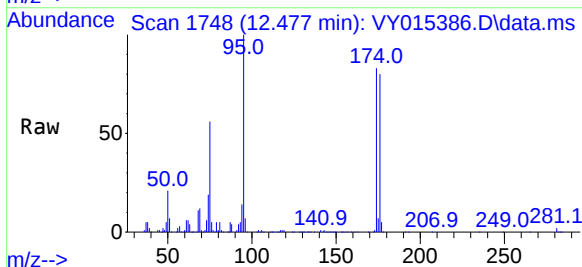


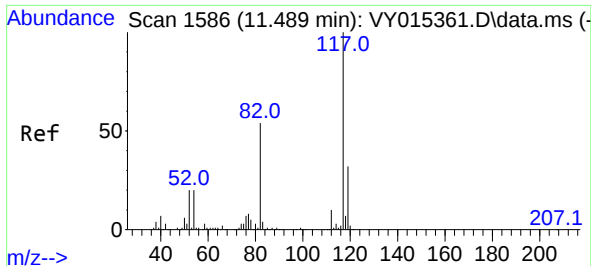

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 117
Delta R.T. -0.000 min
Lab File: VY015386.D
Acq: 30 Aug 2023 18:36

Instrument :
MSVOA_Y
ClientSampleId :
C-2

Tgt Ion:117 Resp: 309565
Ion Ratio Lower Upper
117 100
82 54.0 43.4 65.0
119 32.3 26.3 39.5

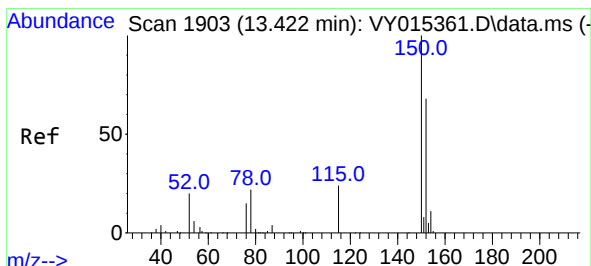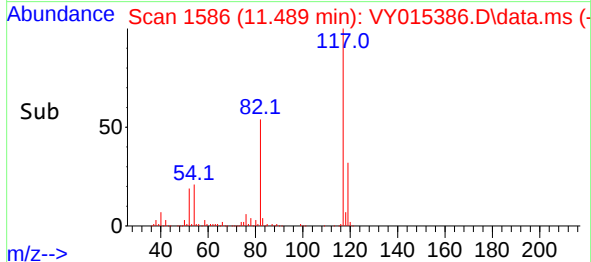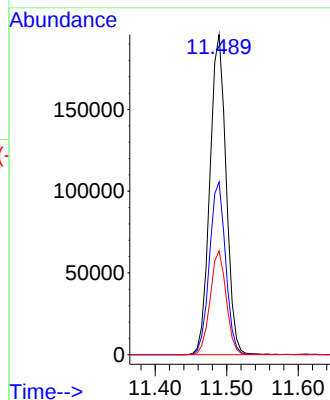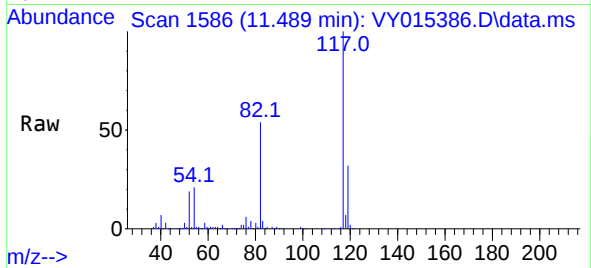

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.000 min
Lab File: VY015386.D
Acq: 30 Aug 2023 18:36

Tgt Ion:152 Resp: 120740
Ion Ratio Lower Upper
152 100
115 57.1 28.8 86.5
150 156.2 0.0 348.8

