

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY083121\
 Data File : VY005912.D
 Acq On : 31 Aug 2021 15:10
 Operator : SY/MD
 Sample : M3602-09
 Misc : 4.83G/5ML/MSVOA_Y/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-1COMP

Quant Time: Sep 01 05:37:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y083121S.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 01 05:32:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.801	168	199038	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	338126	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	358094	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	184866	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	124923	62.282	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	124.560%
35) Dibromofluoromethane	7.728	113	104329	54.942	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	109.880%
50) Toluene-d8	10.185	98	436776	54.807	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	109.620%
62) 4-Bromofluorobenzene	12.483	95	157816	58.975	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	117.960%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY083121\
Data File : VY005912.D
Acq On : 31 Aug 2021 15:10
Operator : SY/MD
Sample : M3602-09
Misc : 4.83G/5ML/MSVOA_Y/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TP-1COMP

Quant Time: Sep 01 05:37:23 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y083121S.M
Quant Title : SW846 8260
QLast Update : Wed Sep 01 05:32:43 2021
Response via : Initial Calibration




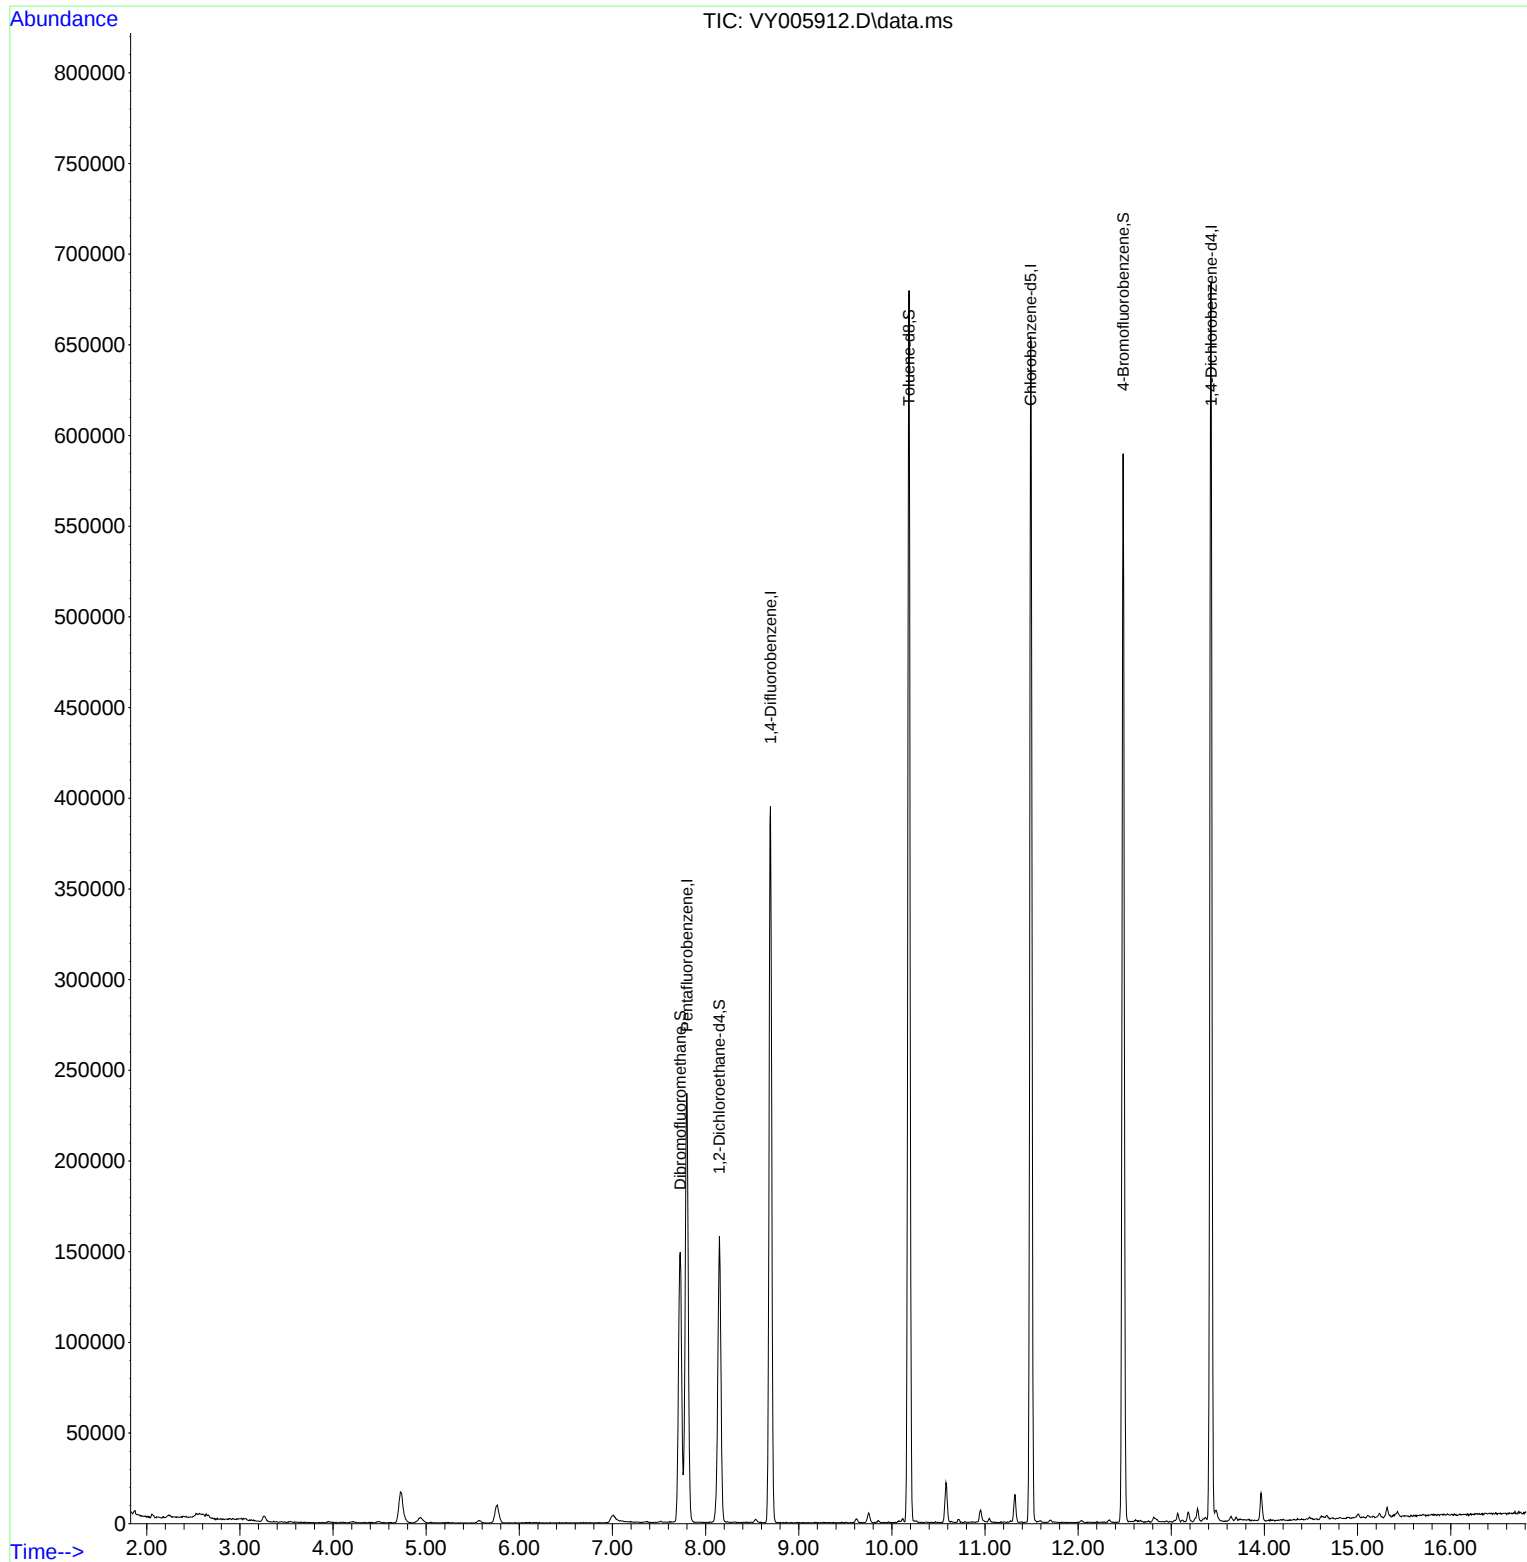


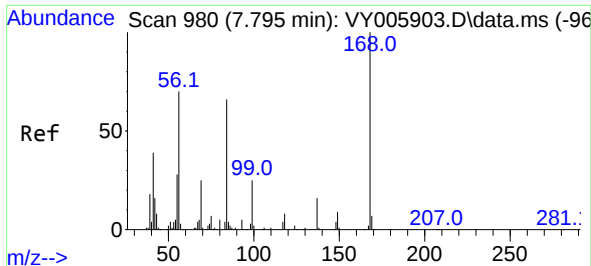

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.801 min Scan# 981
Delta R.T. 0.006 min
Lab File: VY005912.D
Acq: 31 Aug 2021 15:10




Instrument :
MSVOA_Y
ClientSampleId :
TP-1COMP


Tgt Ion:168 Resp: 199038
Ion Ratio Lower Upper
168 100
99 50.3 40.6 60.8

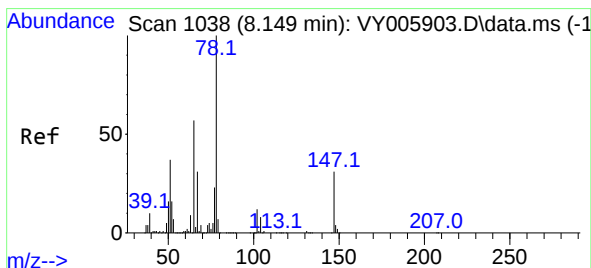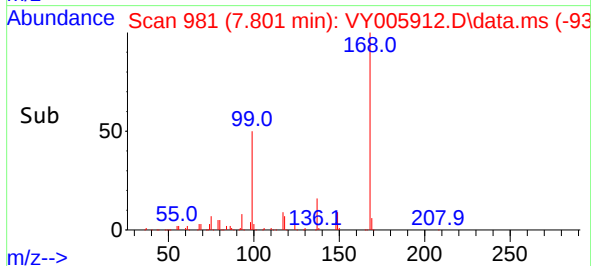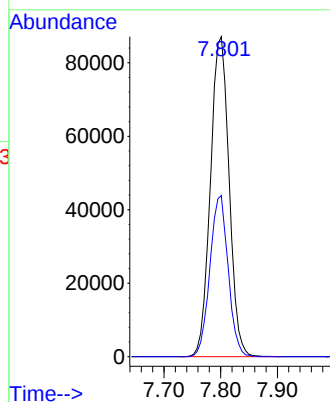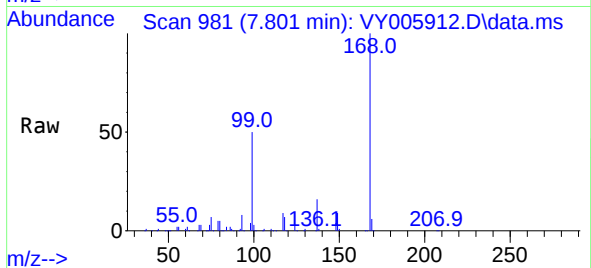

#33
1,2-Dichloroethane-d4
Concen: 62.282 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. 0.000 min
Lab File: VY005912.D
Acq: 31 Aug 2021 15:10

Tgt Ion: 65 Resp: 124923
Ion Ratio Lower Upper
65 100
67 50.5 0.0 105.4

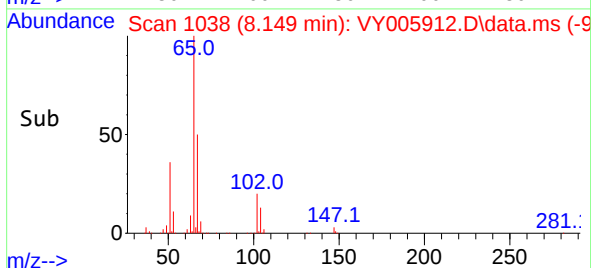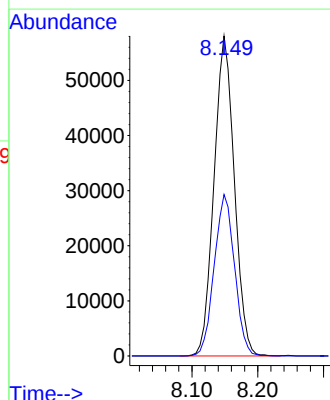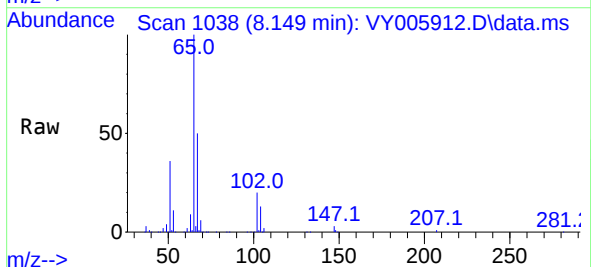




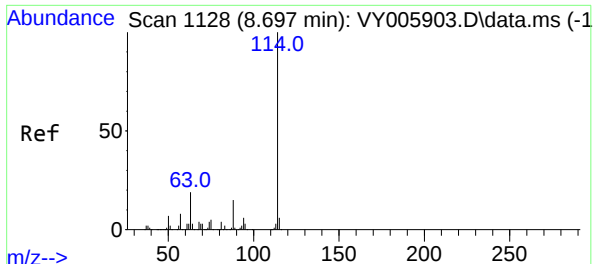


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. 0.000 min
Lab File: VY005912.D
Acq: 31 Aug 2021 15:10

Instrument :
MSVOA_Y
ClientSampleId :
TP-1COMP




Tgt Ion:	114	Resp:	338126
Ion	Ratio	Lower	Upper
114	100		
63	19.8	0.0	38.4
88	14.9	0.0	30.0

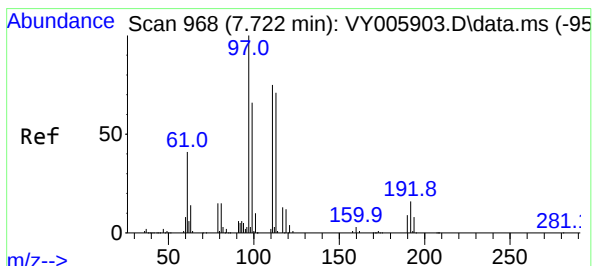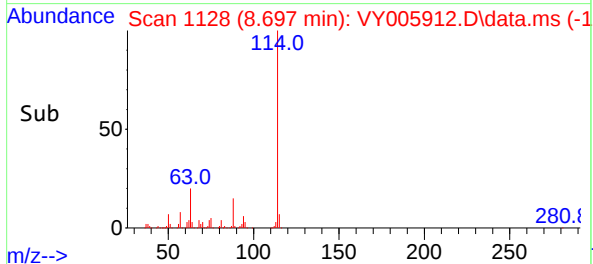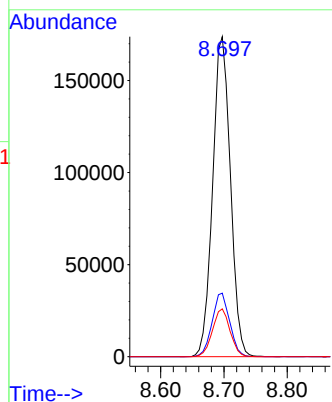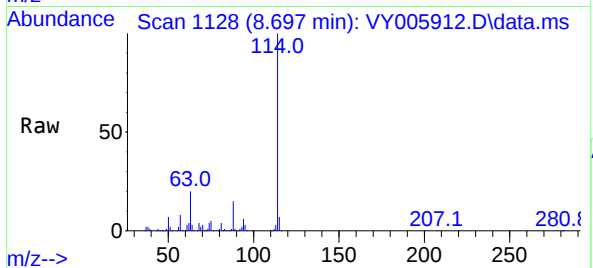


#35

Dibromofluoromethane
Concen: 54.942 ug/l
RT: 7.728 min Scan# 969
Delta R.T. 0.006 min
Lab File: VY005912.D
Acq: 31 Aug 2021 15:10

Tgt Ion:	113	Resp:	104329
Ion	Ratio	Lower	Upper
113	100		
111	101.8	81.9	122.9
192	23.7	19.4	29.0


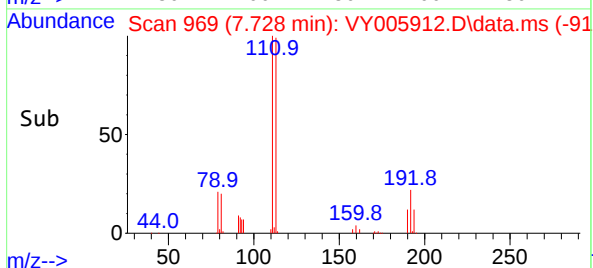
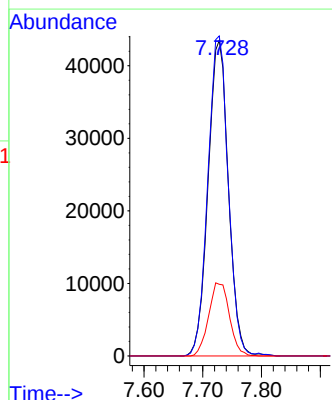
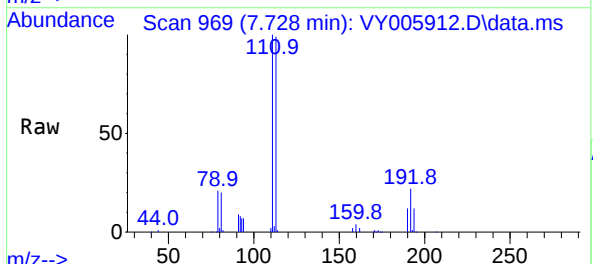


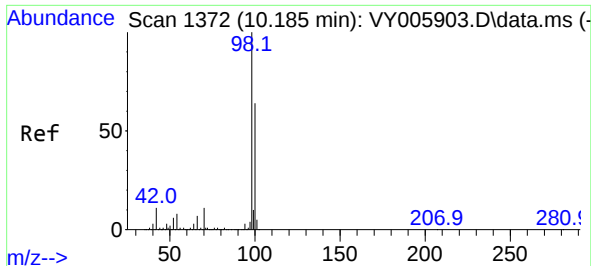

#50
Toluene-d8
Concen: 54.807 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. 0.000 min
Lab File: VY005912.D
Acq: 31 Aug 2021 15:10




Instrument :
MSVOA_Y
ClientSampleId :
TP-1COMP


Tgt Ion: 98 Resp: 436776
Ion Ratio Lower Upper
98 100
100 63.6 50.9 76.3

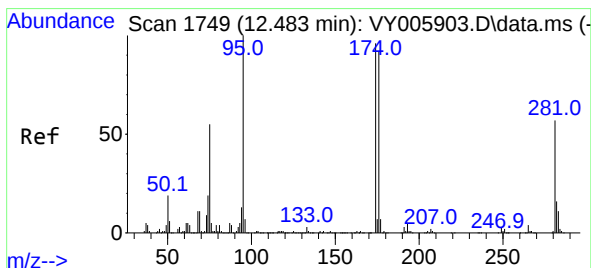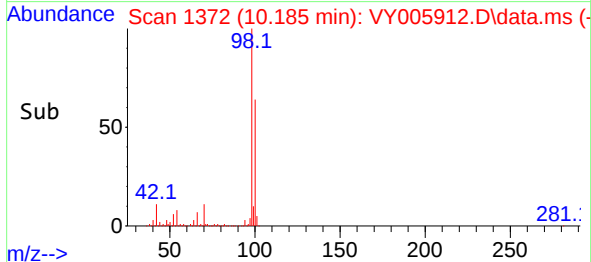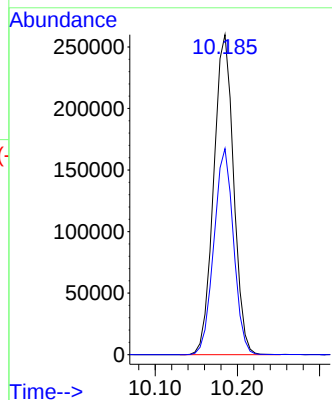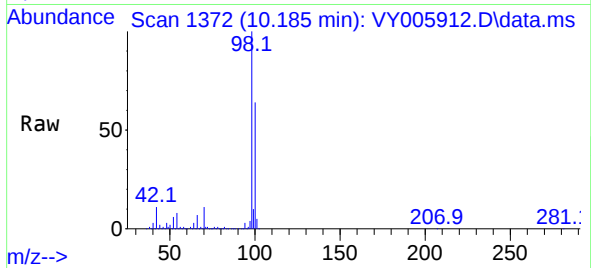

#62
4-Bromofluorobenzene
Concen: 58.975 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY005912.D
Acq: 31 Aug 2021 15:10

Tgt Ion: 95 Resp: 157816
Ion Ratio Lower Upper
95 100
174 99.2 0.0 192.4
176 95.2 0.0 186.8


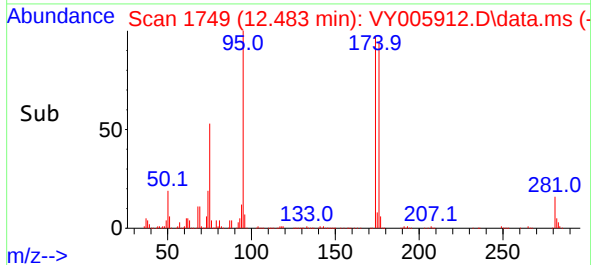
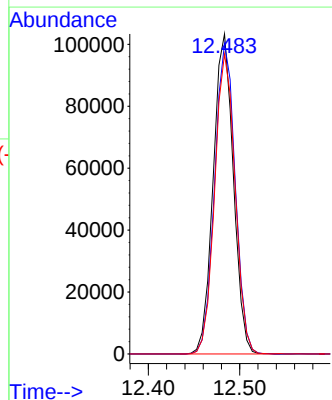
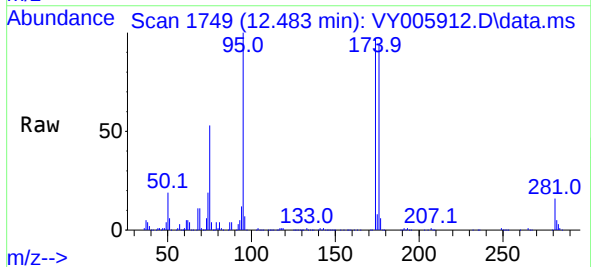


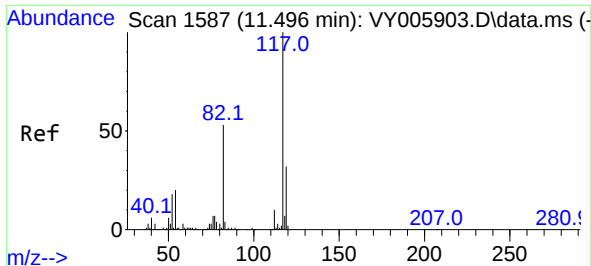

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 1586
Delta R.T. -0.006 min
Lab File: VY005912.D
Acq: 31 Aug 2021 15:10

Instrument :
MSVOA_Y
ClientSampleId :
TP-1COMP

Tgt Ion:	117	Resp:	358094
Ion	Ratio	Lower	Upper
117	100		
82	54.3	42.4	63.6
119	31.9	25.4	38.0

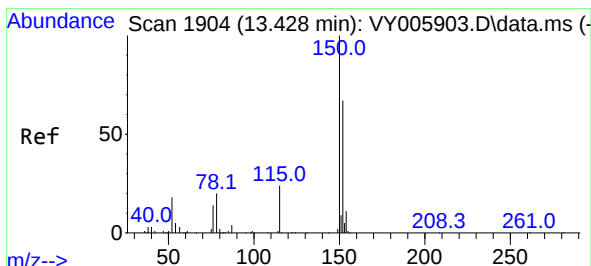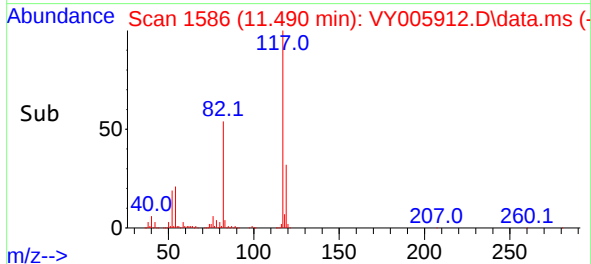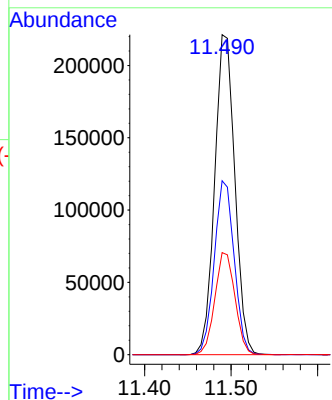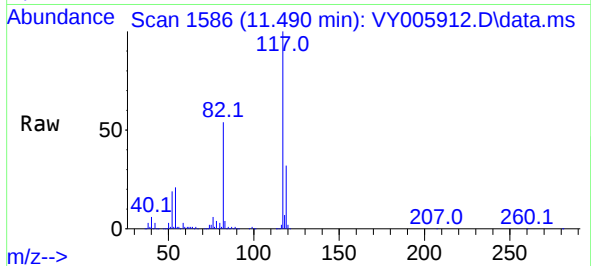

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY005912.D
Acq: 31 Aug 2021 15:10

Tgt Ion:	152	Resp:	184866
Ion	Ratio	Lower	Upper
152	100		
115	53.3	26.8	80.4
150	157.0	0.0	345.6

