
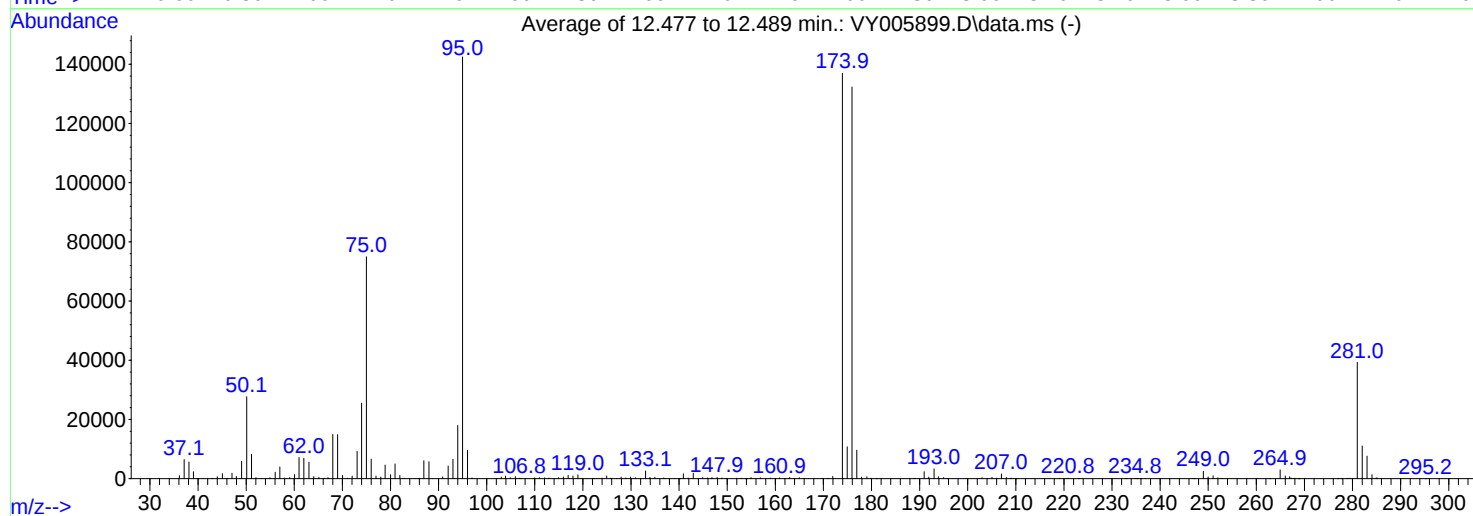


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY083121\
 Data File : VY005899.D
 Acq On : 31 Aug 2021 08:59
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y083121S.M
 Title : SW846 8260
 Last Update : Wed Sep 01 05:32:43 2021

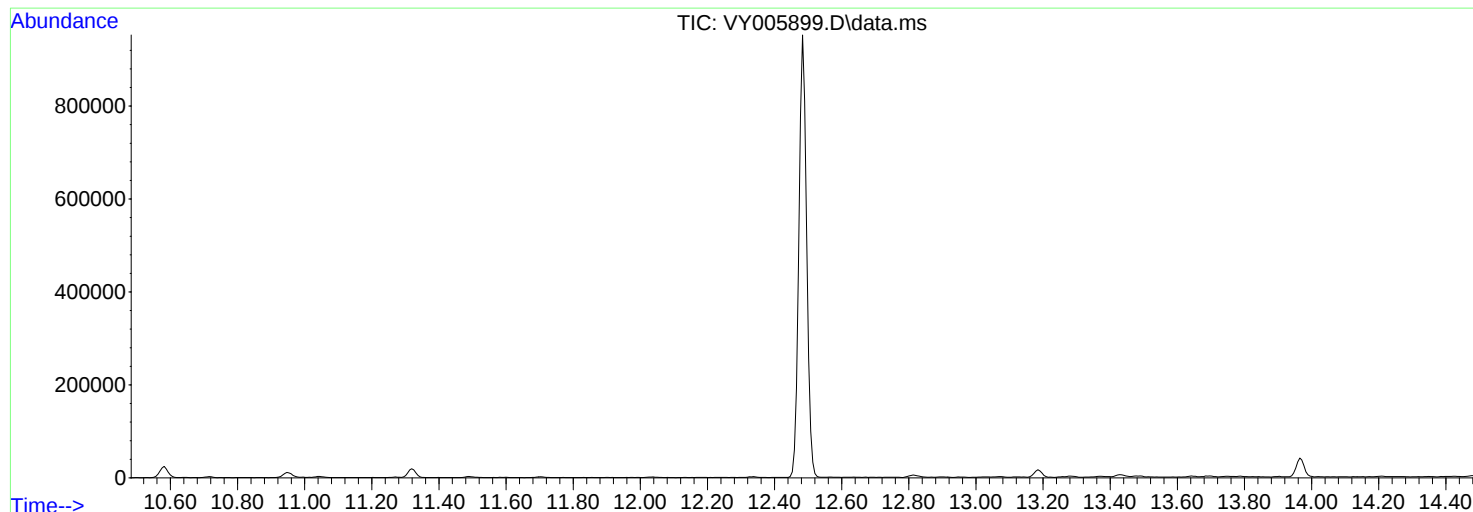

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	27672	PASS
75	95	30	60	52.6	75003	PASS
95	95	100	100	100.0	142528	PASS
96	95	5	9	6.7	9585	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	96.1	136965	PASS
175	174	5	9	7.9	10774	PASS
176	174	95	101	96.6	132363	PASS
177	176	5	9	7.3	9625	PASS