
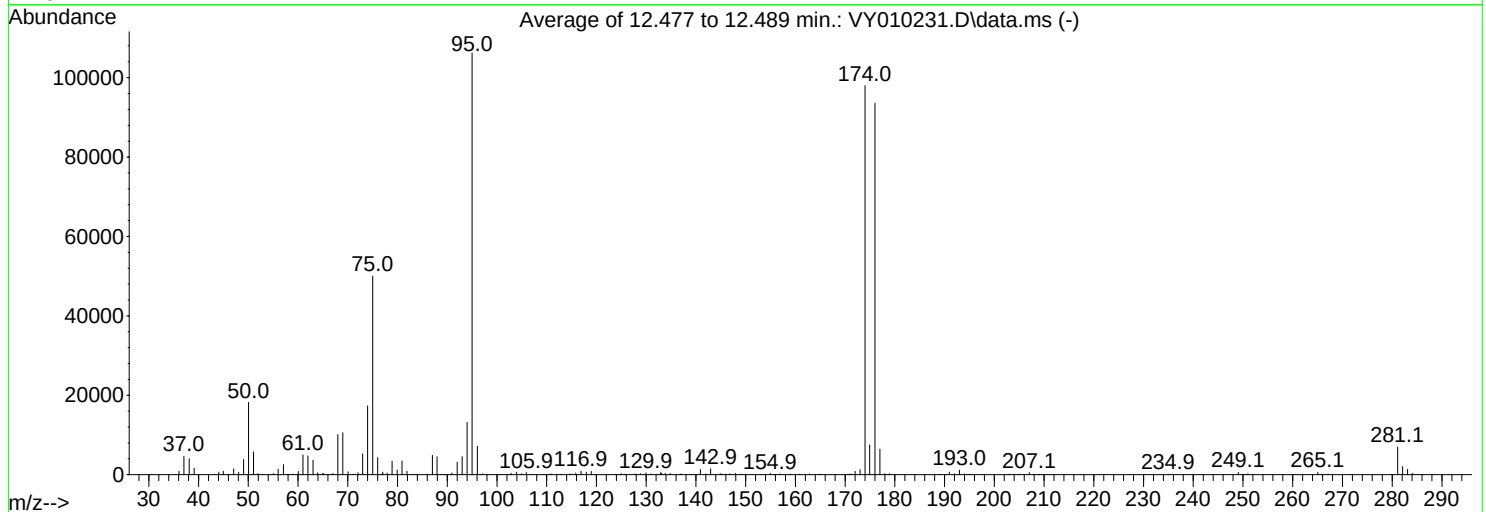


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY083122\
Data File : VY010231.D
Acq On : 31 Aug 2022 08:51
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y083022S.M
Title : SW846 8260
Last Update : Wed Aug 31 02:23:17 2022

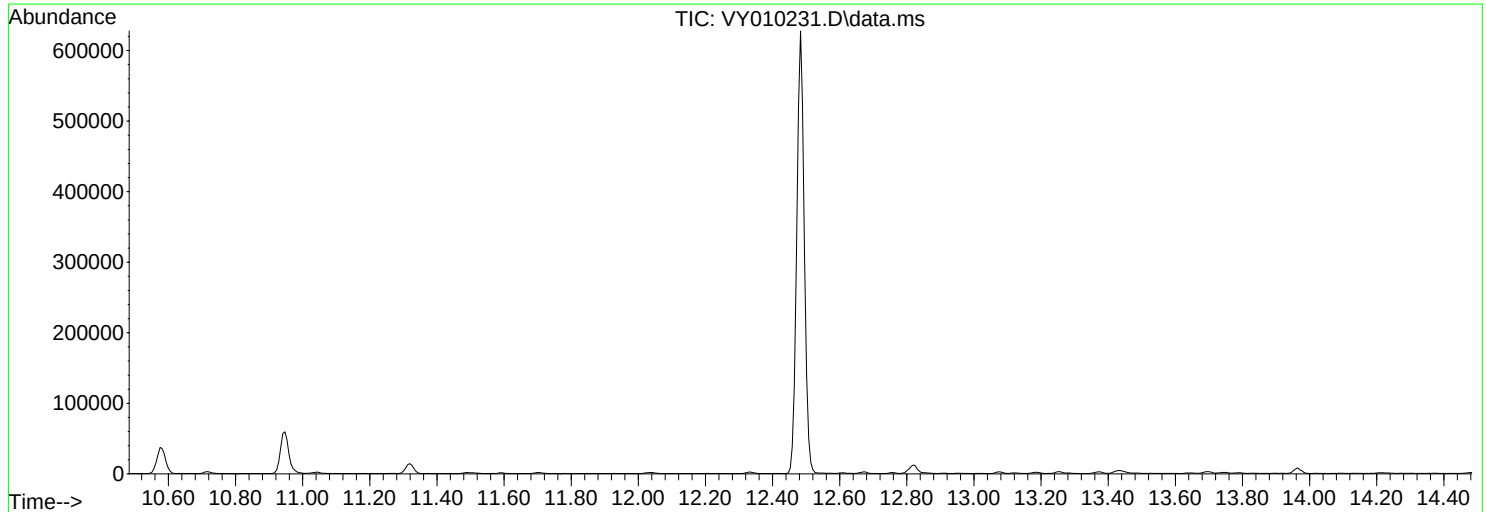

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.1	18203	PASS
75	95	30	60	47.1	50035	PASS
95	95	100	100	100.0	106248	PASS
96	95	5	9	6.8	7182	PASS
173	174	0.00	2	1.3	1269	PASS
174	95	50	100	92.3	98035	PASS
175	174	5	9	7.6	7482	PASS
176	174	95	101	95.5	93592	PASS
177	176	5	9	6.9	6450	PASS