
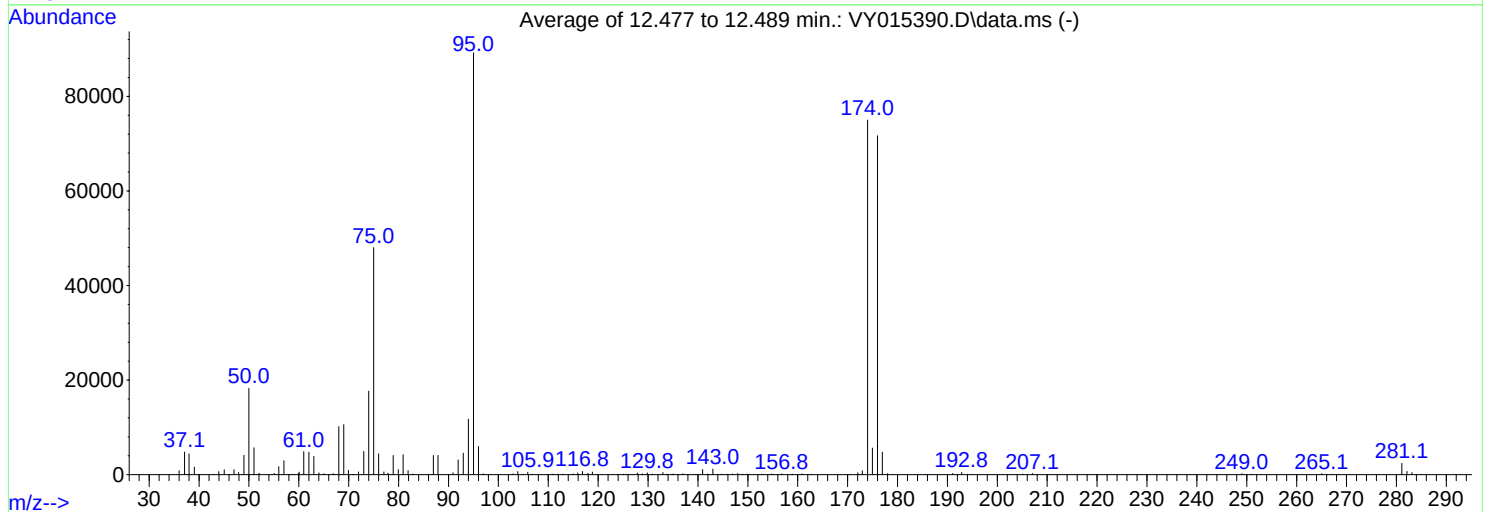


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY083123\
 Data File : VY015390.D
 Acq On : 31 Aug 2023 08:44
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y082923S.M
 Title : SW846 8260
 Last Update : Thu Aug 31 20:01:47 2023

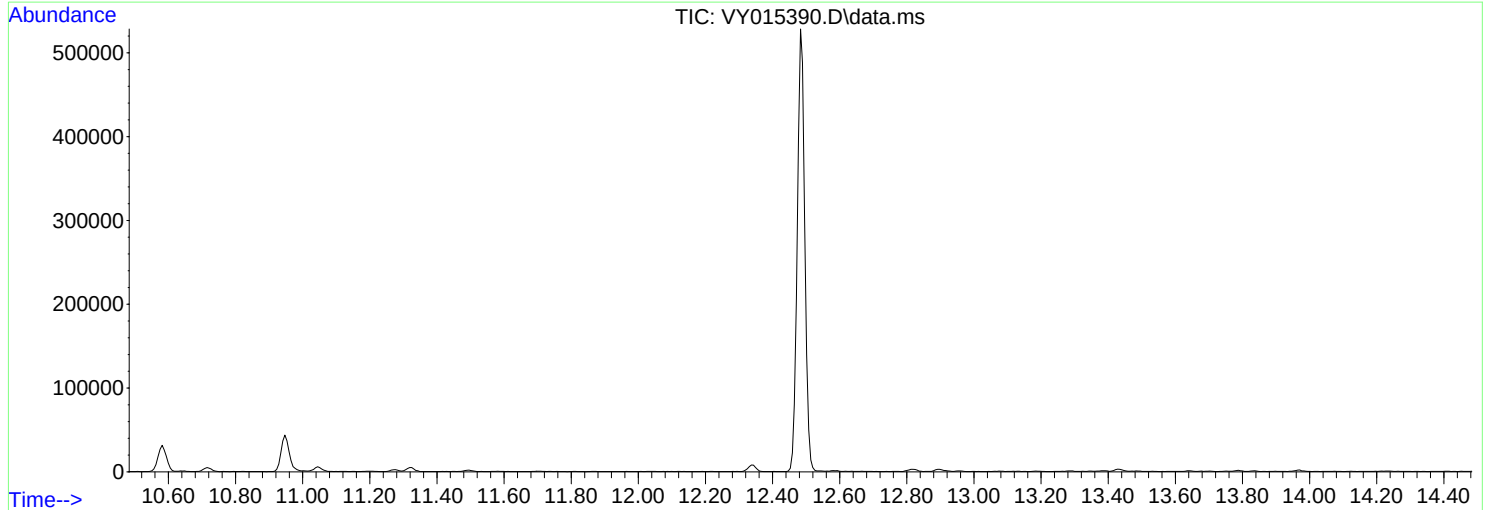

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	18240	PASS
75	95	30	60	53.8	48000	PASS
95	95	100	100	100.0	89200	PASS
96	95	5	9	6.7	5941	PASS
173	174	0.00	2	1.1	803	PASS
174	95	50	100	84.1	74973	PASS
175	174	5	9	7.5	5608	PASS
176	174	95	101	95.6	71661	PASS
177	176	5	9	6.6	4765	PASS