

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY090121\
 Data File : VY005928.D
 Acq On : 01 Sep 2021 14:17
 Operator : SY/MD
 Sample : M3614-01
 Misc : 5.08G/5ML/MSVOA_Y/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 NB-8-083121

Quant Time: Sep 02 07:48:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y083121S.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 01 05:32:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	186159	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	332421	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	357089	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	190910	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	128194	68.335	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	136.660%
35) Dibromofluoromethane	7.722	113	101418	54.325	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	108.660%
50) Toluene-d8	10.185	98	427329	54.541	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	109.080%
62) 4-Bromofluorobenzene	12.483	95	161709	61.467	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	122.940%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY090121\
Data File : VY005928.D
Acq On : 01 Sep 2021 14:17
Operator : SY/MD
Sample : M3614-01
Misc : 5.08G/5ML/MSVOA_Y/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
NB-8-083121

Quant Time: Sep 02 07:48:23 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y083121S.M
Quant Title : SW846 8260
QLast Update : Wed Sep 01 05:32:43 2021
Response via : Initial Calibration




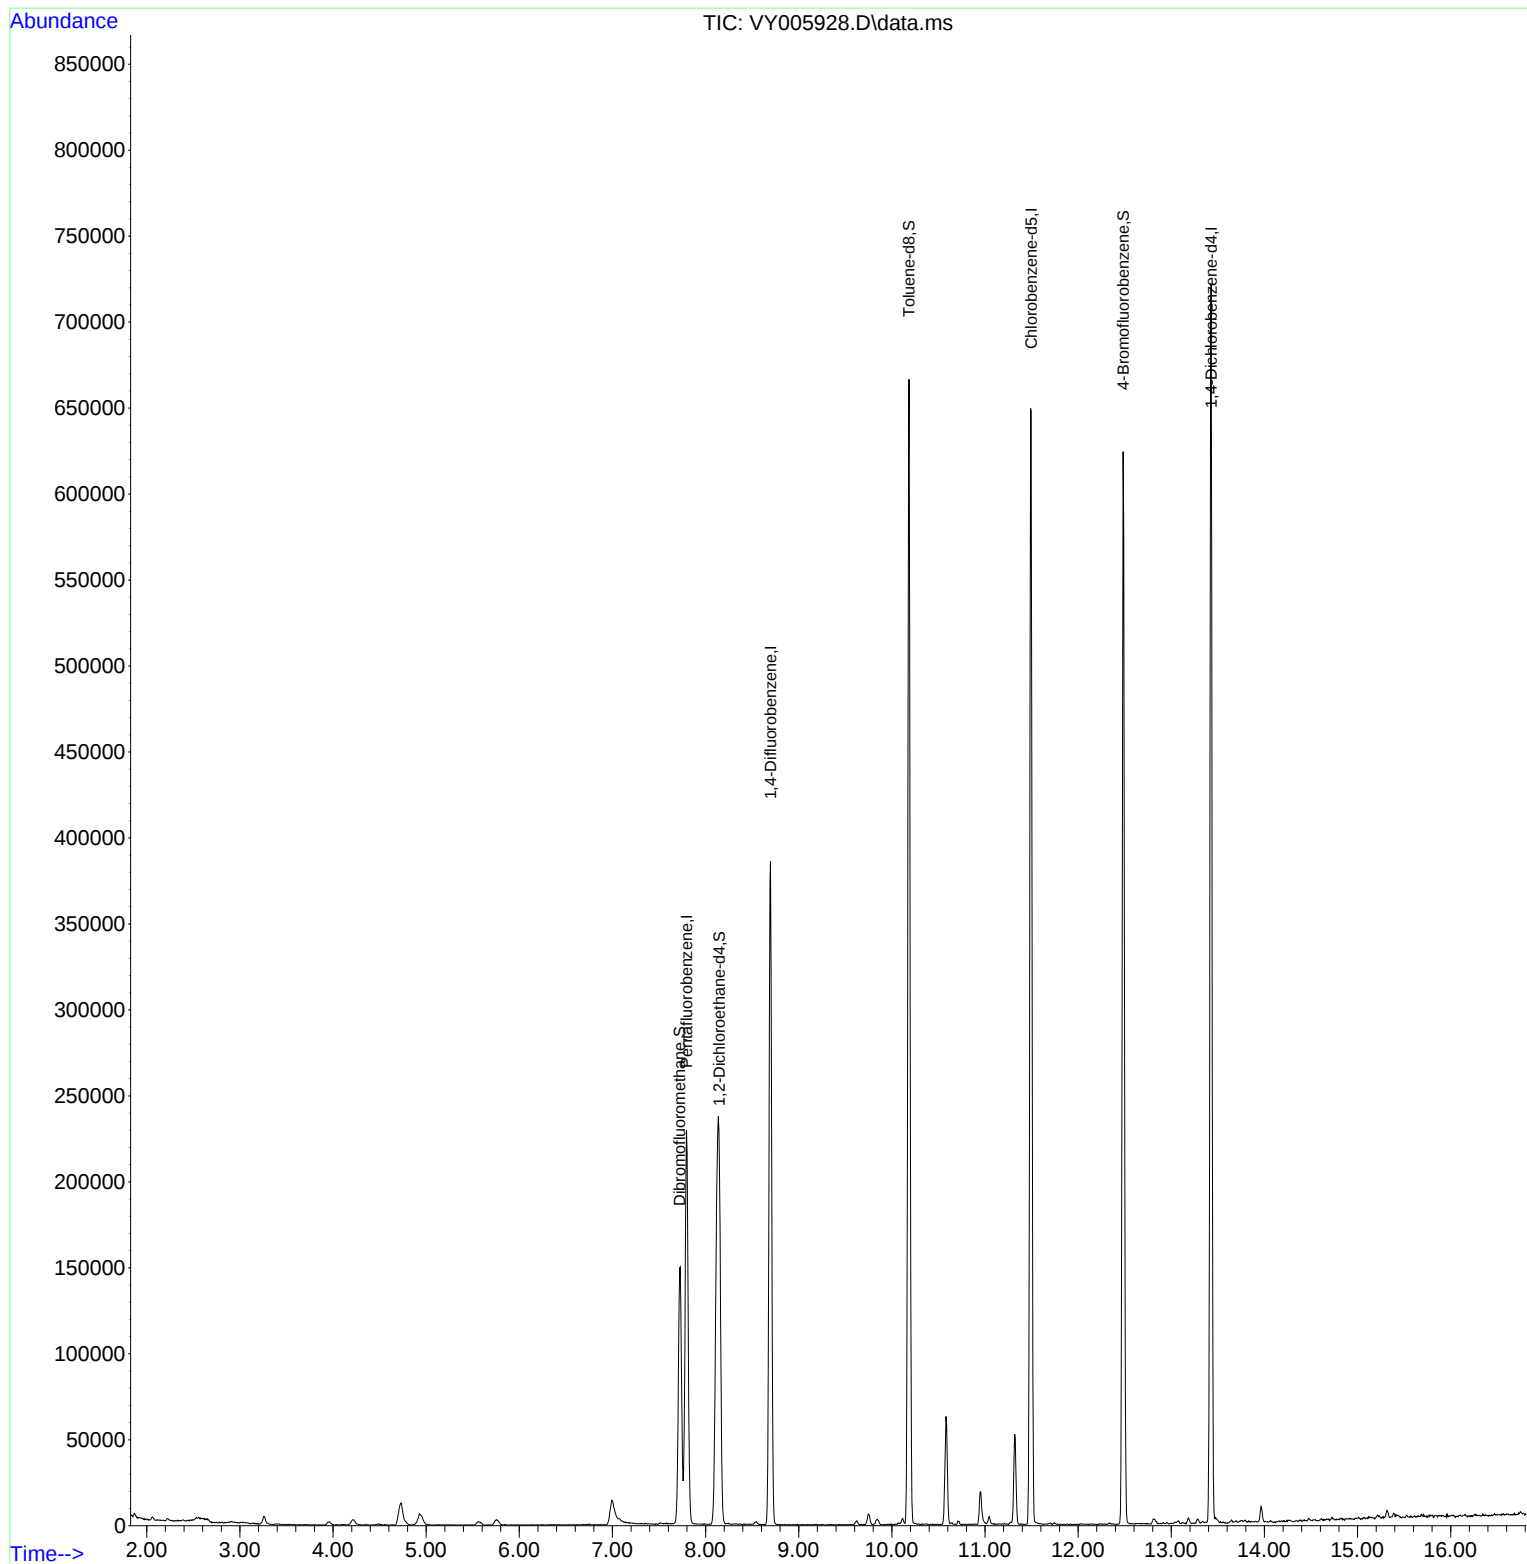


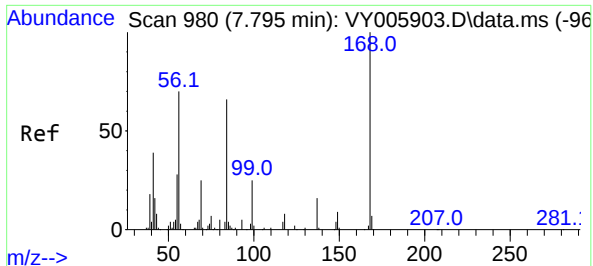

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.795 min Scan# 980
Delta R.T. 0.000 min
Lab File: VY005928.D
Acq: 01 Sep 2021 14:17




Instrument :
MSVOA_Y
ClientSampleId :
NB-8-083121


Tgt Ion:168 Resp: 186159
Ion Ratio Lower Upper
168 100
99 51.4 40.6 60.8

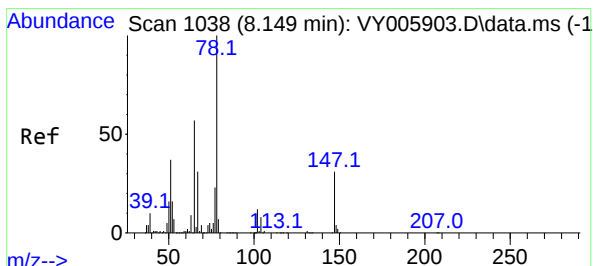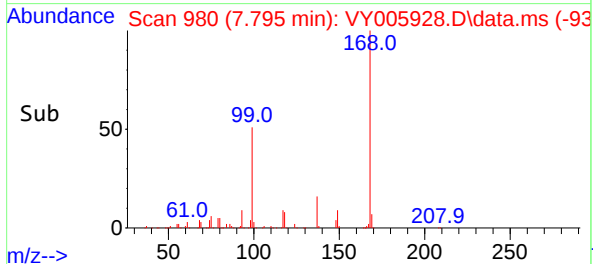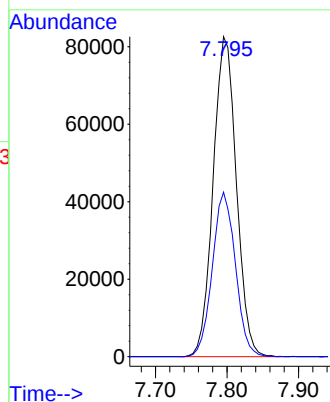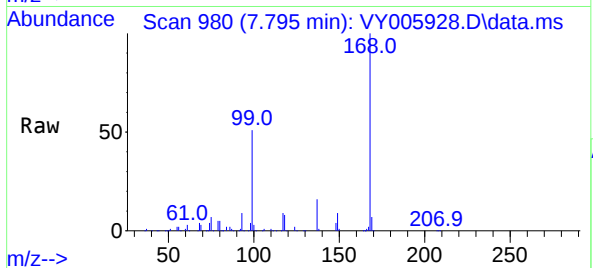

#33
1,2-Dichloroethane-d4
Concen: 68.335 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VY005928.D
Acq: 01 Sep 2021 14:17

Tgt Ion: 65 Resp: 128194
Ion Ratio Lower Upper
65 100
67 51.7 0.0 105.4

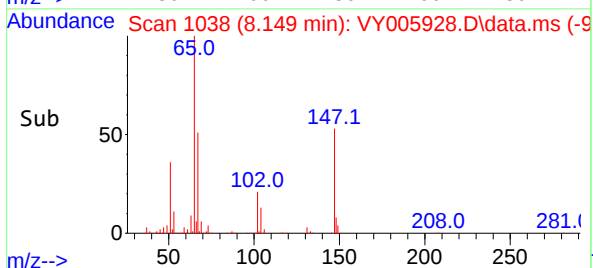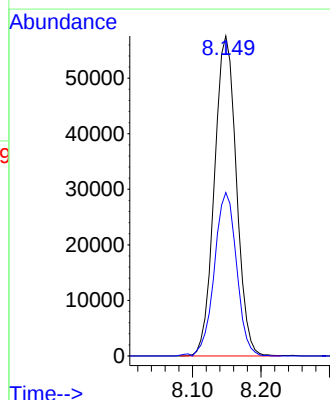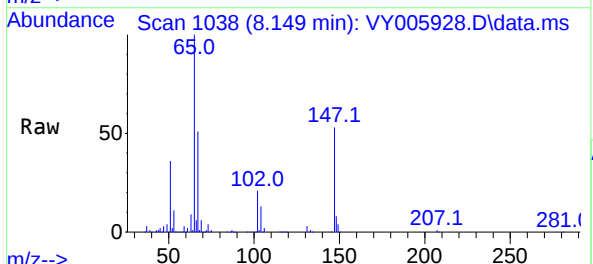




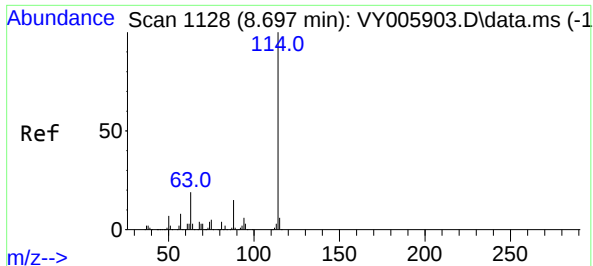


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VY005928.D
Acq: 01 Sep 2021 14:17

Instrument :
MSVOA_Y
ClientSampleId :
NB-8-083121




Tgt Ion:	114	Resp:	332421
Ion	Ratio	Lower	Upper
114	100		
63	19.7	0.0	38.4
88	14.9	0.0	30.0

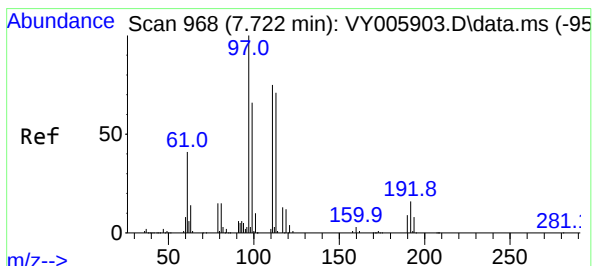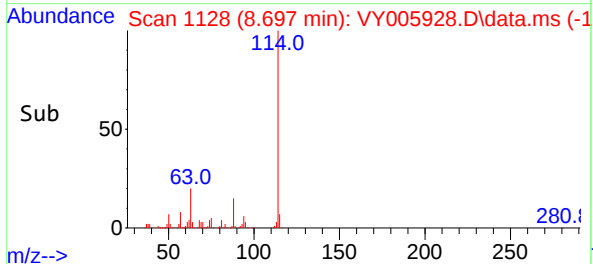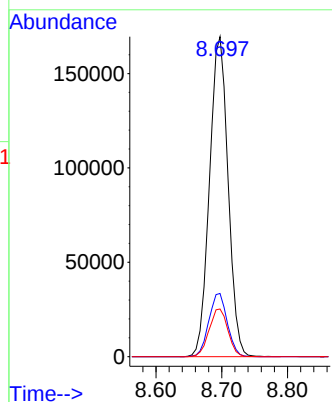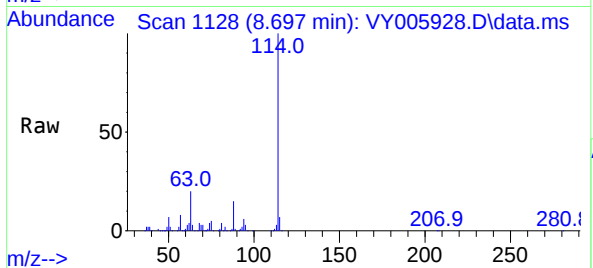


#35

Dibromofluoromethane
Concen: 54.325 ug/l
RT: 7.722 min Scan# 968
Delta R.T. -0.000 min
Lab File: VY005928.D
Acq: 01 Sep 2021 14:17

Tgt Ion:	113	Resp:	101418
Ion	Ratio	Lower	Upper
113	100		
111	104.2	81.9	122.9
192	24.0	19.4	29.0


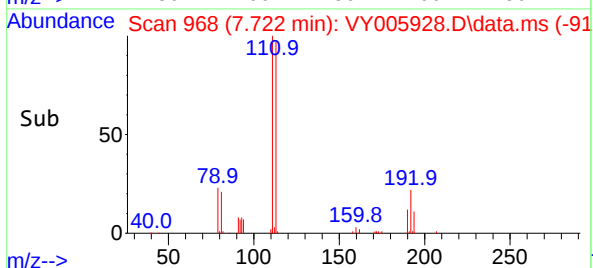
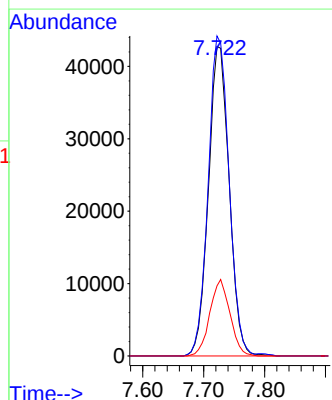
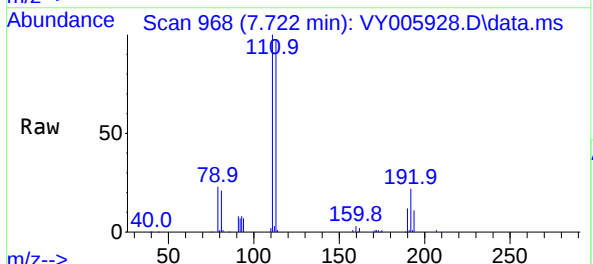


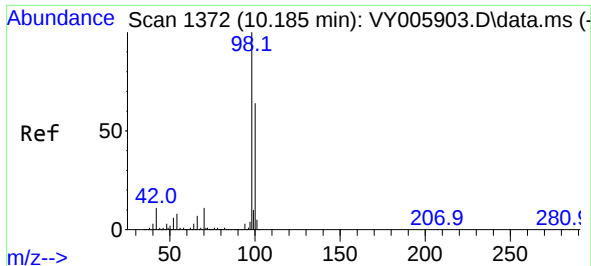

#50
Toluene-d8
Concen: 54.541 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY005928.D
Acq: 01 Sep 2021 14:17




Instrument :
MSVOA_Y
ClientSampleId :
NB-8-083121


Tgt Ion: 98 Resp: 427329
Ion Ratio Lower Upper
98 100
100 63.6 50.9 76.3

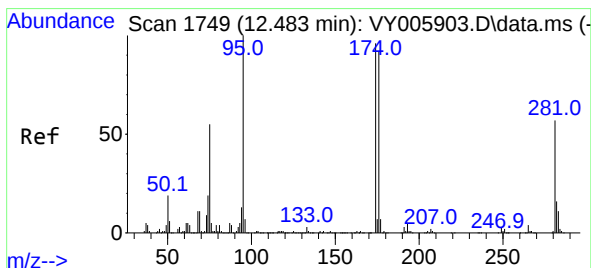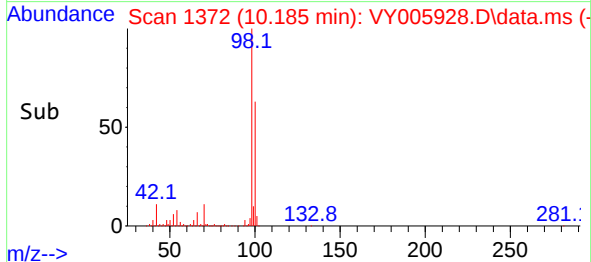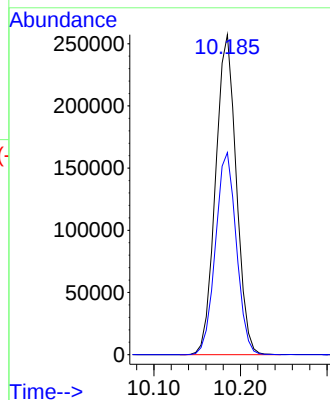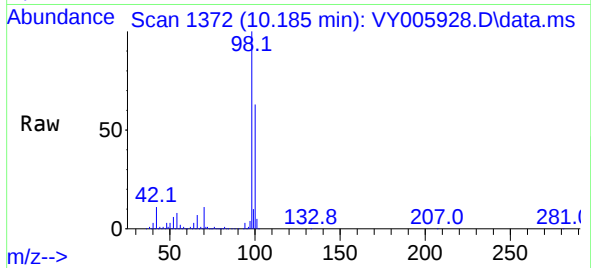

#62
4-Bromofluorobenzene
Concen: 61.467 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY005928.D
Acq: 01 Sep 2021 14:17

Tgt Ion: 95 Resp: 161709
Ion Ratio Lower Upper
95 100
174 96.4 0.0 192.4
176 93.5 0.0 186.8


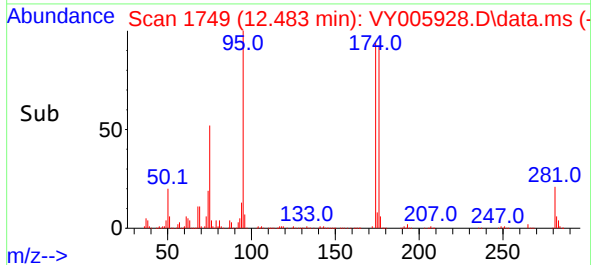
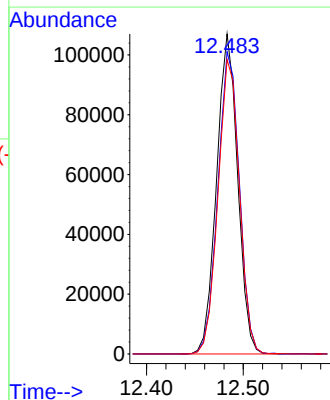
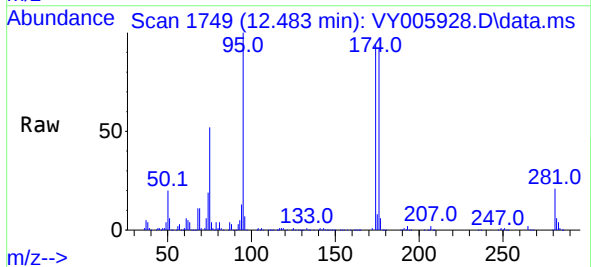


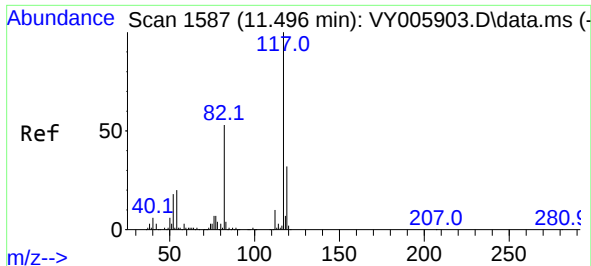

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.496 min Scan# 1587
Delta R.T. -0.000 min
Lab File: VY005928.D
Acq: 01 Sep 2021 14:17

Instrument :
MSVOA_Y
ClientSampleId :
NB-8-083121

Tgt Ion:117 Resp: 357089
Ion Ratio Lower Upper
117 100
82 54.6 42.4 63.6
119 33.1 25.4 38.0

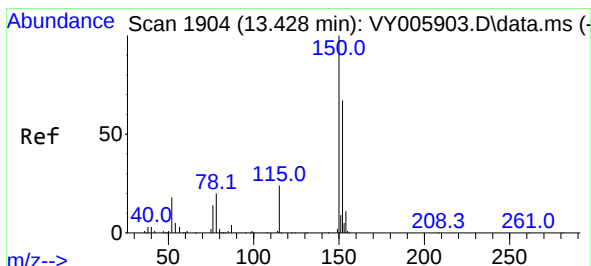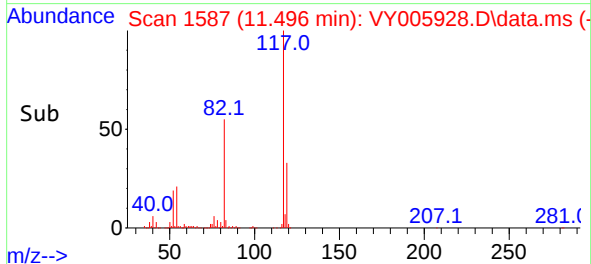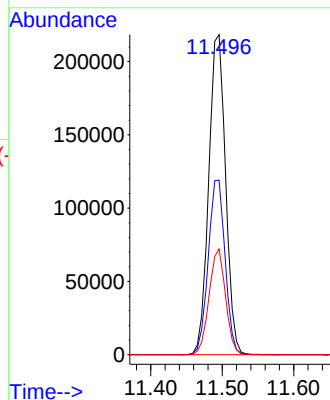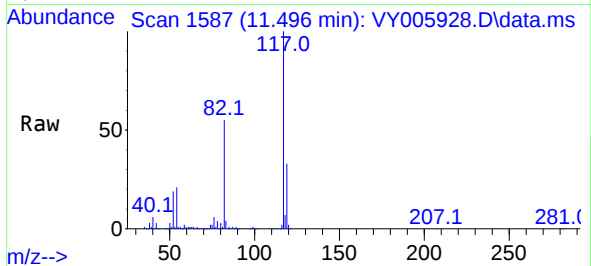

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY005928.D
Acq: 01 Sep 2021 14:17

Tgt Ion:152 Resp: 190910
Ion Ratio Lower Upper
152 100
115 54.5 26.8 80.4
150 157.0 0.0 345.6

