


Bromomethane

Response Ratio

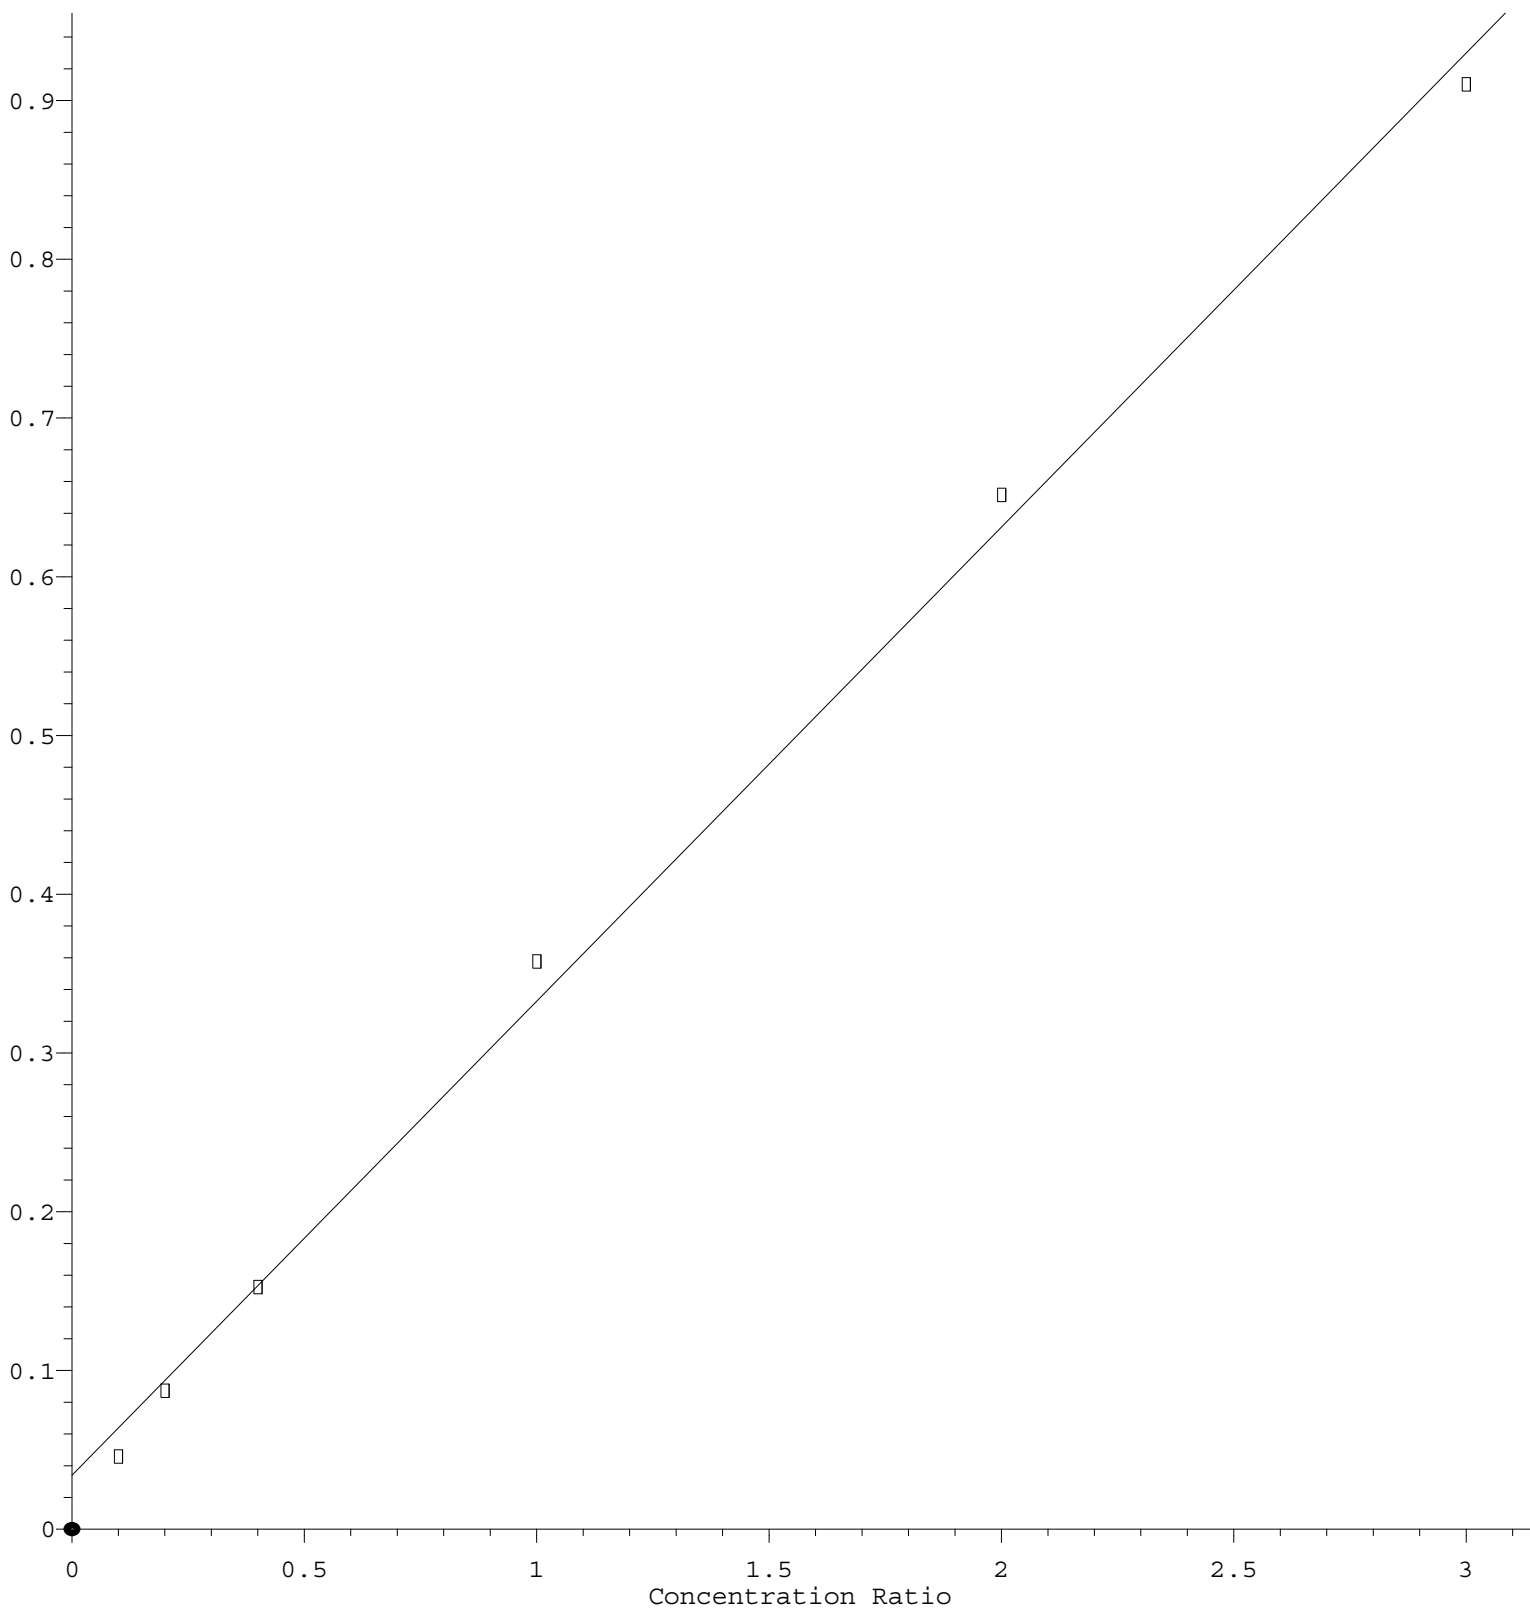

$$\text{Response} = 2.990\text{e-}001 * \text{Amt} + 3.352\text{e-}002$$


Coef of Det (r^2) = 0.997024 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y090222S.M

Calibration Table Last Updated: Fri Sep 02 16:41:46 2022

Bromochloromethane

Response Ratio

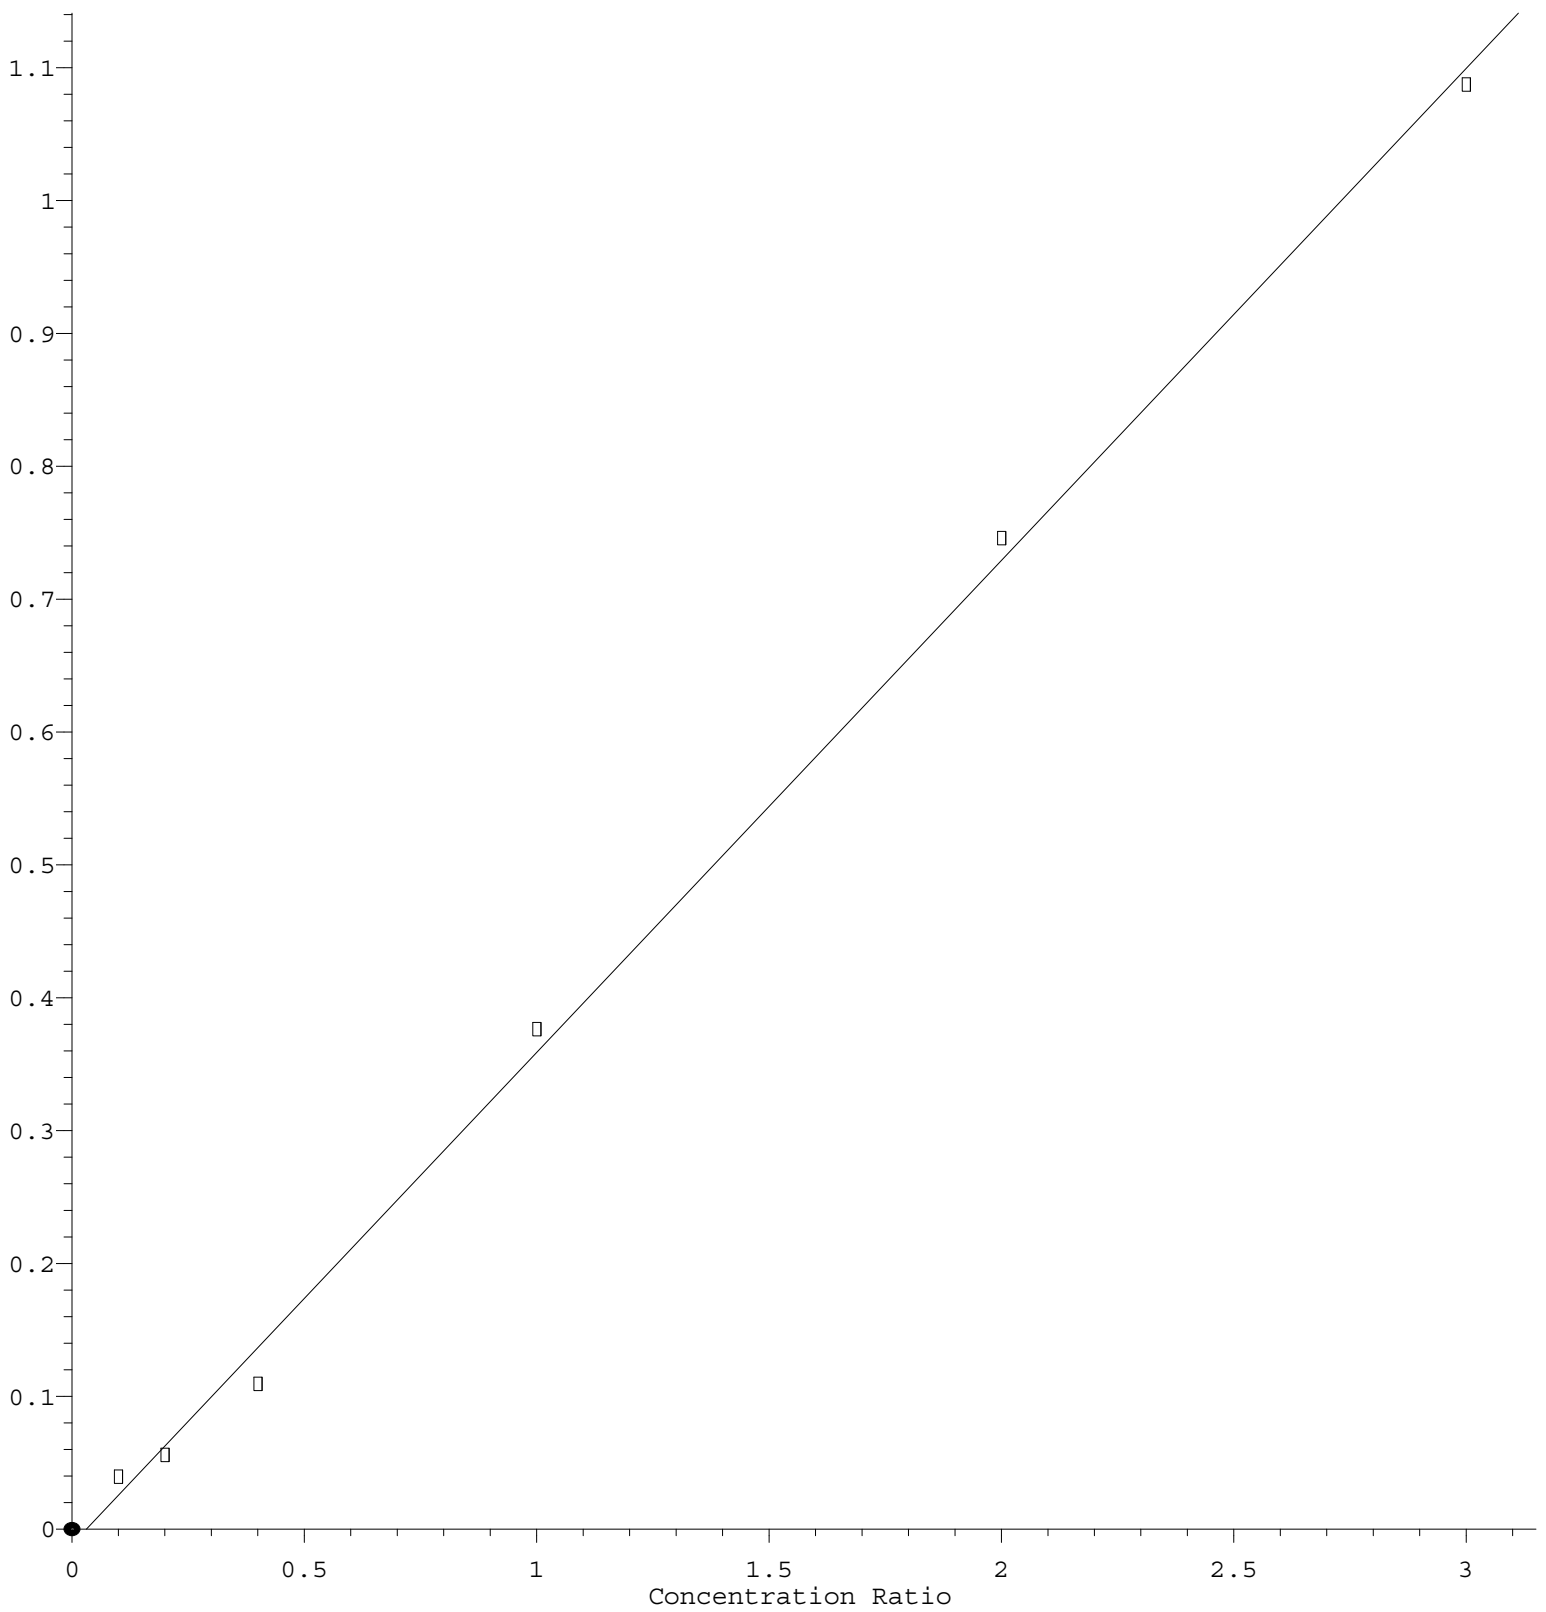

$$\text{Response} = 3.705\text{e-}001 * \text{Amt} - 1.138\text{e-}002$$


Coef of Det (r^2) = 0.998144 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y090222S.M

Calibration Table Last Updated: Fri Sep 02 16:41:46 2022

2-Chloroethyl Vinyl ether

Response Ratio

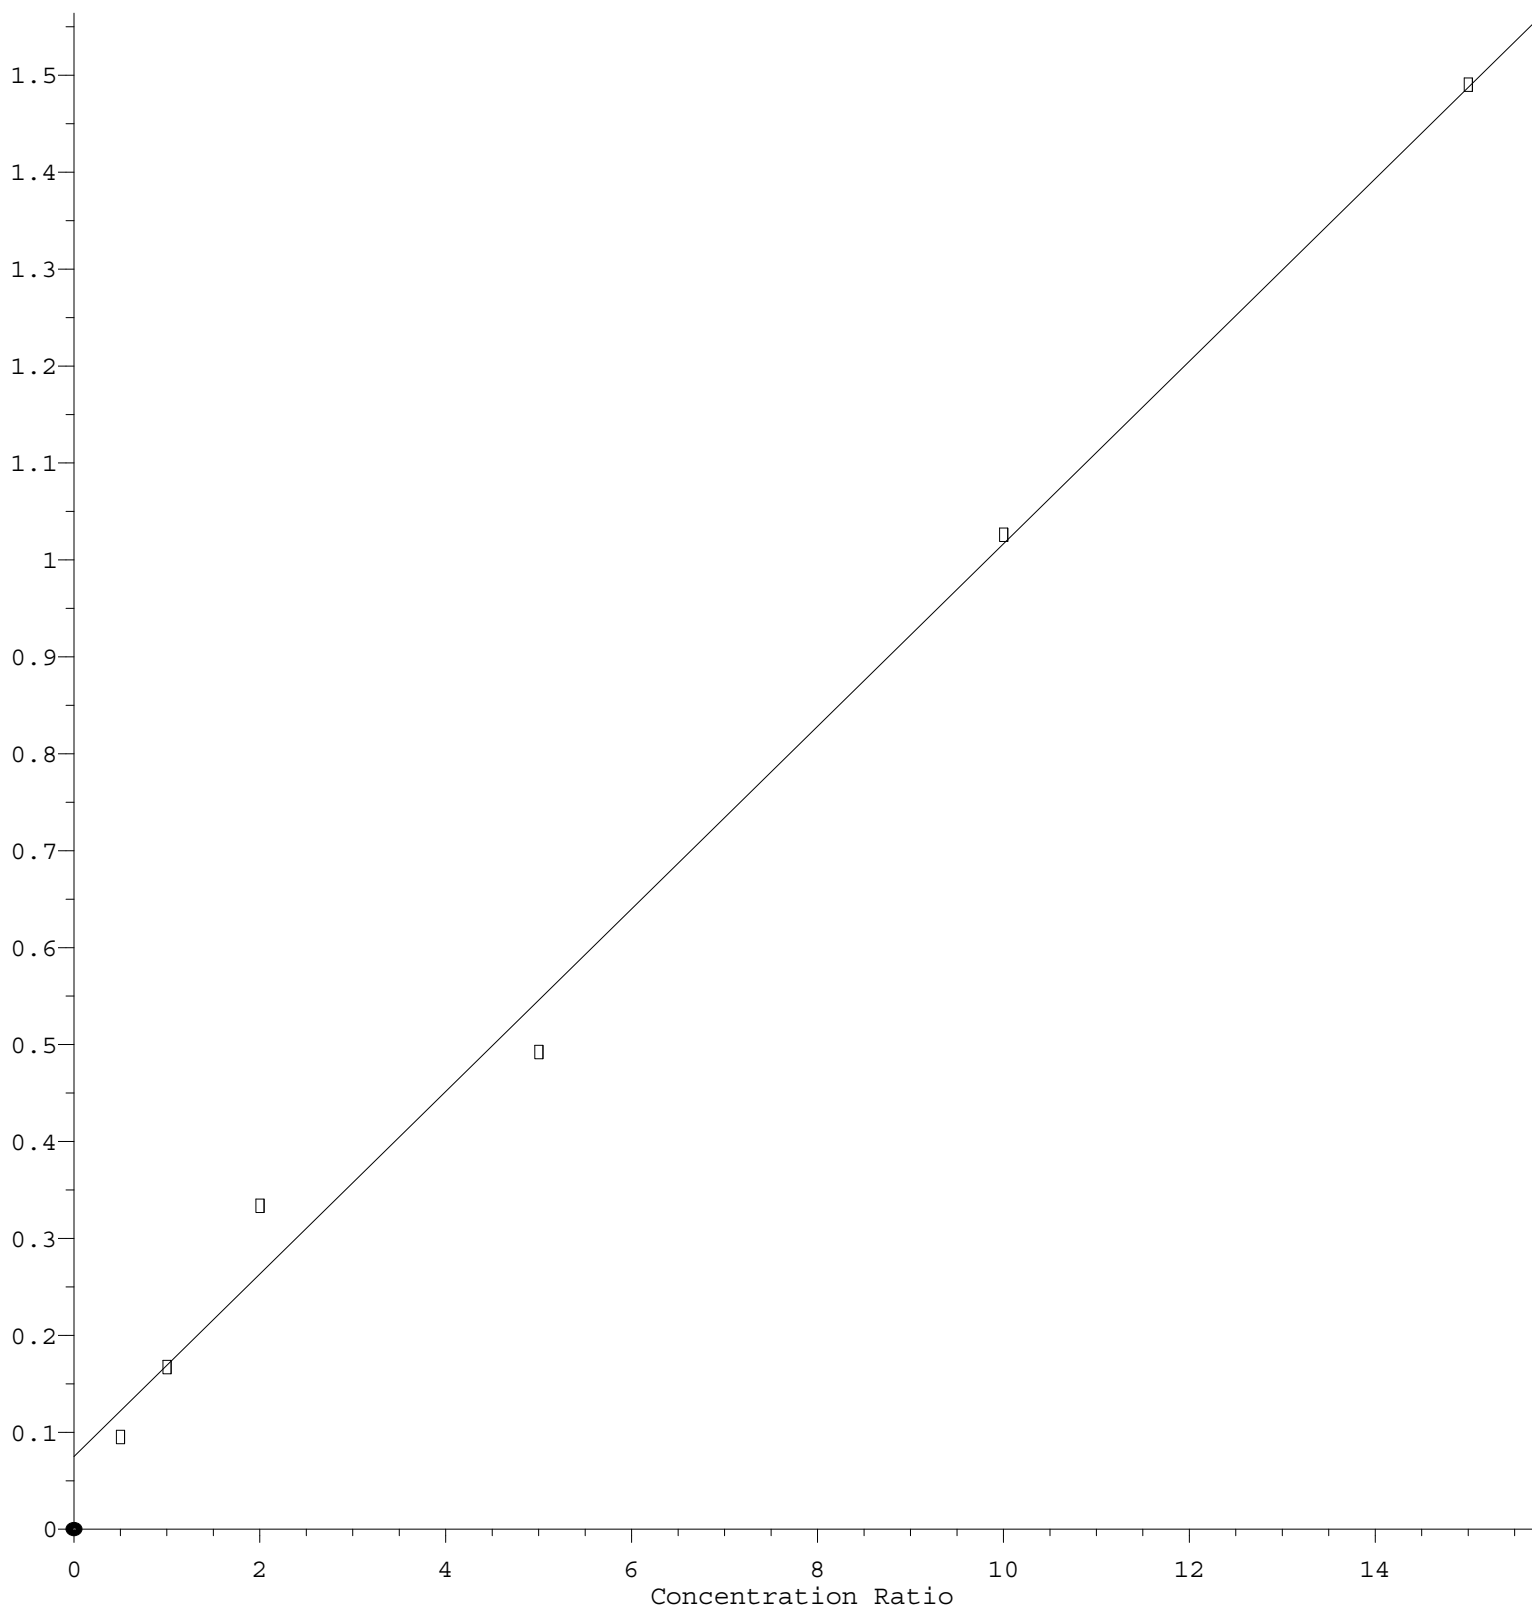

$$\text{Response} = 9.412\text{e-}002 * \text{Amt} + 7.519\text{e-}002$$


Coef of Det (r^2) = 0.994224 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y090222S.M

Calibration Table Last Updated: Fri Sep 02 16:41:46 2022

4-Bromofluorobenzene

Response Ratio

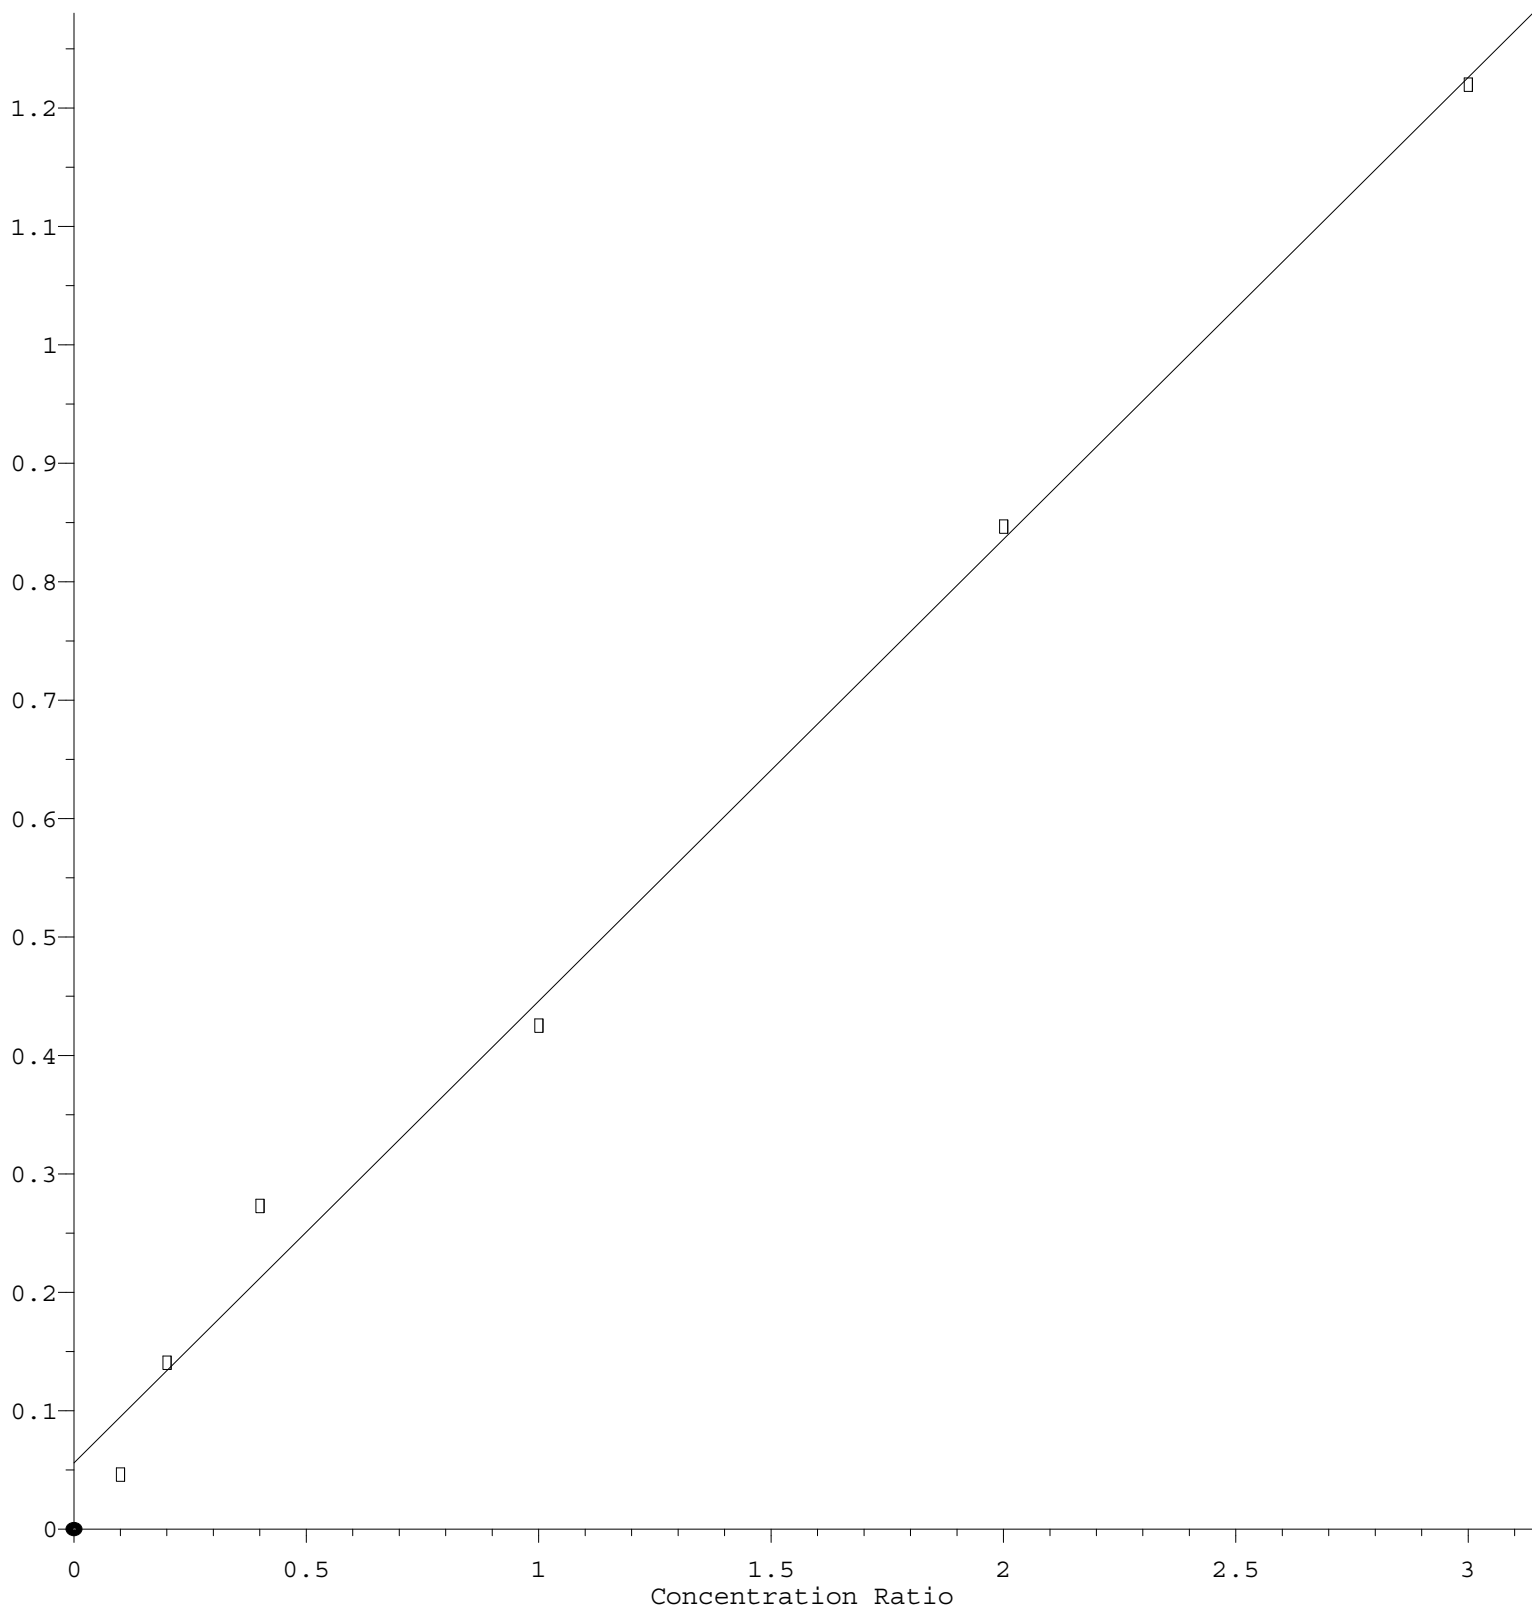

$$\text{Response} = 3.900\text{e-}001 * \text{Amt} + 5.634\text{e-}002$$


Coef of Det (r^2) = 0.993463 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y090222S.M

Calibration Table Last Updated: Fri Sep 02 16:41:46 2022

Tetrachloroethene

Response Ratio

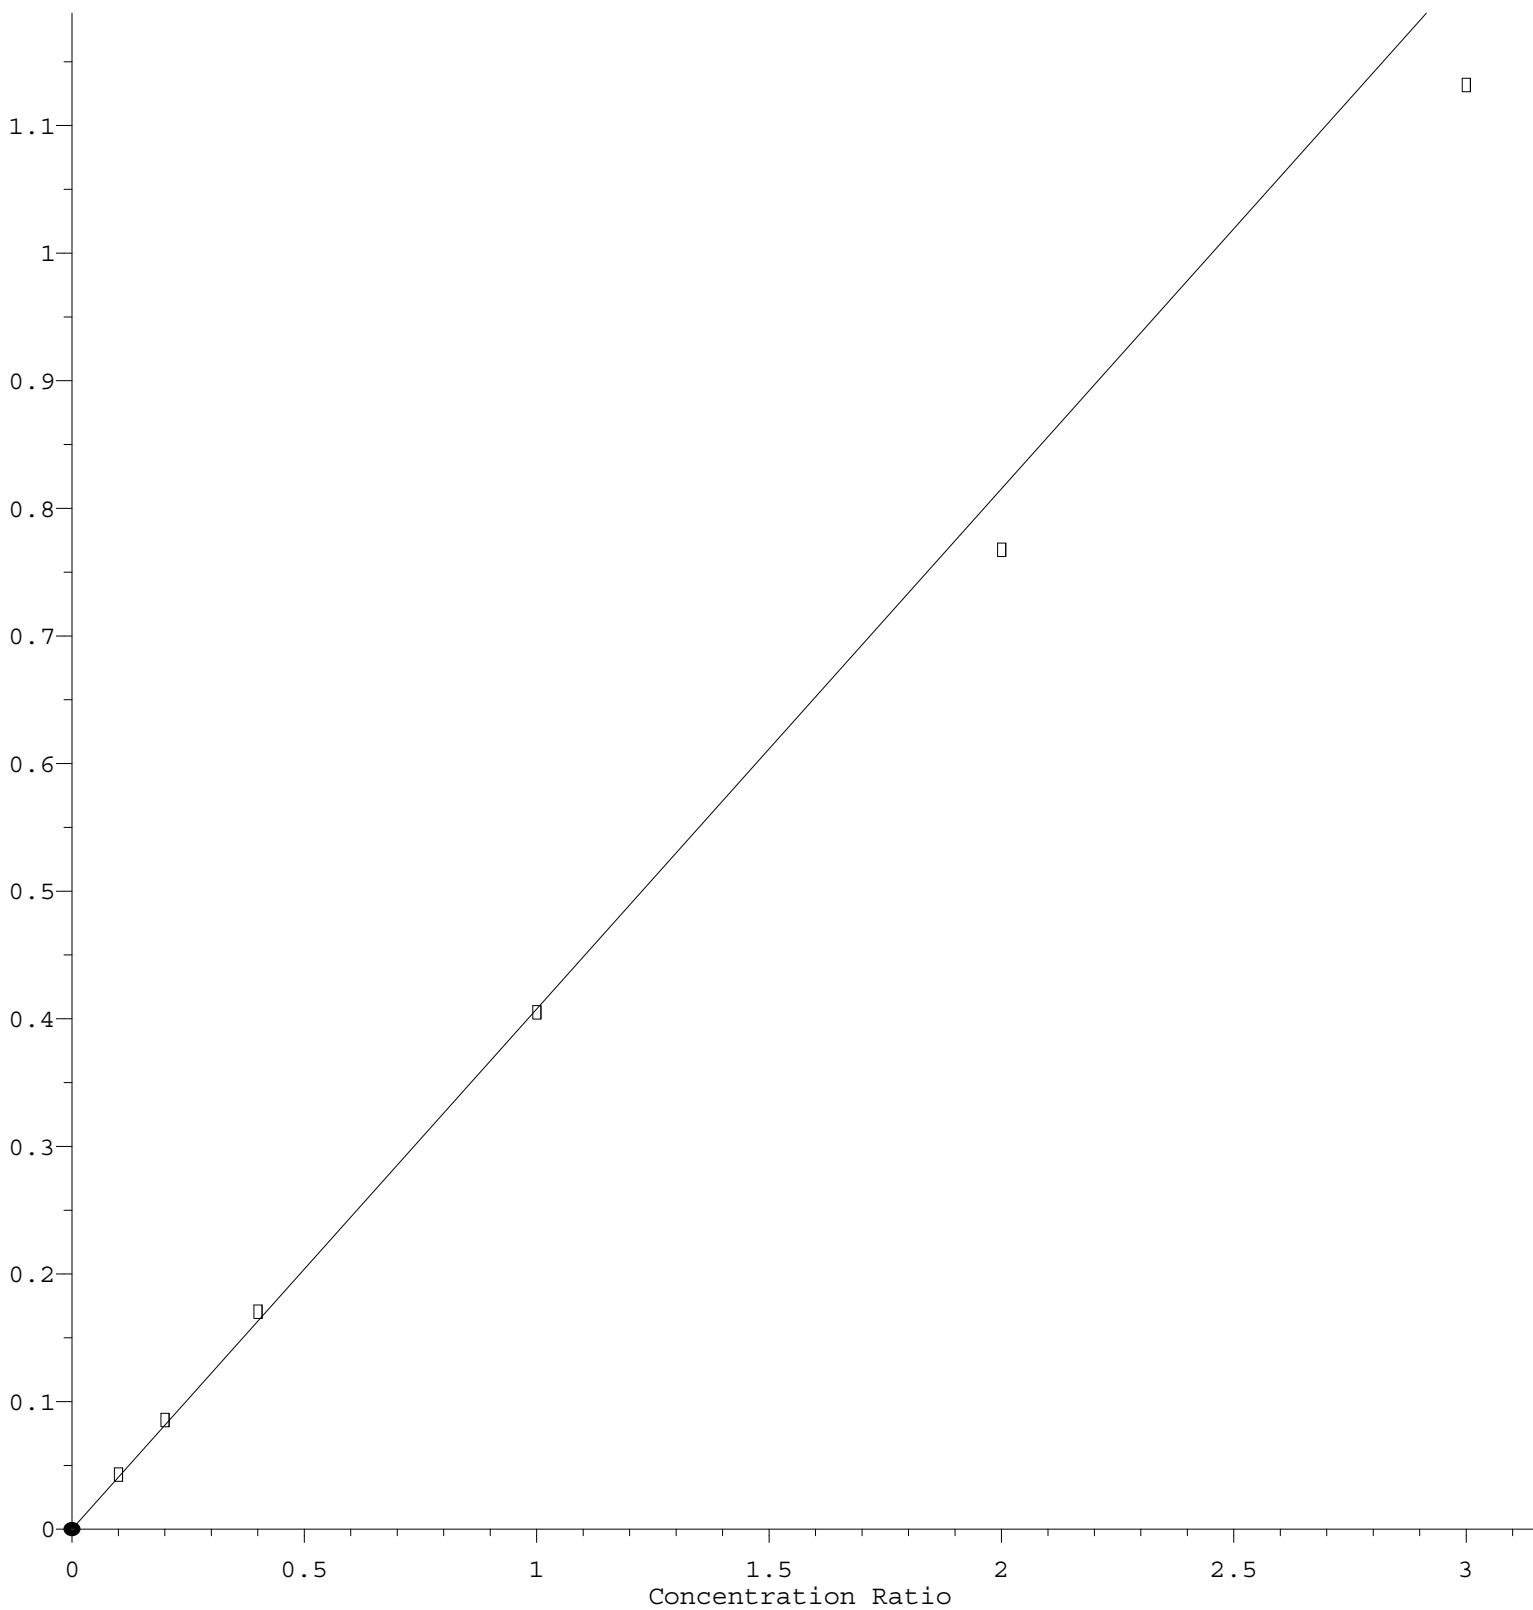

$$\text{Response} = 4.078\text{e-}001 * \text{Amt}$$

RF Rel Std Dev = 5.607% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y090222S.M

Calibration Table Last Updated: Fri Sep 02 16:41:46 2022