


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY090222\
Data File : VY010268.D
Acq On : 02 Sep 2022 09:02
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090222S.M
Title : SW846 8260
Last Update : Fri Sep 02 16:41:46 2022

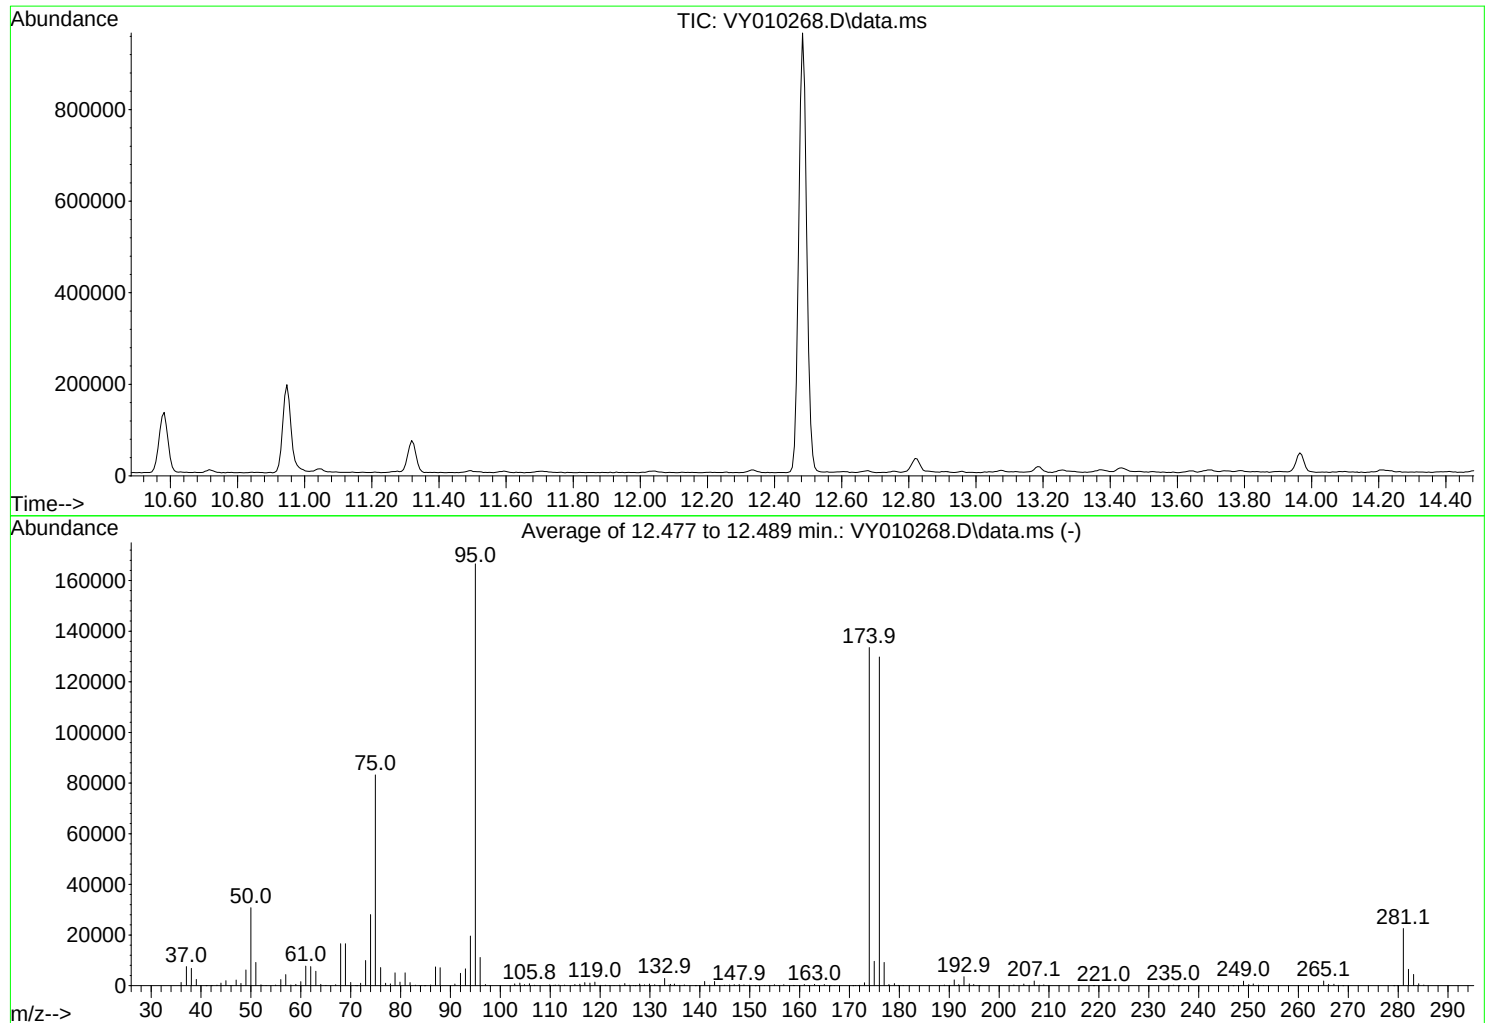

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1737

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	30797	PASS
75	95	30	60	50.0	83216	PASS
95	95	100	100	100.0	166592	PASS
96	95	5	9	6.7	11116	PASS
173	174	0.00	2	0.9	1140	PASS
174	95	50	100	80.2	133565	PASS
175	174	5	9	7.2	9609	PASS
176	174	95	101	97.2	129837	PASS
177	176	5	9	7.1	9161	PASS