
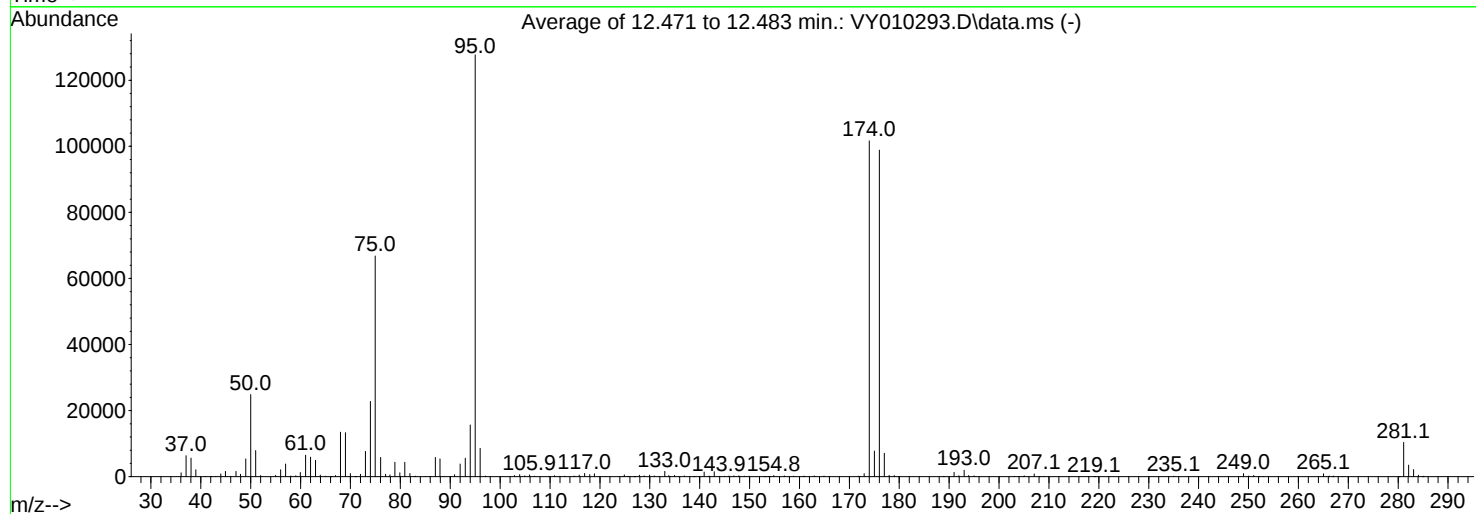


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY090222\  
 Data File : VY010293.D  
 Acq On : 02 Sep 2022 21:09  
 Operator : KP/MD  
 Sample : BFB  
 Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
 ALS Vial : 29 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y090222S.M  
 Title : SW846 8260  
 Last Update : Fri Sep 02 16:41:46 2022

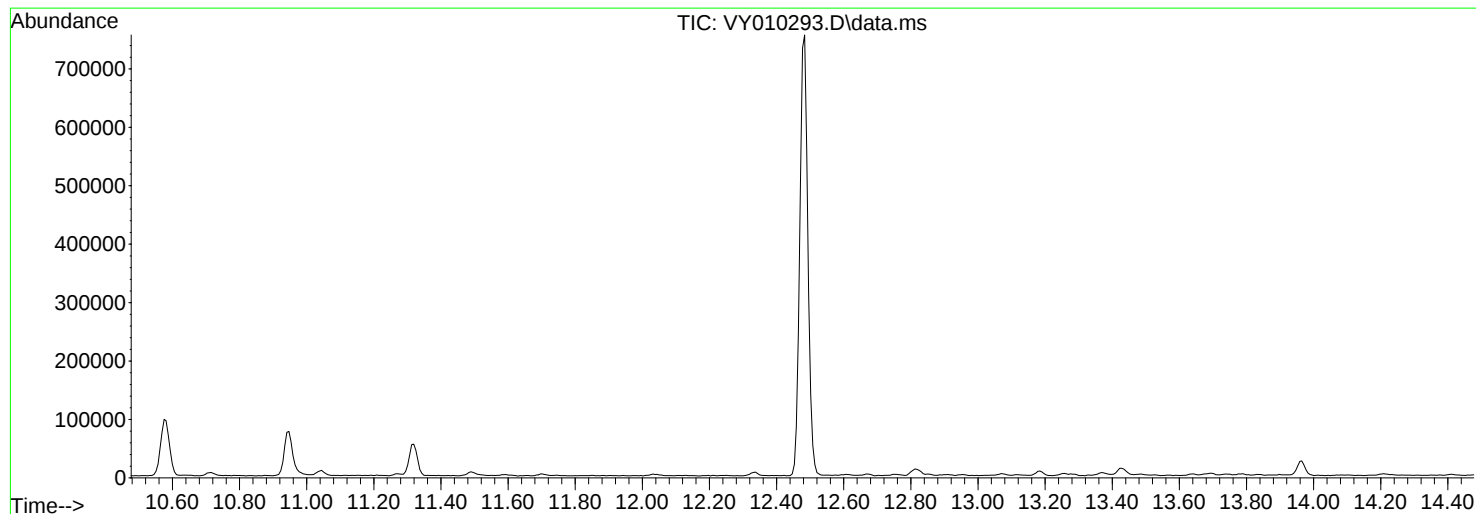

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 19.5         | 24851      | PASS                |
| 75             | 95              | 30              | 60              | 52.3         | 66807      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 127691     | PASS                |
| 96             | 95              | 5               | 9               | 6.7          | 8563       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.9          | 907        | PASS                |
| 174            | 95              | 50              | 100             | 79.6         | 101659     | PASS                |
| 175            | 174             | 5               | 9               | 7.6          | 7775       | PASS                |
| 176            | 174             | 95              | 101             | 97.3         | 98869      | PASS                |
| 177            | 176             | 5               | 9               | 7.2          | 7086       | PASS                |