
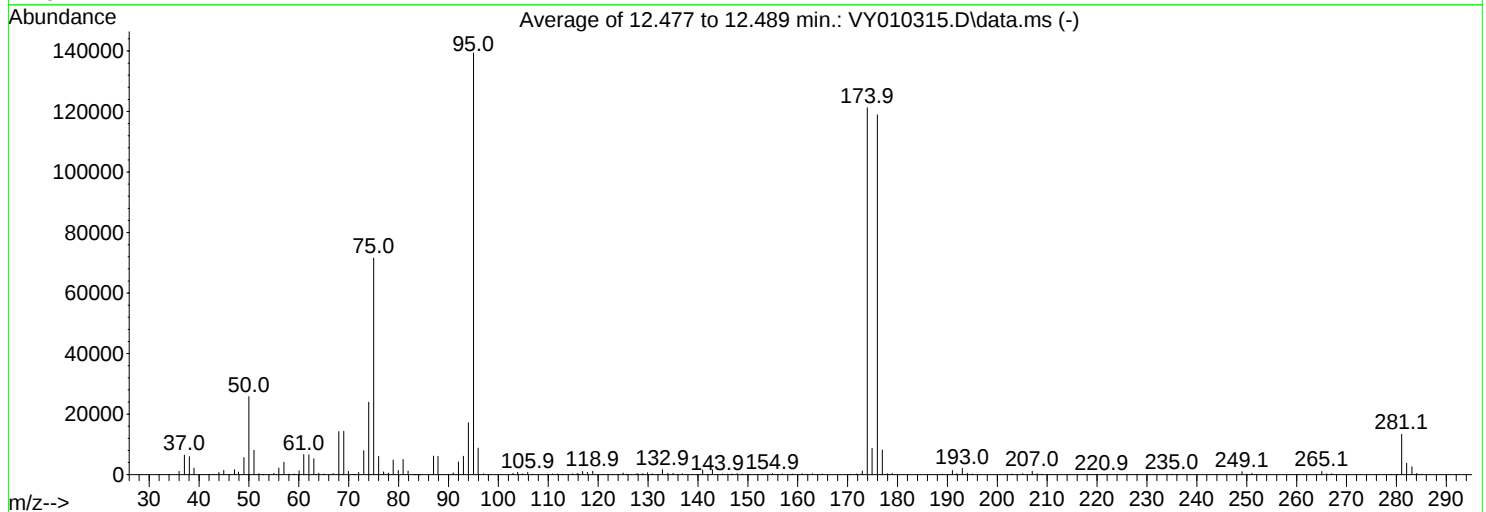


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY090322\
 Data File : VY010315.D
 Acq On : 03 Sep 2022 12:30
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090222S.M
 Title : SW846 8260
 Last Update : Fri Sep 02 16:41:46 2022

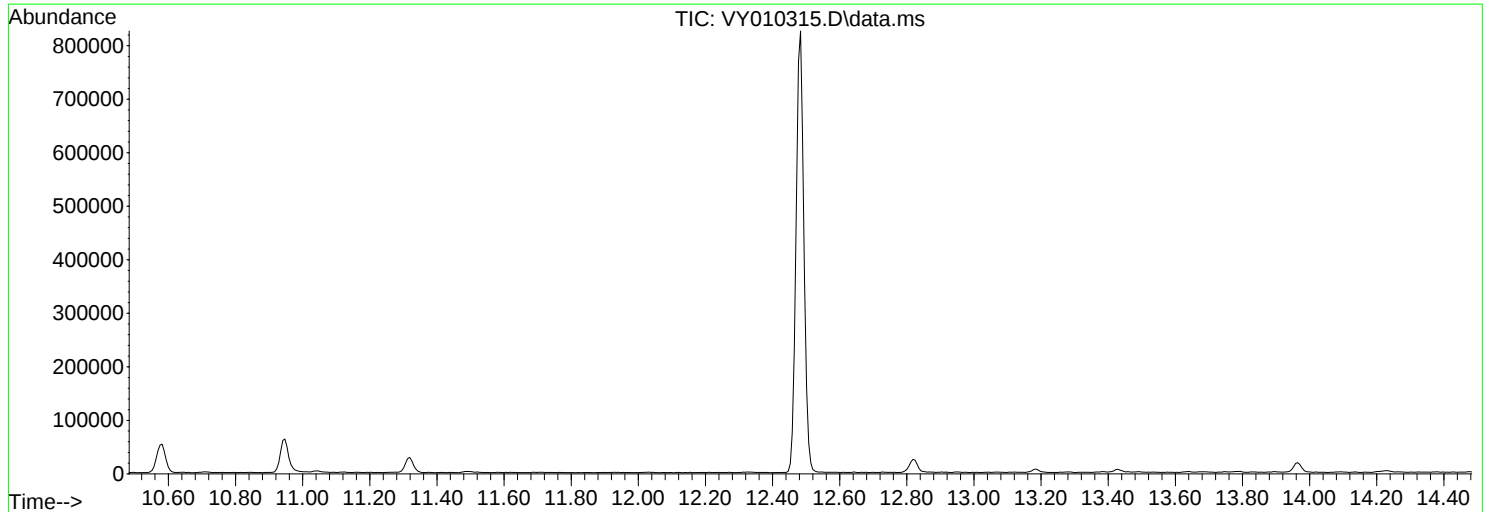

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	25800	PASS
75	95	30	60	51.3	71560	PASS
95	95	100	100	100.0	139376	PASS
96	95	5	9	6.3	8789	PASS
173	174	0.00	2	1.0	1206	PASS
174	95	50	100	87.0	121261	PASS
175	174	5	9	7.2	8673	PASS
176	174	95	101	98.1	118915	PASS
177	176	5	9	6.8	8139	PASS