



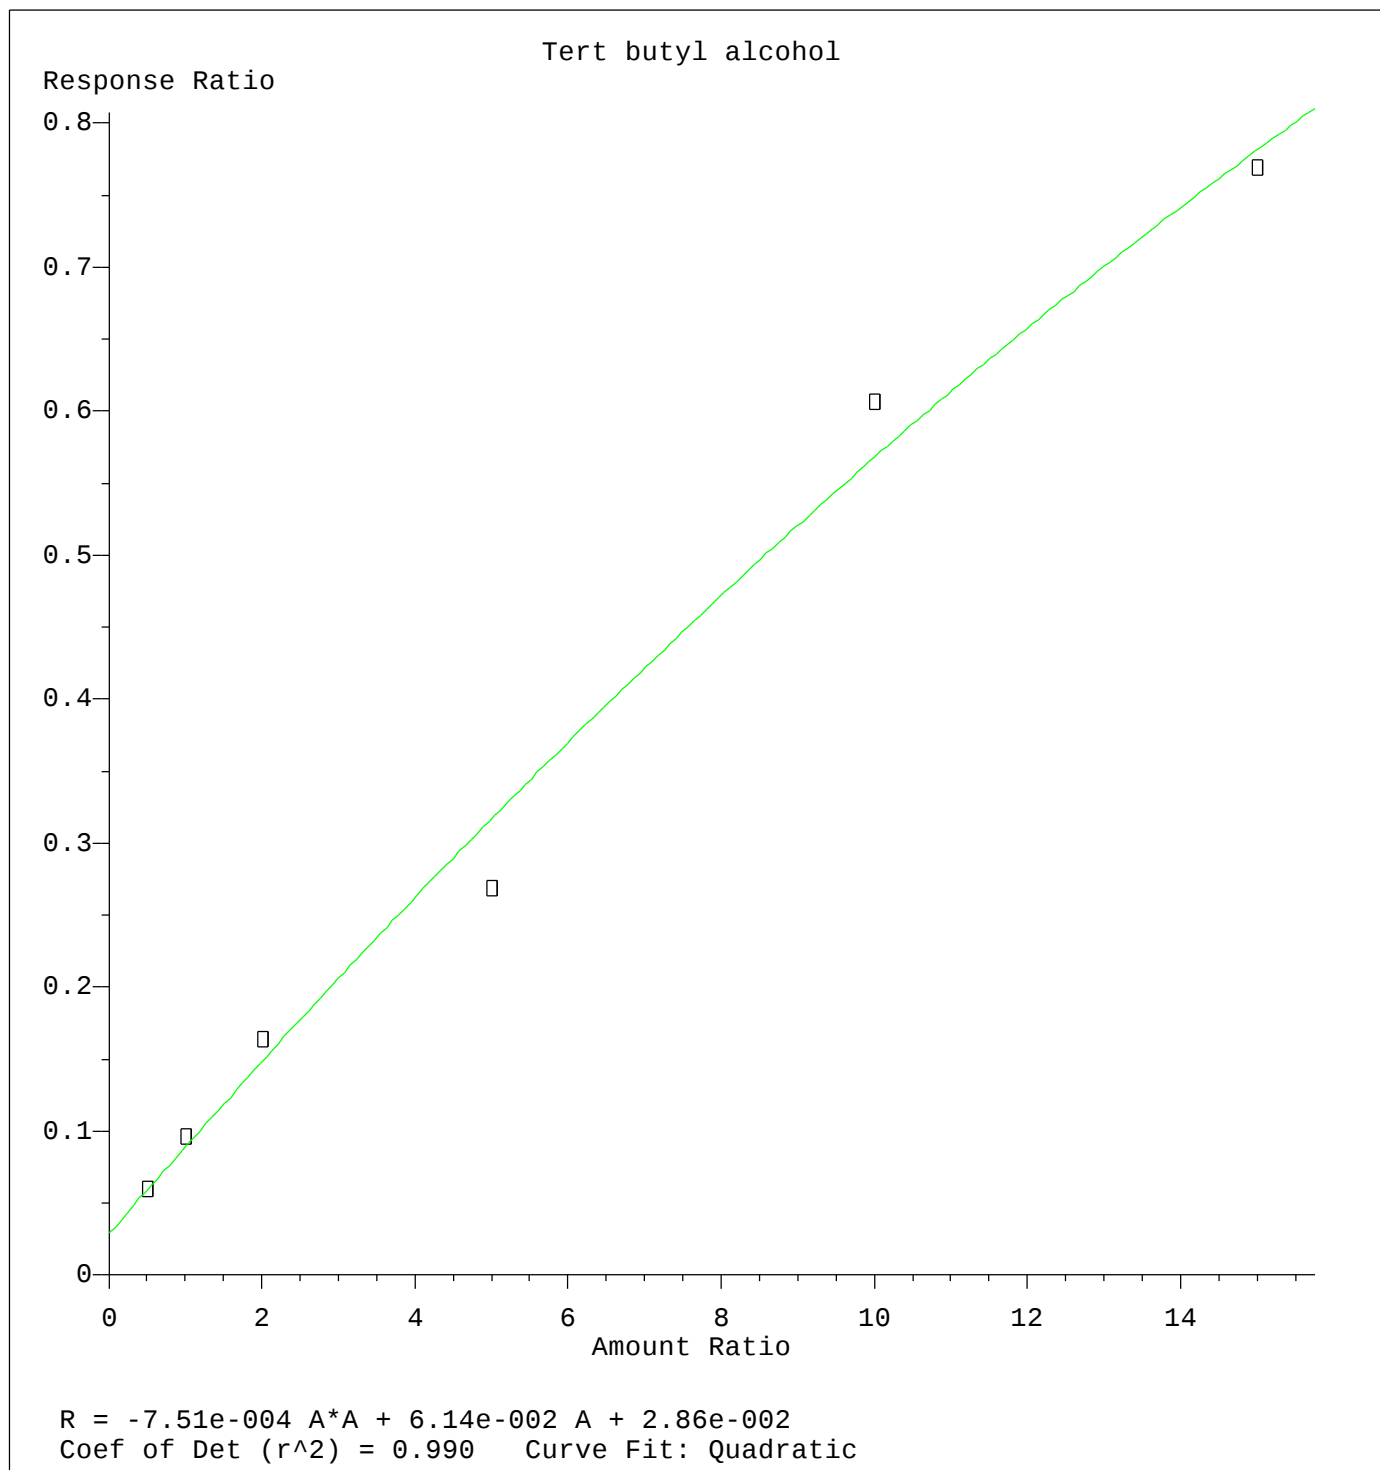

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_Y\METHODS\82Y090420S.M  
Calibration Table Last Updated: Sat Sep 05 00:58:02 2020

# Methylene Chloride

Response Ratio

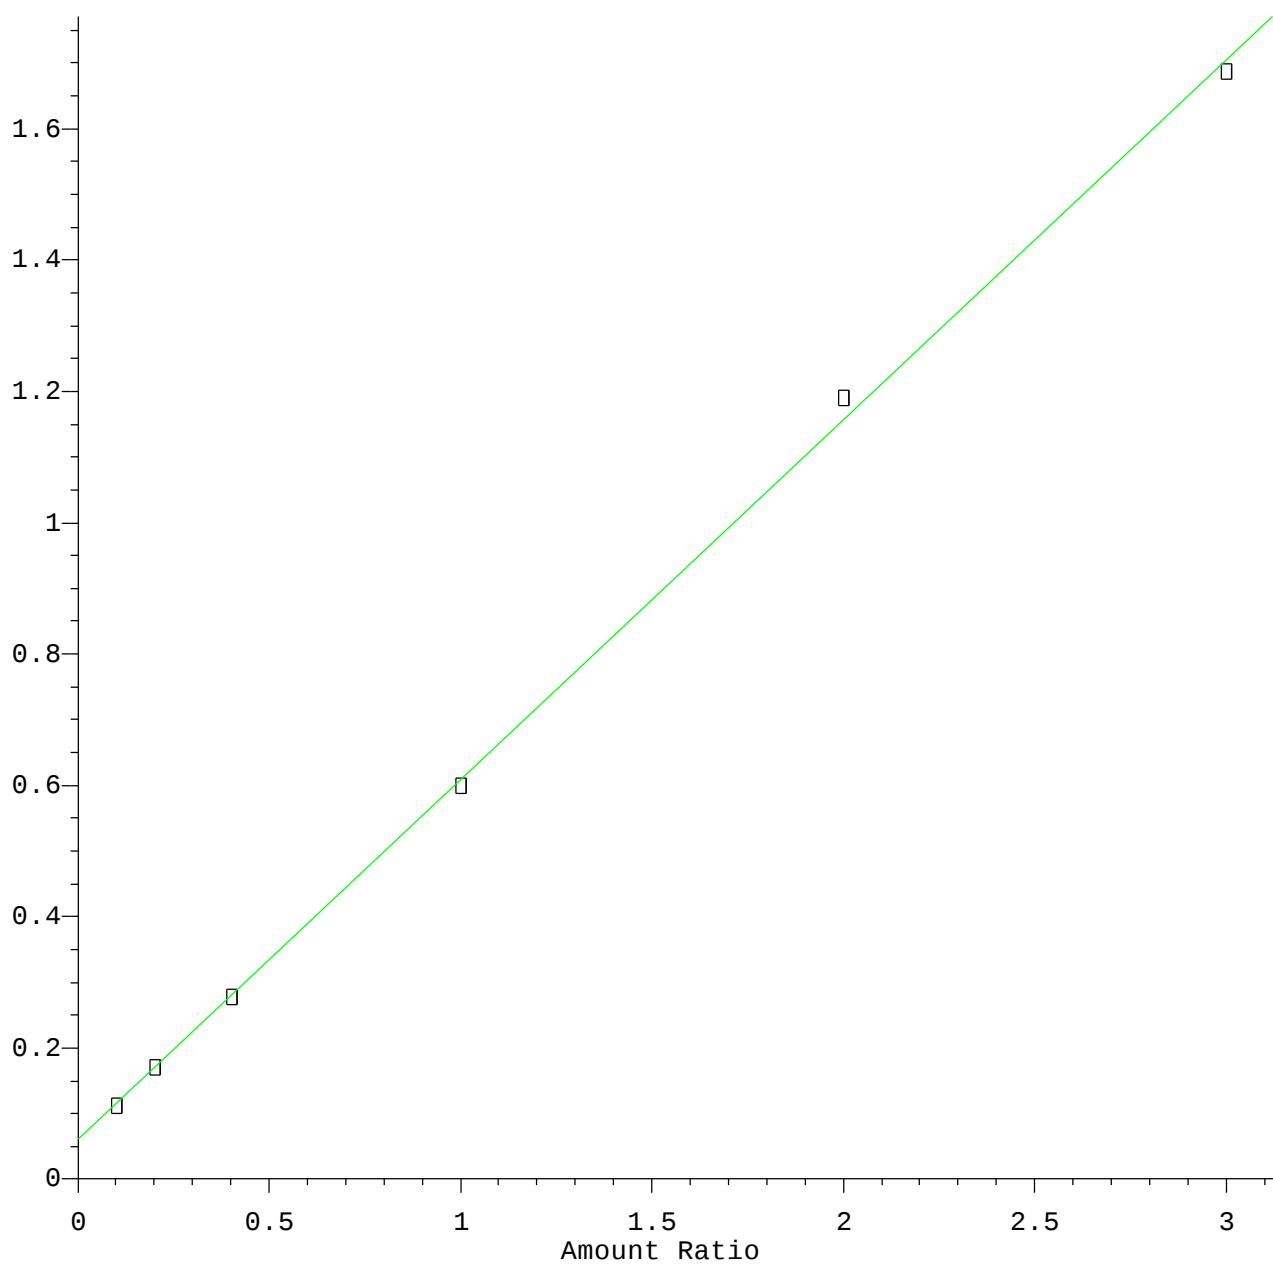


Resp Ratio =  $5.48 \times 10^{-1} \times \text{Amt} + 5.97 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.999    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_Y\METHODS\82Y090420S.M  
Calibration Table Last Updated: Sat Sep 05 00:58:02 2020


# Dichlorodifluoromethane

Response Ratio

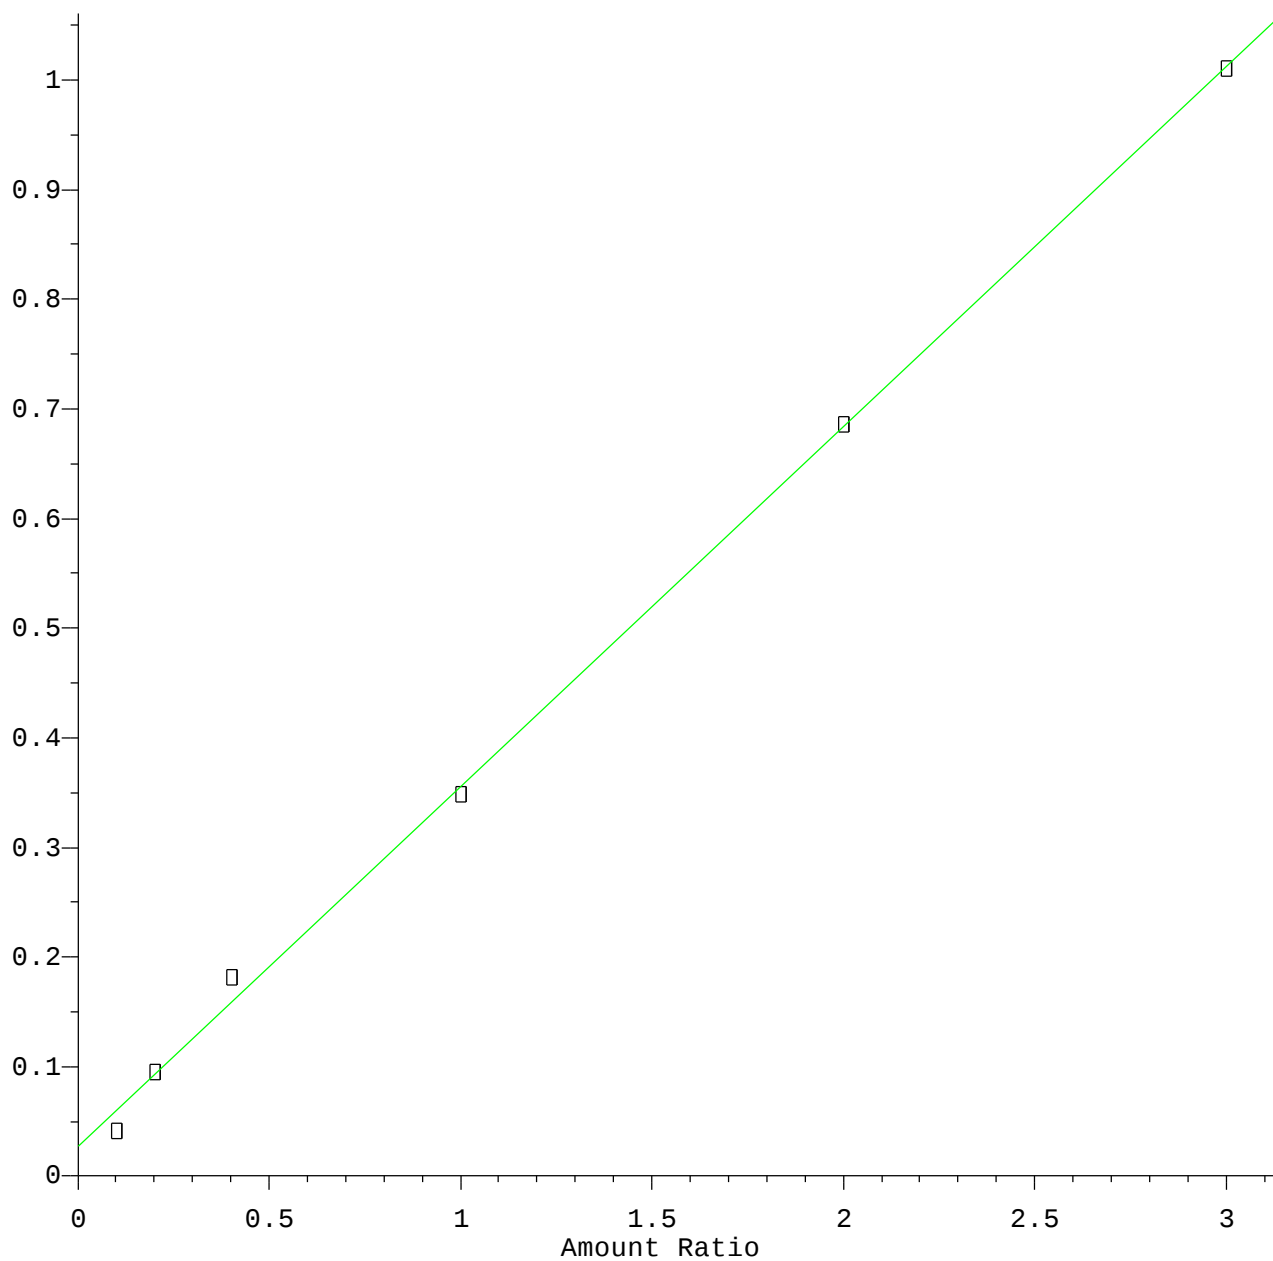


Resp Ratio =  $3.28 \times 10^{-1} \times \text{Amt} + 2.68 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.999    Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_Y\METHODS\82Y090420S.M  
Calibration Table Last Updated: Sat Sep 05 00:58:02 2020

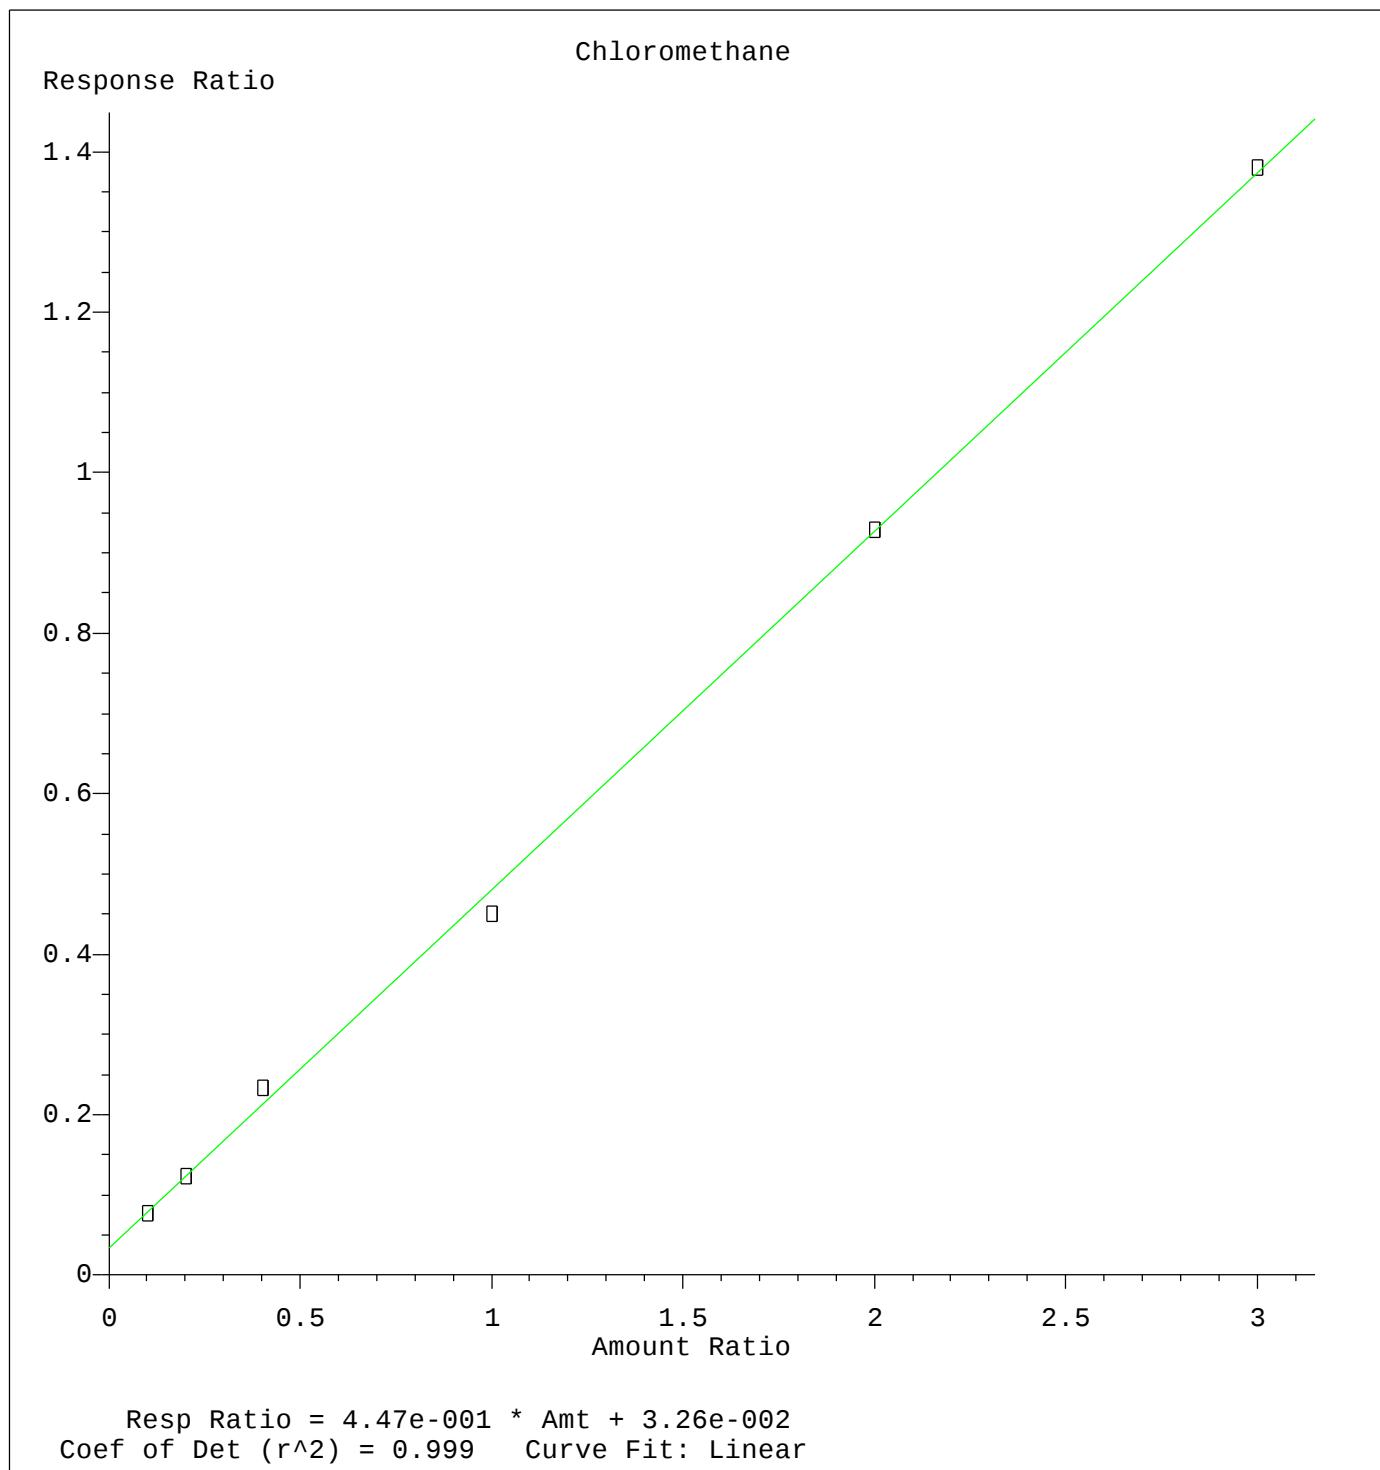

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_Y\METHODS\82Y090420S.M  
Calibration Table Last Updated: Sat Sep 05 00:58:02 2020

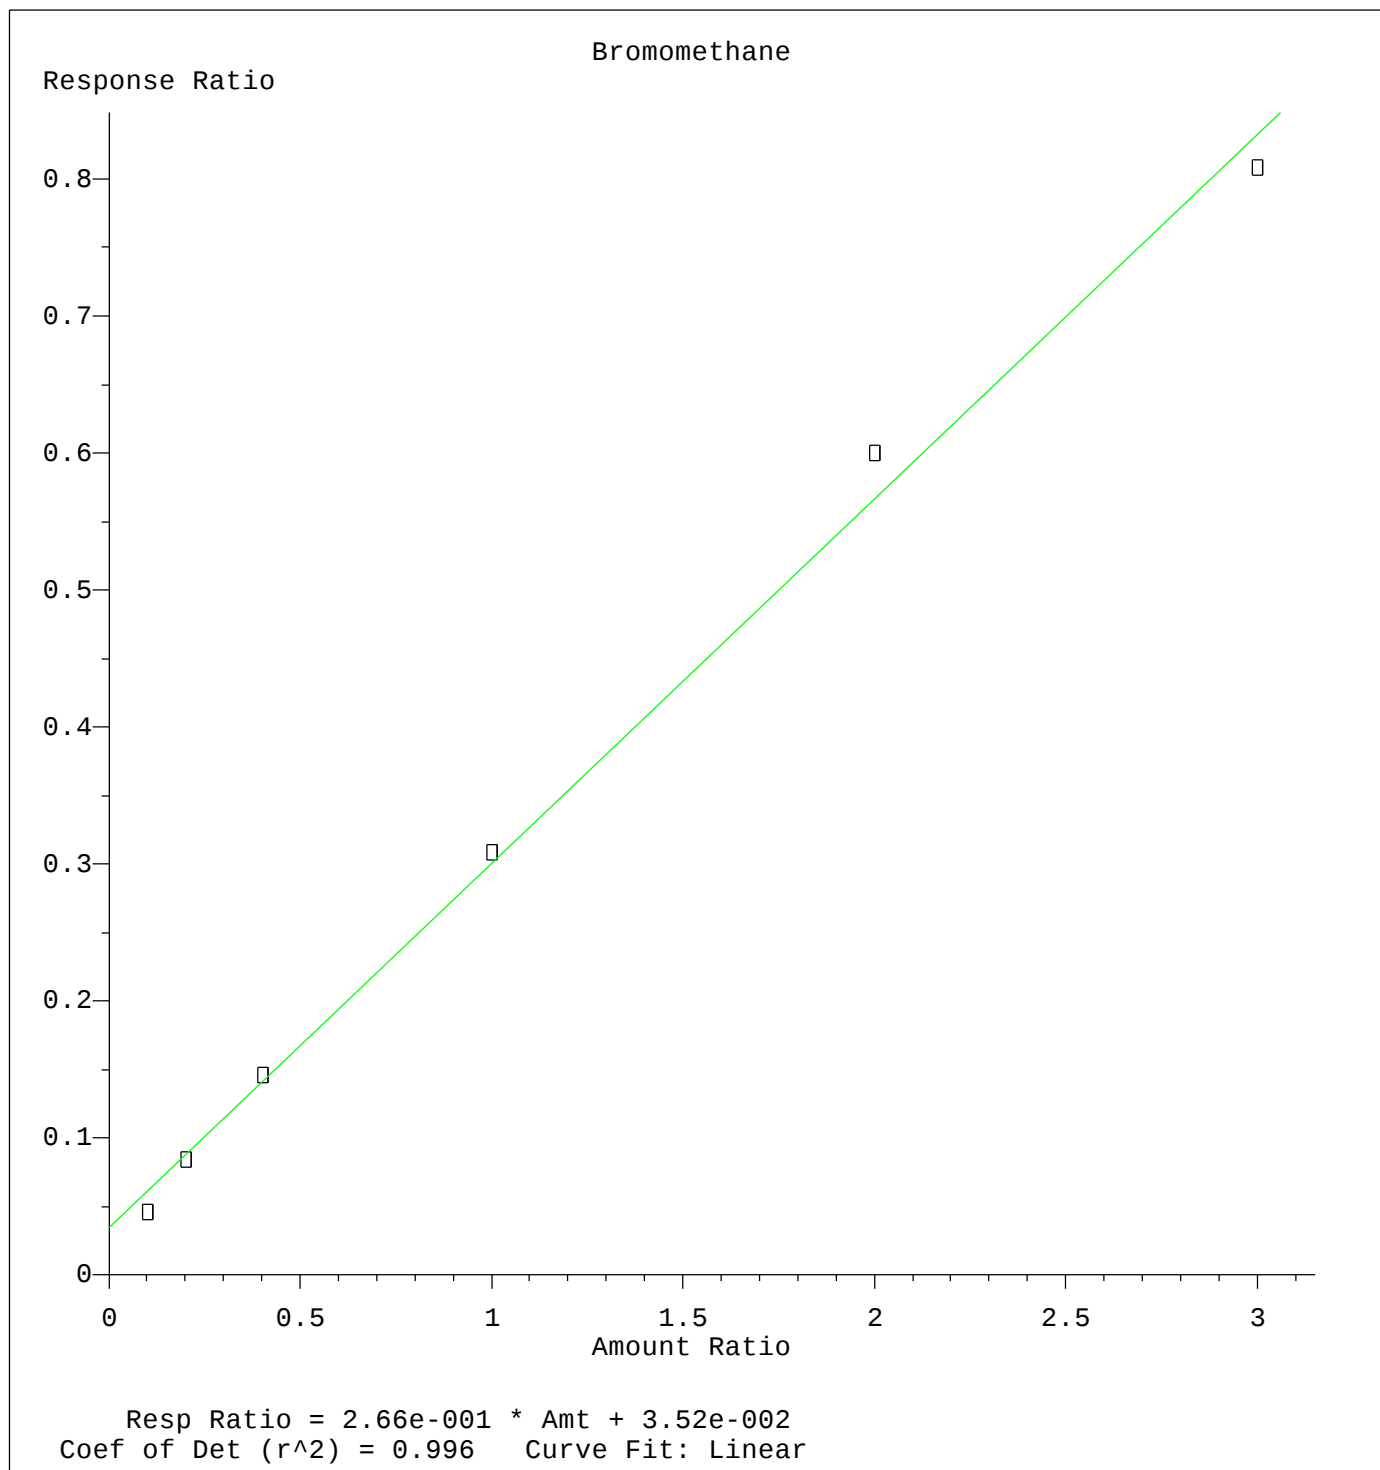

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_Y\METHODS\82Y090420S.M  
Calibration Table Last Updated: Sat Sep 05 00:58:02 2020

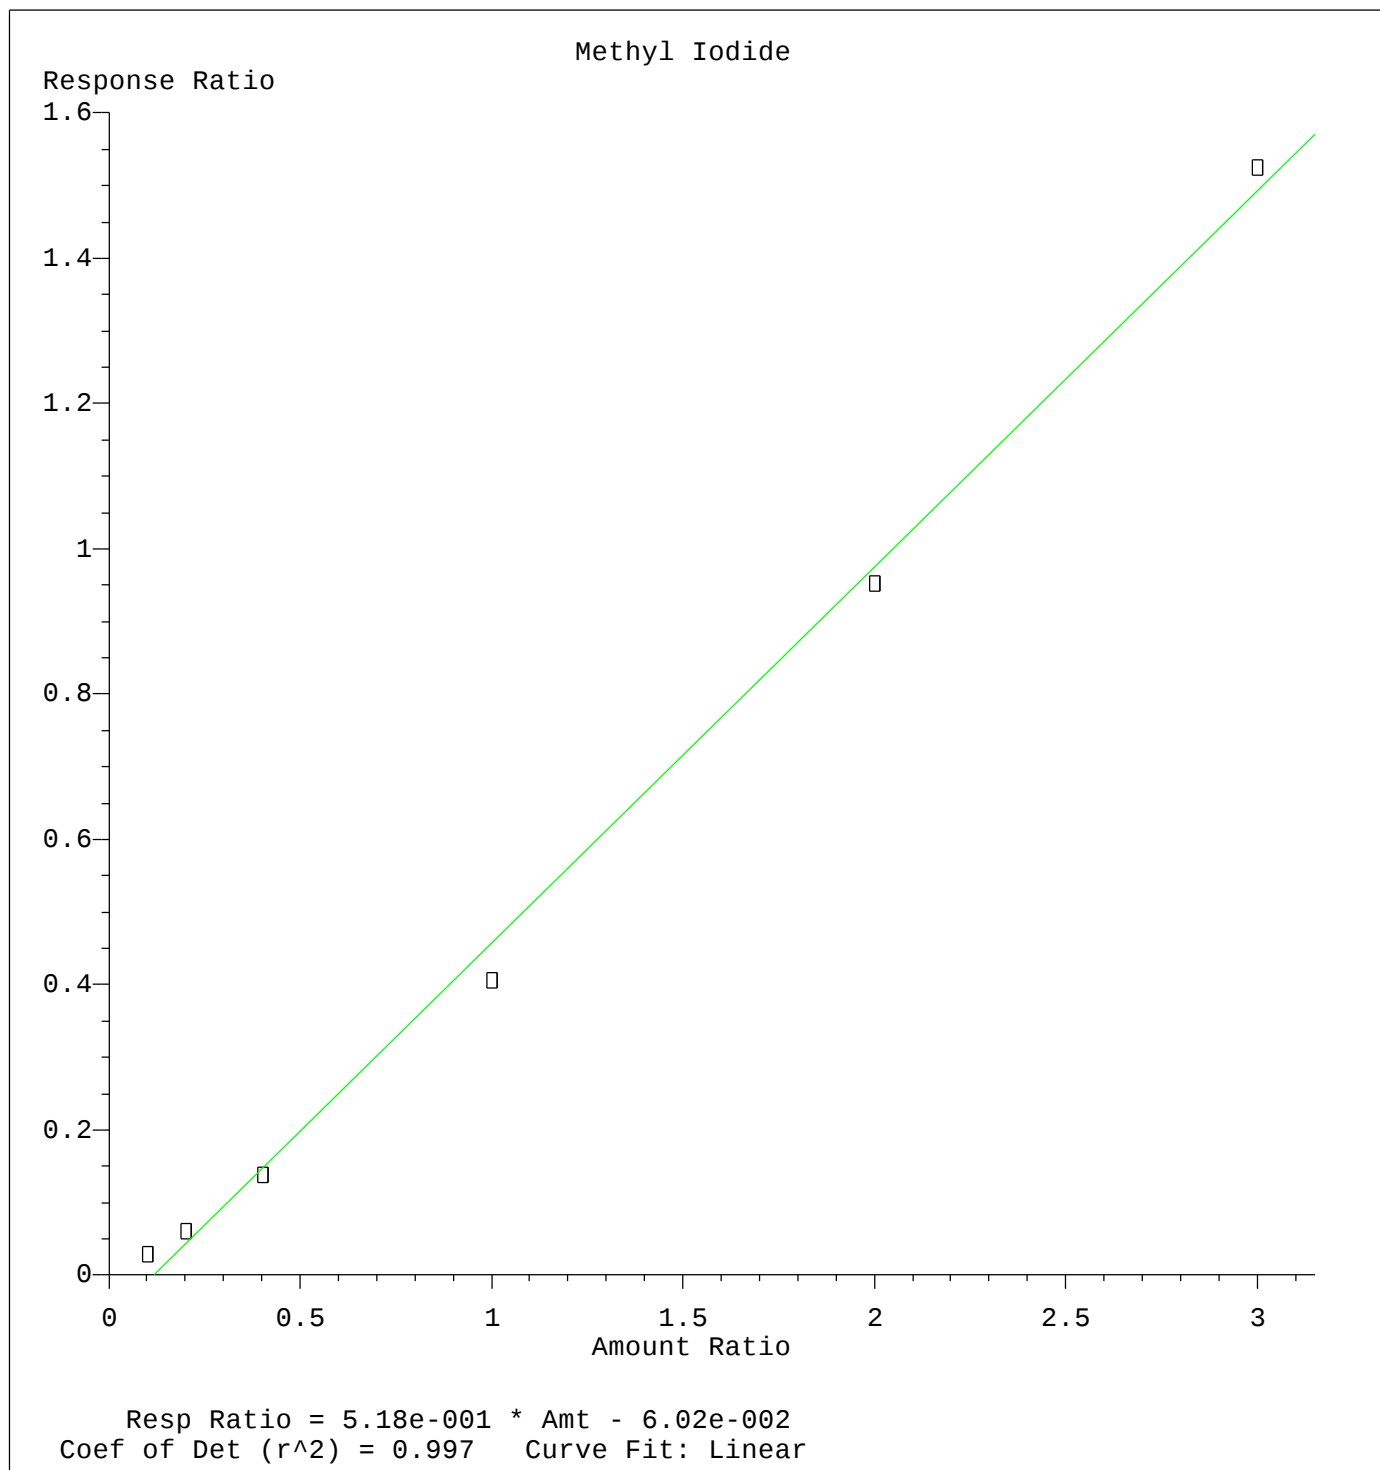

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_Y\METHODS\82Y090420S.M  
Calibration Table Last Updated: Sat Sep 05 00:58:02 2020