


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\VY090420\  
 Data File : VY003430.D  
 Acq On : 04 Sep 2020 13:36  
 Operator : SY/MD  
 Sample : BFB  
 Misc : 5.00G/5ML/MSVOA Y/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_Y\METHODS\82Y090420S.M  
 Title : SW846 8260  
 Last Update : Sat Sep 05 00:58:02 2020

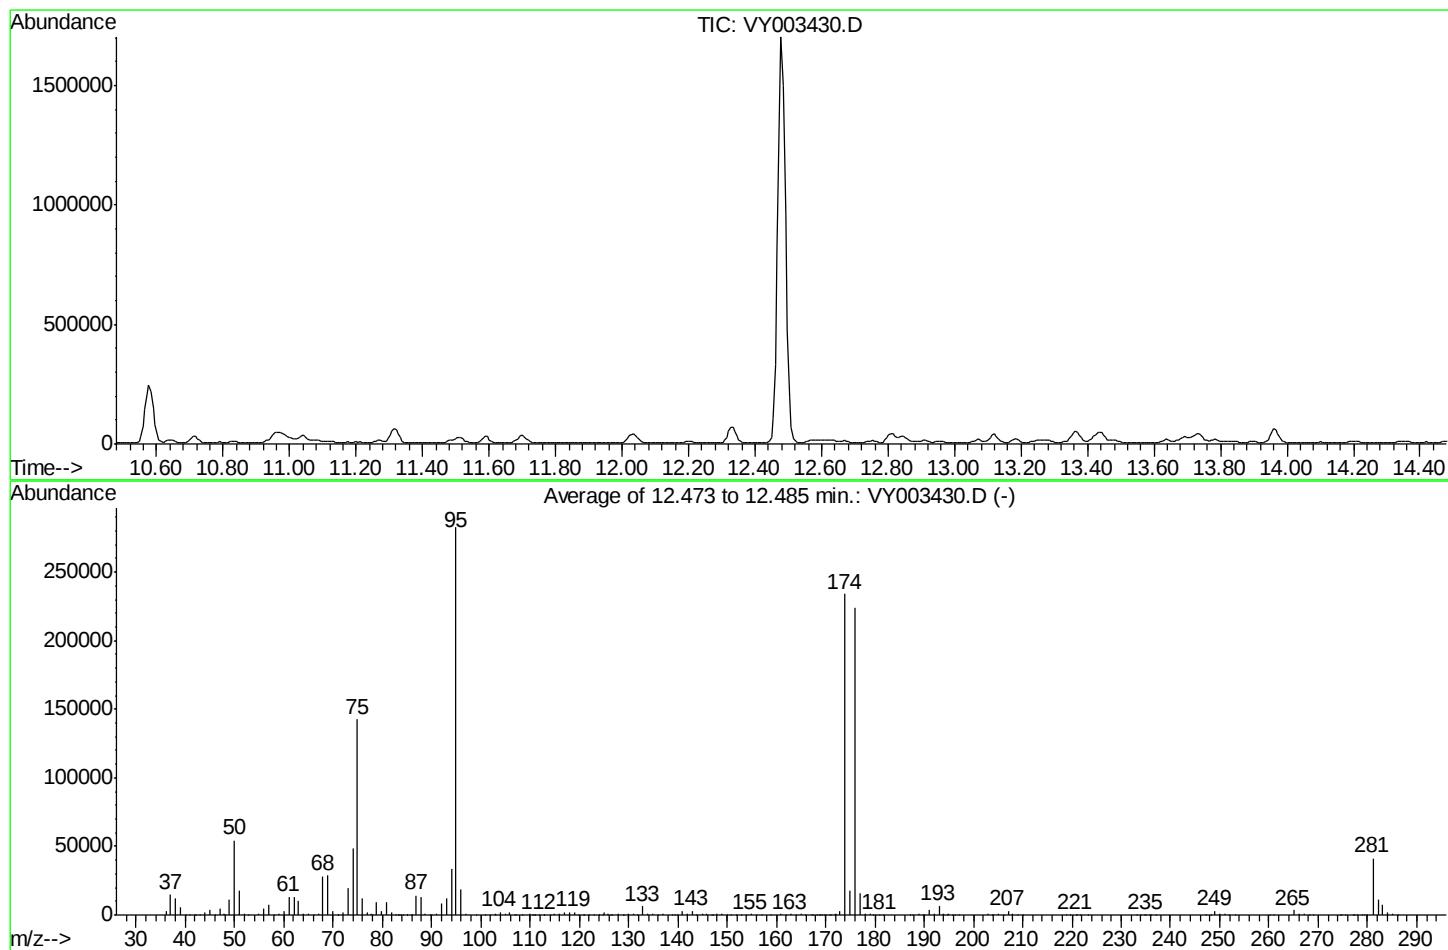

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1750

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 19.3      | 54482   | PASS             |
| 75          | 95           | 30           | 60           | 50.4      | 142532  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 282602  | PASS             |
| 96          | 95           | 5            | 9            | 6.6       | 18712   | PASS             |
| 173         | 174          | 0.00         | 2            | 1.1       | 2490    | PASS             |
| 174         | 95           | 50           | 100          | 82.9      | 234176  | PASS             |
| 175         | 174          | 5            | 9            | 7.5       | 17586   | PASS             |
| 176         | 174          | 95           | 101          | 95.8      | 224362  | PASS             |
| 177         | 176          | 5            | 9            | 7.1       | 15896   | PASS             |