
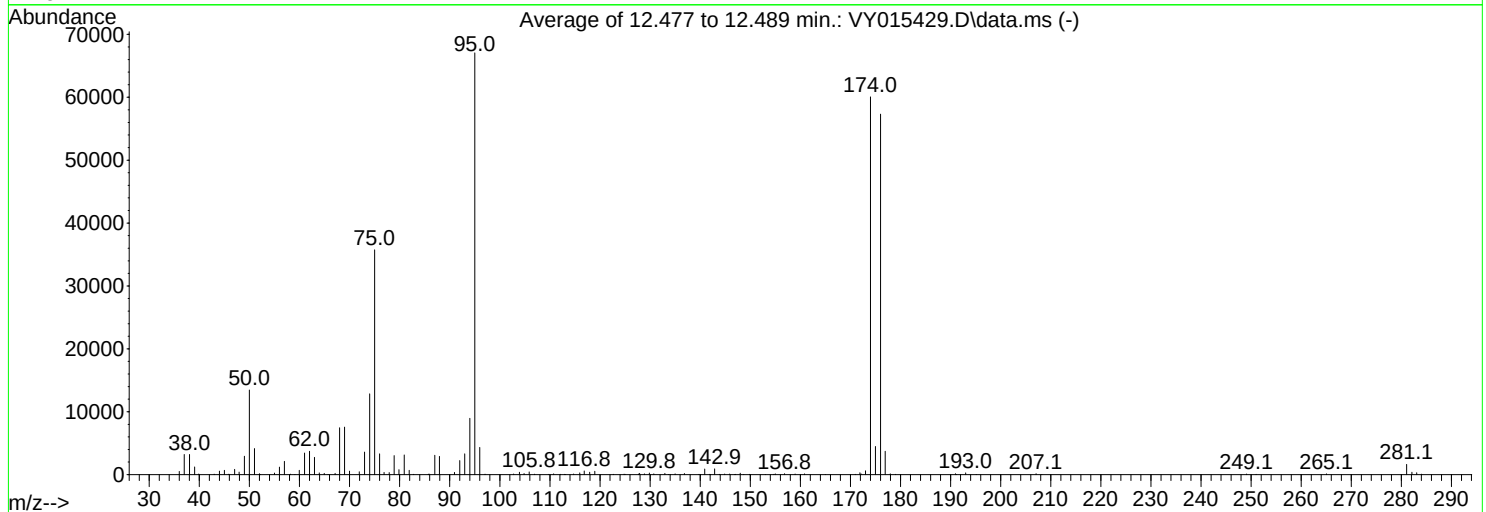


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY090523\
Data File : VY015429.D
Acq On : 05 Sep 2023 09:19
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y082923S.M
Title : SW846 8260
Last Update : Thu Aug 31 20:01:47 2023

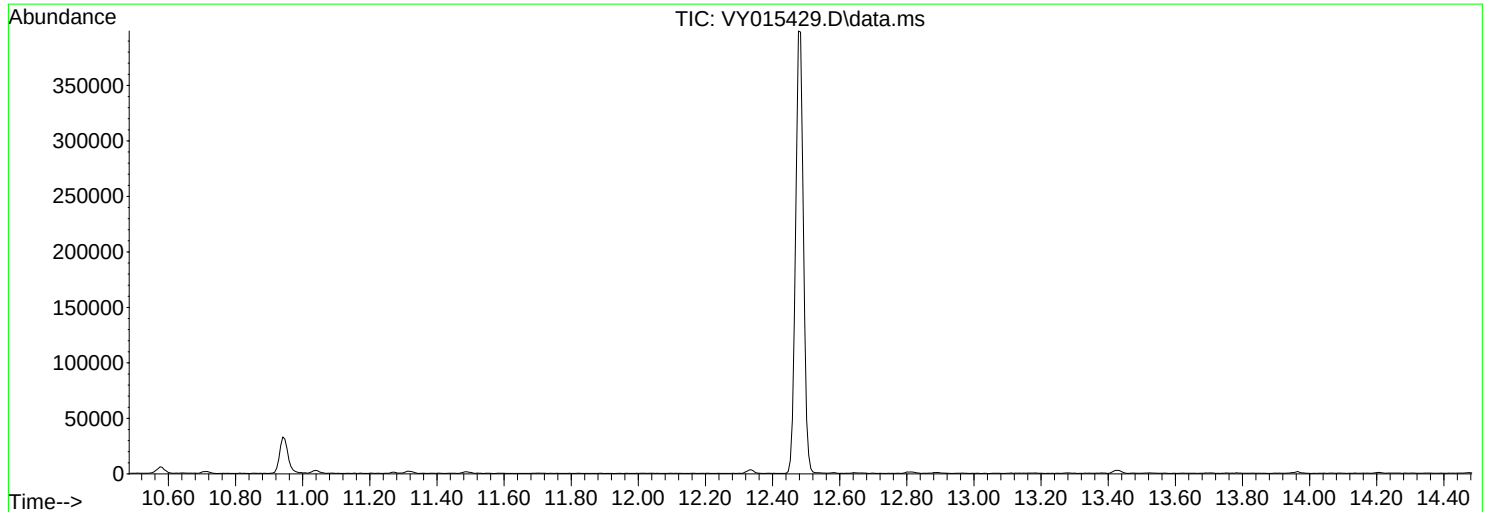

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	13450	PASS
75	95	30	60	53.3	35733	PASS
95	95	100	100	100.0	67064	PASS
96	95	5	9	6.5	4326	PASS
173	174	0.00	2	1.0	610	PASS
174	95	50	100	89.6	60075	PASS
175	174	5	9	7.5	4488	PASS
176	174	95	101	95.4	57323	PASS
177	176	5	9	6.5	3725	PASS