
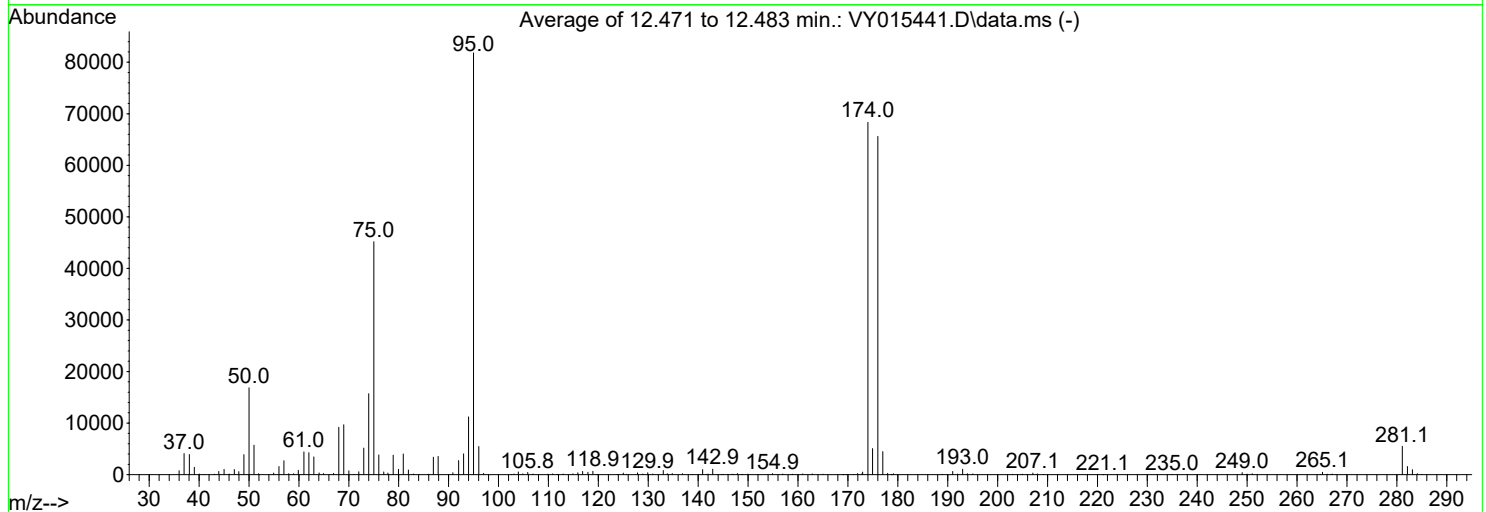


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY090623\
Data File : VY015441.D
Acq On : 06 Sep 2023 09:03
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y082923S.M
Title : SW846 8260
Last Update : Thu Aug 31 20:01:47 2023

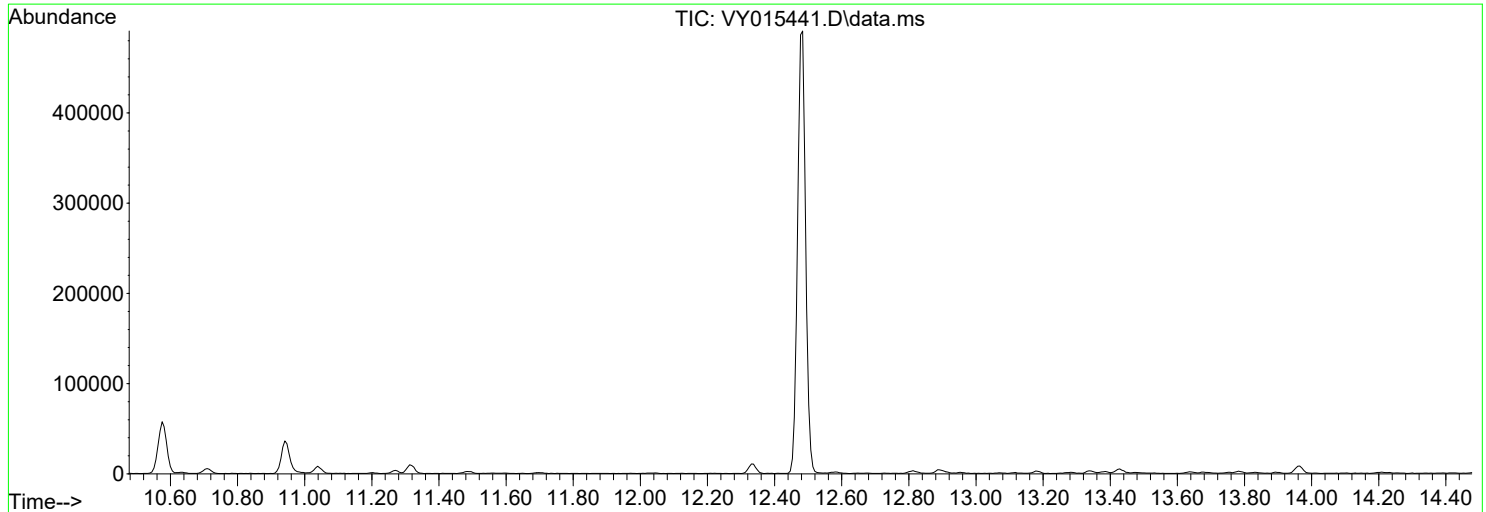

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	16857	PASS
75	95	30	60	55.2	45203	PASS
95	95	100	100	100.0	81819	PASS
96	95	5	9	6.7	5461	PASS
173	174	0.00	2	0.7	509	PASS
174	95	50	100	83.5	68352	PASS
175	174	5	9	7.4	5068	PASS
176	174	95	101	96.0	65611	PASS
177	176	5	9	6.8	4463	PASS