

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY090722\
 Data File : VY010369.D
 Acq On : 07 Sep 2022 14:04
 Operator : KP/MD
 Sample : N4474-03
 Misc : 5.26g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BEACONPOINT-BF-VOC-03

Quant Time: Sep 08 04:10:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090222S.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 02 16:41:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	243057	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	406226	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	377274	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	172634	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	126224	50.646	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	101.300%
35) Dibromofluoromethane	7.716	113	121785	45.033	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	90.060%
50) Toluene-d8	10.179	98	475784	52.549	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	105.100%
62) 4-Bromofluorobenzene	12.483	95	161608	43.784	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	87.560%
Target Compounds						
					Qvalue	
5) Bromomethane	2.668	94	574	Below Cal		87
36) 1,1-Dichloropropene	7.789	75	16875	4.253	ug/l #	50
38) Carbon Tetrachloride	7.783	117	22565	5.518	ug/l #	15
76) 1,2,3-Trichloropropane	12.483	75	82749	40.279	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.483	75	82749	84.026	ug/l #	7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY090722\
Data File : VY010369.D
Acq On : 07 Sep 2022 14:04
Operator : KP/MD
Sample : N4474-03
Misc : 5.26g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BF-VOC-03

Quant Time: Sep 08 04:10:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090222S.M
Quant Title : SW846 8260
QLast Update : Fri Sep 02 16:41:46 2022
Response via : Initial Calibration




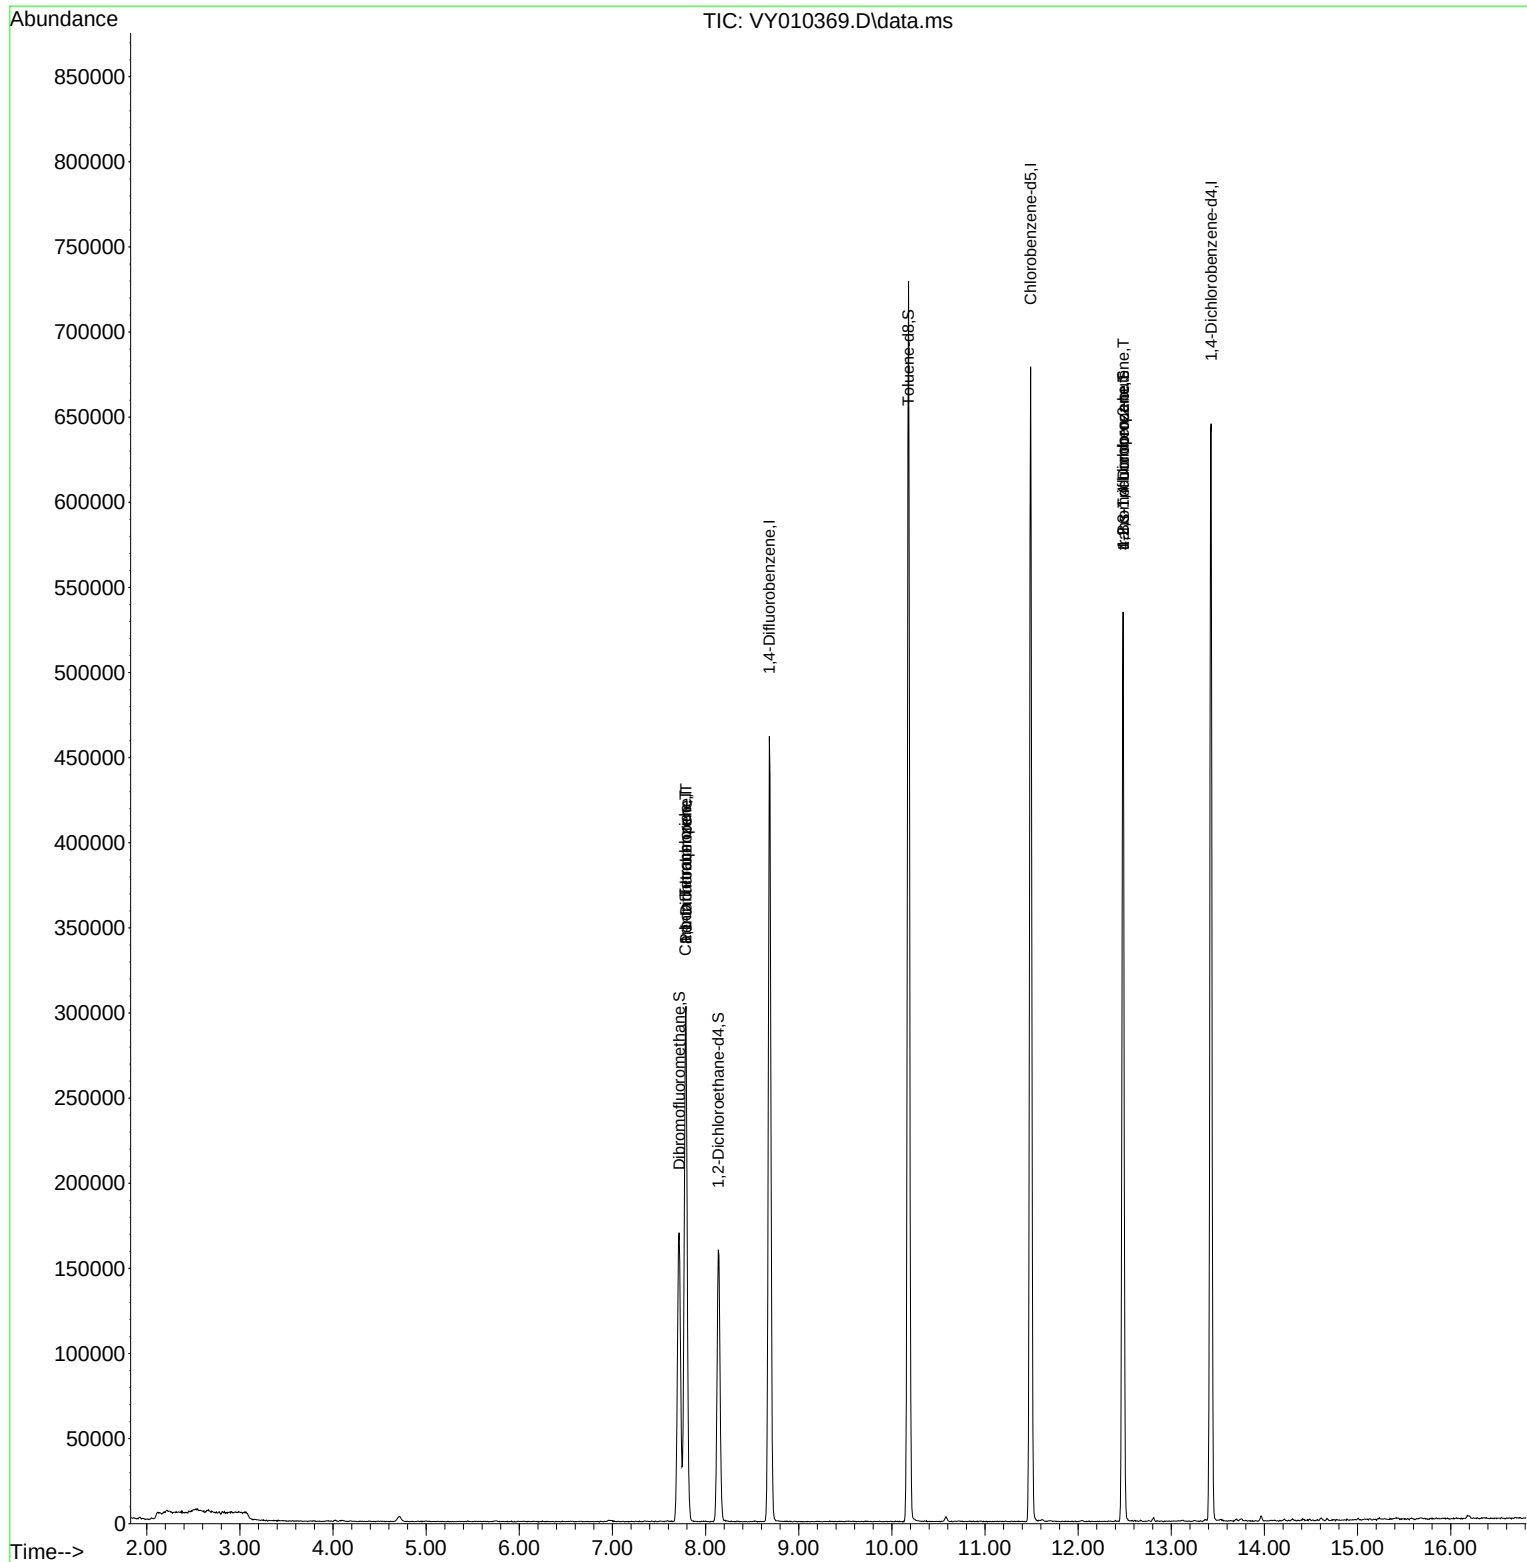


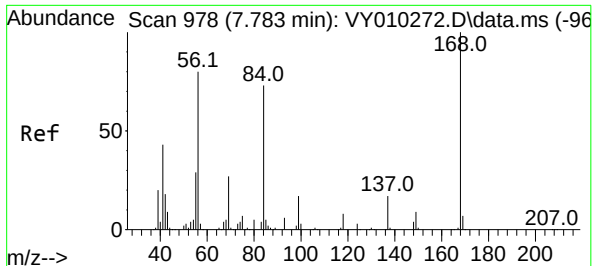

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY010369.D
Acq: 07 Sep 2022 14:04




Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BF-VOC-03


Tgt Ion:168 Resp: 243057
Ion Ratio Lower Upper
168 100
99 53.2 46.9 70.3

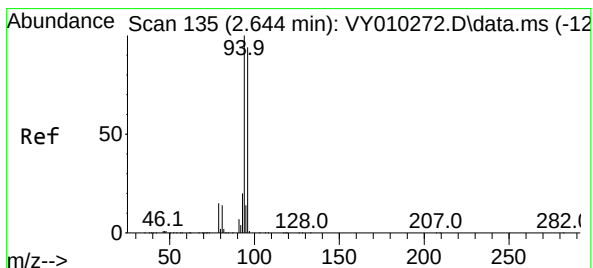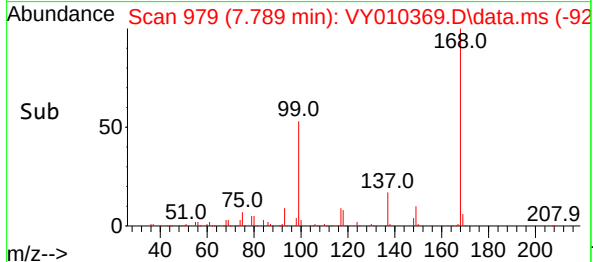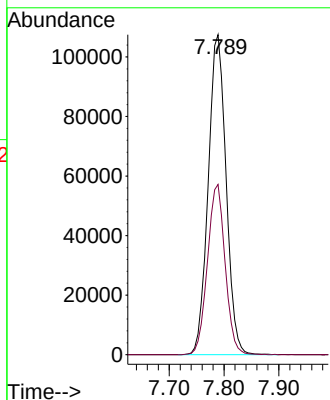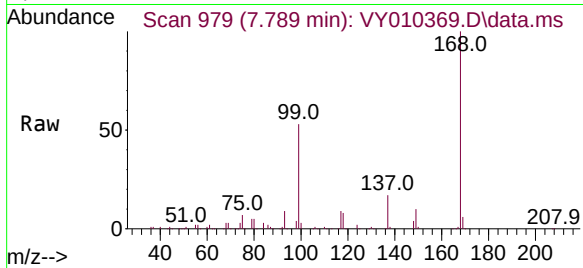

#5
Bromomethane
Concen: Below Cal
RT: 2.668 min Scan# 139
Delta R.T. 0.024 min
Lab File: VY010369.D
Acq: 07 Sep 2022 14:04

Tgt Ion: 94 Resp: 574
Ion Ratio Lower Upper
94 100
96 79.2 73.5 110.3

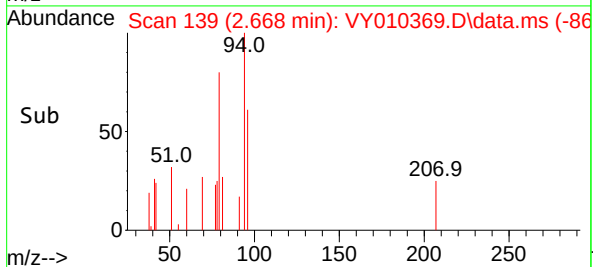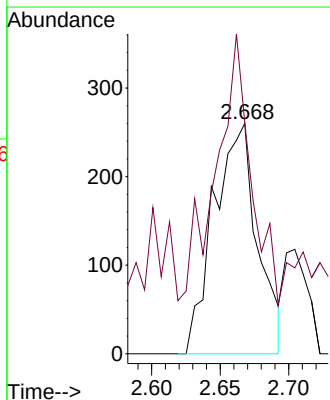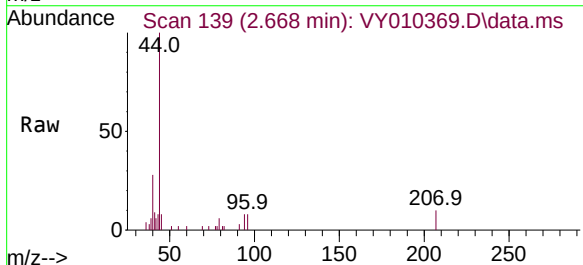

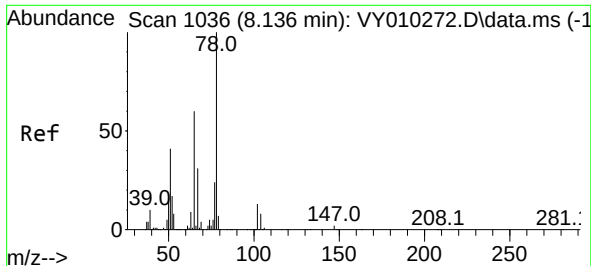

#33

1,2-Dichloroethane-d4

Concen: 50.646 ug/l

RT: 8.136 min Scan# 1036

Delta R.T. 0.000 min

Lab File: VY010369.D

Acq: 07 Sep 2022 14:04

Instrument :

MSVOA_Y

ClientSampleId :





BEACONPOINT-BF-VOC-03

Tgt Ion: 65 Resp: 126224

Ion Ratio Lower Upper

65 100

67 52.4 0.0 99.4

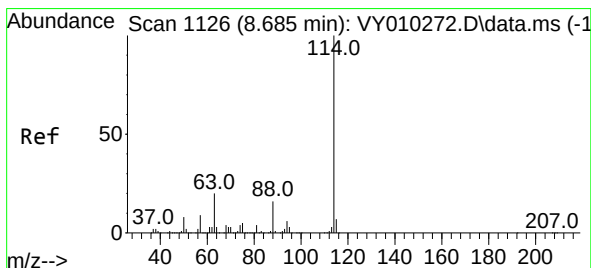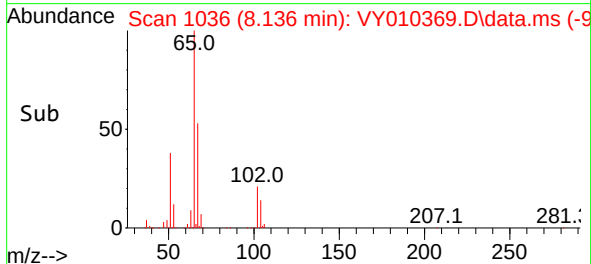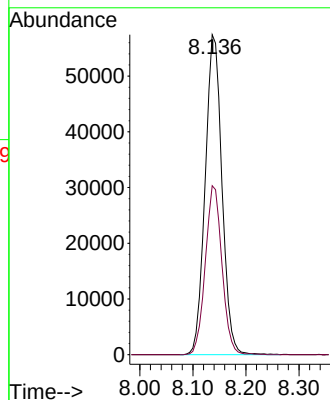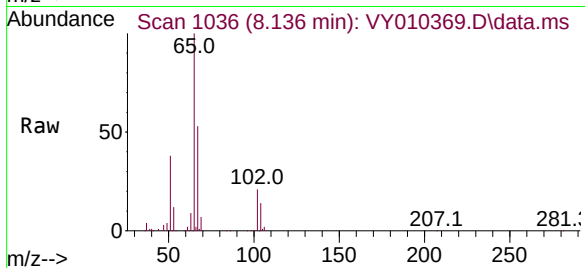

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VY010369.D

Acq: 07 Sep 2022 14:04




Tgt Ion: 114 Resp: 406226


Ion Ratio Lower Upper

114 100

63 19.1 0.0 43.2

88 15.0 0.0 31.8


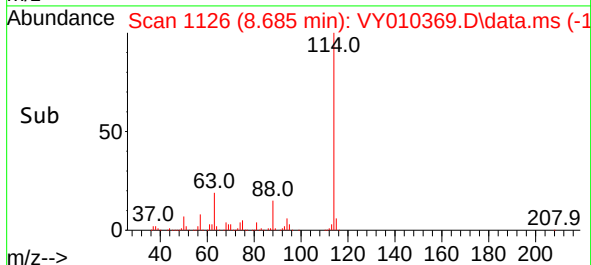
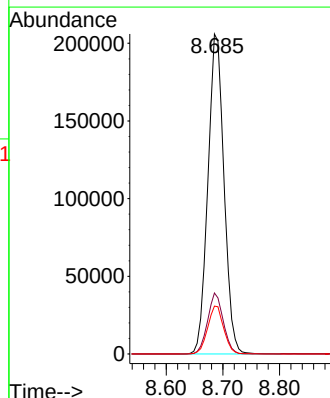
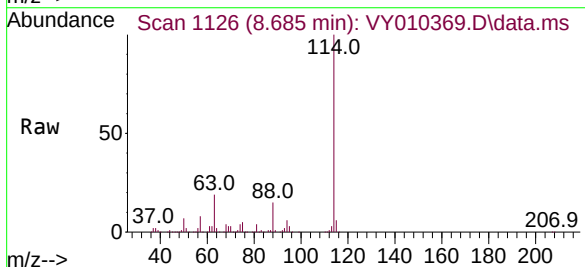


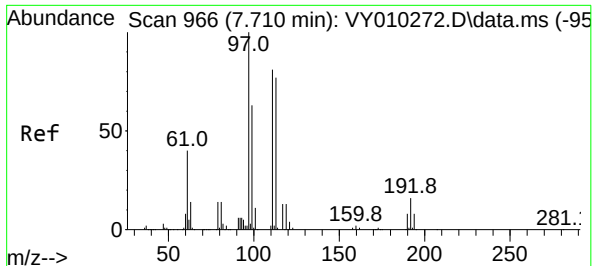

#35
Dibromofluoromethane
Concen: 45.033 ug/l
RT: 7.716 min Scan# 910
Delta R.T. 0.006 min
Lab File: VY010369.D
Acq: 07 Sep 2022 14:04




Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BF-VOC-03


Tgt Ion:113 Resp: 121785
Ion Ratio Lower Upper
113 100
111 102.6 82.6 124.0
192 20.3 17.6 26.4

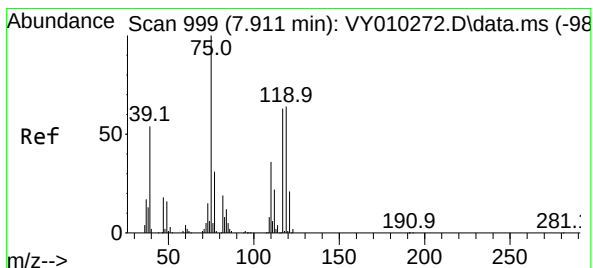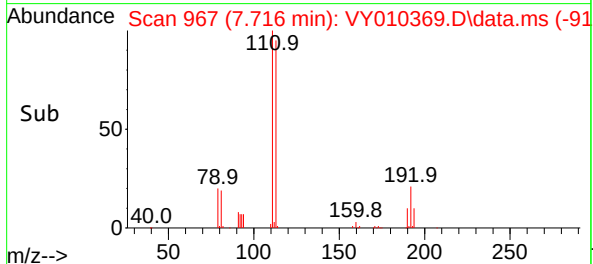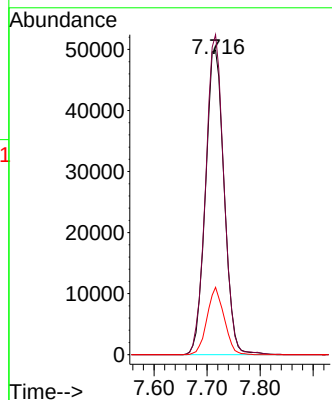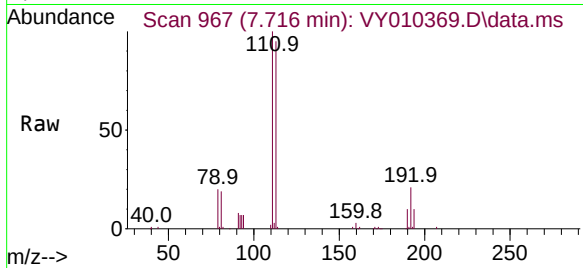

#36
1,1-Dichloropropene
Concen: 4.253 ug/l
RT: 7.789 min Scan# 979
Delta R.T. -0.122 min
Lab File: VY010369.D
Acq: 07 Sep 2022 14:04

Tgt Ion: 75 Resp: 16875
Ion Ratio Lower Upper
75 100
110 8.9 17.1 51.2#
77 0.0 24.4 36.6#


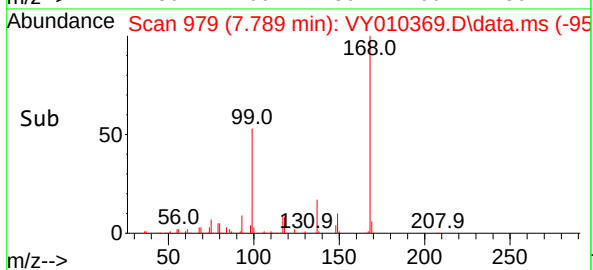
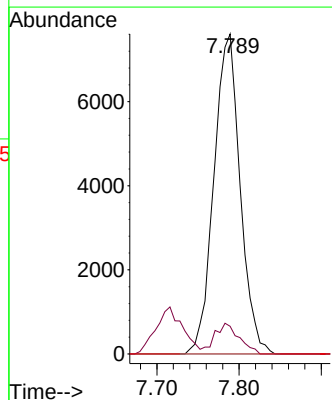
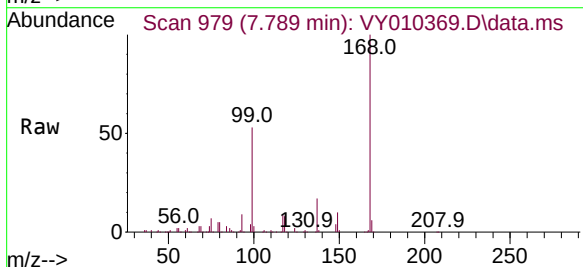


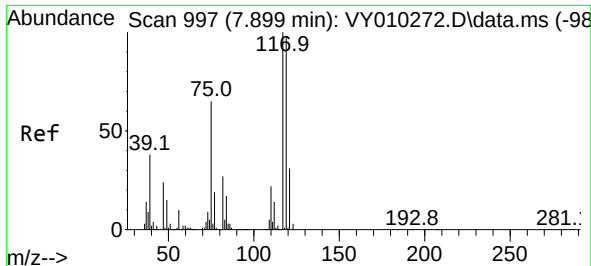

#38
Carbon Tetrachloride
Concen: 5.518 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.116 min
Lab File: VY010369.D
Acq: 07 Sep 2022 14:04




Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BF-VOC-03


Tgt Ion:117 Resp: 22565
Ion Ratio Lower Upper
117 100
119 5.2 77.9 116.9#
121 0.0 24.8 37.2#

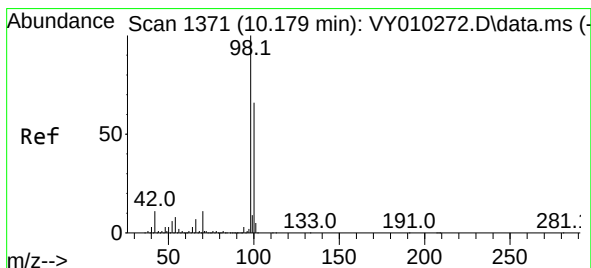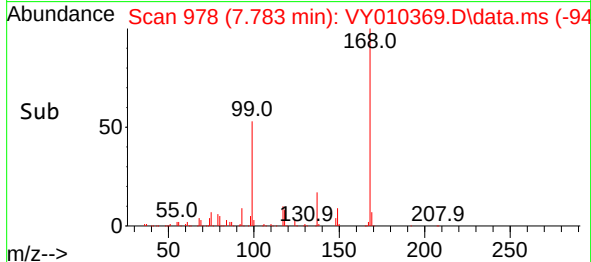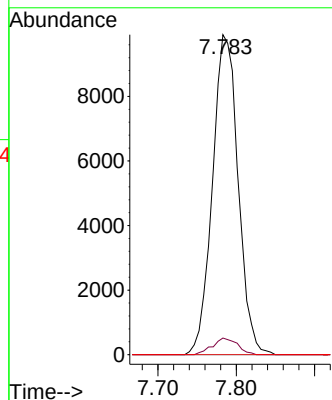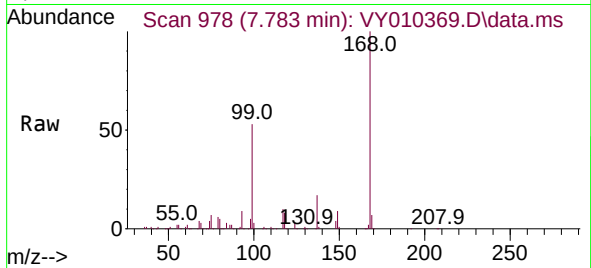

#50
Toluene-d8
Concen: 52.549 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY010369.D
Acq: 07 Sep 2022 14:04

Tgt Ion: 98 Resp: 475784
Ion Ratio Lower Upper
98 100
100 65.6 50.2 75.2


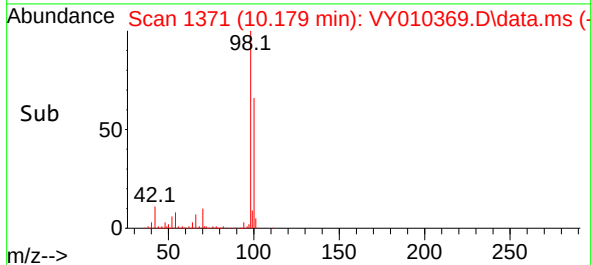
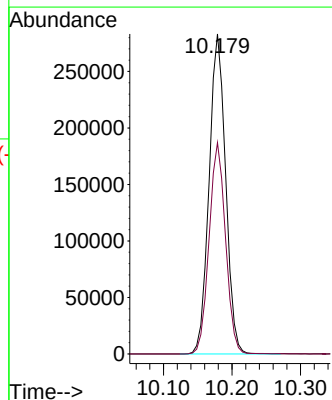
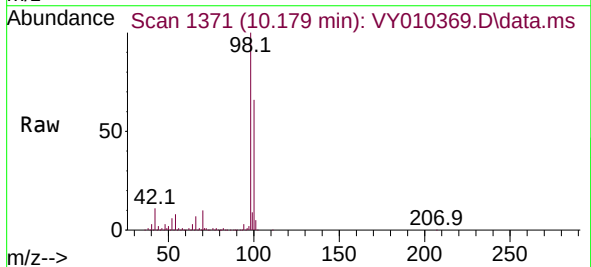


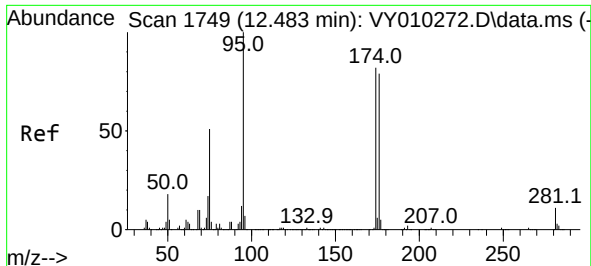

#62
4-Bromofluorobenzene
Concen: 43.784 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY010369.D
Acq: 07 Sep 2022 14:04




Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BF-VOC-03


Tgt Ion: 95 Resp: 161608
Ion Ratio Lower Upper
95 100
174 87.9 0.0 177.0
176 85.1 0.0 175.8

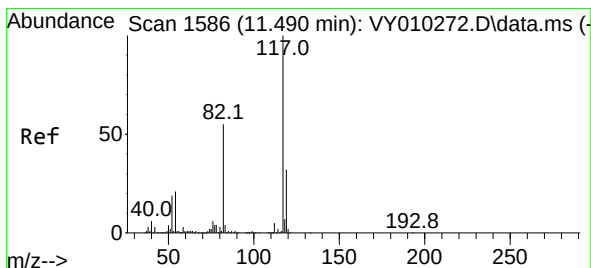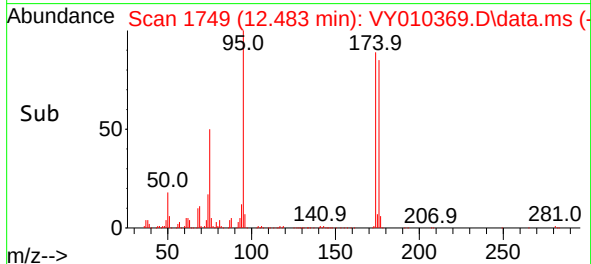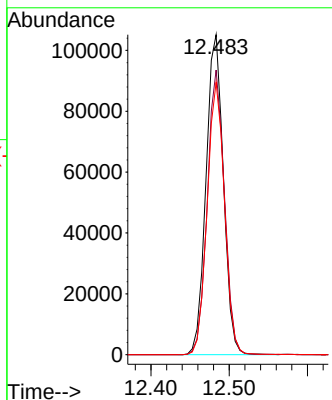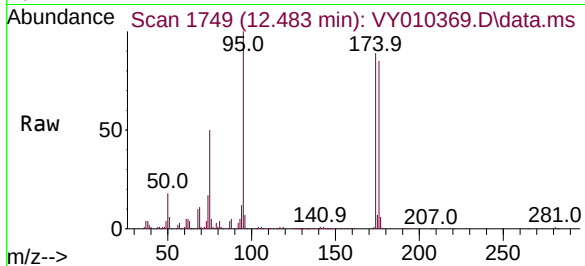

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 1586
Delta R.T. -0.001 min
Lab File: VY010369.D
Acq: 07 Sep 2022 14:04

Tgt Ion: 117 Resp: 377274
Ion Ratio Lower Upper
117 100
82 53.7 43.0 64.4
119 31.8 25.4 38.0

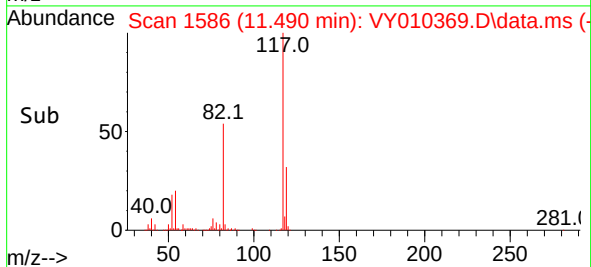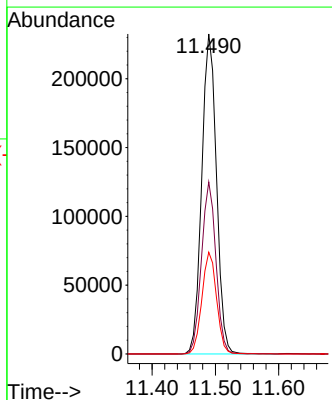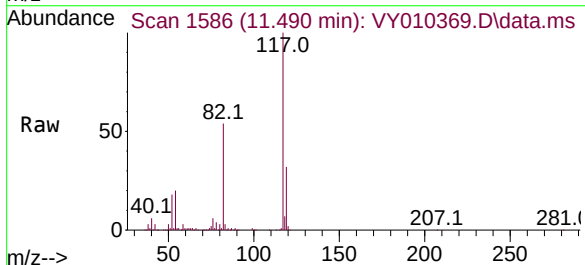

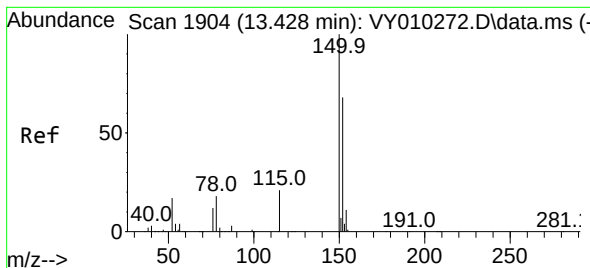

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.000 min

Lab File: VY010369.D


Acq: 07 Sep 2022 14:04

Instrument :

MSVOA_Y

ClientSampleId :

BEACONPOINT-BF-VOC-03

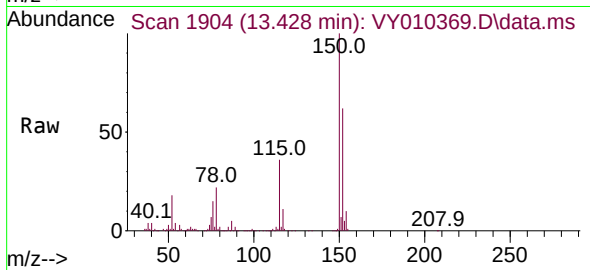




Tgt Ion:152 Resp: 172634

Ion Ratio Lower Upper

152 100

115 57.9 28.2 84.7

150 158.3 0.0 347.6

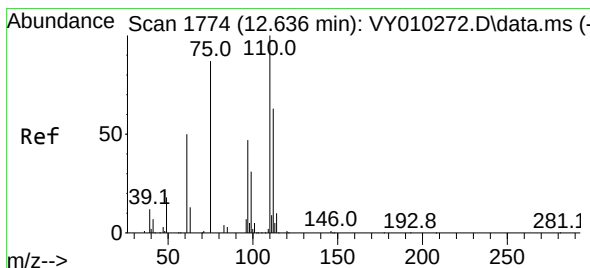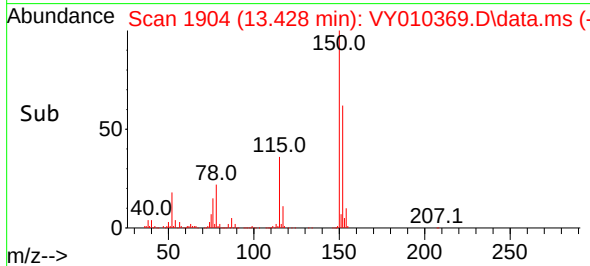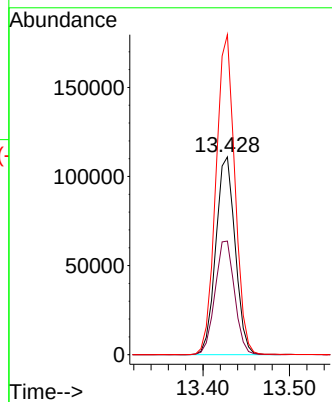

#76

1,2,3-Trichloropropane

Concen: 40.279 ug/l

RT: 12.483 min Scan# 1749

Delta R.T. -0.153 min

Lab File: VY010369.D




Acq: 07 Sep 2022 14:04


Tgt Ion: 75 Resp: 82749

Ion Ratio Lower Upper

75 100


77 1.2 0.0 0.0#

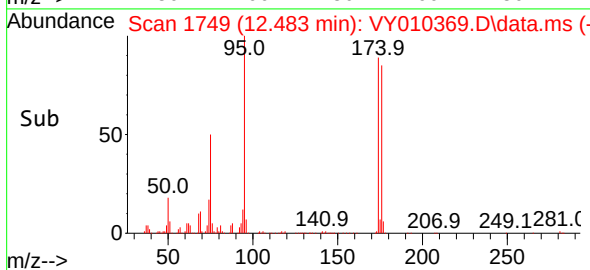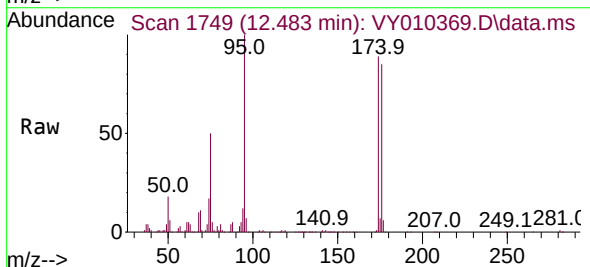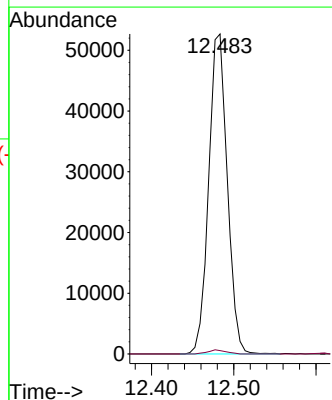

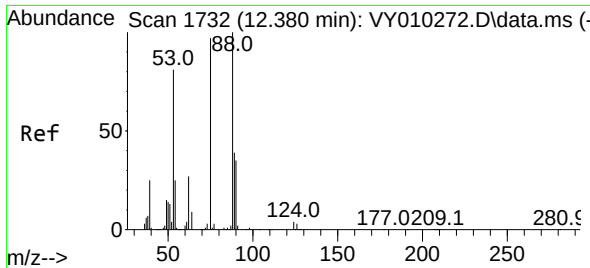

#81
 trans-1,4-Dichloro-2-butene
 Concen: 84.026 ug/l
 RT: 12.483 min Scan# 11
 Delta R.T. 0.103 min
 Lab File: VY010369.D
 Acq: 07 Sep 2022 14:04

Instrument :
 MSVOA_Y
 ClientSampleId :
 BEACONPOINT-BF-VOC-03

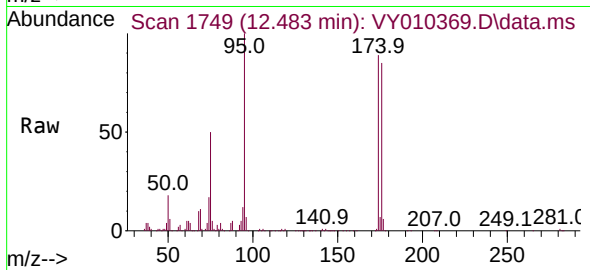

Tgt Ion: 75 Resp: 82749
 Ion Ratio Lower Upper
 75 100
 53 0.0 85.3 127.9#
 89 0.0 37.0 55.4#

