

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY090722\
 Data File : VY010371.D
 Acq On : 07 Sep 2022 14:50
 Operator : KP/MD
 Sample : N4474-05
 Misc : 5.56g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BEACONPOINT-BF-VOC-05

Quant Time: Sep 08 04:11:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090222S.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 02 16:41:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	239994	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	399128	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	375547	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	175027	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	129071	52.449	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 104.900%	
35) Dibromofluoromethane	7.716	113	122269	46.016	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 92.040%	
50) Toluene-d8	10.179	98	470632	52.904	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 105.800%	
62) 4-Bromofluorobenzene	12.483	95	162149	44.865	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 89.740%	


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY090722\
Data File : VY010371.D
Acq On : 07 Sep 2022 14:50
Operator : KP/MD
Sample : N4474-05
Misc : 5.56g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BF-VOC-05

Quant Time: Sep 08 04:11:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090222S.M
Quant Title : SW846 8260
QLast Update : Fri Sep 02 16:41:46 2022
Response via : Initial Calibration




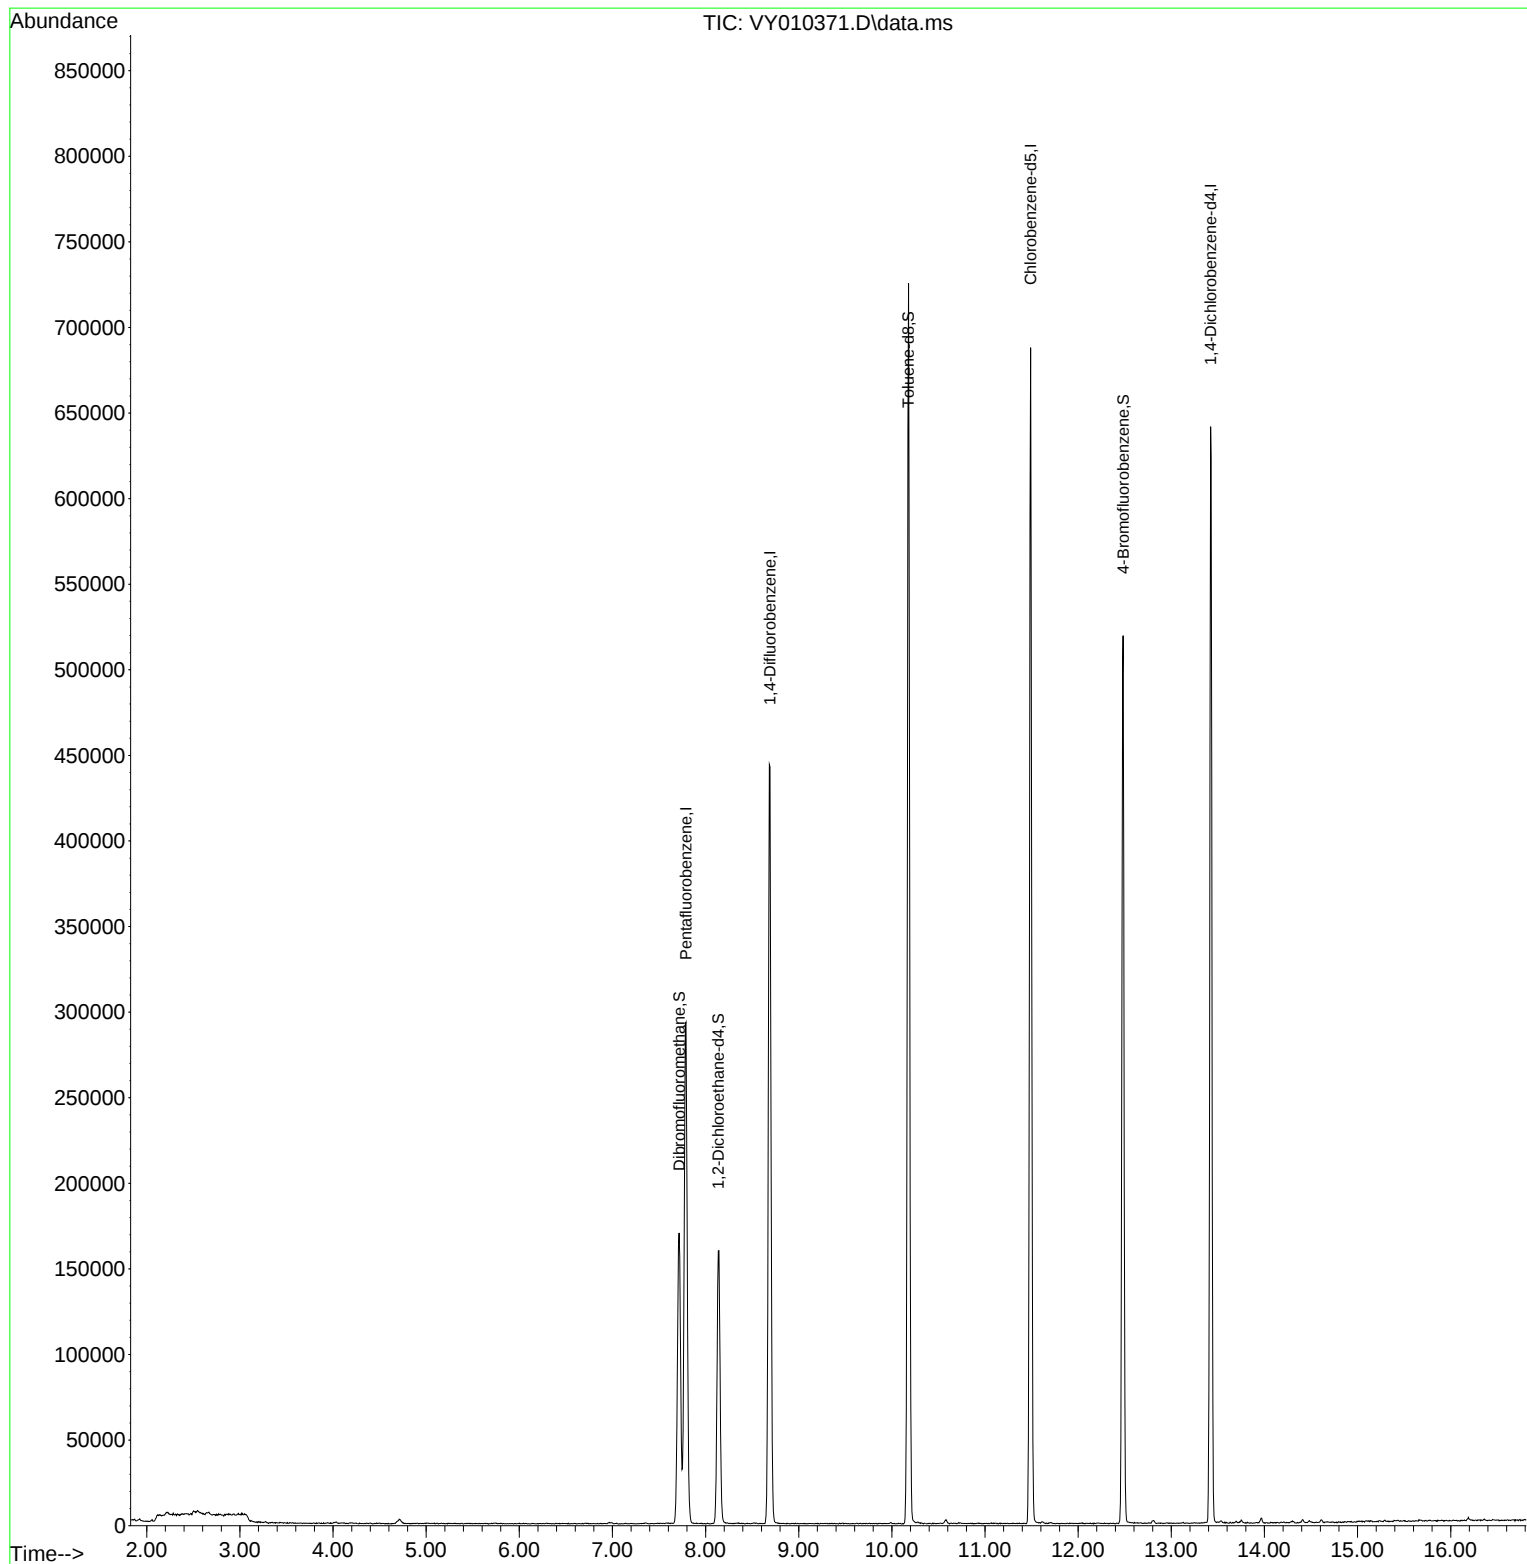


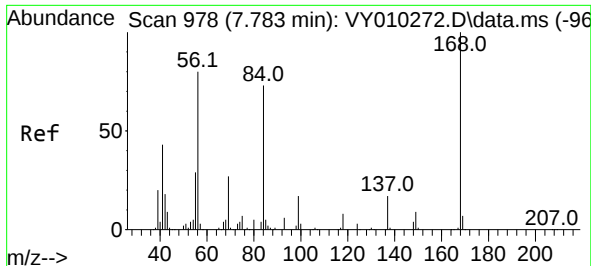

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY010371.D
Acq: 07 Sep 2022 14:50




Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BF-VOC-05


Tgt Ion:168 Resp: 239994
Ion Ratio Lower Upper
168 100
99 52.5 46.9 70.3

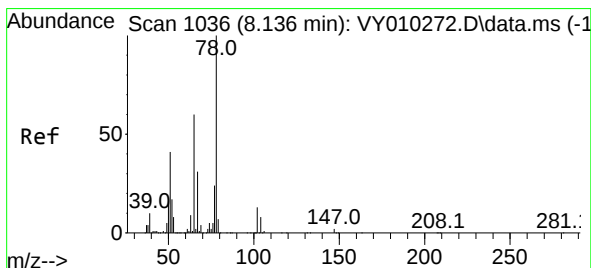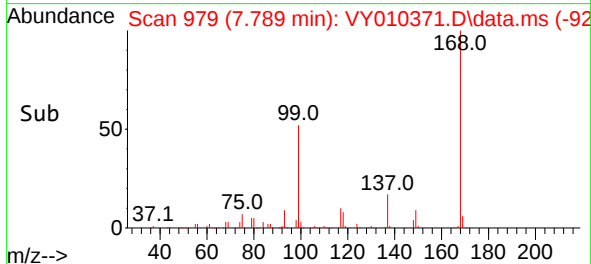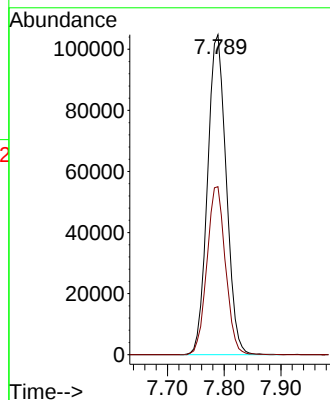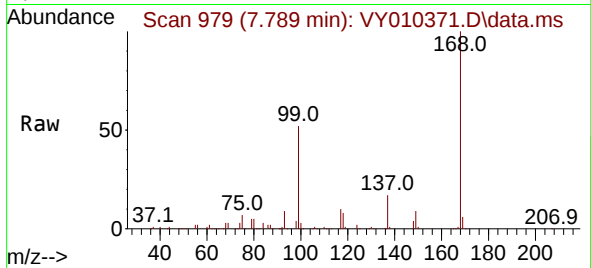

#33
1,2-Dichloroethane-d4
Concen: 52.449 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. 0.000 min
Lab File: VY010371.D
Acq: 07 Sep 2022 14:50

Tgt Ion: 65 Resp: 129071
Ion Ratio Lower Upper
65 100
67 52.4 0.0 99.4


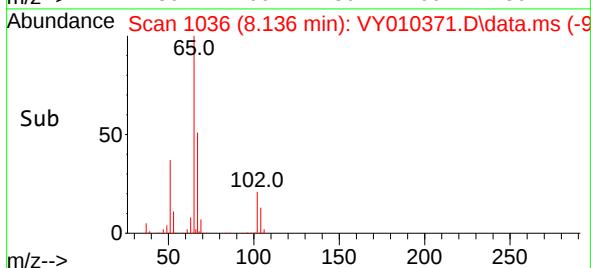
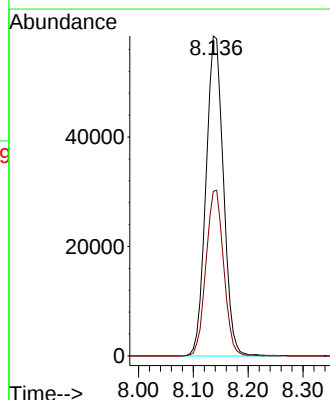
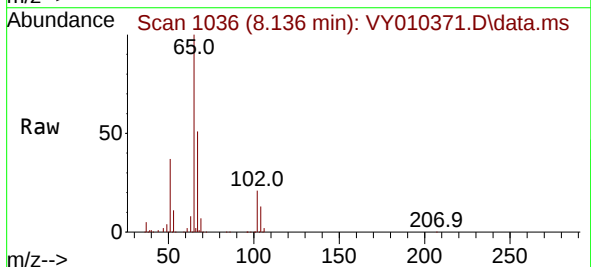


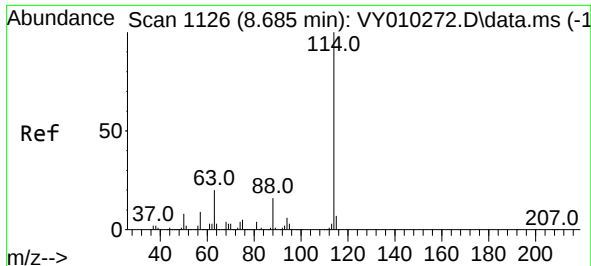

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.691 min Scan# 1127
Delta R.T. 0.006 min
Lab File: VY010371.D
Acq: 07 Sep 2022 14:50




Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BF-VOC-05


Tgt Ion:114 Resp: 399128
Ion Ratio Lower Upper
114 100
63 18.3 0.0 43.2
88 14.6 0.0 31.8

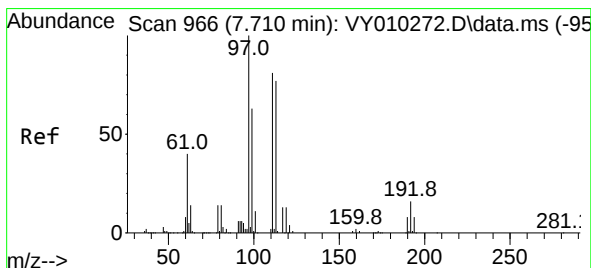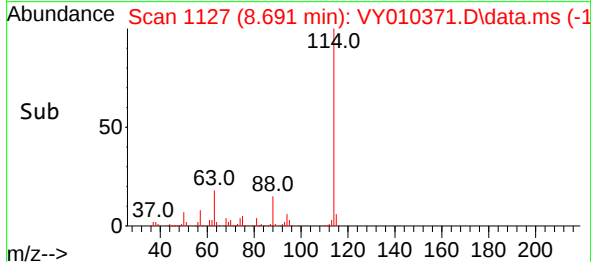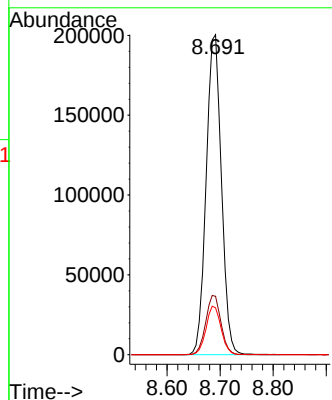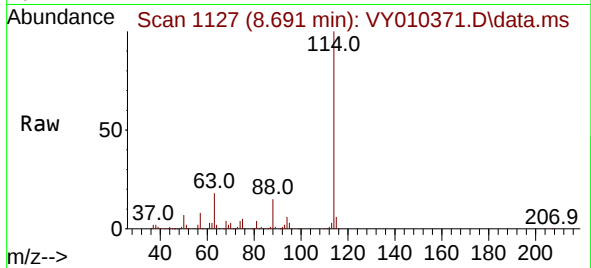

#35
Dibromofluoromethane
Concen: 46.016 ug/l
RT: 7.716 min Scan# 967
Delta R.T. 0.006 min
Lab File: VY010371.D
Acq: 07 Sep 2022 14:50

Tgt Ion:113 Resp: 122269
Ion Ratio Lower Upper
113 100
111 101.8 82.6 124.0
192 20.8 17.6 26.4


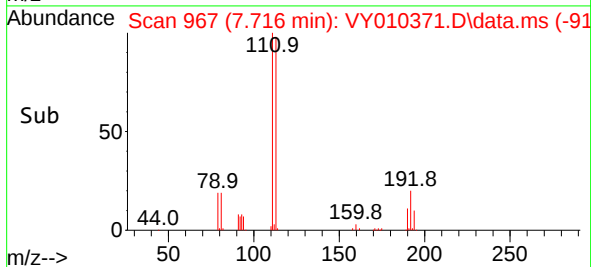
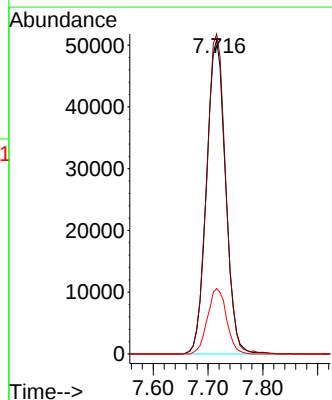
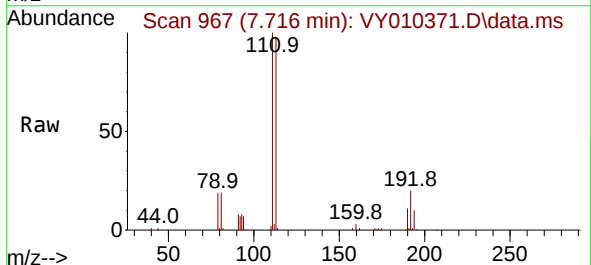


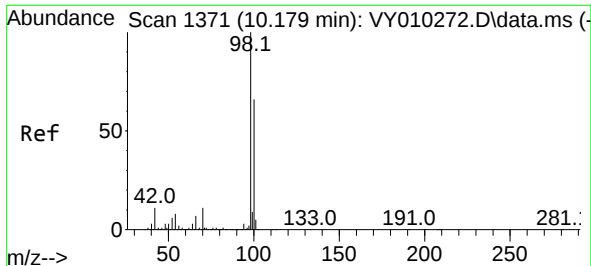

#50
Toluene-d8
Concen: 52.904 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY010371.D
Acq: 07 Sep 2022 14:50




Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BF-VOC-05


Tgt Ion: 98 Resp: 470632
Ion Ratio Lower Upper
98 100
100 65.8 50.2 75.2

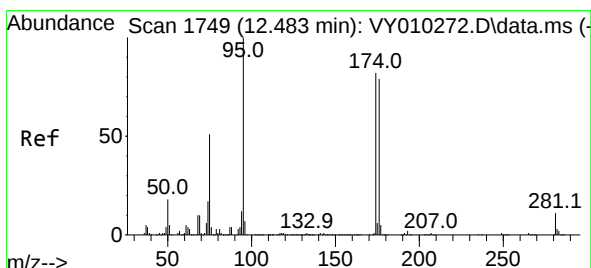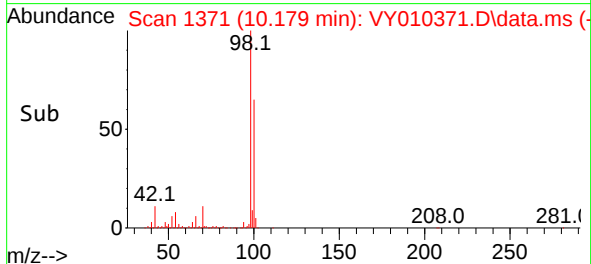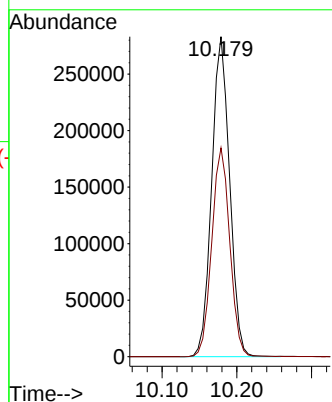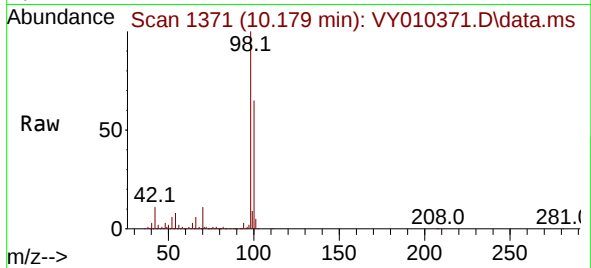

#62
4-Bromofluorobenzene
Concen: 44.865 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY010371.D
Acq: 07 Sep 2022 14:50

Tgt Ion: 95 Resp: 162149
Ion Ratio Lower Upper
95 100
174 87.5 0.0 177.0
176 85.5 0.0 175.8

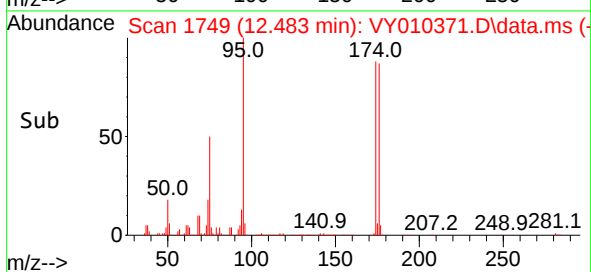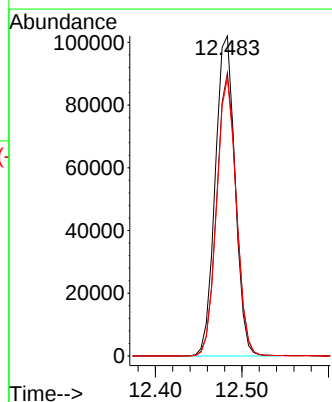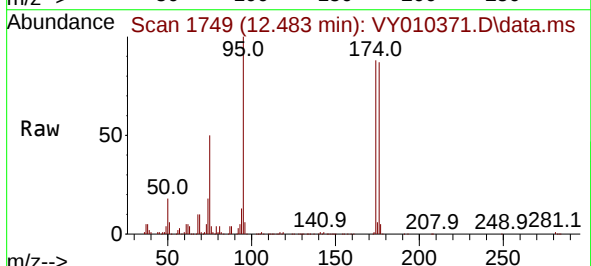

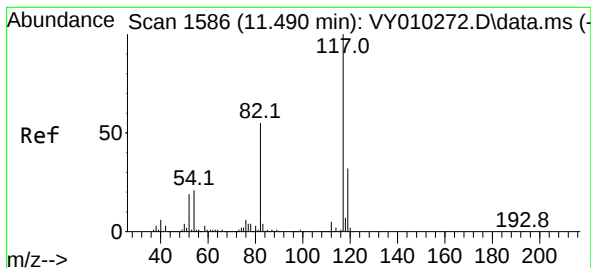

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.489 min Scan# 11

Delta R.T. -0.001 min

Lab File: VY010371.D

Acq: 07 Sep 2022 14:50

Instrument :

MSVOA_Y

ClientSampleId :

BEACONPOINT-BF-VOC-05





Tgt Ion:117 Resp: 375547

Ion Ratio Lower Upper

117 100

82 51.9 43.0 64.4

119 31.5 25.4 38.0

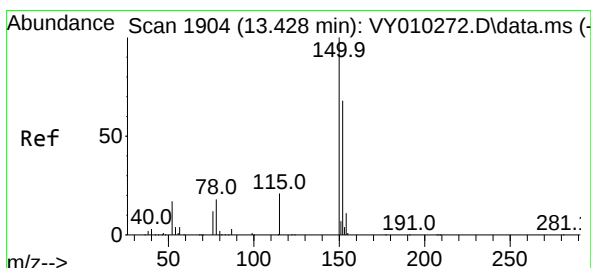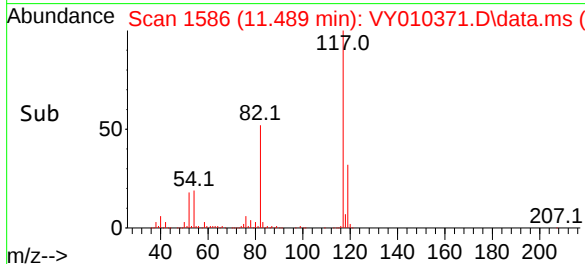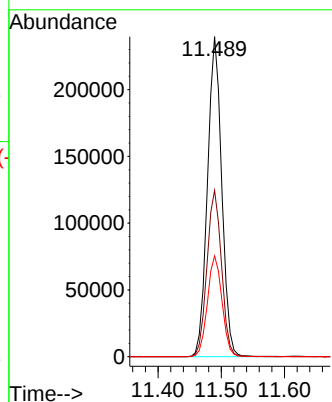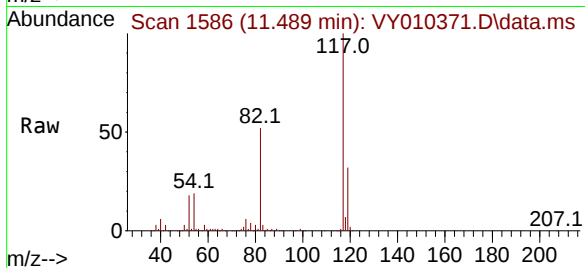

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. -0.006 min

Lab File: VY010371.D

Acq: 07 Sep 2022 14:50

Tgt Ion:152 Resp: 175027

Ion Ratio Lower Upper

152 100

115 56.0 28.2 84.7

150 157.1 0.0 347.6

