
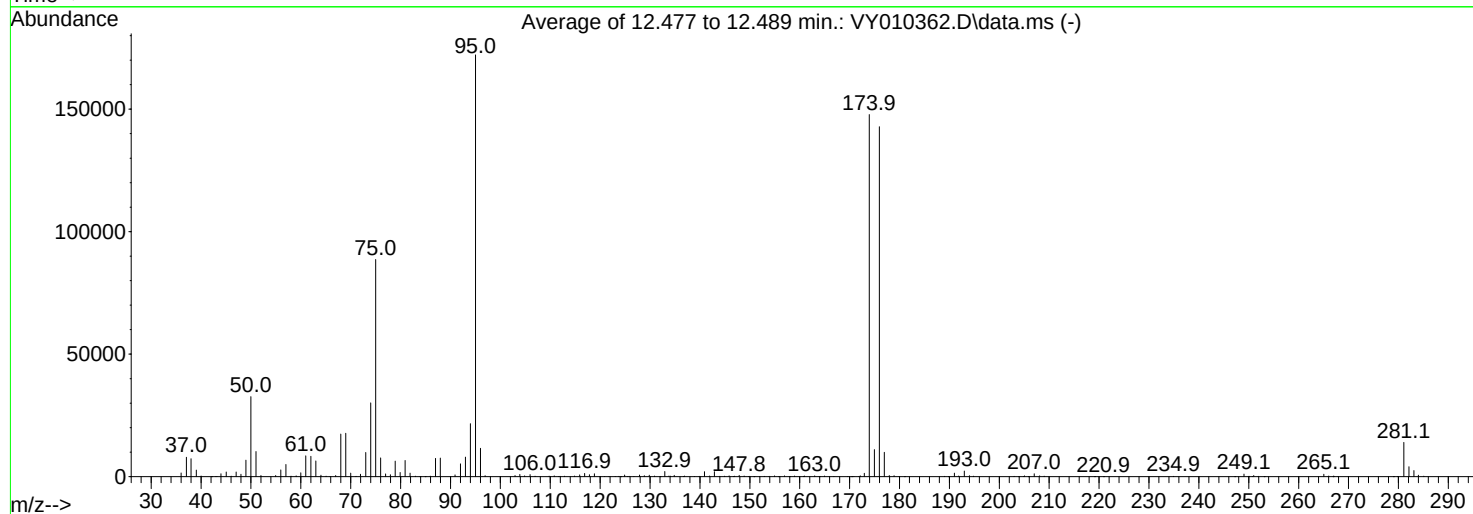


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY090722\  
Data File : VY010362.D  
Acq On : 07 Sep 2022 08:28  
Operator : KP/MD  
Sample : BFB  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y090222S.M  
Title : SW846 8260  
Last Update : Fri Sep 02 16:41:46 2022

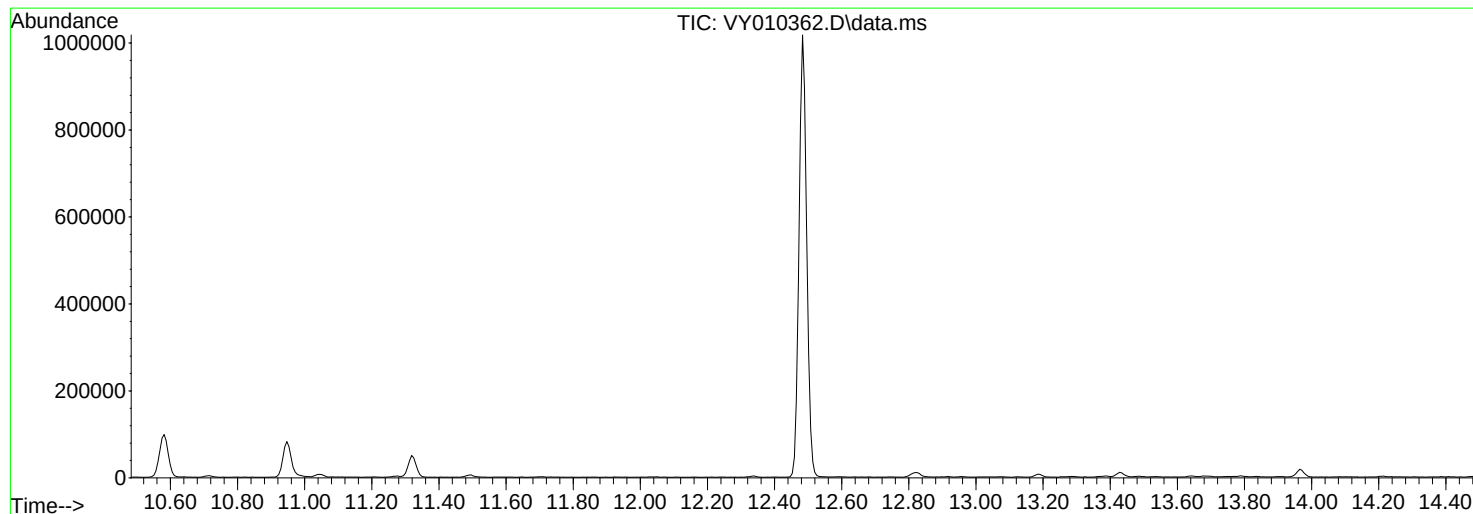

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 50     | 95      | 15     | 40     | 19.0  | 32632  | PASS      |
| 75     | 95      | 30     | 60     | 51.5  | 88600  | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 172181 | PASS      |
| 96     | 95      | 5      | 9      | 6.7   | 11588  | PASS      |
| 173    | 174     | 0.00   | 2      | 0.9   | 1363   | PASS      |
| 174    | 95      | 50     | 100    | 85.8  | 147795 | PASS      |
| 175    | 174     | 5      | 9      | 7.5   | 11045  | PASS      |
| 176    | 174     | 95     | 101    | 96.6  | 142837 | PASS      |
| 177    | 176     | 5      | 9      | 7.0   | 9930   | PASS      |