

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY090723\
 Data File : VY015468.D
 Acq On : 07 Sep 2023 15:27
 Operator : SY/MD
 Sample : 04333-01
 Misc : 5.05g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-1

Quant Time: Sep 07 23:09:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y082923S.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 31 20:01:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.777	168	297435	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.679	114	490605	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.483	117	443824	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	215096	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.130	65	184472	57.856	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	115.720%
35) Dibromofluoromethane	7.703	113	152519	53.974	ug/l	-0.01
Spiked Amount	50.000	Range	54 - 147	Recovery	=	107.940%
50) Toluene-d8	10.173	98	571417	55.840	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	111.680%
62) 4-Bromofluorobenzene	12.477	95	202789	53.380	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	106.760%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY090723\
Data File : VY015468.D
Acq On : 07 Sep 2023 15:27
Operator : SY/MD
Sample : 04333-01
Misc : 5.05g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
WC-1

Quant Time: Sep 07 23:09:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y082923S.M
Quant Title : SW846 8260
QLast Update : Thu Aug 31 20:01:47 2023
Response via : Initial Calibration




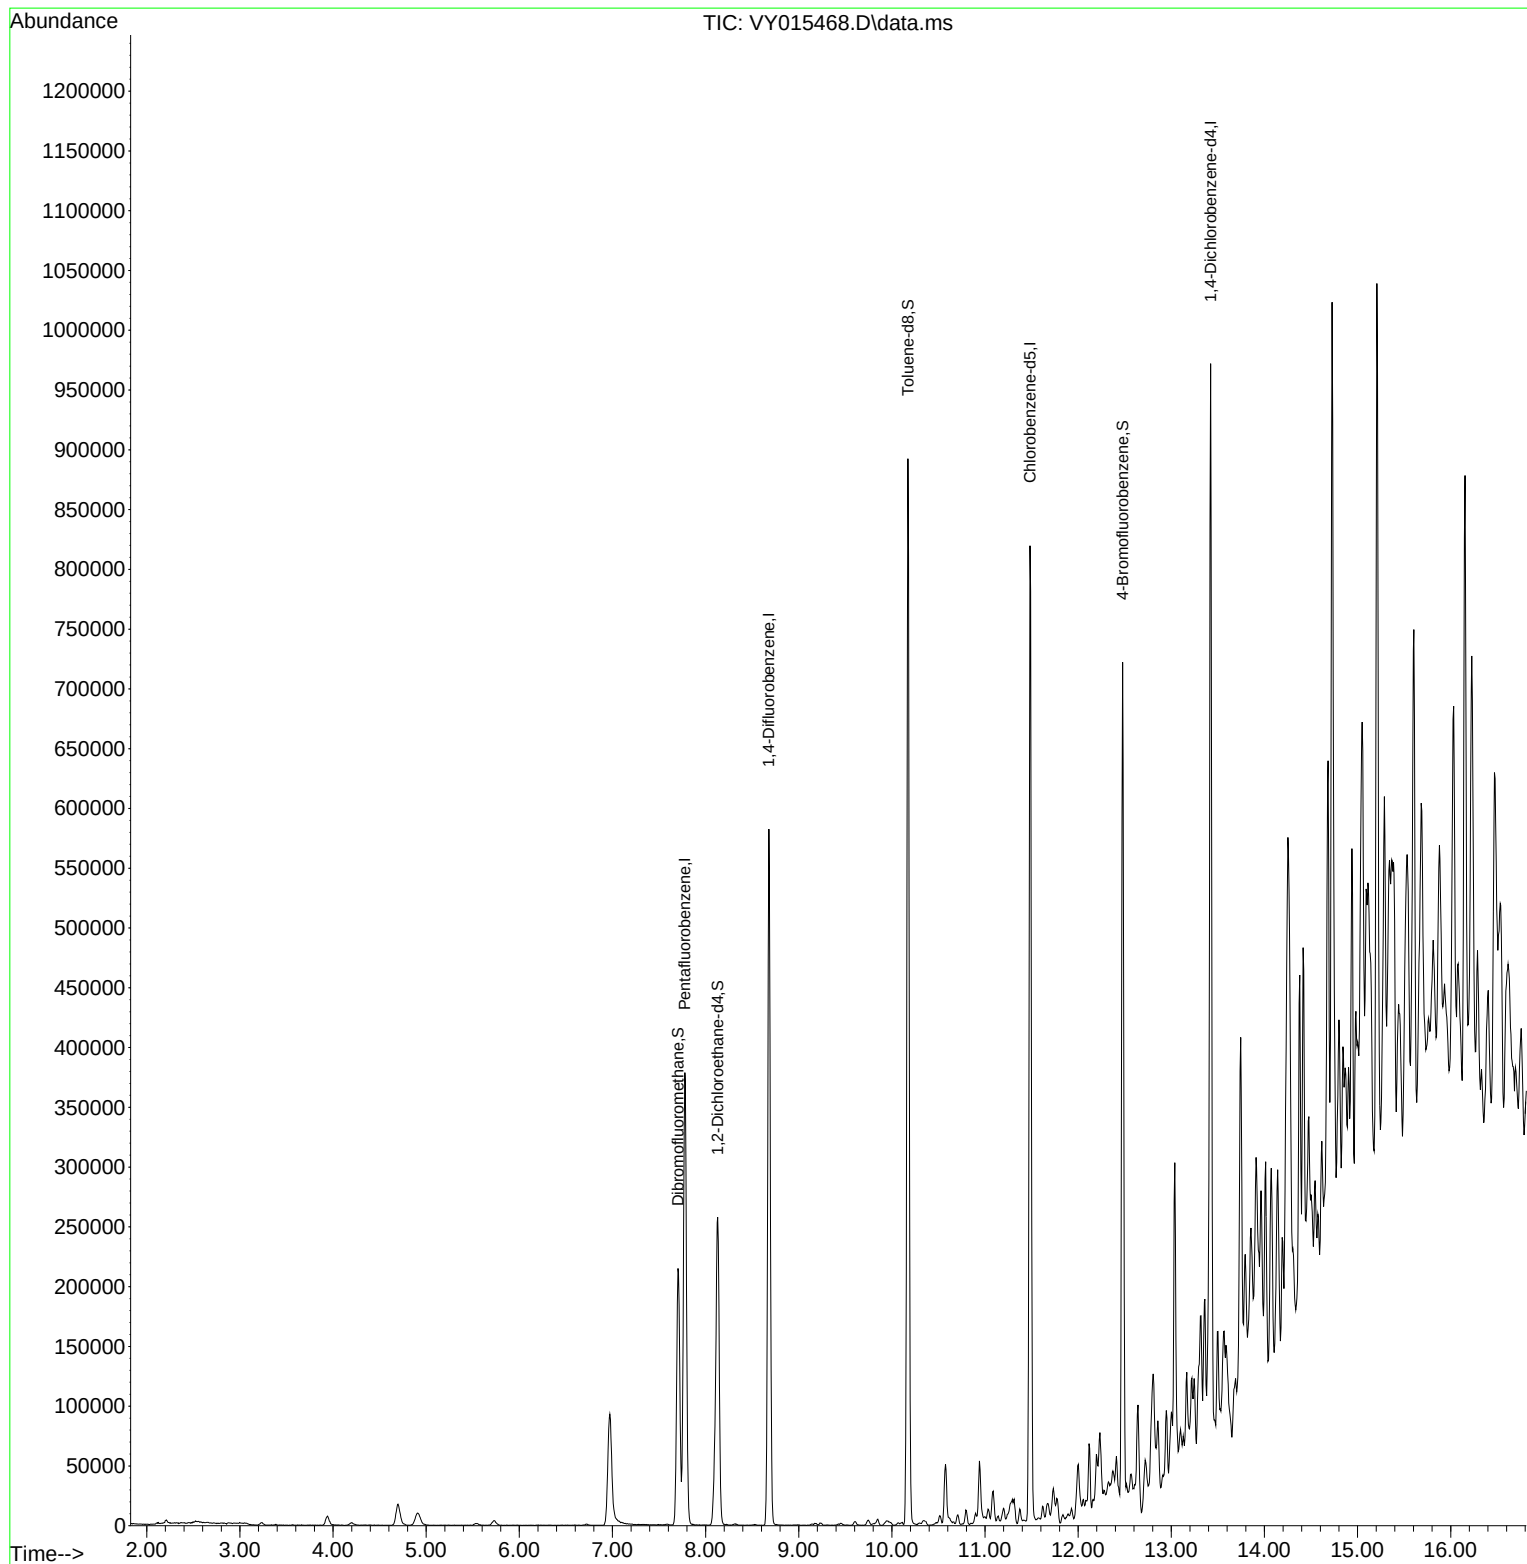


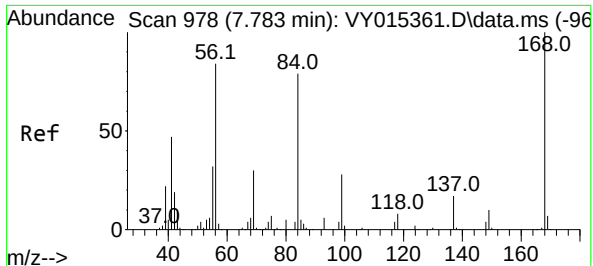

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.777 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY015468.D
Acq: 07 Sep 2023 15:27




Instrument :
MSVOA_Y
ClientSampleId :
WC-1


Tgt Ion:168 Resp: 297435
Ion Ratio Lower Upper
168 100
99 55.8 43.4 65.0

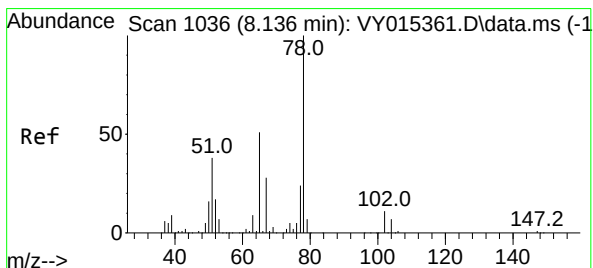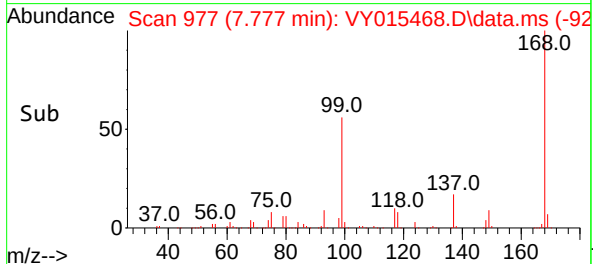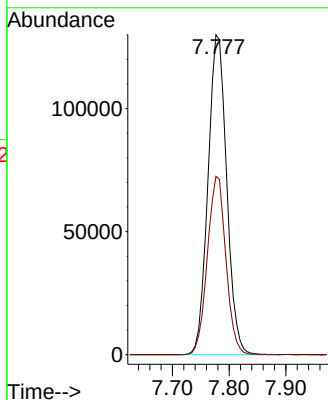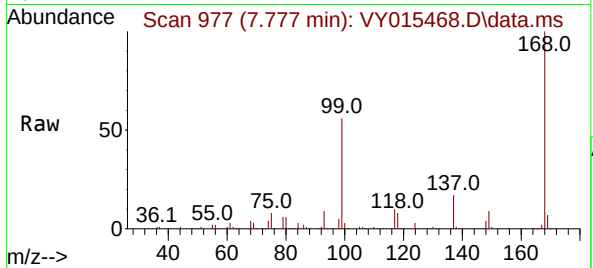

#33
1,2-Dichloroethane-d4
Concen: 57.856 ug/l
RT: 8.130 min Scan# 1035
Delta R.T. -0.006 min
Lab File: VY015468.D
Acq: 07 Sep 2023 15:27

Tgt Ion: 65 Resp: 184472
Ion Ratio Lower Upper
65 100
67 52.1 0.0 101.8

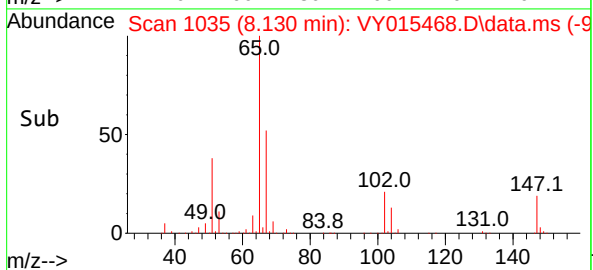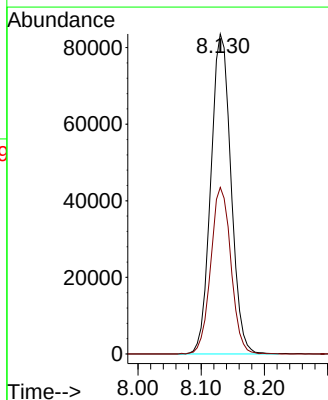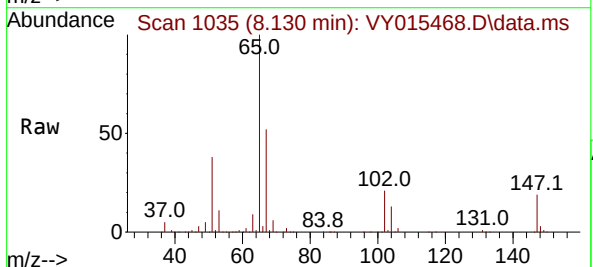

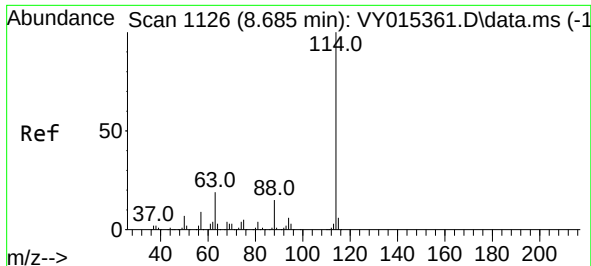

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.679 min Scan# 1125

Delta R.T. -0.006 min

Lab File: VY015468.D

Acq: 07 Sep 2023 15:27

Instrument :

MSVOA_Y

ClientSampleId :

WC-1





Tgt Ion:114 Resp: 490605

Ion Ratio Lower Upper

114 100

63 20.0 0.0 42.4

88 15.2 0.0 30.6

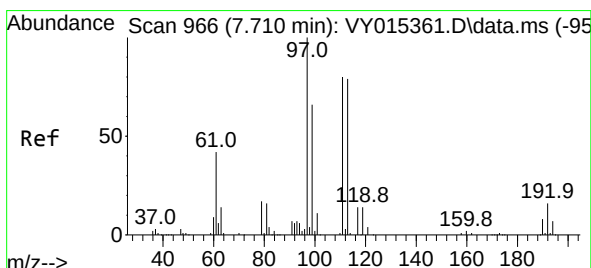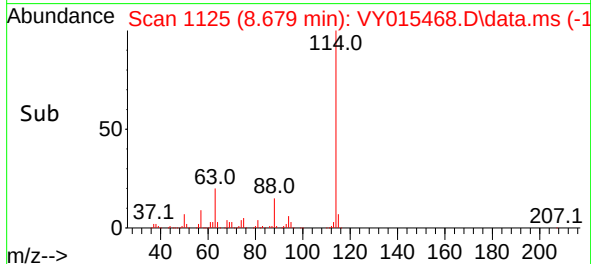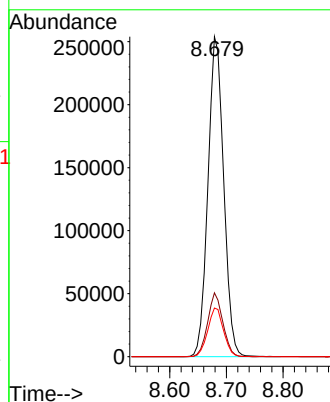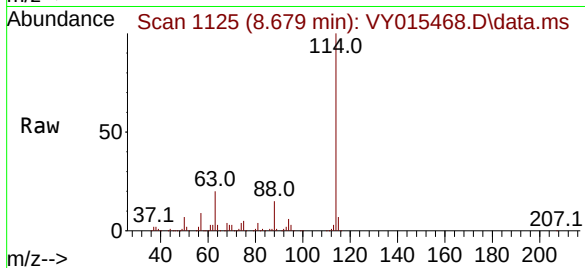

#35

Dibromofluoromethane

Concen: 53.974 ug/l

RT: 7.703 min Scan# 965

Delta R.T. -0.012 min

Lab File: VY015468.D

Acq: 07 Sep 2023 15:27




Tgt Ion:113 Resp: 152519


Ion Ratio Lower Upper

113 100

111 103.2 81.3 121.9

192 20.0 16.9 25.3

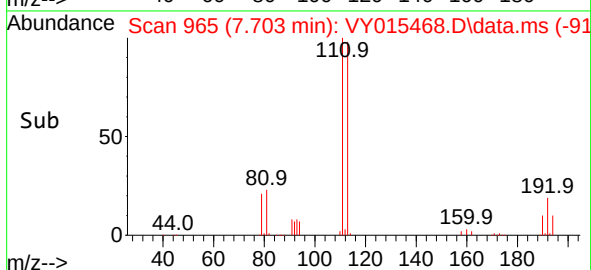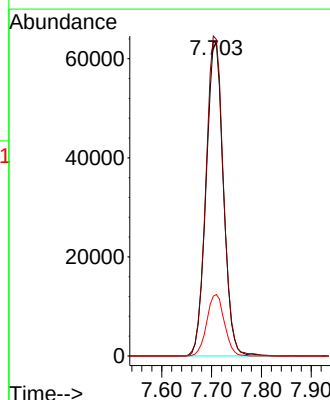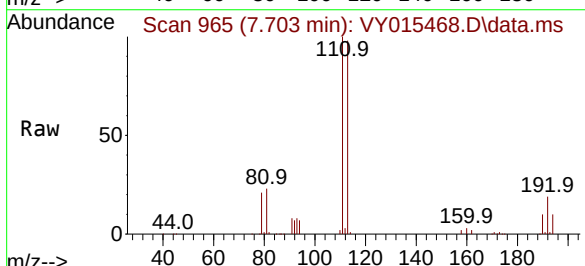

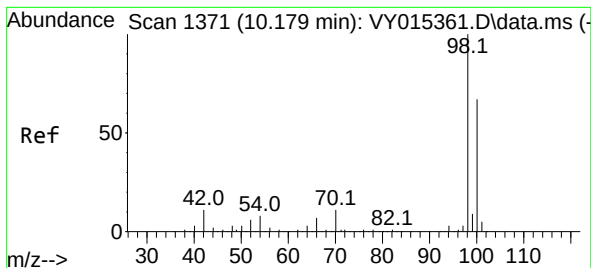

#50

Toluene-d8

Concen: 55.840 ug/l

RT: 10.173 min Scan# 1

Delta R.T. -0.006 min

Lab File: VY015468.D

Acq: 07 Sep 2023 15:27

Instrument :

MSVOA_Y

ClientSampleId :





WC-1

Tgt Ion: 98 Resp: 571417

Ion Ratio Lower Upper

98 100

100 65.5 50.1 75.1

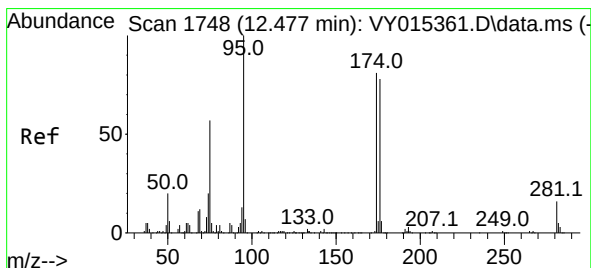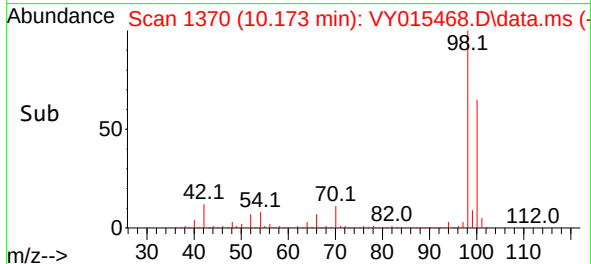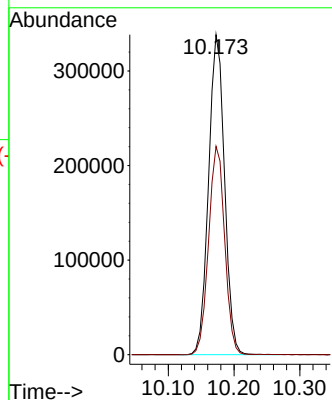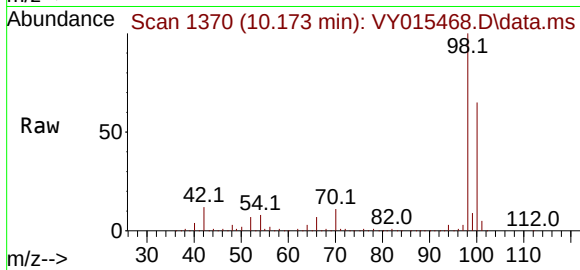

#62

4-Bromofluorobenzene

Concen: 53.380 ug/l

RT: 12.477 min Scan# 1748

Delta R.T. -0.000 min

Lab File: VY015468.D

Acq: 07 Sep 2023 15:27




Tgt Ion: 95 Resp: 202789


Ion Ratio Lower Upper

95 100

174 84.7 0.0 178.2

176 82.9 0.0 173.8

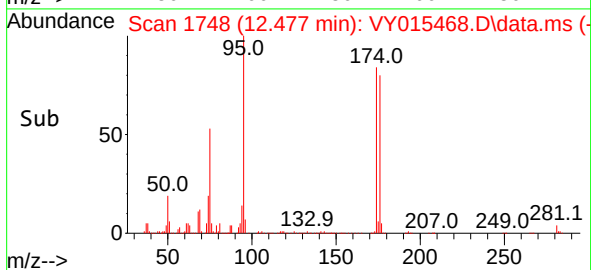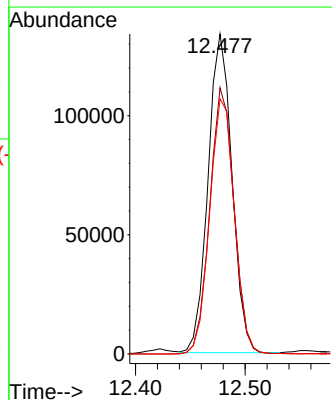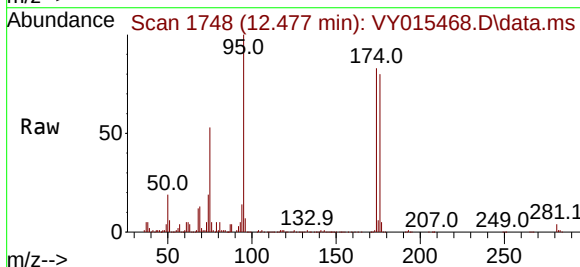

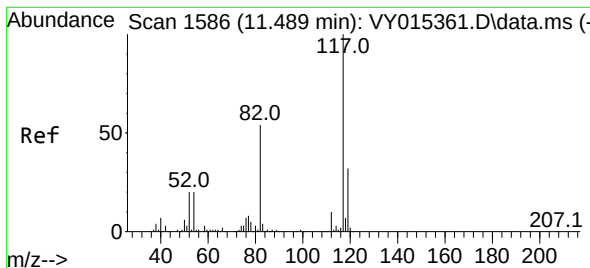

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.483 min Scan# 11

Delta R.T. -0.006 min

Lab File: VY015468.D

Acq: 07 Sep 2023 15:27

Instrument :

MSVOA_Y

ClientSampleId :

WC-1





Tgt Ion:117 Resp: 443824

Ion Ratio Lower Upper

117 100

82 55.5 43.4 65.0

119 32.8 26.3 39.5

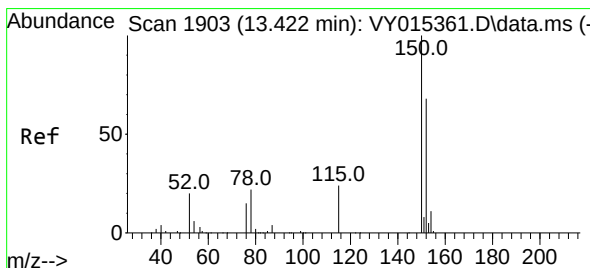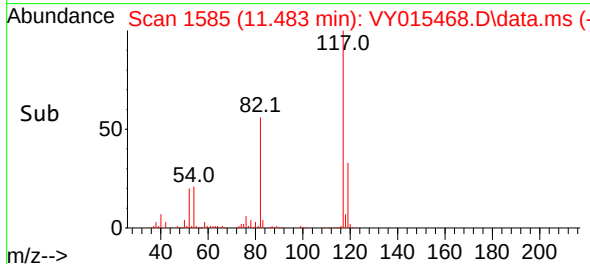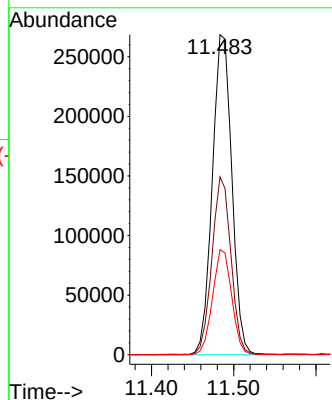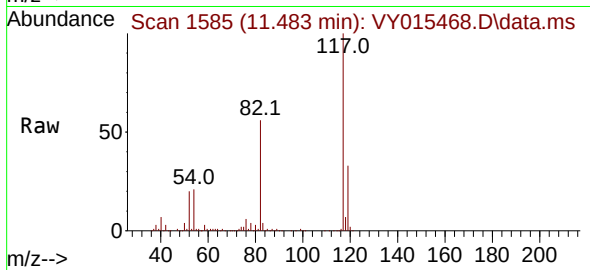

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. -0.000 min

Lab File: VY015468.D

Acq: 07 Sep 2023 15:27

Tgt Ion:152 Resp: 215096

Ion Ratio Lower Upper

152 100

115 57.4 28.8 86.5

150 155.1 0.0 348.8

