
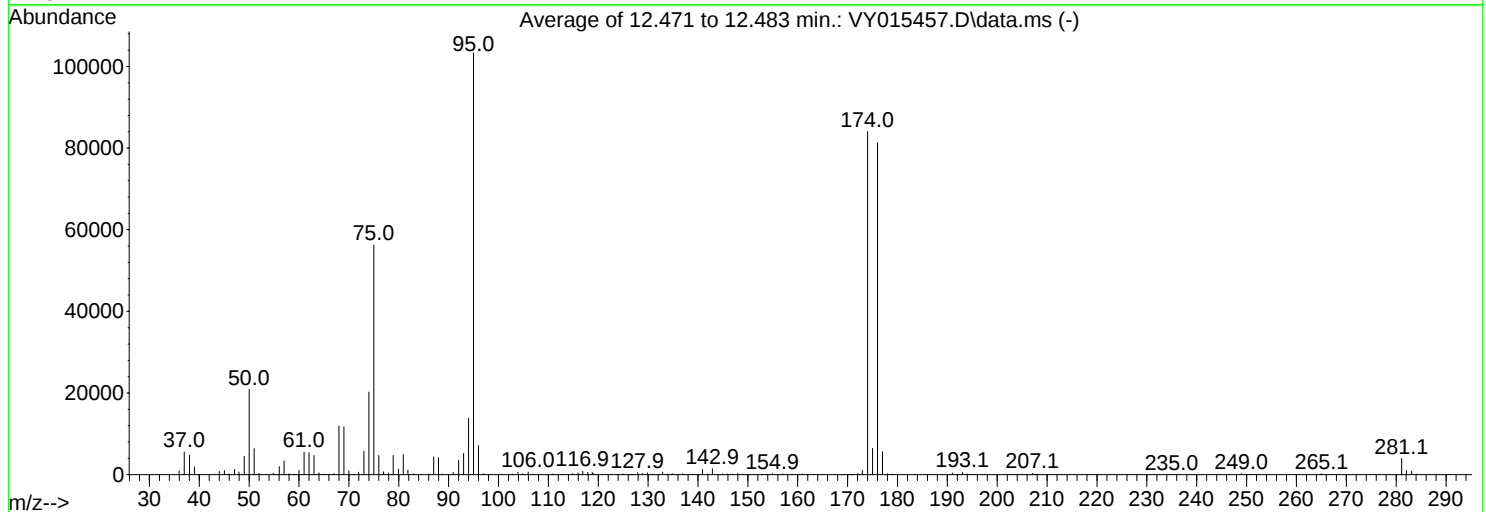


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY090723\
Data File : VY015457.D
Acq On : 07 Sep 2023 08:45
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y082923S.M
Title : SW846 8260
Last Update : Thu Aug 31 20:01:47 2023

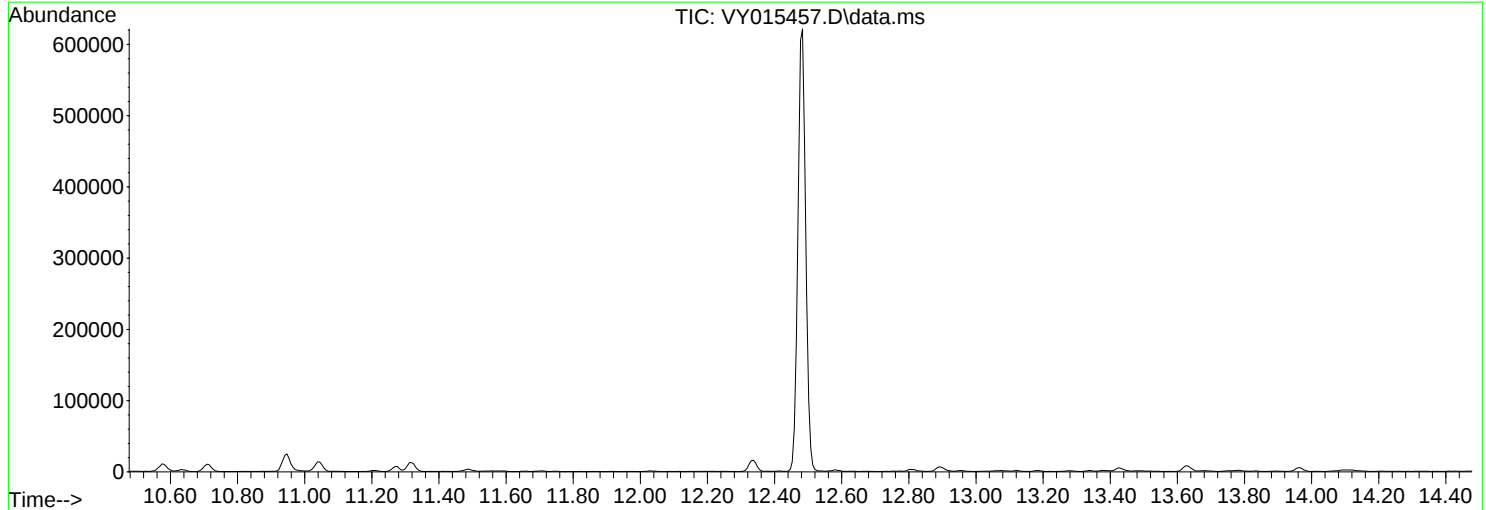

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	20877	PASS
75	95	30	60	54.4	56240	PASS
95	95	100	100	100.0	103328	PASS
96	95	5	9	6.9	7105	PASS
173	174	0.00	2	1.3	1080	PASS
174	95	50	100	81.3	84029	PASS
175	174	5	9	7.7	6429	PASS
176	174	95	101	96.8	81328	PASS
177	176	5	9	6.9	5588	PASS