
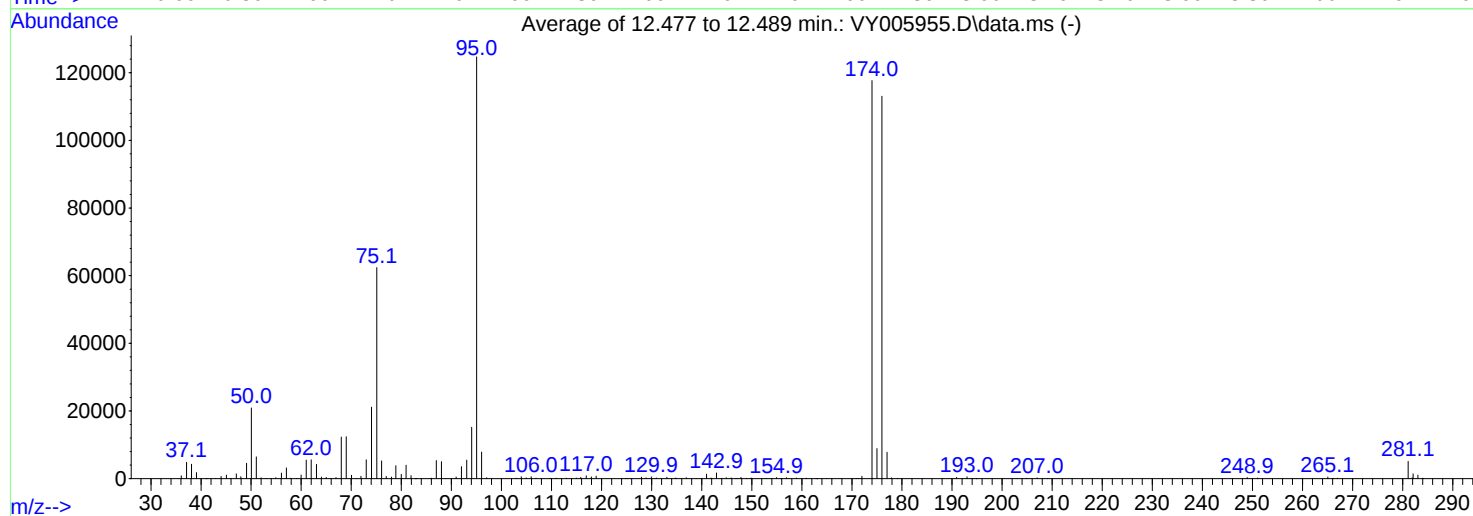


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY090821\
Data File : VY005955.D
Acq On : 08 Sep 2021 08:09
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y0831215.M
Title : SW846 8260
Last Update : Wed Sep 01 05:32:43 2021

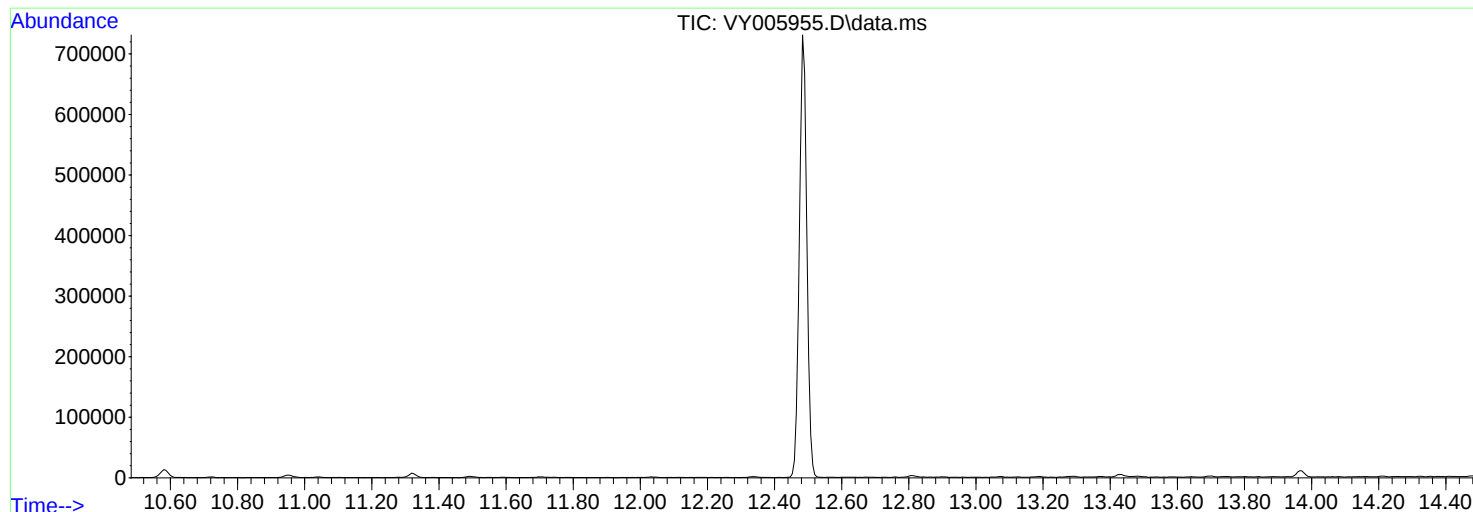

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.8	20907	PASS
75	95	30	60	50.0	62373	PASS
95	95	100	100	100.0	124683	PASS
96	95	5	9	6.3	7835	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	94.4	117656	PASS
175	174	5	9	7.6	8891	PASS
176	174	95	101	96.1	113024	PASS
177	176	5	9	6.9	7792	PASS