

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY090822\
 Data File : VY010395.D
 Acq On : 08 Sep 2022 15:01
 Operator : KP/MD
 Sample : N4474-01
 Misc : 5.51g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BEACONPOINT-BF-VOC-01

Quant Time: Sep 09 06:26:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090222S.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 02 16:41:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	322762	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	556520	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	540910	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	267972	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	153058	46.247	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	92.500%
35) Dibromofluoromethane	7.716	113	140936	38.041	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	76.080%
50) Toluene-d8	10.179	98	545647	43.990	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	87.980%
62) 4-Bromofluorobenzene	12.477	95	197217	38.213	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	76.420%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY090822\
Data File : VY010395.D
Acq On : 08 Sep 2022 15:01
Operator : KP/MD
Sample : N4474-01
Misc : 5.51g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BF-VOC-01

Quant Time: Sep 09 06:26:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090222S.M
Quant Title : SW846 8260
QLast Update : Fri Sep 02 16:41:46 2022
Response via : Initial Calibration




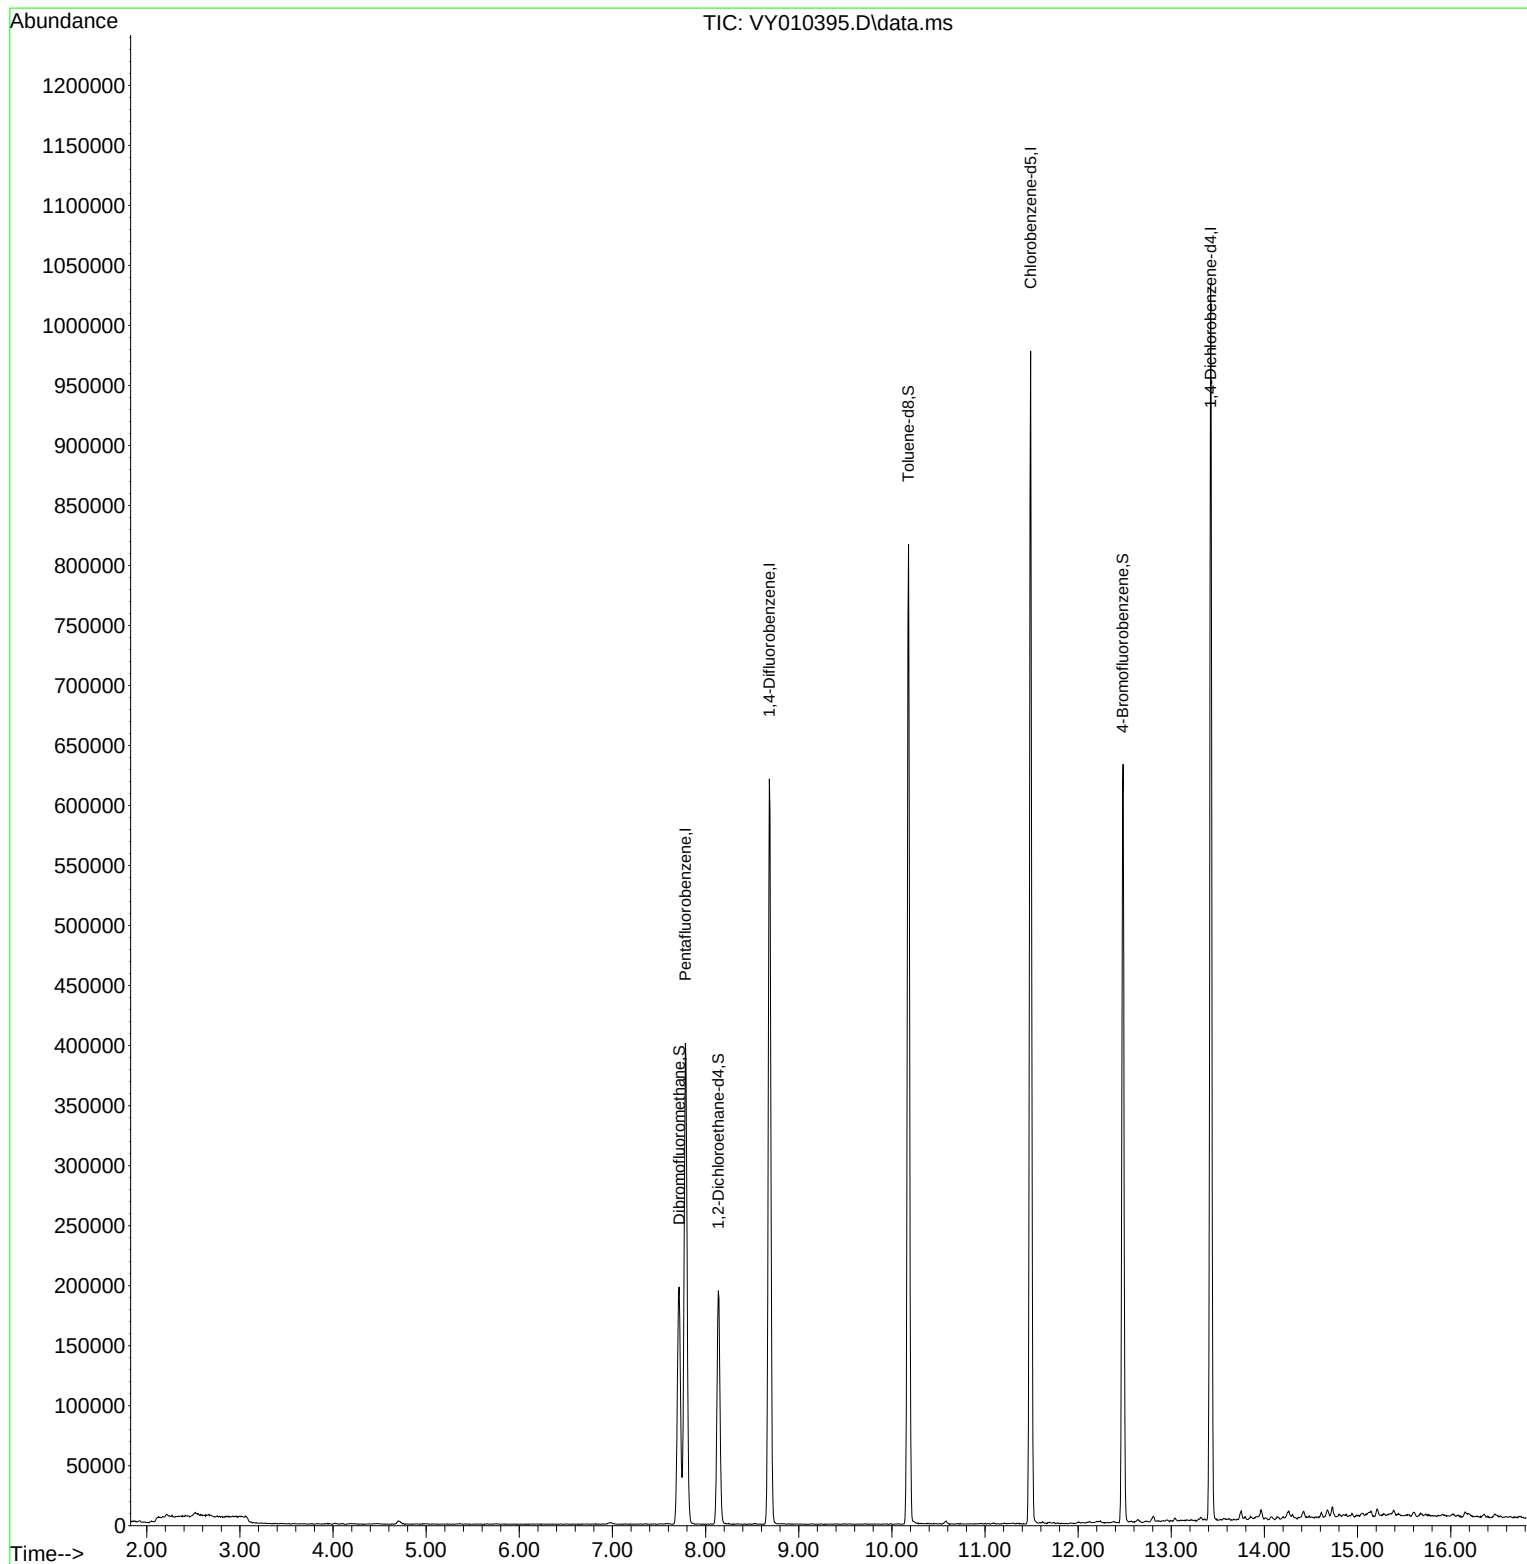


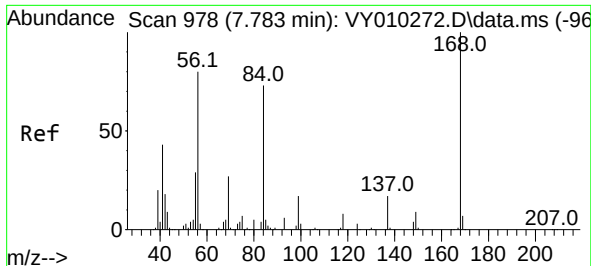

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY010395.D
Acq: 08 Sep 2022 15:01




Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BF-VOC-01


Tgt Ion:168 Resp: 322762
Ion Ratio Lower Upper
168 100
99 54.4 46.9 70.3

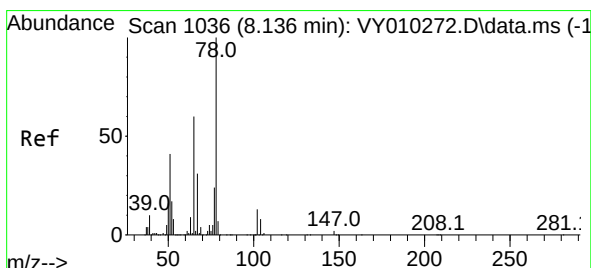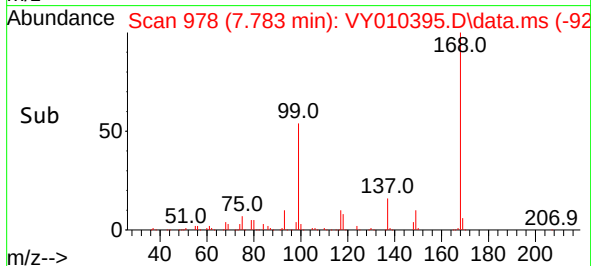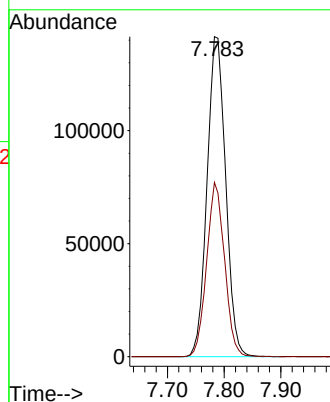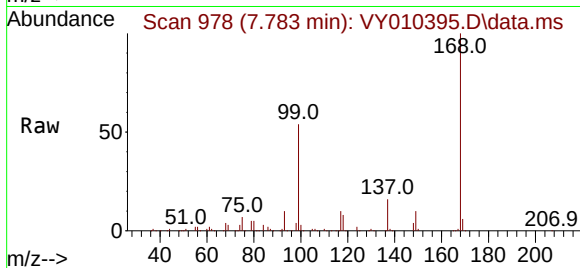

#33
1,2-Dichloroethane-d4
Concen: 46.247 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. 0.000 min
Lab File: VY010395.D
Acq: 08 Sep 2022 15:01

Tgt Ion: 65 Resp: 153058
Ion Ratio Lower Upper
65 100
67 52.6 0.0 99.4


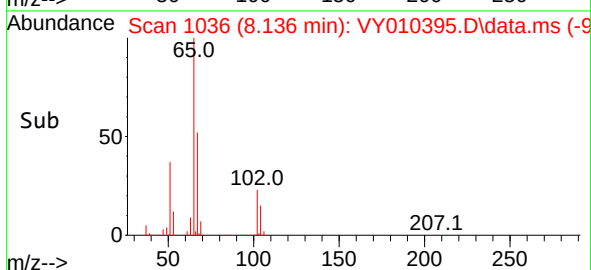
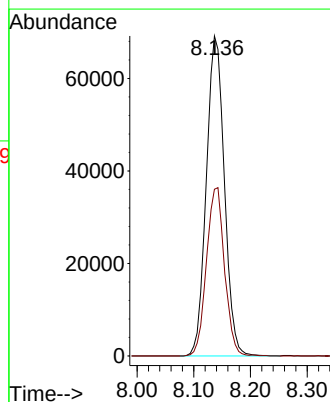
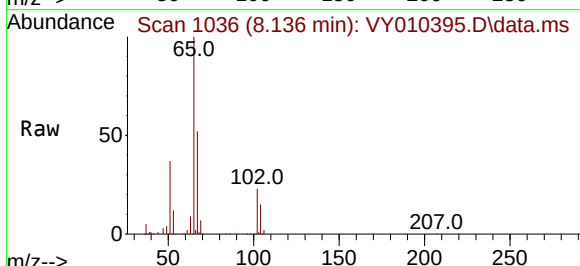


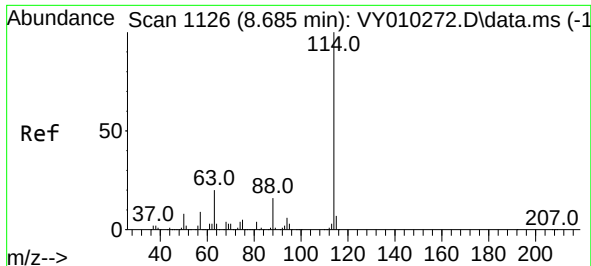

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.685 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VY010395.D
Acq: 08 Sep 2022 15:01




Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BF-VOC-01


Tgt Ion:114 Resp: 556520
Ion Ratio Lower Upper
114 100
63 18.7 0.0 43.2
88 14.7 0.0 31.8

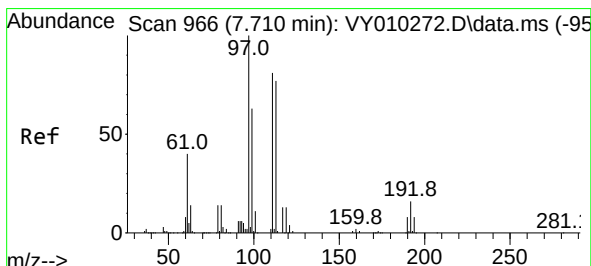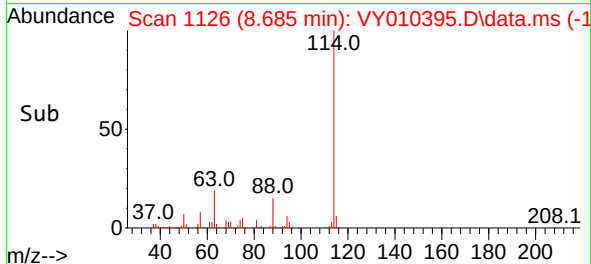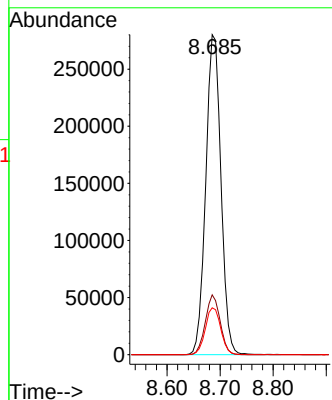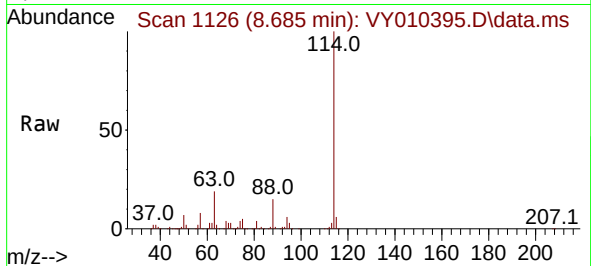

#35
Dibromofluoromethane
Concen: 38.041 ug/l
RT: 7.716 min Scan# 967
Delta R.T. 0.006 min
Lab File: VY010395.D
Acq: 08 Sep 2022 15:01

Tgt Ion:113 Resp: 140936
Ion Ratio Lower Upper
113 100
111 102.4 82.6 124.0
192 20.7 17.6 26.4


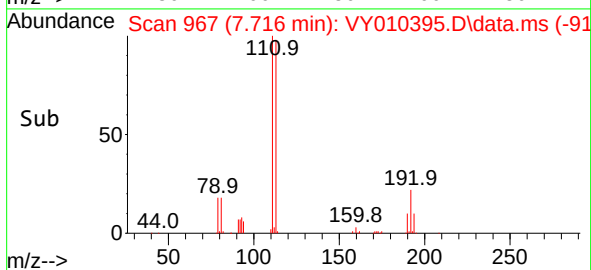
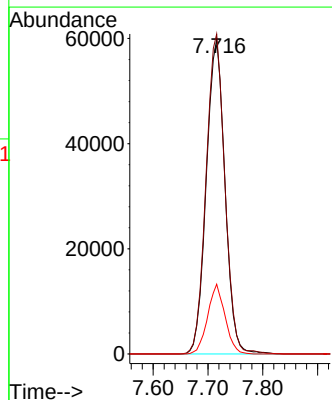
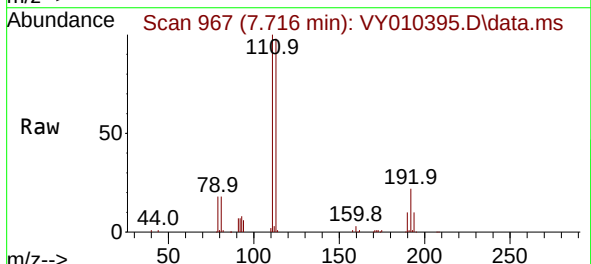


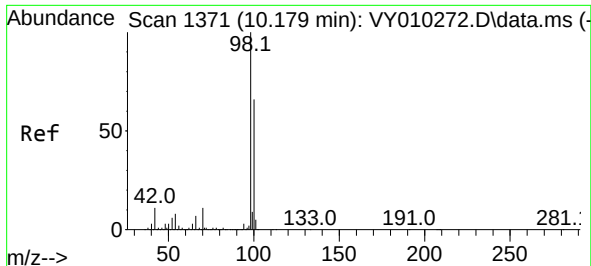

#50
Toluene-d8
Concen: 43.990 ug/l
RT: 10.179 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY010395.D
Acq: 08 Sep 2022 15:01




Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BF-VOC-01


Tgt Ion: 98 Resp: 545647
Ion Ratio Lower Upper
98 100
100 65.6 50.2 75.2

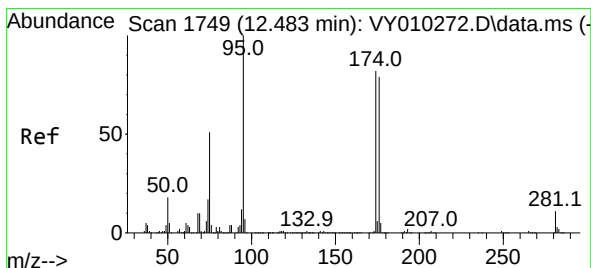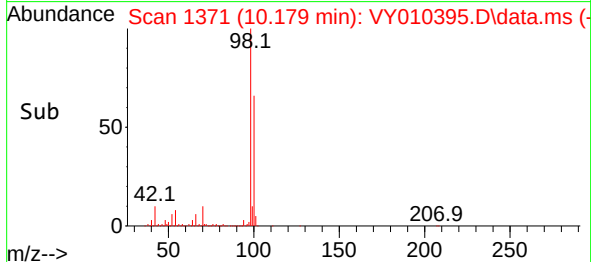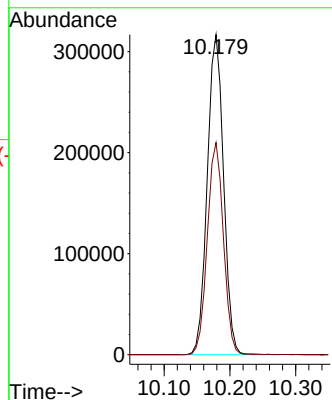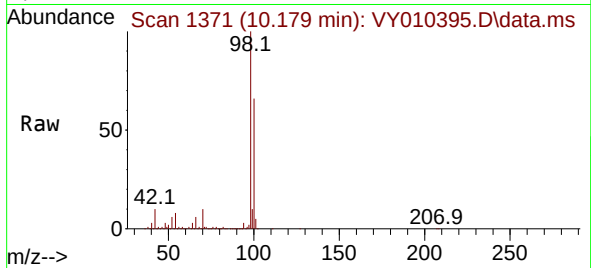

#62
4-Bromofluorobenzene
Concen: 38.213 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.006 min
Lab File: VY010395.D
Acq: 08 Sep 2022 15:01

Tgt Ion: 95 Resp: 197217
Ion Ratio Lower Upper
95 100
174 87.9 0.0 177.0
176 84.9 0.0 175.8


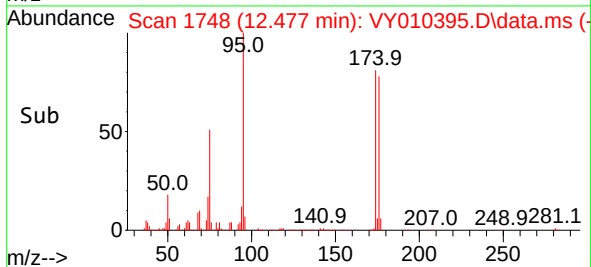
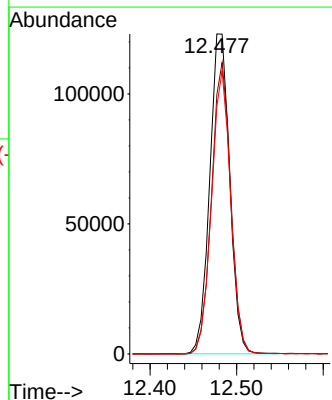
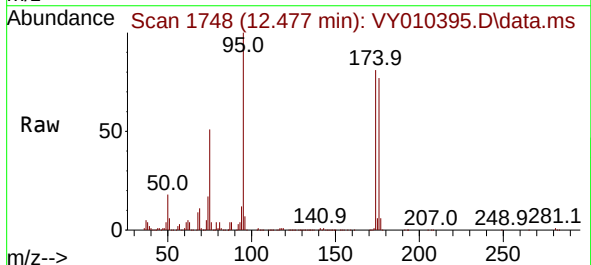


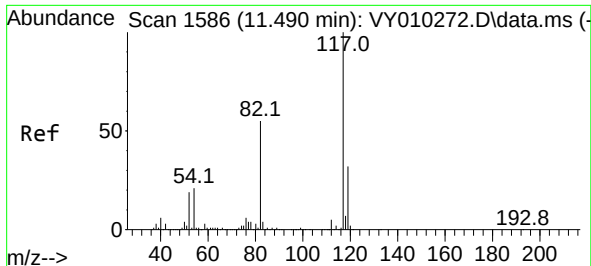

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 11
Delta R.T. -0.000 min
Lab File: VY010395.D
Acq: 08 Sep 2022 15:01

Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BF-VOC-01

Tgt Ion:117 Resp: 540910
Ion Ratio Lower Upper
117 100
82 52.8 43.0 64.4
119 32.1 25.4 38.0

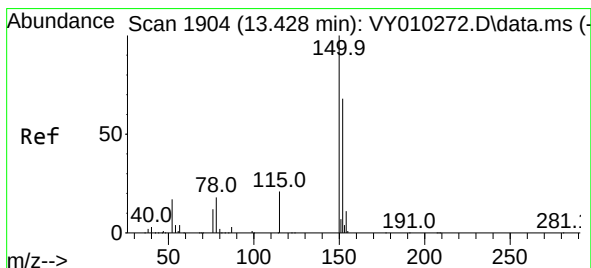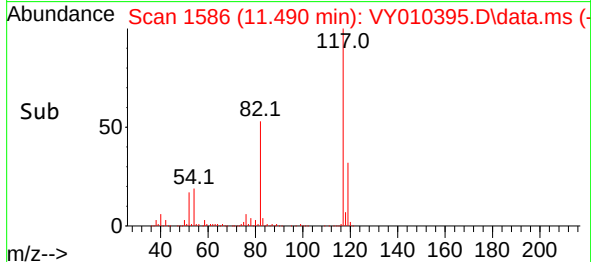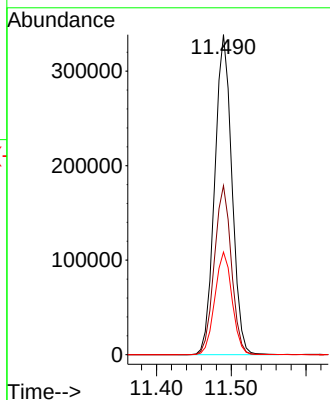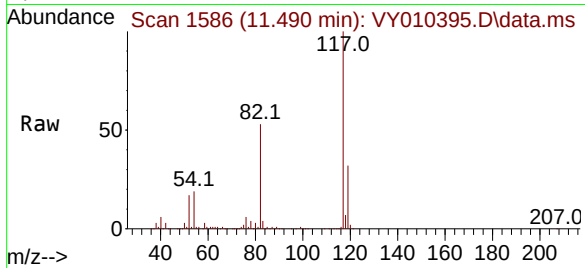

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.006 min
Lab File: VY010395.D
Acq: 08 Sep 2022 15:01

Tgt Ion:152 Resp: 267972
Ion Ratio Lower Upper
152 100
115 56.8 28.2 84.7
150 155.7 0.0 347.6

