

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY090822\  
 Data File : VY010404.D  
 Acq On : 08 Sep 2022 18:32  
 Operator : KP/MD  
 Sample : N4512-01  
 Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 VNJ-214

Quant Time: Sep 09 06:27:23 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y090222S.M  
 Quant Title : SW846 8260  
 QLast Update : Fri Sep 02 16:41:46 2022  
 Response via : Initial Calibration

| Compound                   | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|----------------------------|--------|------|----------|--------|-------|----------|
| -----                      |        |      |          |        |       |          |
| Internal Standards         |        |      |          |        |       |          |
| 1) Pentafluorobenzene      | 7.782  | 168  | 286948   | 50.000 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 8.685  | 114  | 490543   | 50.000 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.489 | 117  | 480672   | 50.000 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 13.428 | 152  | 234068   | 50.000 | ug/l  | 0.00     |

|                             |        |       |          |          |      |         |
|-----------------------------|--------|-------|----------|----------|------|---------|
| System Monitoring Compounds |        |       |          |          |      |         |
| 33) 1,2-Dichloroethane-d4   | 8.136  | 65    | 131067   | 44.545   | ug/l | 0.00    |
| Spiked Amount               | 50.000 | Range | 50 - 163 | Recovery | =    | 89.100% |
| 35) Dibromofluoromethane    | 7.715  | 113   | 124603   | 38.156   | ug/l | 0.00    |
| Spiked Amount               | 50.000 | Range | 54 - 147 | Recovery | =    | 76.320% |
| 50) Toluene-d8              | 10.178 | 98    | 481148   | 44.007   | ug/l | 0.00    |
| Spiked Amount               | 50.000 | Range | 49 - 140 | Recovery | =    | 88.020% |
| 62) 4-Bromofluorobenzene    | 12.477 | 95    | 171642   | 37.640   | ug/l | 0.00    |
| Spiked Amount               | 50.000 | Range | 25 - 144 | Recovery | =    | 75.280% |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY090822\  
Data File : VY010404.D  
Acq On : 08 Sep 2022 18:32  
Operator : KP/MD  
Sample : N4512-01  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
VNJ-214

Quant Time: Sep 09 06:27:23 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y090222S.M  
Quant Title : SW846 8260  
QLast Update : Fri Sep 02 16:41:46 2022  
Response via : Initial Calibration




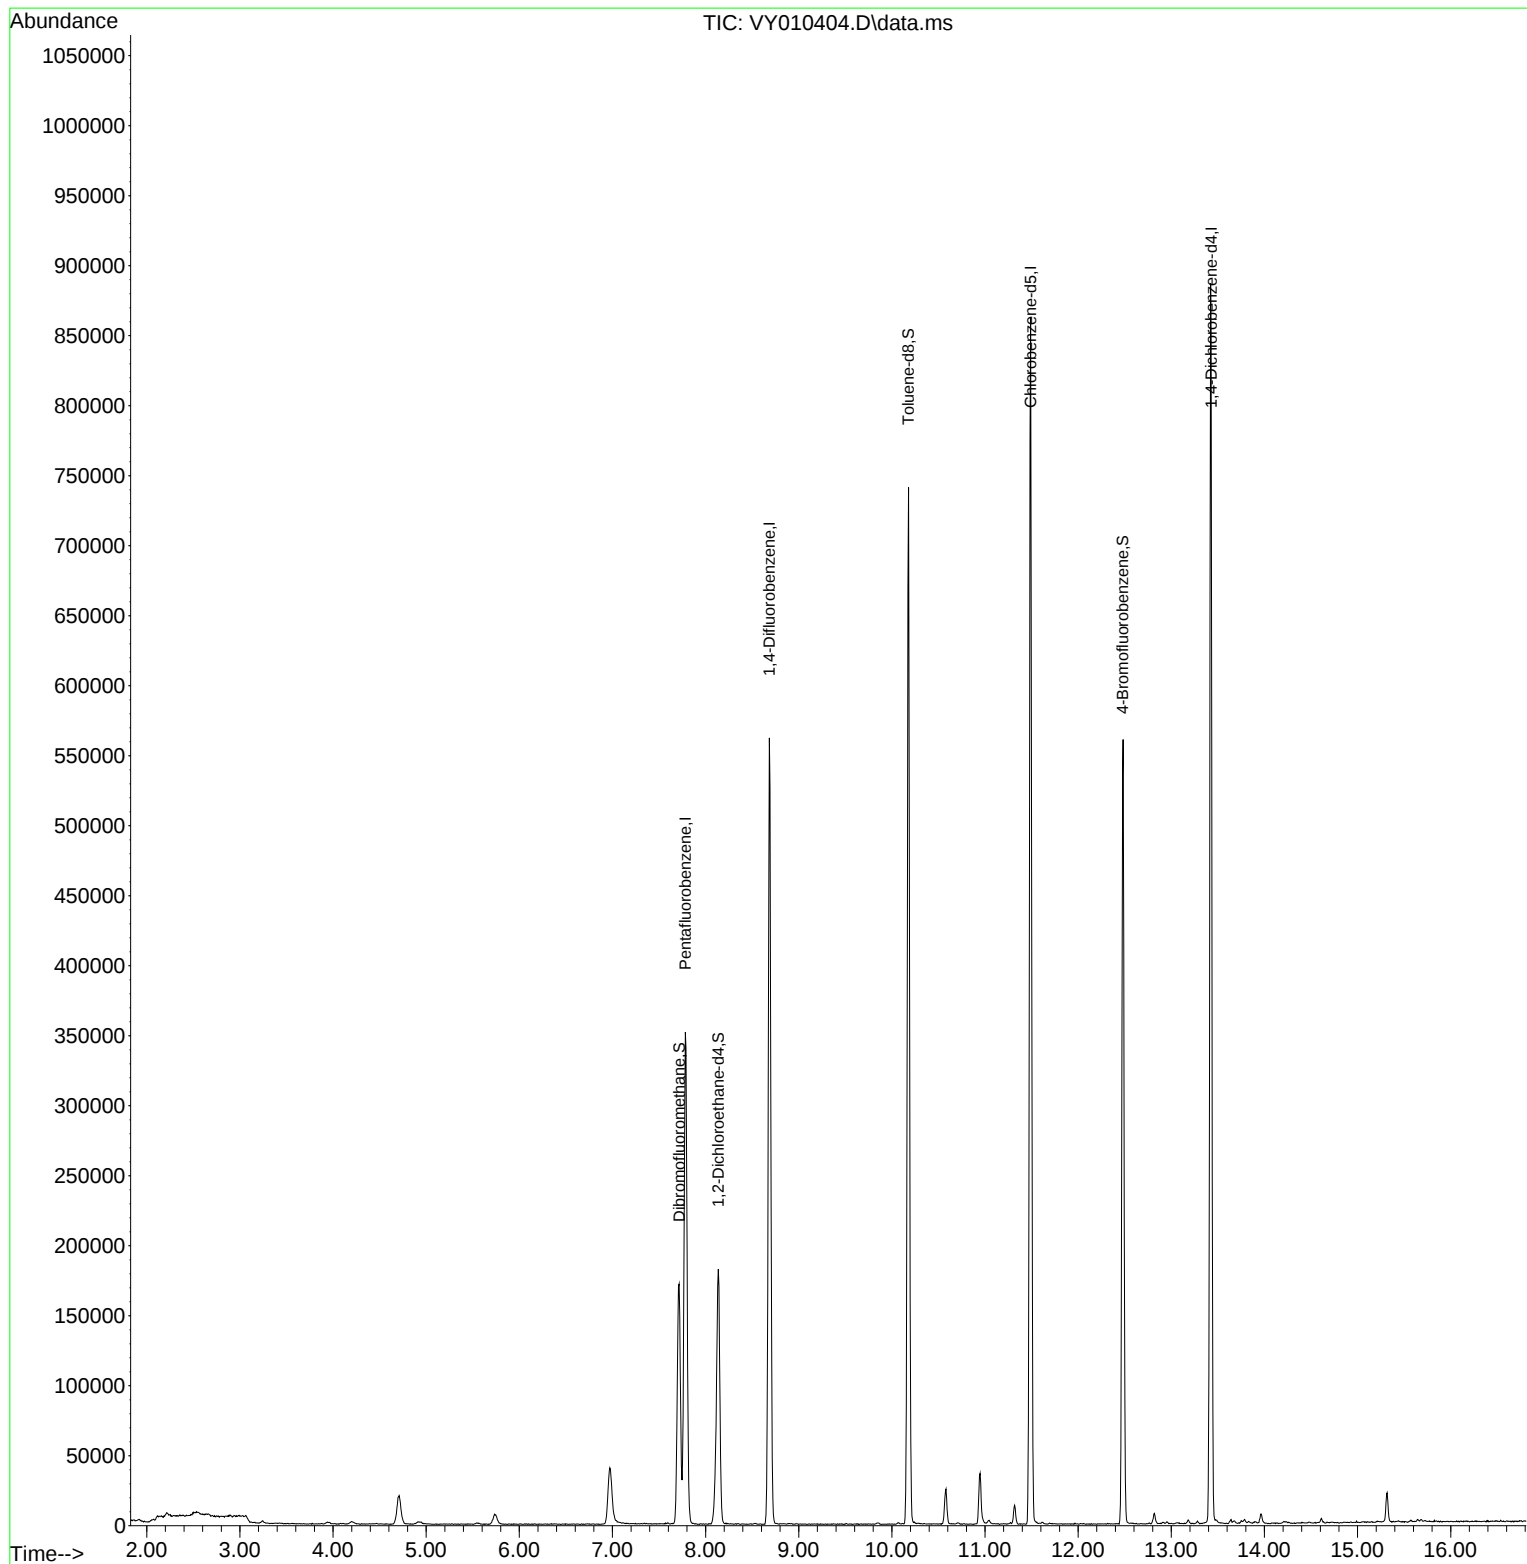


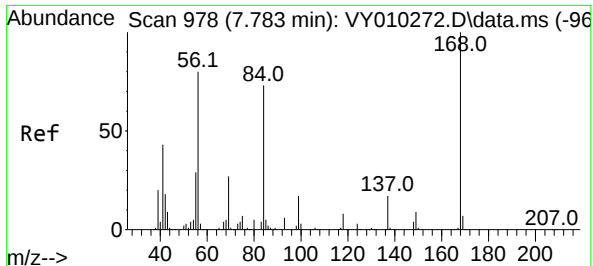

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 7.782 min Scan# 91  
Delta R.T. -0.001 min  
Lab File: VY010404.D  
Acq: 08 Sep 2022 18:32




Instrument :  
MSVOA\_Y  
ClientSampleId :  
VNJ-214


Tgt Ion:168 Resp: 286948  
Ion Ratio Lower Upper  
168 100  
99 52.6 46.9 70.3

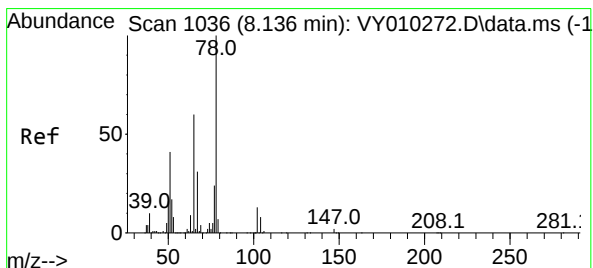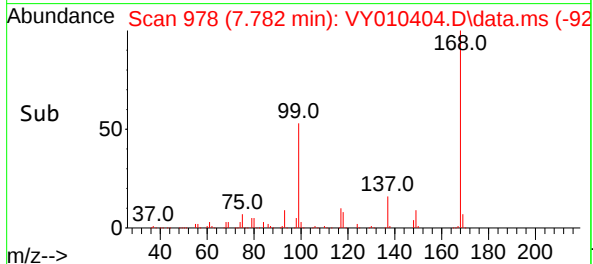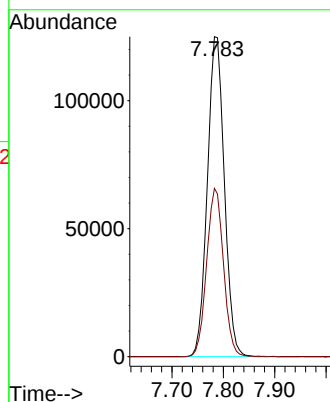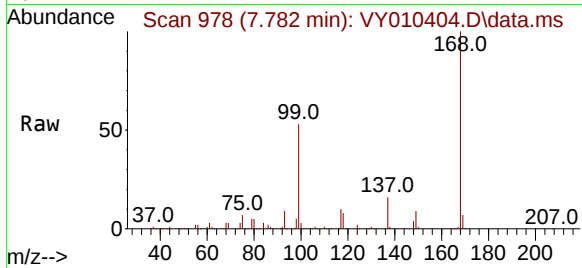

#33  
1,2-Dichloroethane-d4  
Concen: 44.545 ug/l  
RT: 8.136 min Scan# 1036  
Delta R.T. 0.000 min  
Lab File: VY010404.D  
Acq: 08 Sep 2022 18:32

Tgt Ion: 65 Resp: 131067  
Ion Ratio Lower Upper  
65 100  
67 52.2 0.0 99.4


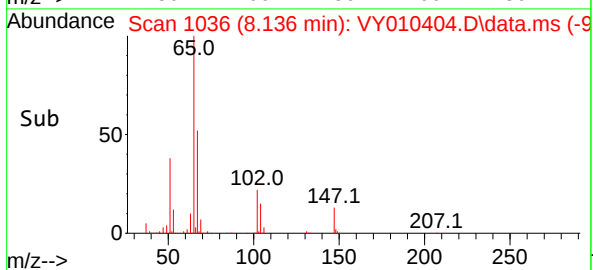
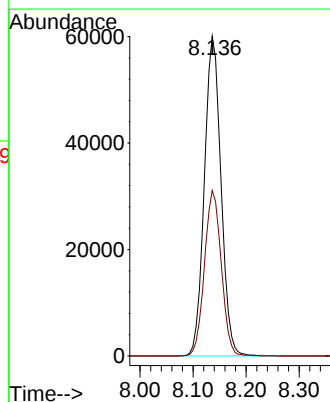
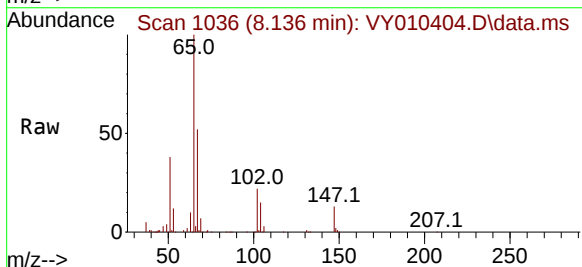


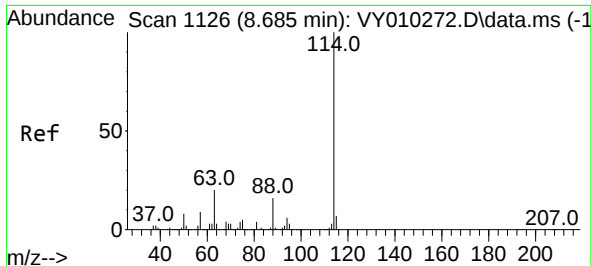

#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 8.685 min Scan# 1126  
Delta R.T. -0.000 min  
Lab File: VY010404.D  
Acq: 08 Sep 2022 18:32




Instrument :  
MSVOA\_Y  
ClientSampleId :  
VNJ-214


Tgt Ion:114 Resp: 490543  
Ion Ratio Lower Upper  
114 100  
63 18.4 0.0 43.2  
88 15.2 0.0 31.8

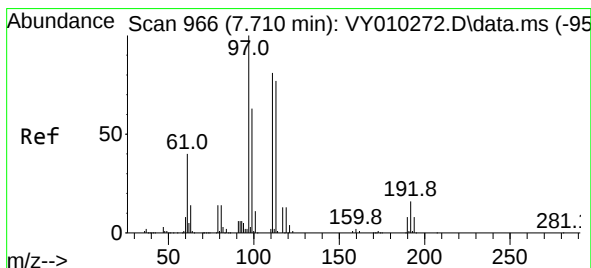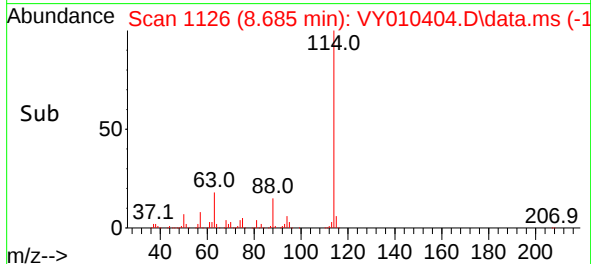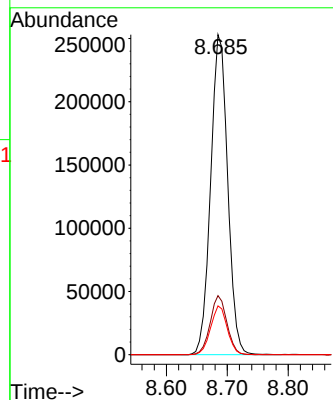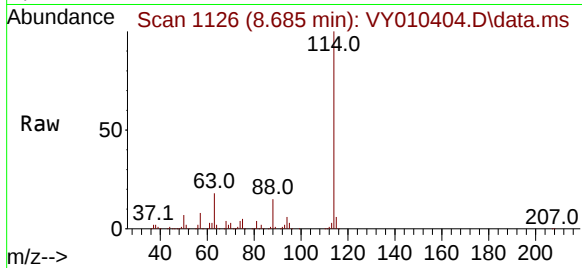

#35  
Dibromofluoromethane  
Concen: 38.156 ug/l  
RT: 7.715 min Scan# 967  
Delta R.T. 0.005 min  
Lab File: VY010404.D  
Acq: 08 Sep 2022 18:32

Tgt Ion:113 Resp: 124603  
Ion Ratio Lower Upper  
113 100  
111 101.9 82.6 124.0  
192 21.0 17.6 26.4


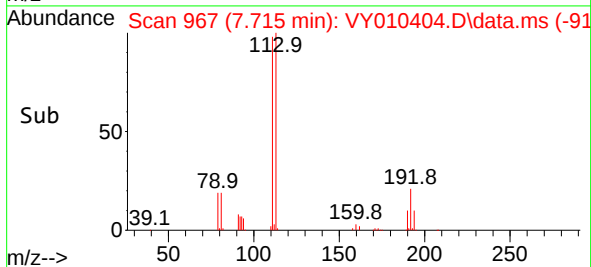
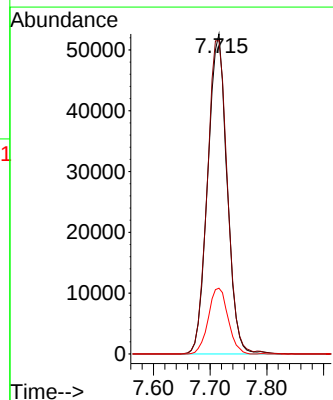
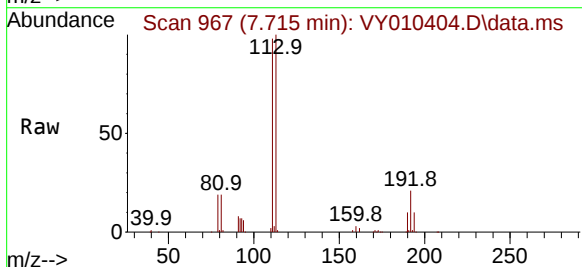


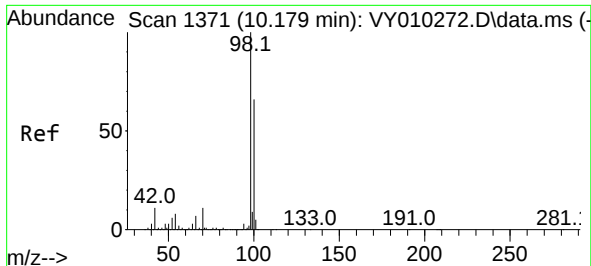

#50  
Toluene-d8  
Concen: 44.007 ug/l  
RT: 10.178 min Scan# 11  
Delta R.T. -0.001 min  
Lab File: VY010404.D  
Acq: 08 Sep 2022 18:32




Instrument :  
MSVOA\_Y  
ClientSampleId :  
VNJ-214


Tgt Ion: 98 Resp: 481148  
Ion Ratio Lower Upper  
98 100  
100 65.4 50.2 75.2

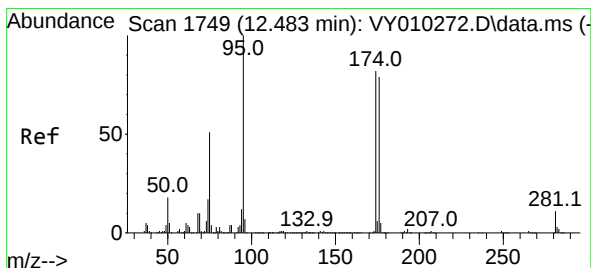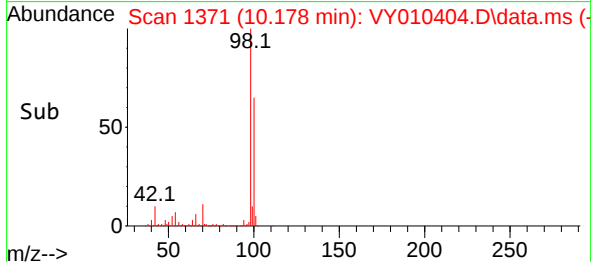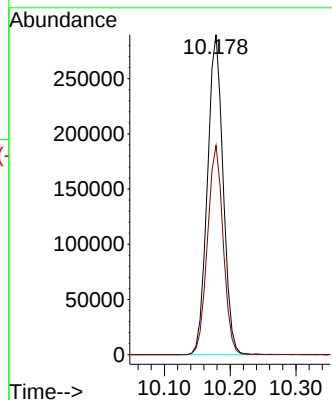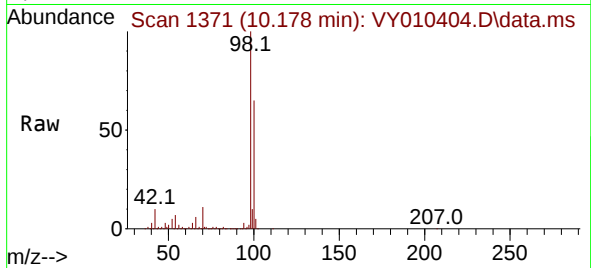

#62  
4-Bromofluorobenzene  
Concen: 37.640 ug/l  
RT: 12.477 min Scan# 1748  
Delta R.T. -0.006 min  
Lab File: VY010404.D  
Acq: 08 Sep 2022 18:32

Tgt Ion: 95 Resp: 171642  
Ion Ratio Lower Upper  
95 100  
174 86.7 0.0 177.0  
176 84.9 0.0 175.8


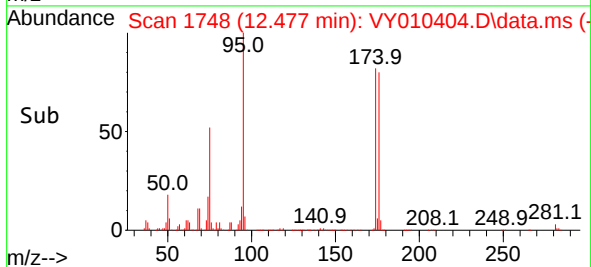
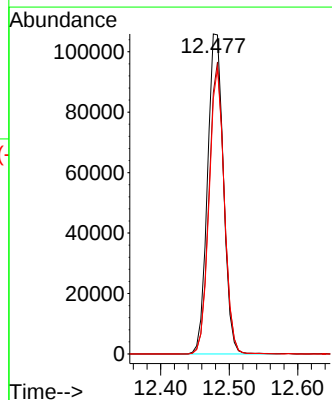
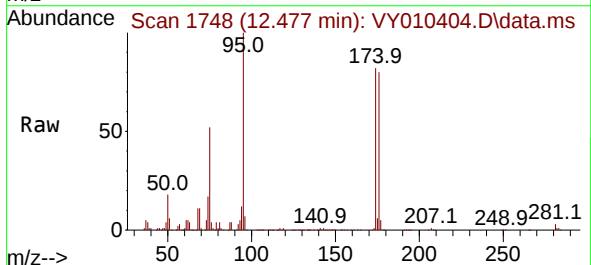


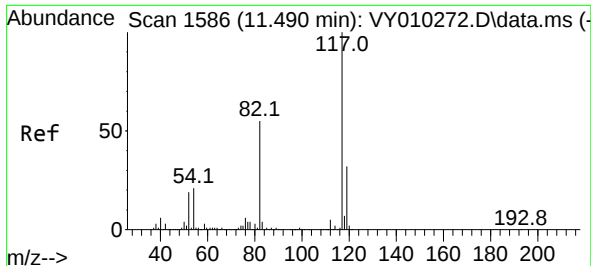

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.489 min Scan# 117  
Delta R.T. -0.001 min  
Lab File: VY010404.D  
Acq: 08 Sep 2022 18:32

Instrument :  
MSVOA\_Y  
ClientSampleId :  
VNJ-214

Tgt Ion:117 Resp: 480672  
Ion Ratio Lower Upper  
117 100  
82 52.6 43.0 64.4  
119 33.1 25.4 38.0

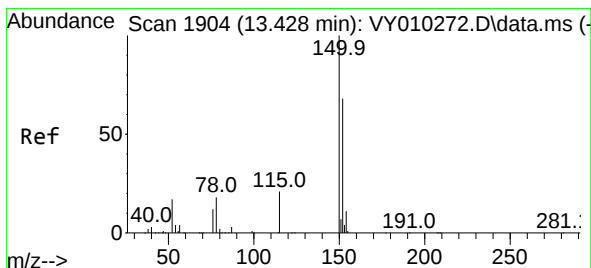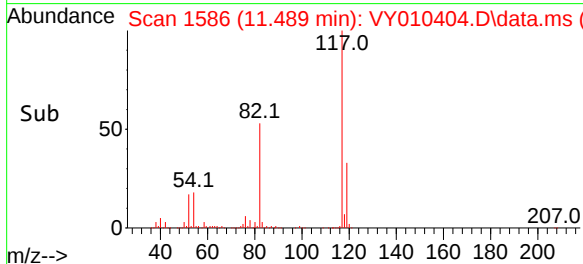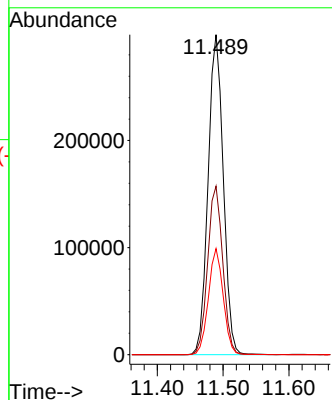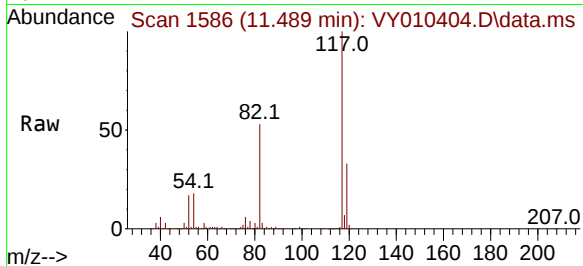

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.428 min Scan# 1904  
Delta R.T. -0.000 min  
Lab File: VY010404.D  
Acq: 08 Sep 2022 18:32

Tgt Ion:152 Resp: 234068  
Ion Ratio Lower Upper  
152 100  
115 57.2 28.2 84.7  
150 158.6 0.0 347.6

