
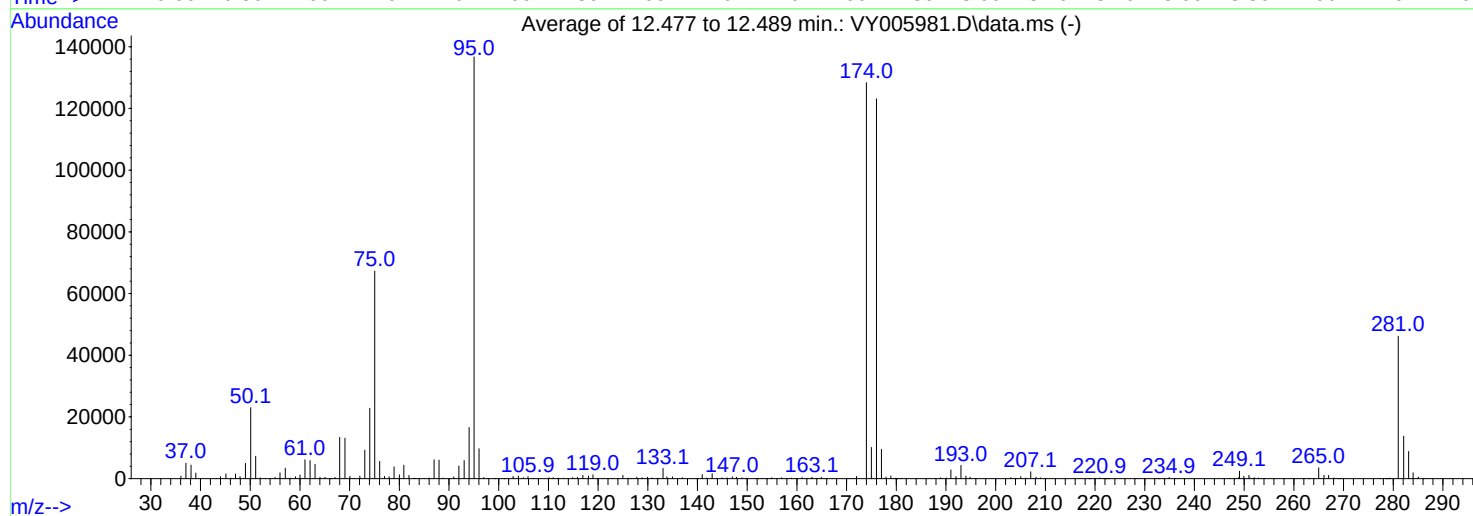


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091021\
 Data File : VY005981.D
 Acq On : 10 Sep 2021 11:12
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y0831215.M
 Title : SW846 8260
 Last Update : Wed Sep 01 05:32:43 2021

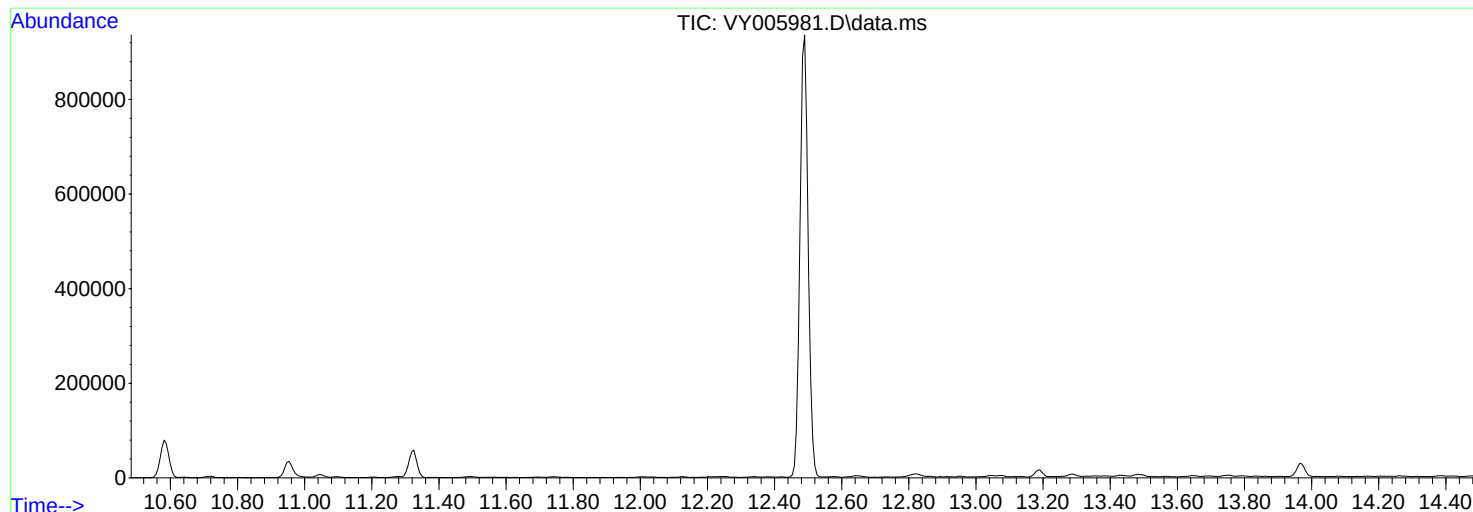

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1737

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	23035	PASS
75	95	30	60	49.2	67272	PASS
95	95	100	100	100.0	136728	PASS
96	95	5	9	7.1	9695	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	93.9	128347	PASS
175	174	5	9	7.9	10113	PASS
176	174	95	101	95.9	123133	PASS
177	176	5	9	7.7	9478	PASS