



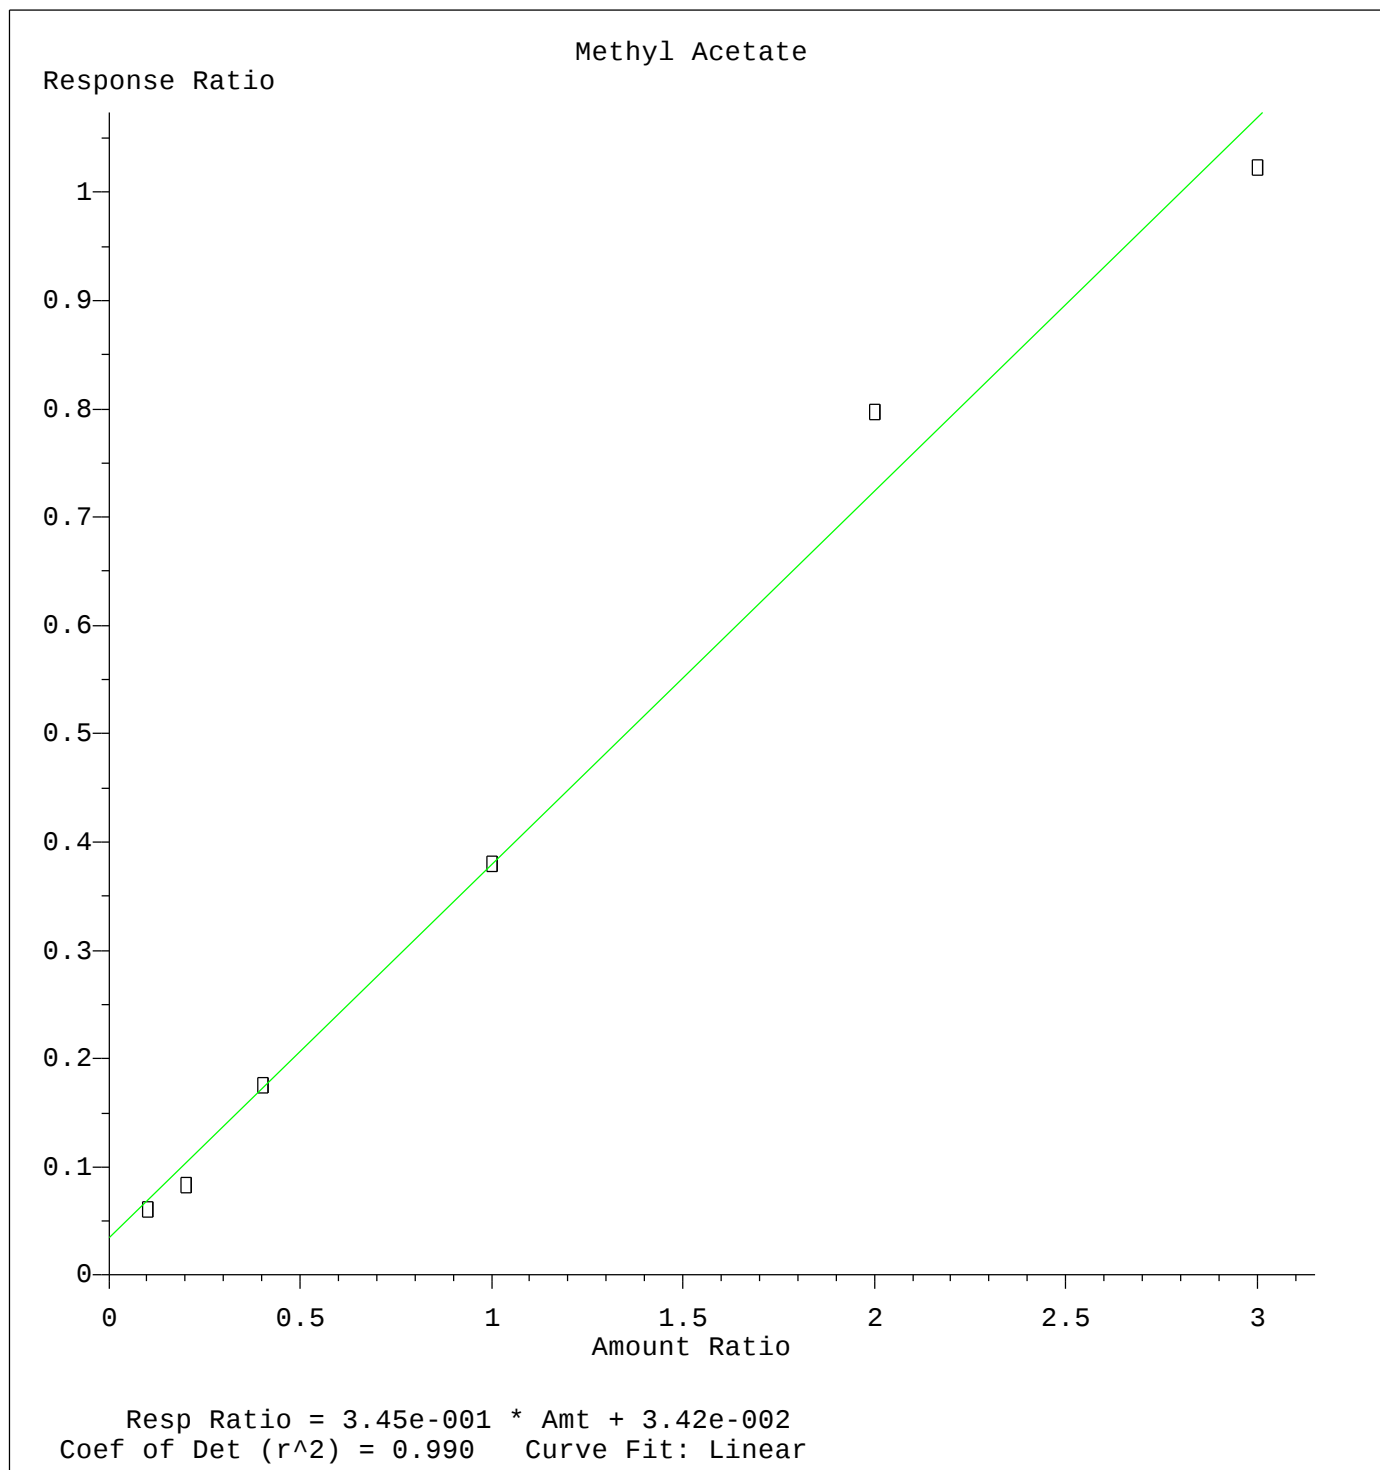

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y091119S.M
Calibration Table Last Updated: Thu Sep 19 11:25:13 2019


Methylene Chloride

Response Ratio

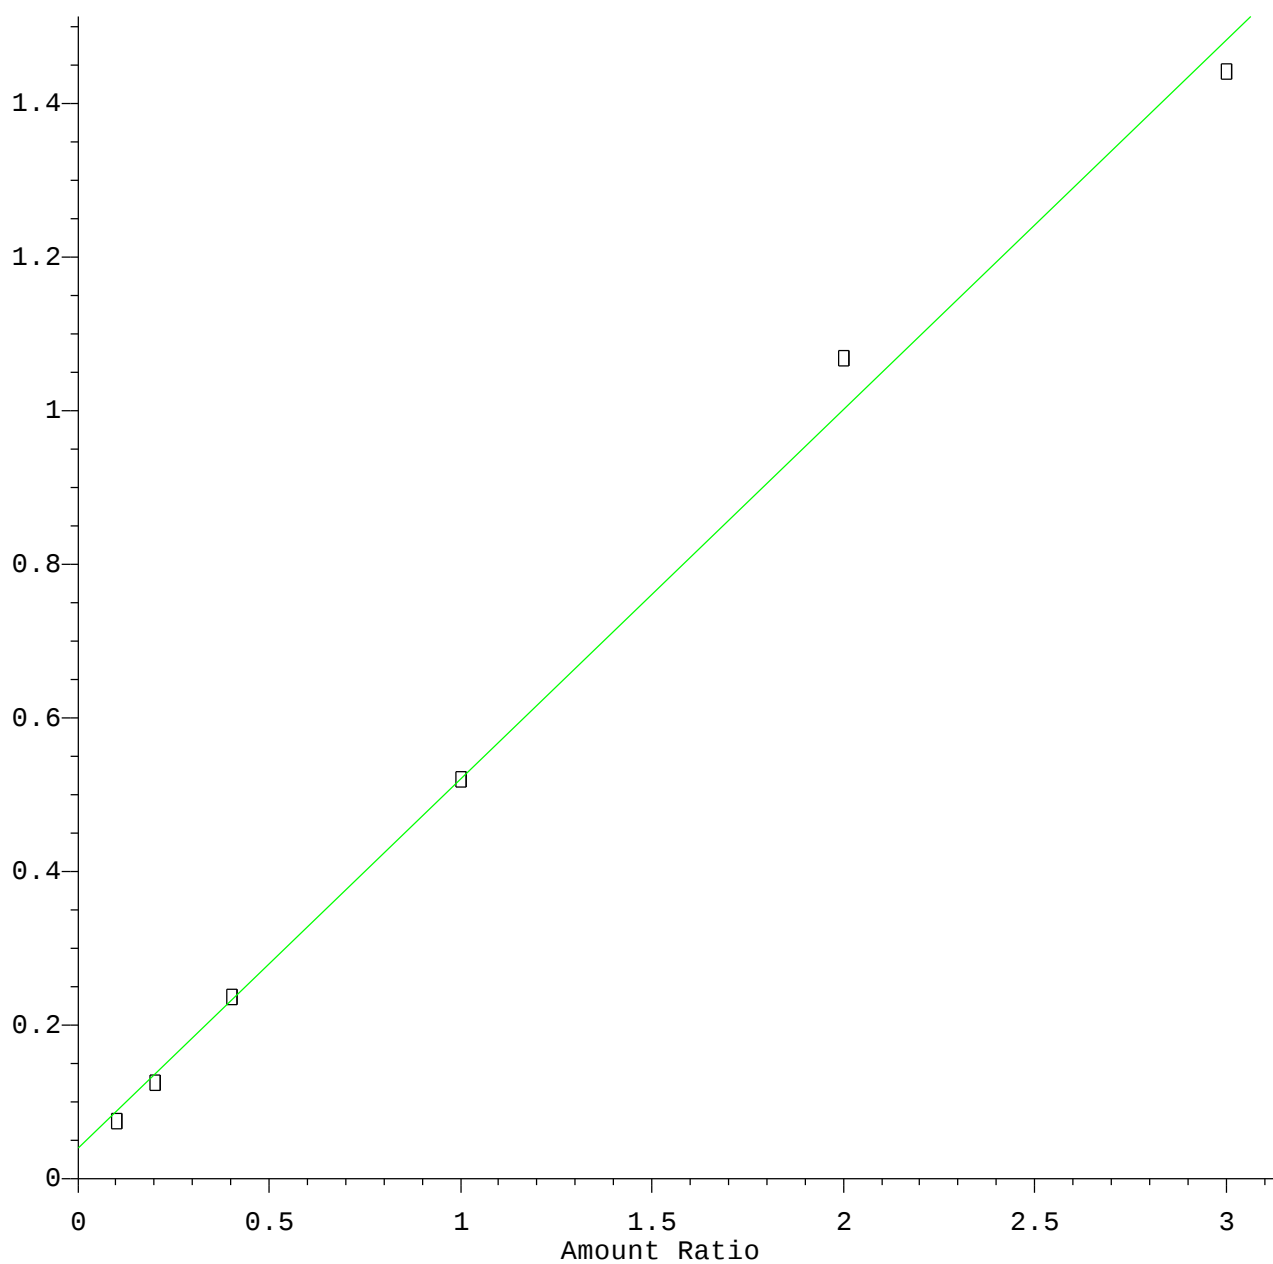

Resp Ratio = $4.81 \times 10^{-1} \times \text{Amt} + 4.00 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y091119S.M
Calibration Table Last Updated: Thu Sep 19 11:25:13 2019

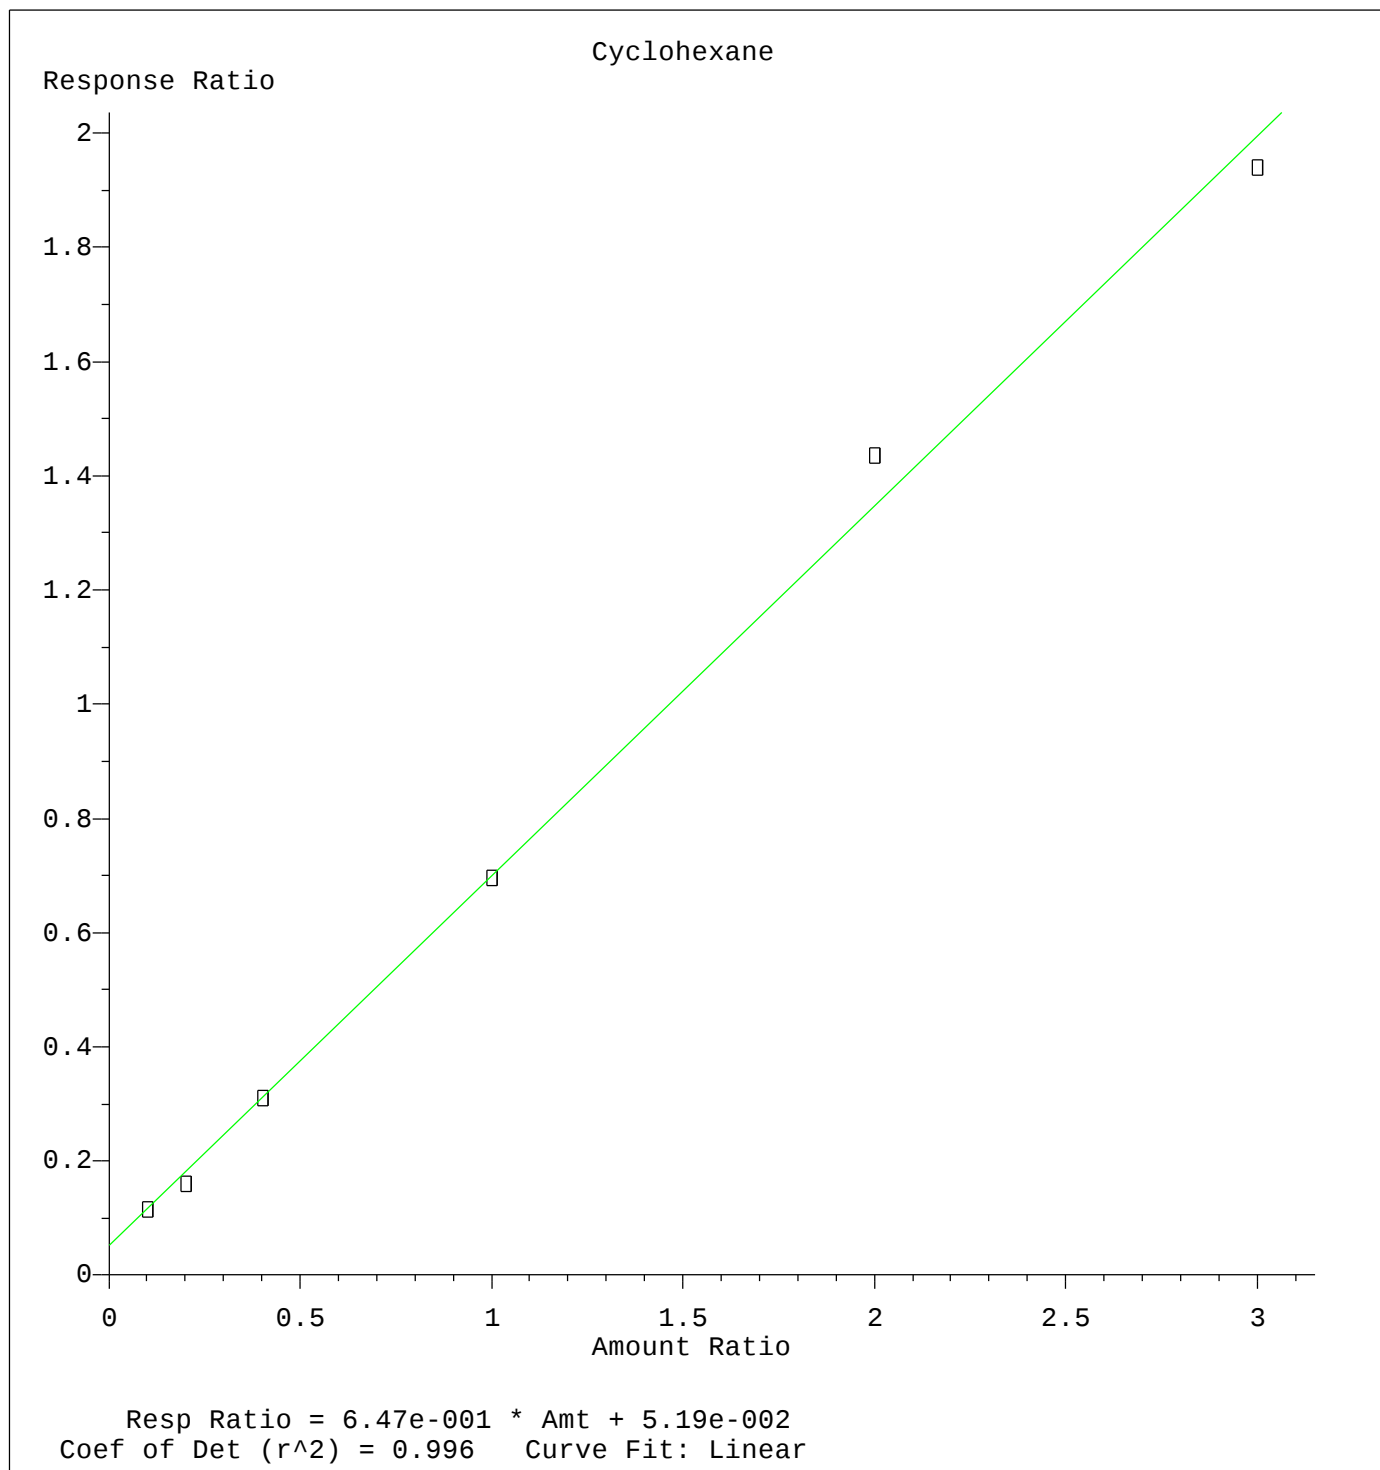

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y091119S.M
Calibration Table Last Updated: Thu Sep 19 11:25:13 2019


Dichlorodifluoromethane

Response Ratio

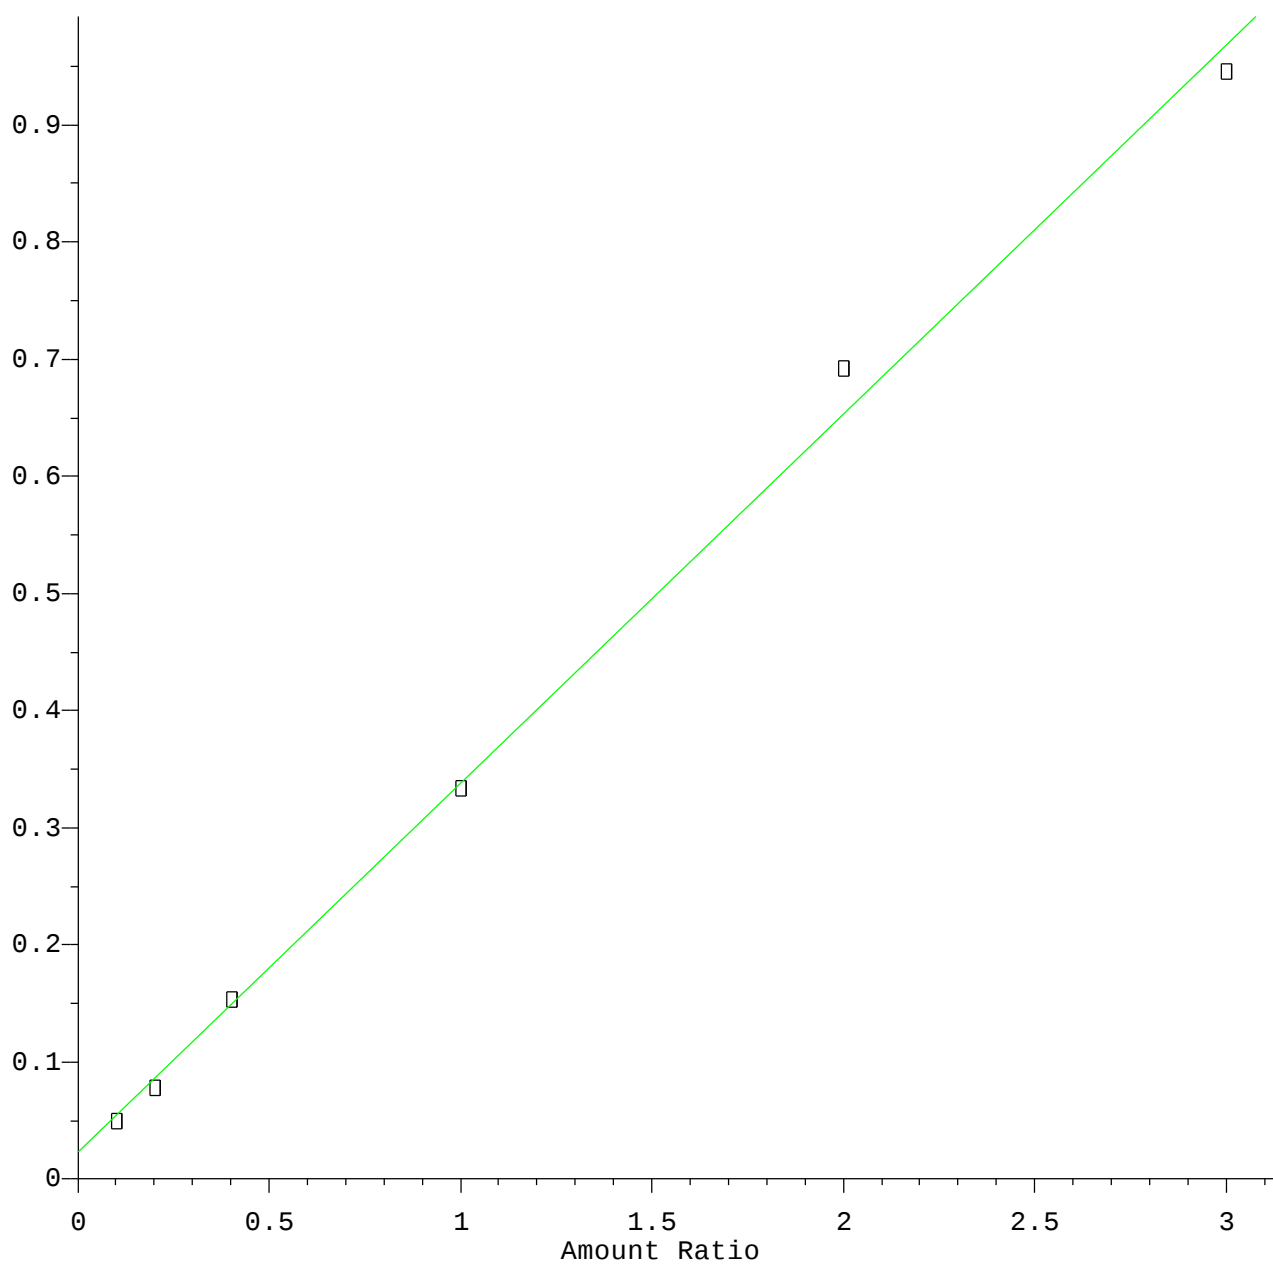

Resp Ratio = $3.15 \times 10^{-1} \times \text{Amt} + 2.26 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y091119S.M
Calibration Table Last Updated: Thu Sep 19 11:25:13 2019

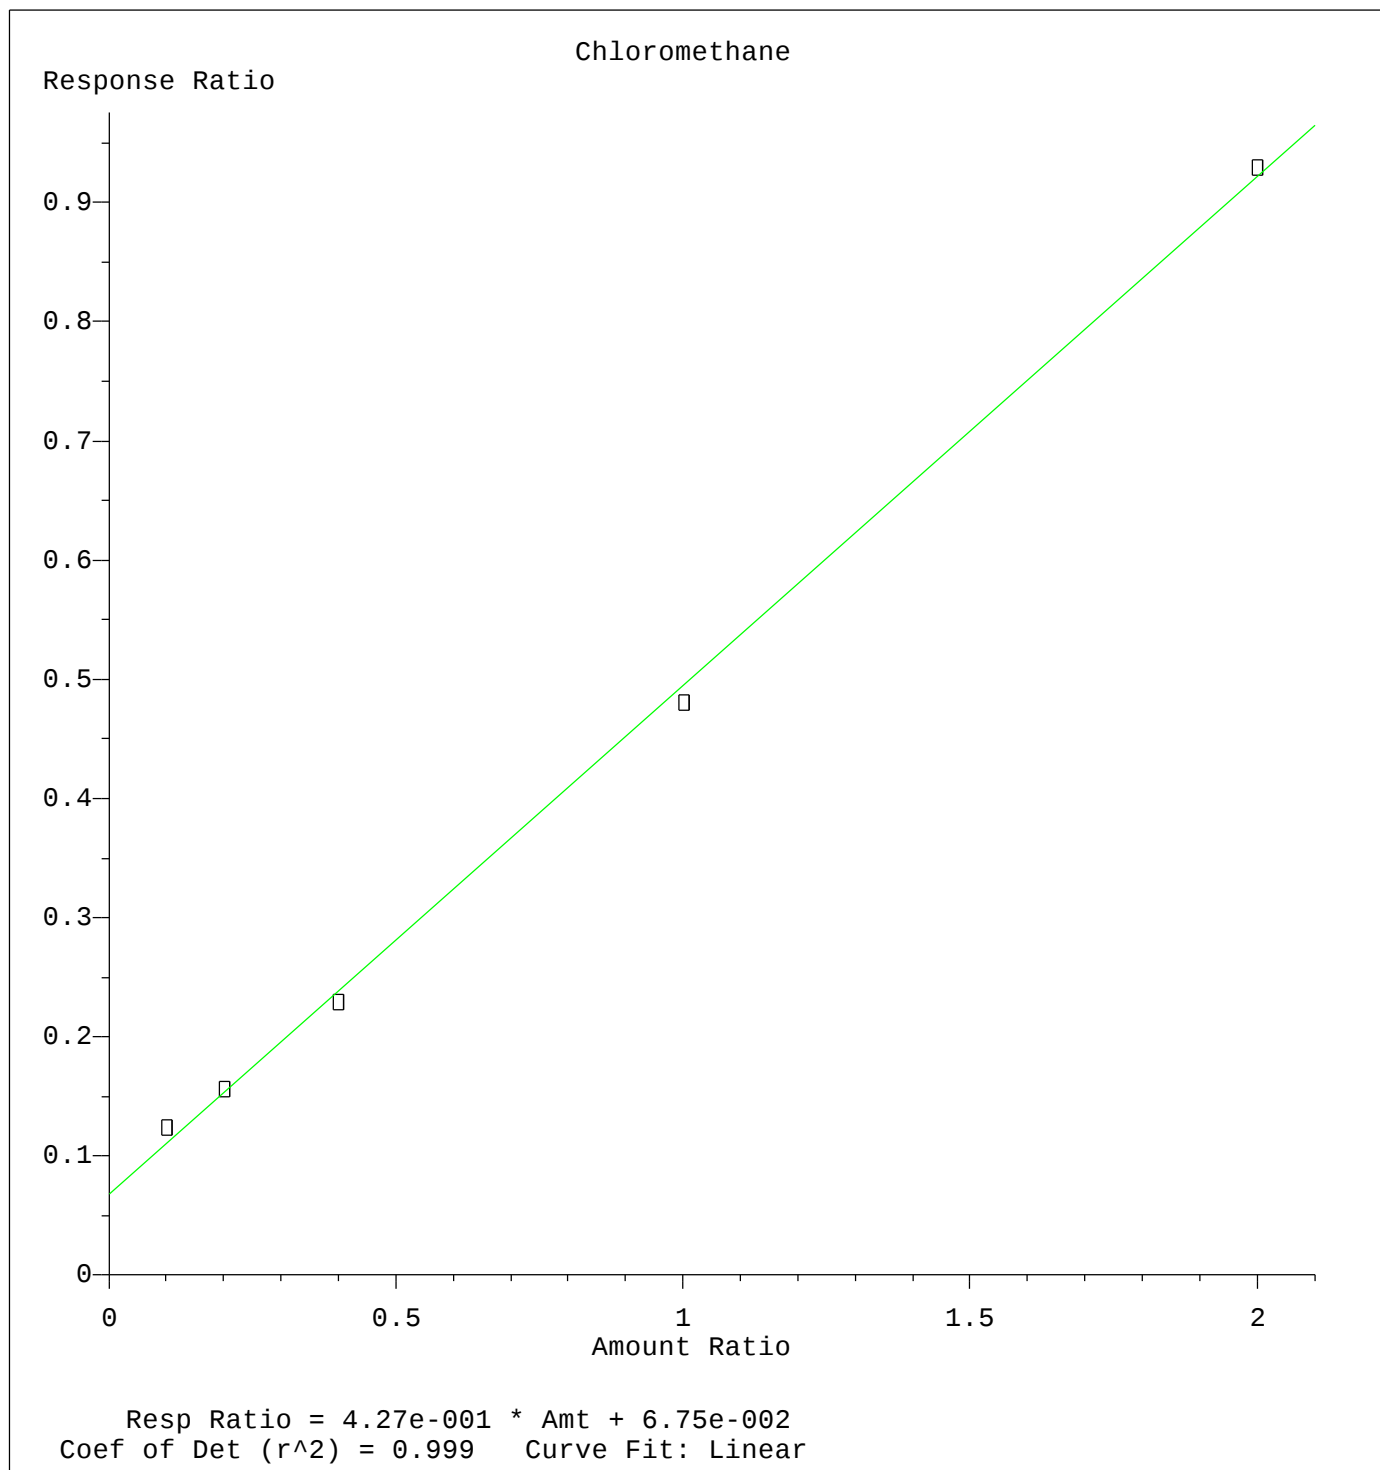

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y091119S.M
Calibration Table Last Updated: Thu Sep 19 11:25:13 2019


Acrolein

Response Ratio

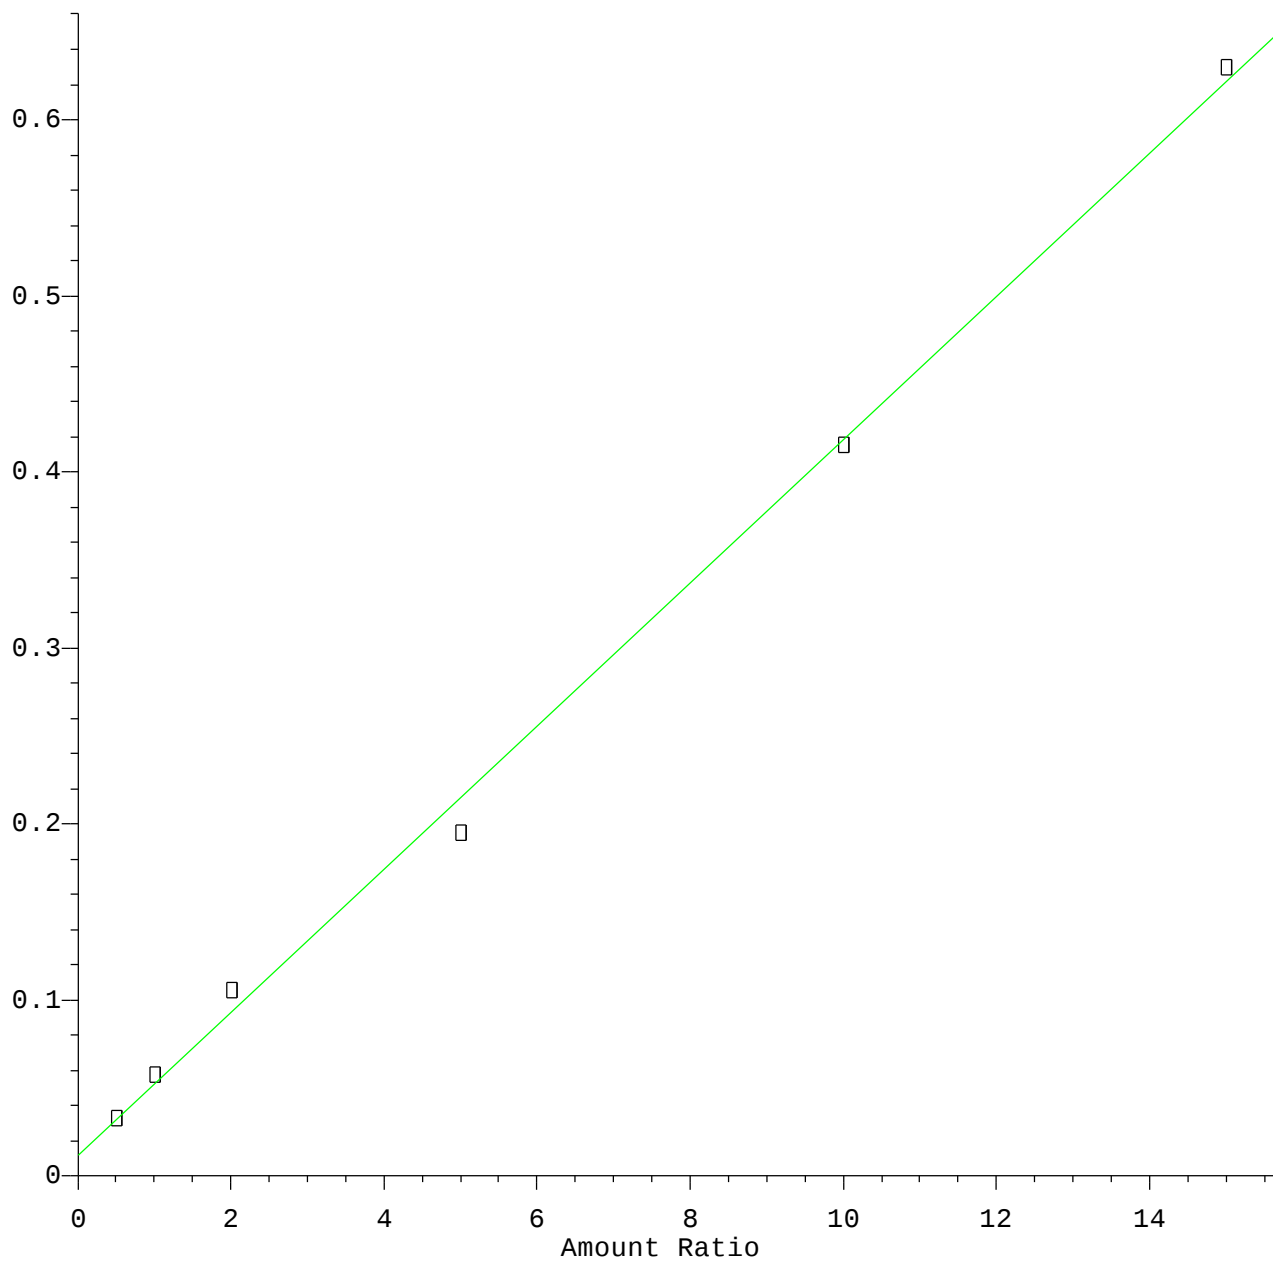

Resp Ratio = $4.07 \times 10^{-2} \times \text{Amt} + 1.21 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y091119S.M
Calibration Table Last Updated: Thu Sep 19 11:25:13 2019

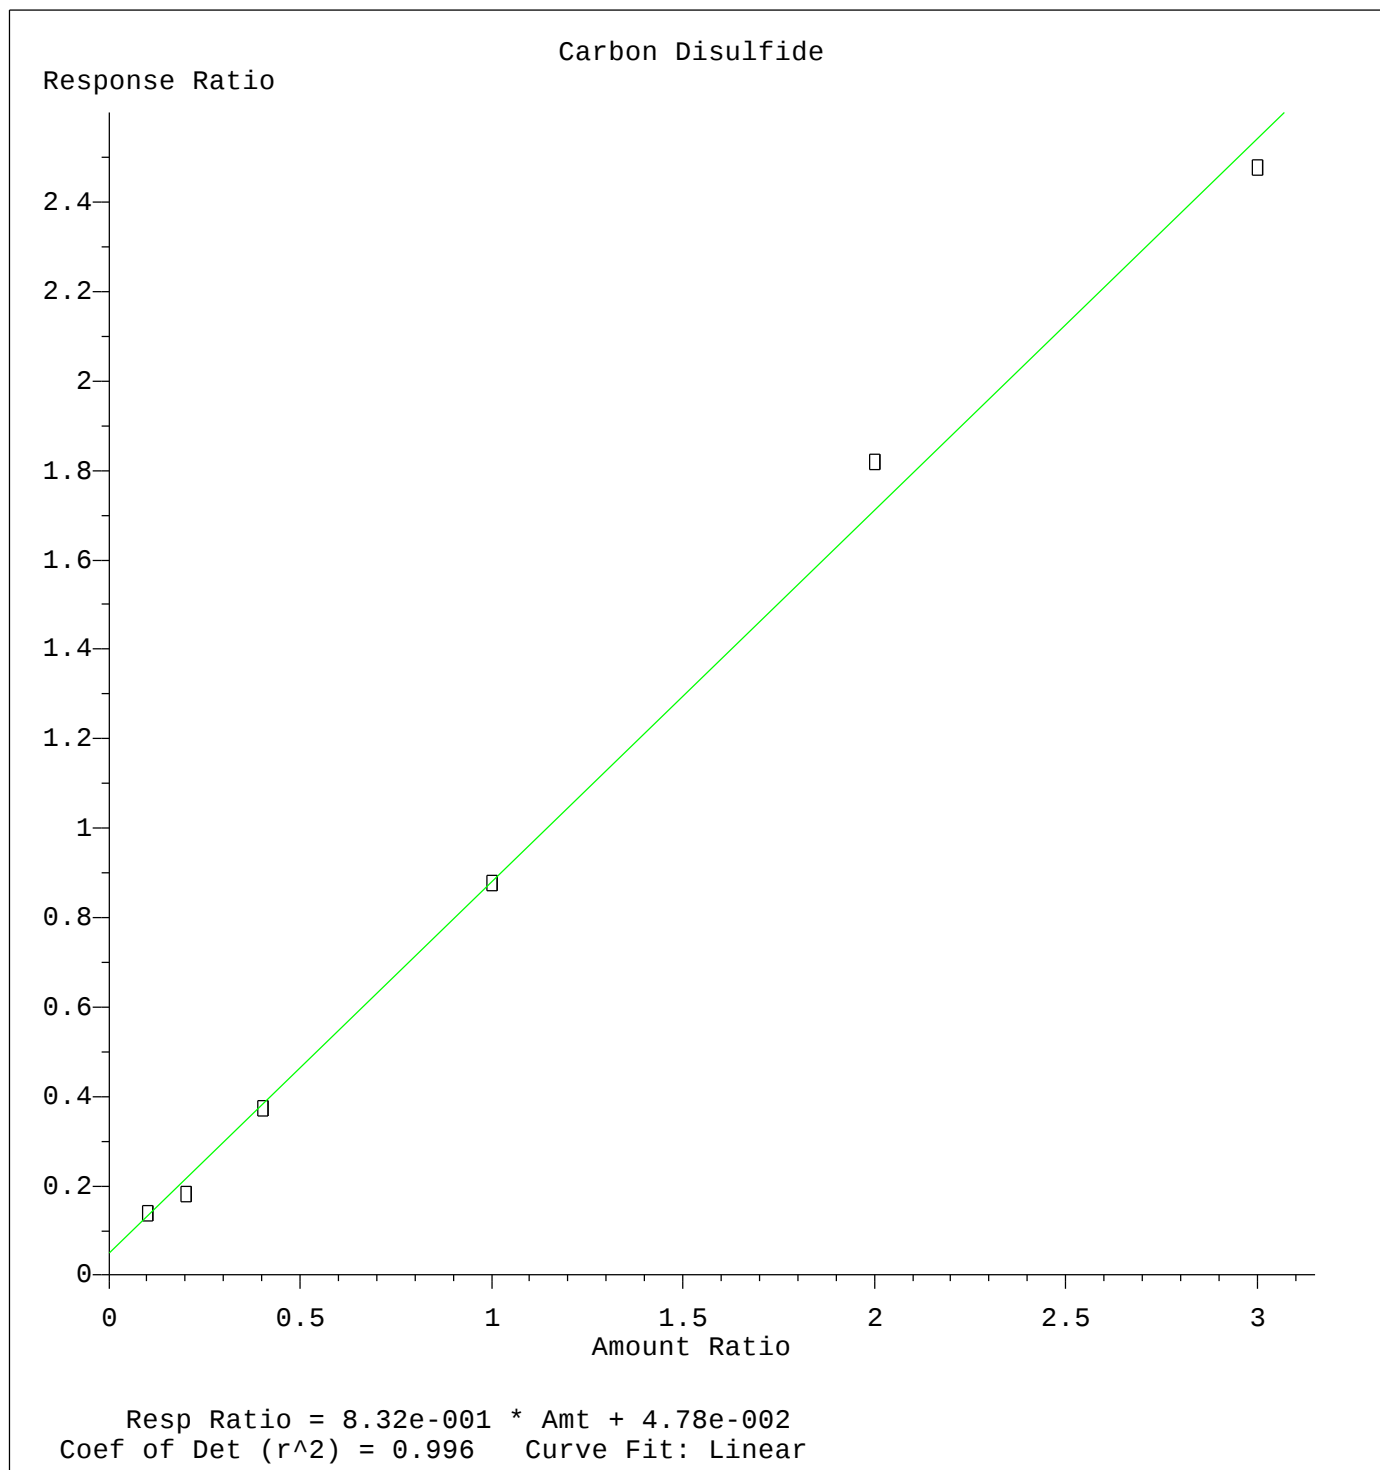

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y091119S.M
Calibration Table Last Updated: Thu Sep 19 11:25:13 2019