


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\VY091119\
Data File : VY000001.D
Acq On : 11 Sep 2019 12:40
Operator :
Sample : BFB
Misc : 5.00µl/5.00ml
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y091119S.M
Title : SW846 8260
Last Update : Thu Sep 12 09:07:31 2019

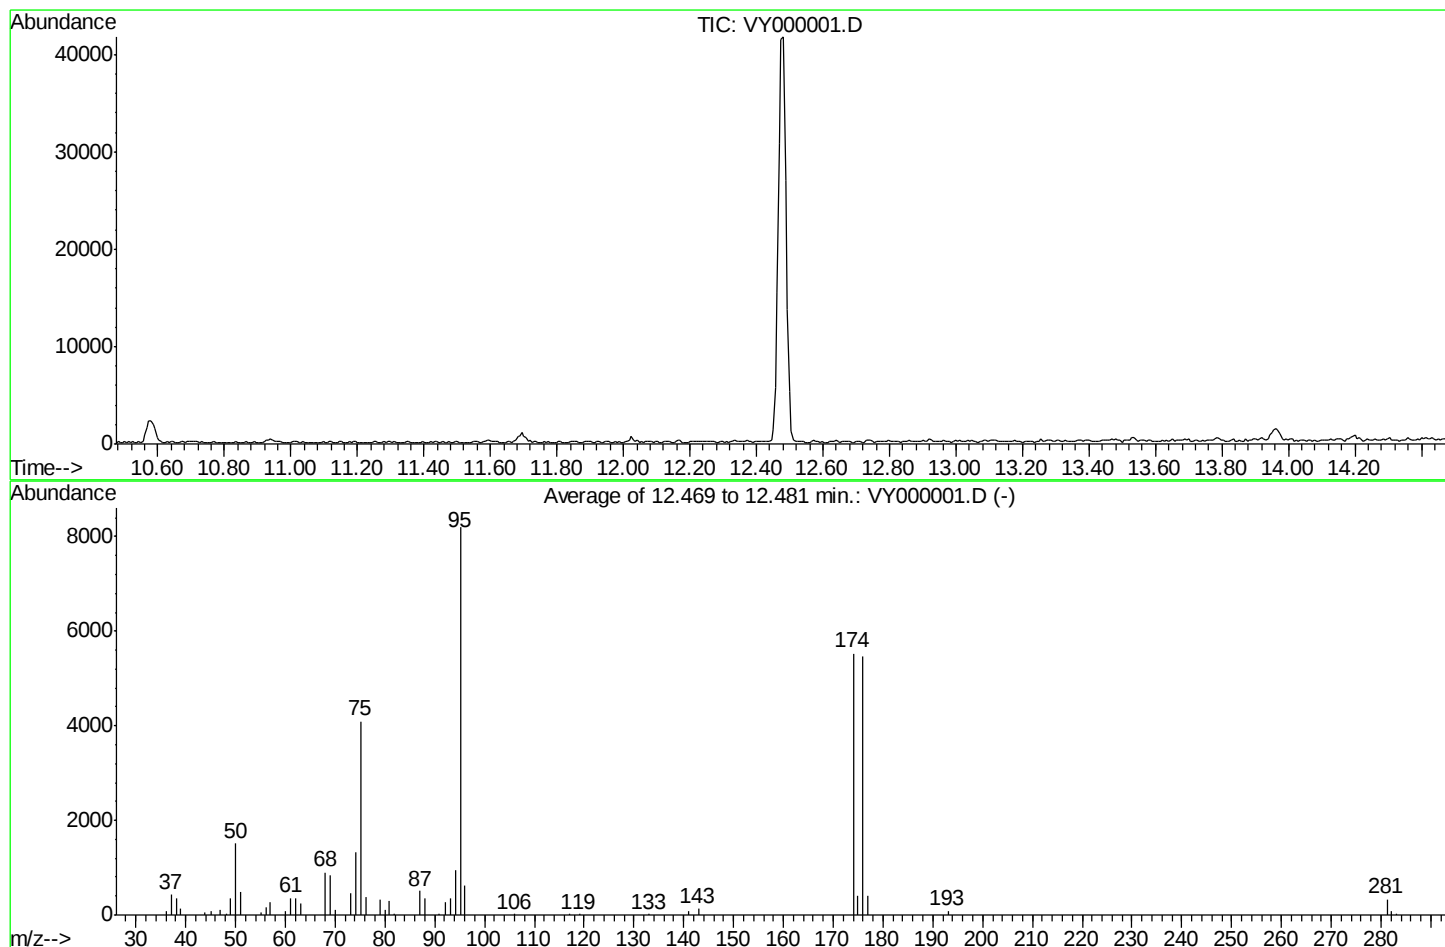

AutoFind: Scans 1733, 1734, 1735; Background Corrected with Scan 1726

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	1514	PASS
75	95	30	60	50.0	4095	PASS
95	95	100	100	100.0	8197	PASS
96	95	5	9	7.7	633	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	67.4	5526	PASS
175	174	5	9	7.1	394	PASS
176	174	95	101	99.1	5476	PASS
177	176	5	9	7.4	406	PASS