



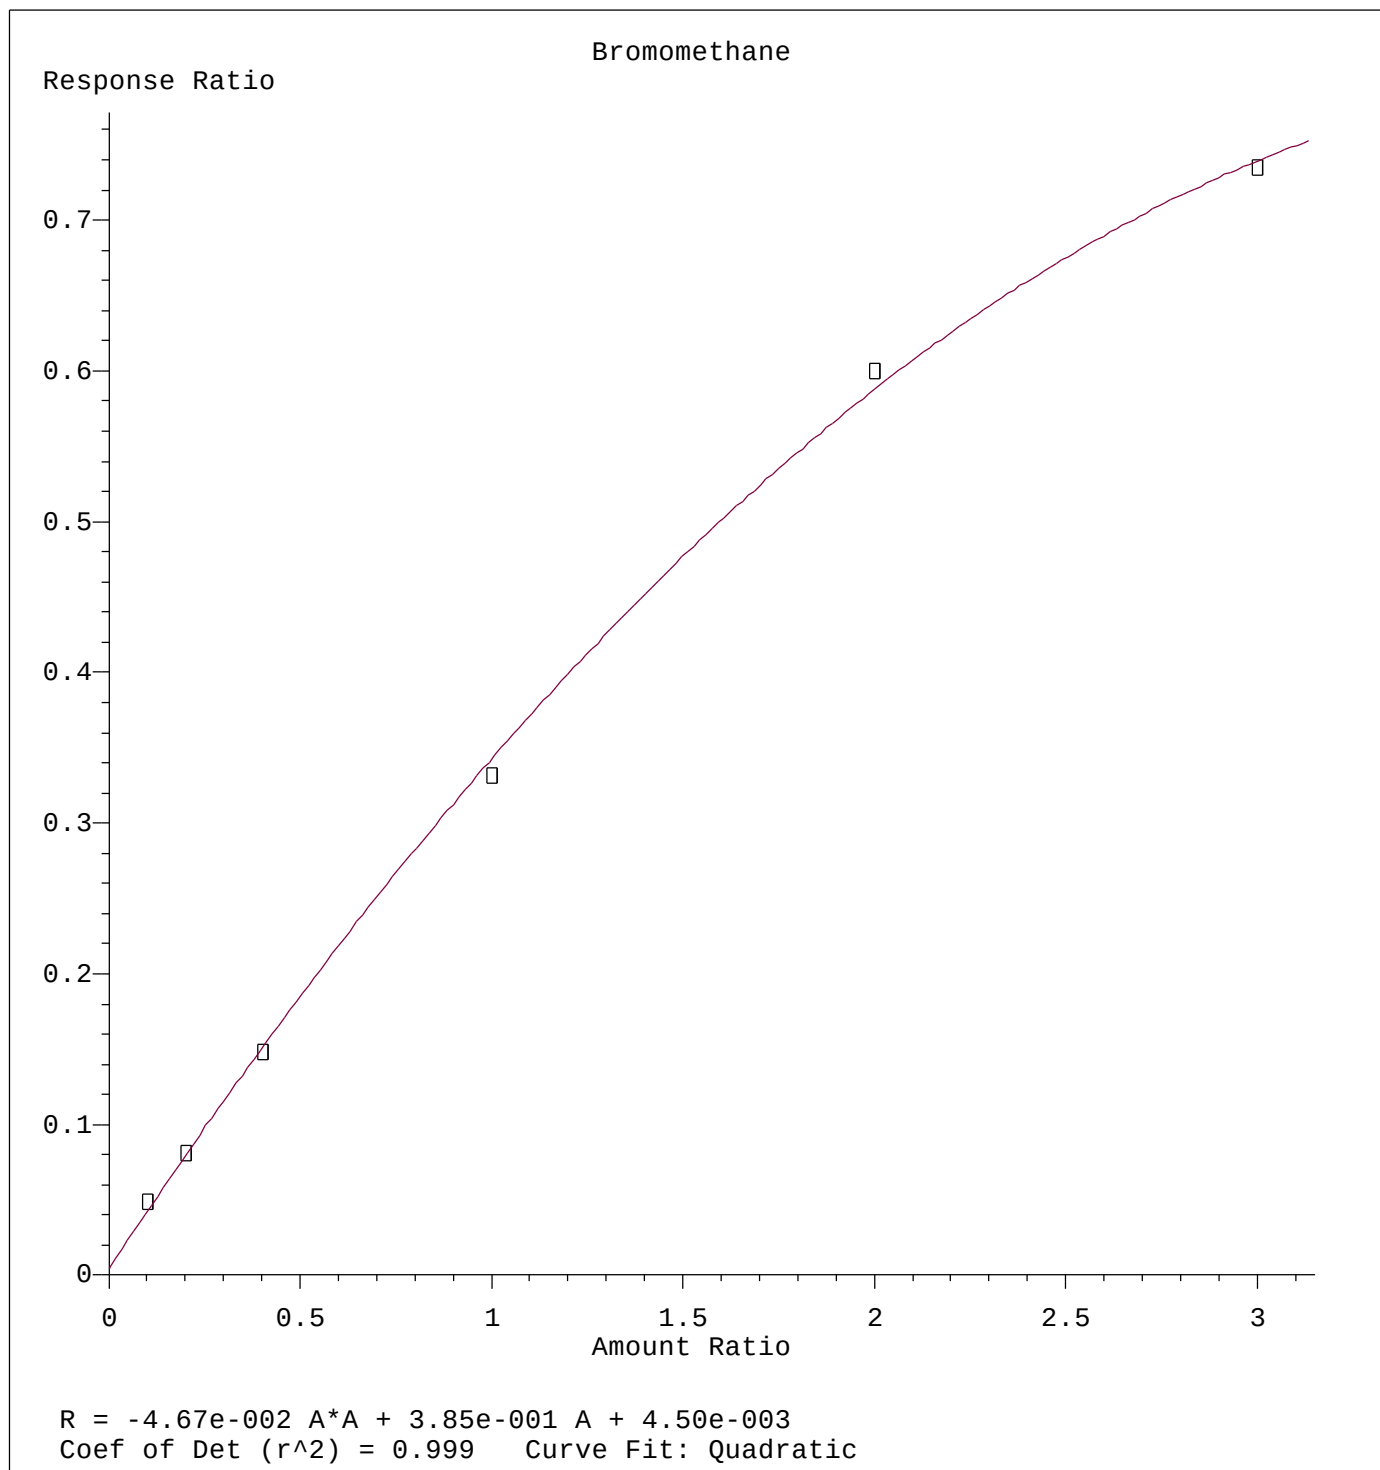


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y091219S.M
Calibration Table Last Updated: Thu Sep 12 16:17:30 2019

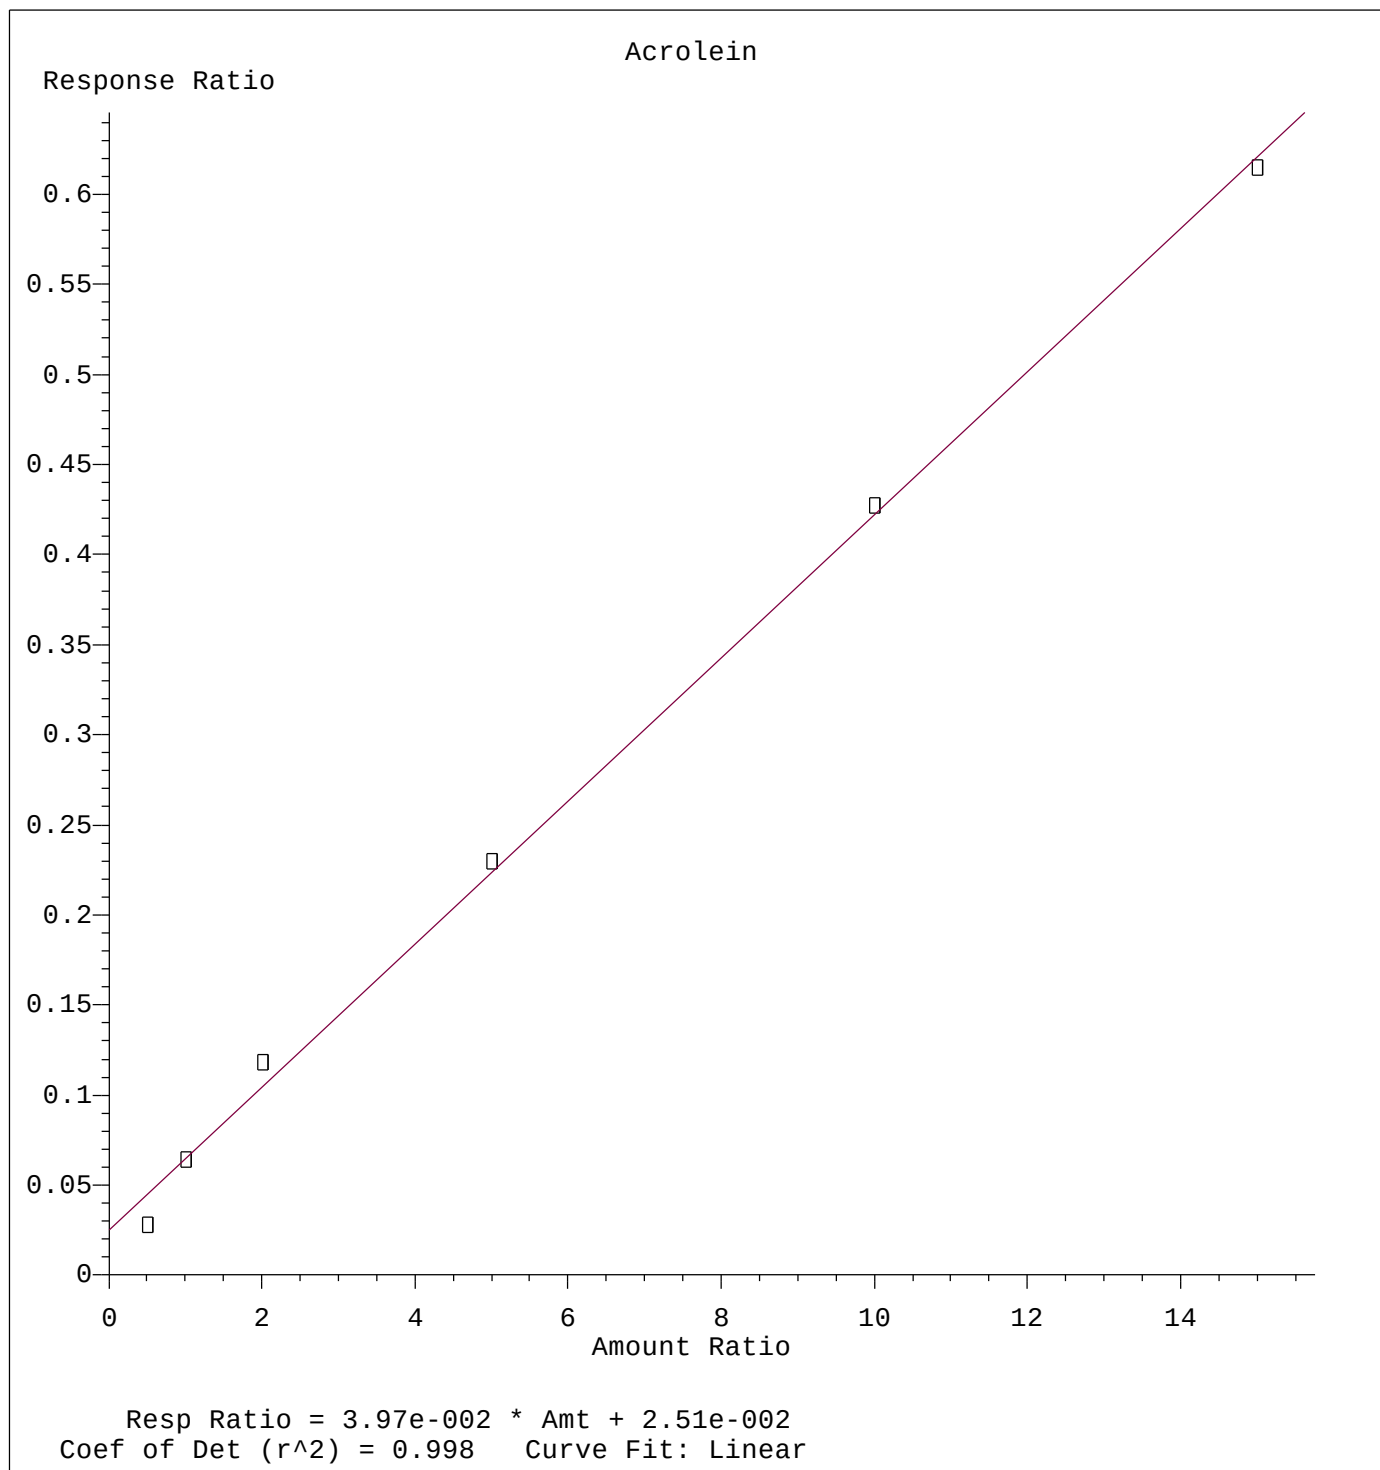

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y091219S.M
Calibration Table Last Updated: Thu Sep 12 16:17:30 2019


Methylene Chloride

Response Ratio

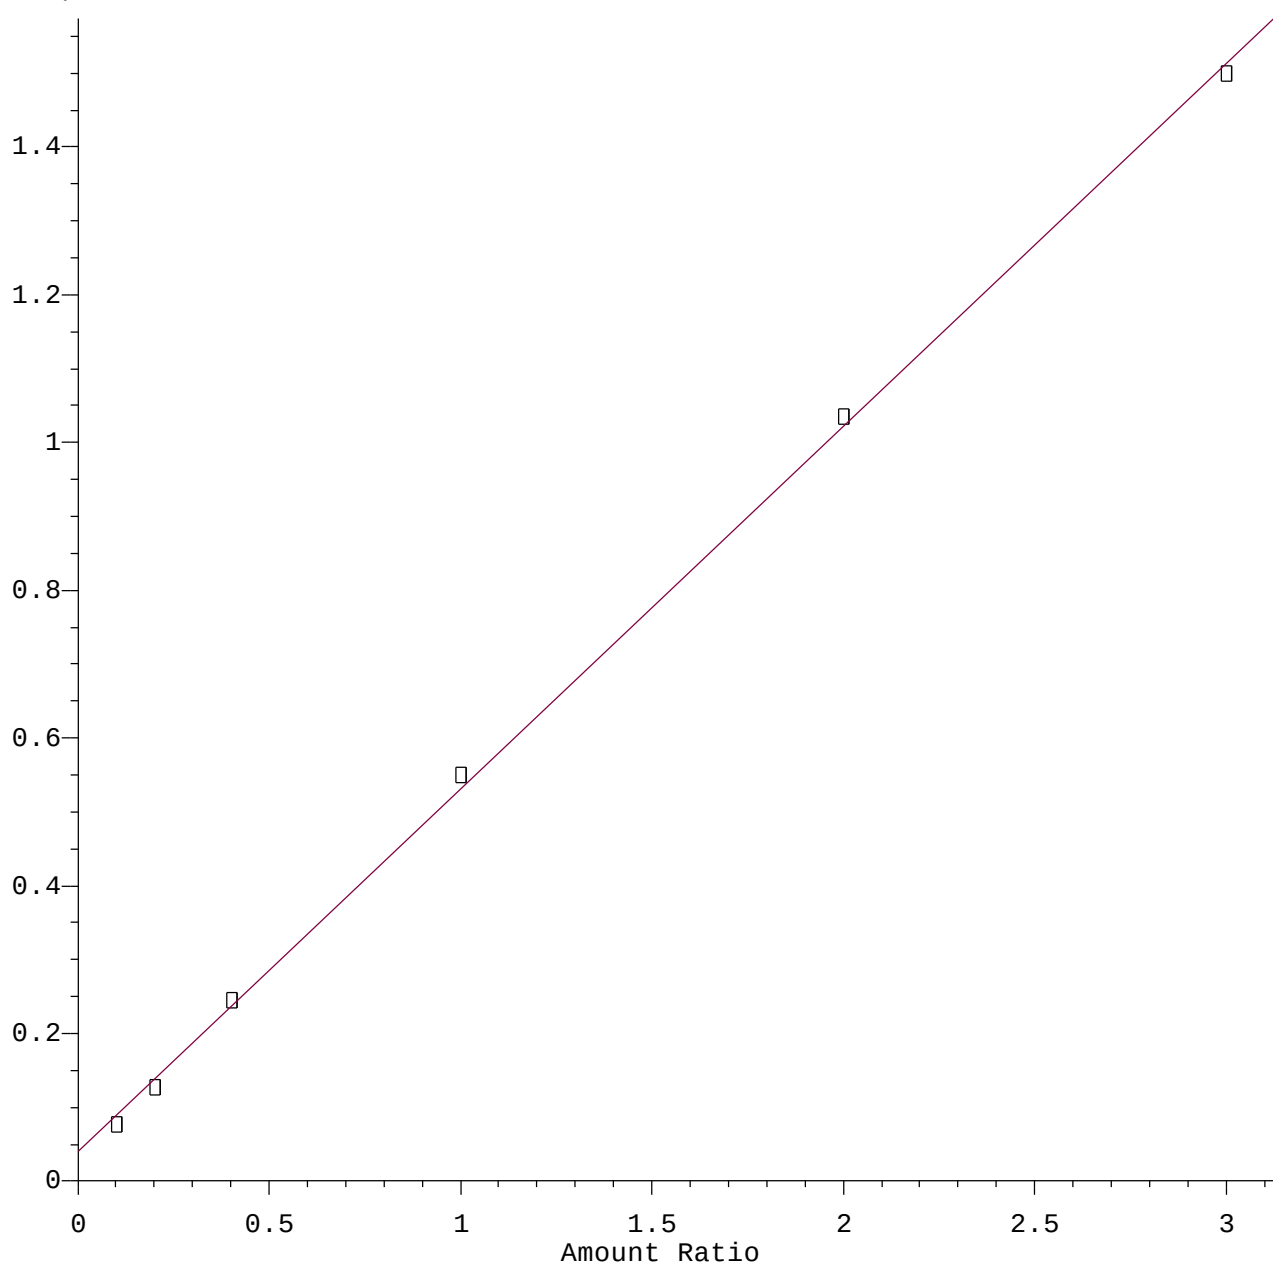


Resp Ratio = $4.91 \times 10^{-1} \times \text{Amt} + 3.99 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y091219S.M
Calibration Table Last Updated: Thu Sep 12 16:17:30 2019

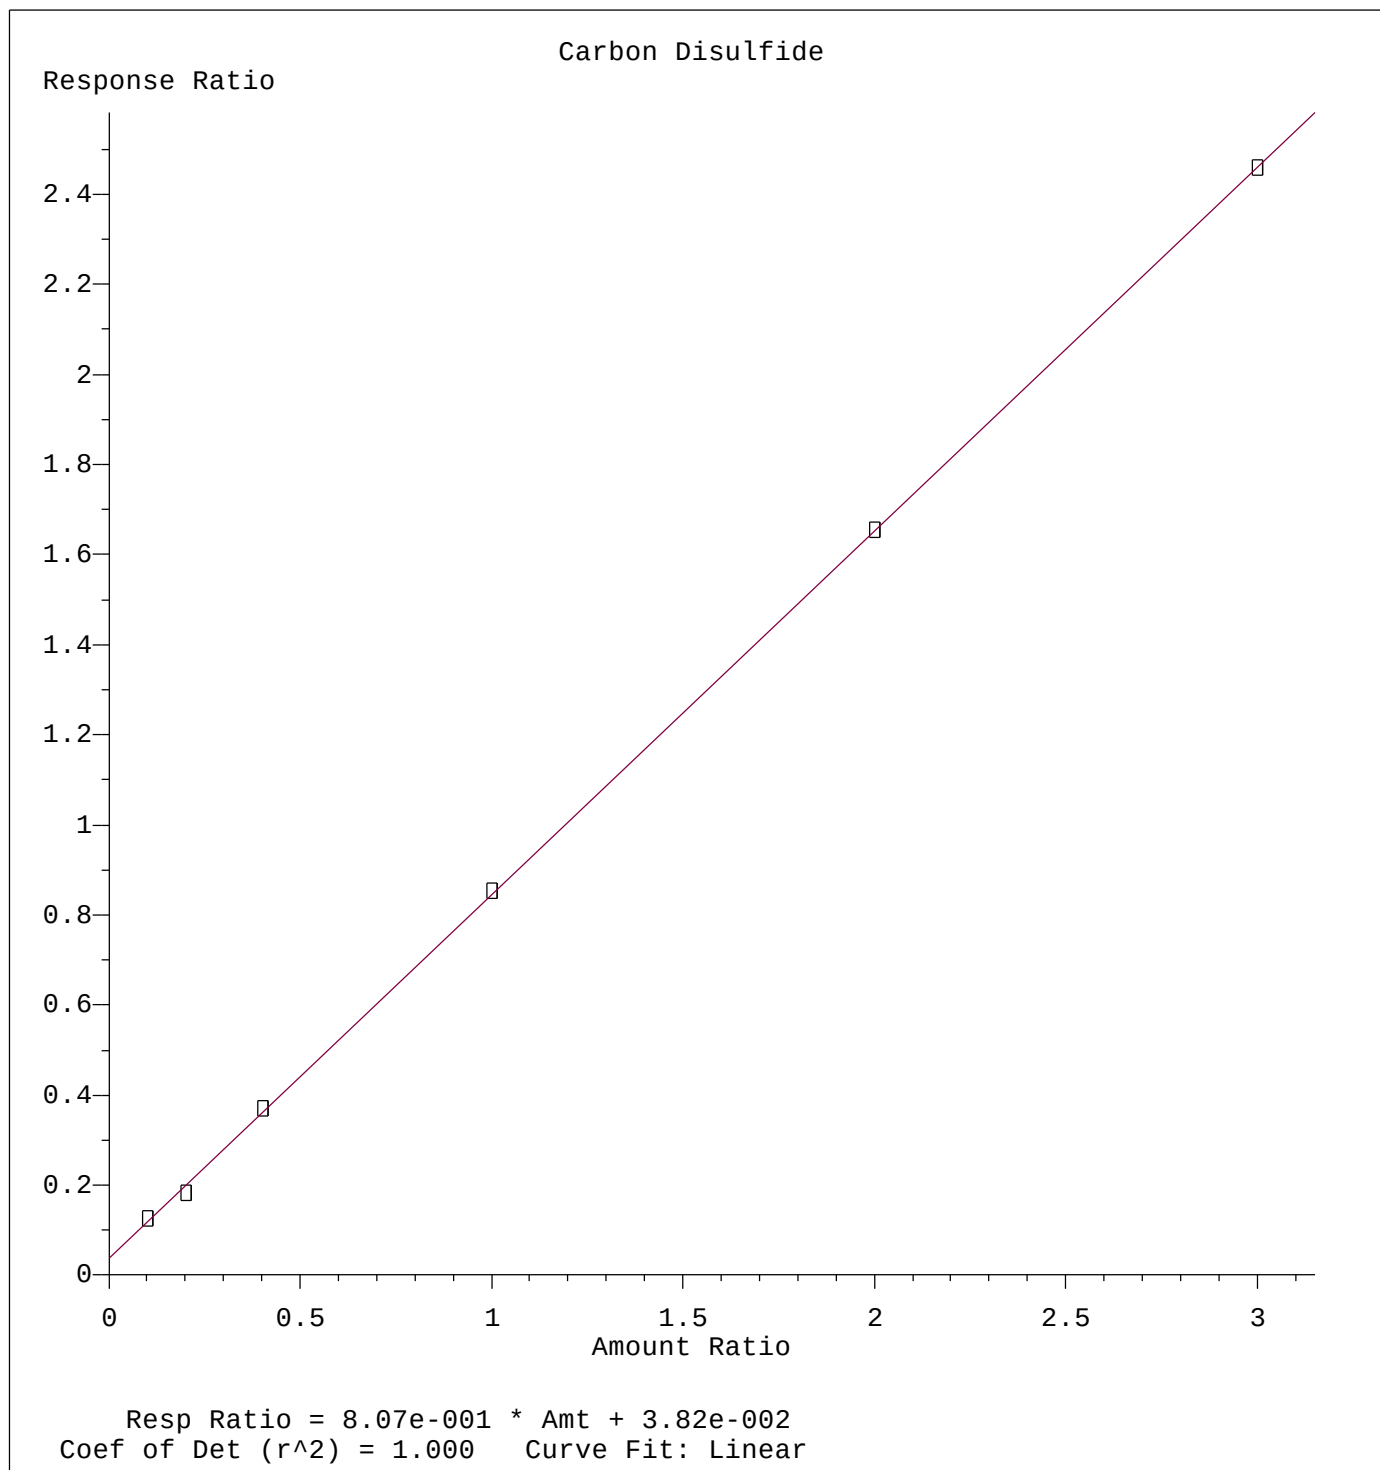


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y091219S.M
Calibration Table Last Updated: Thu Sep 12 16:17:30 2019

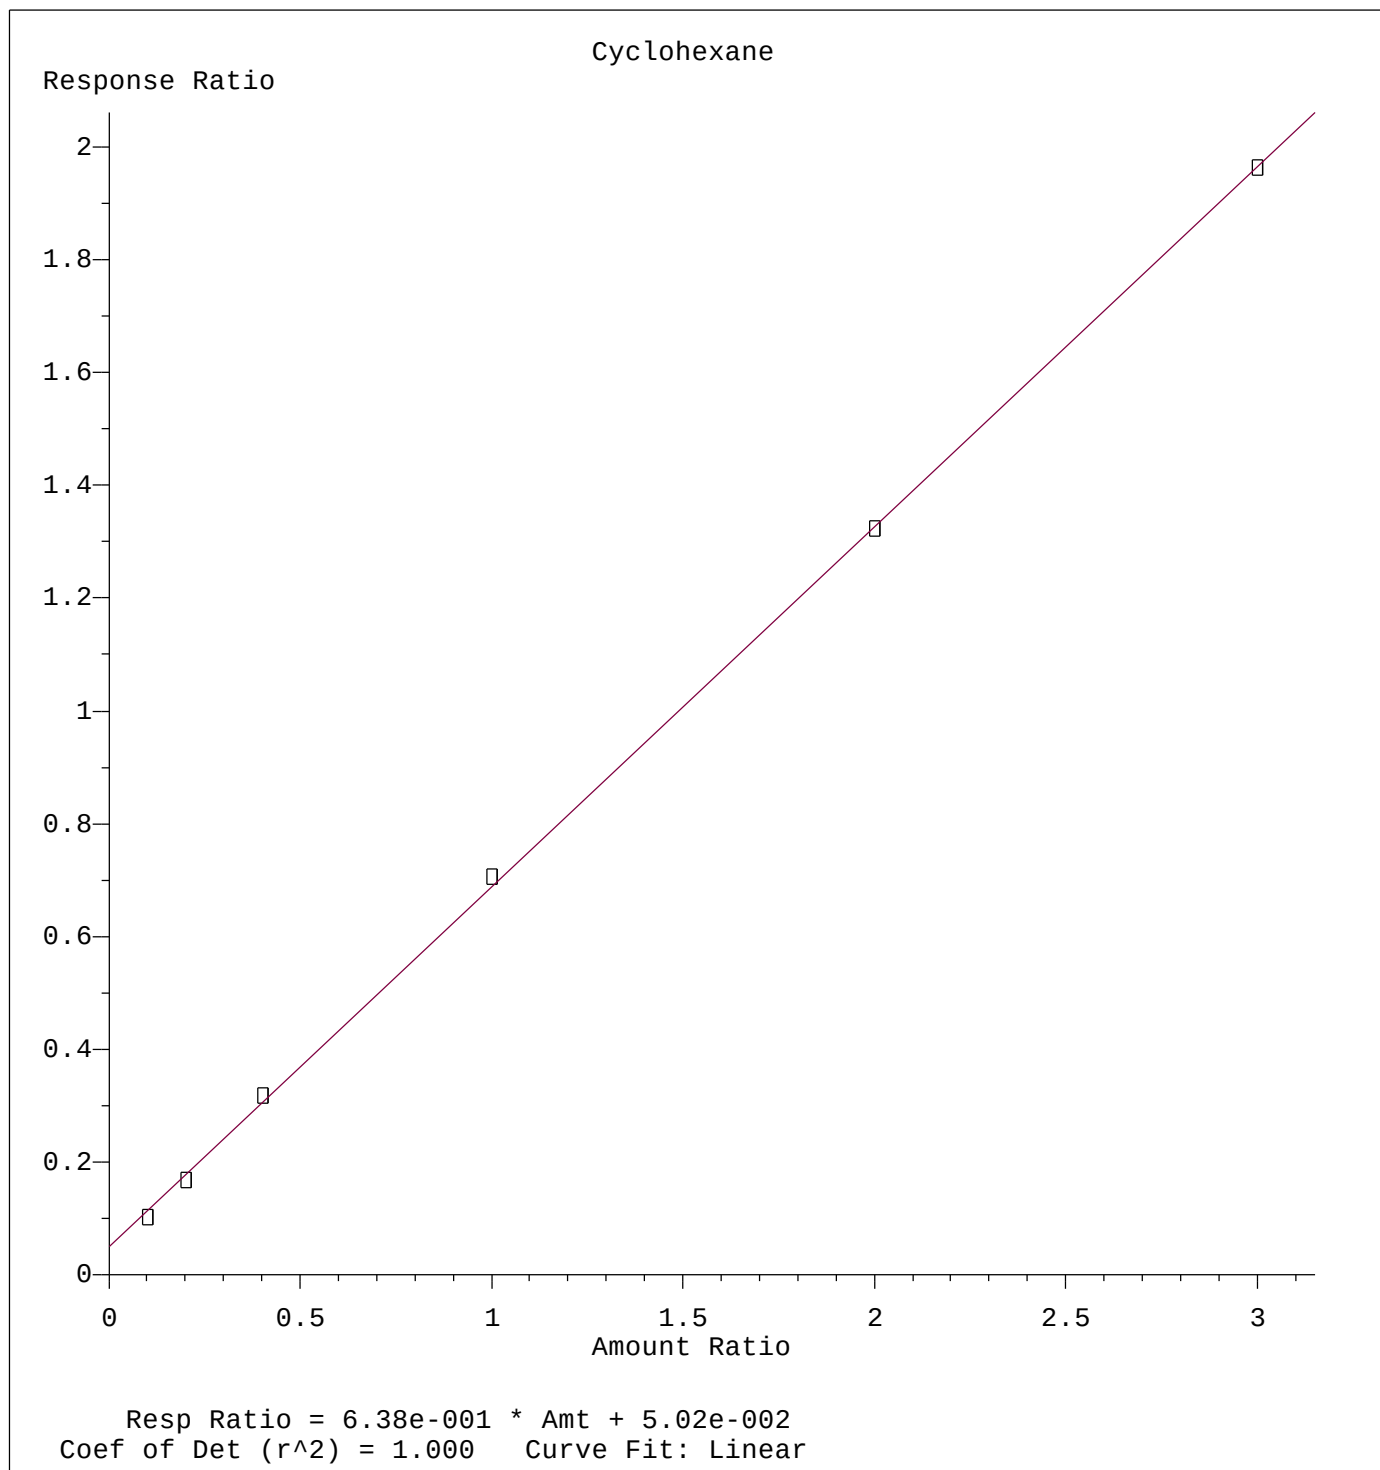


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y091219S.M
Calibration Table Last Updated: Thu Sep 12 16:17:30 2019

1,2-Dibromo-3-Chloropropane

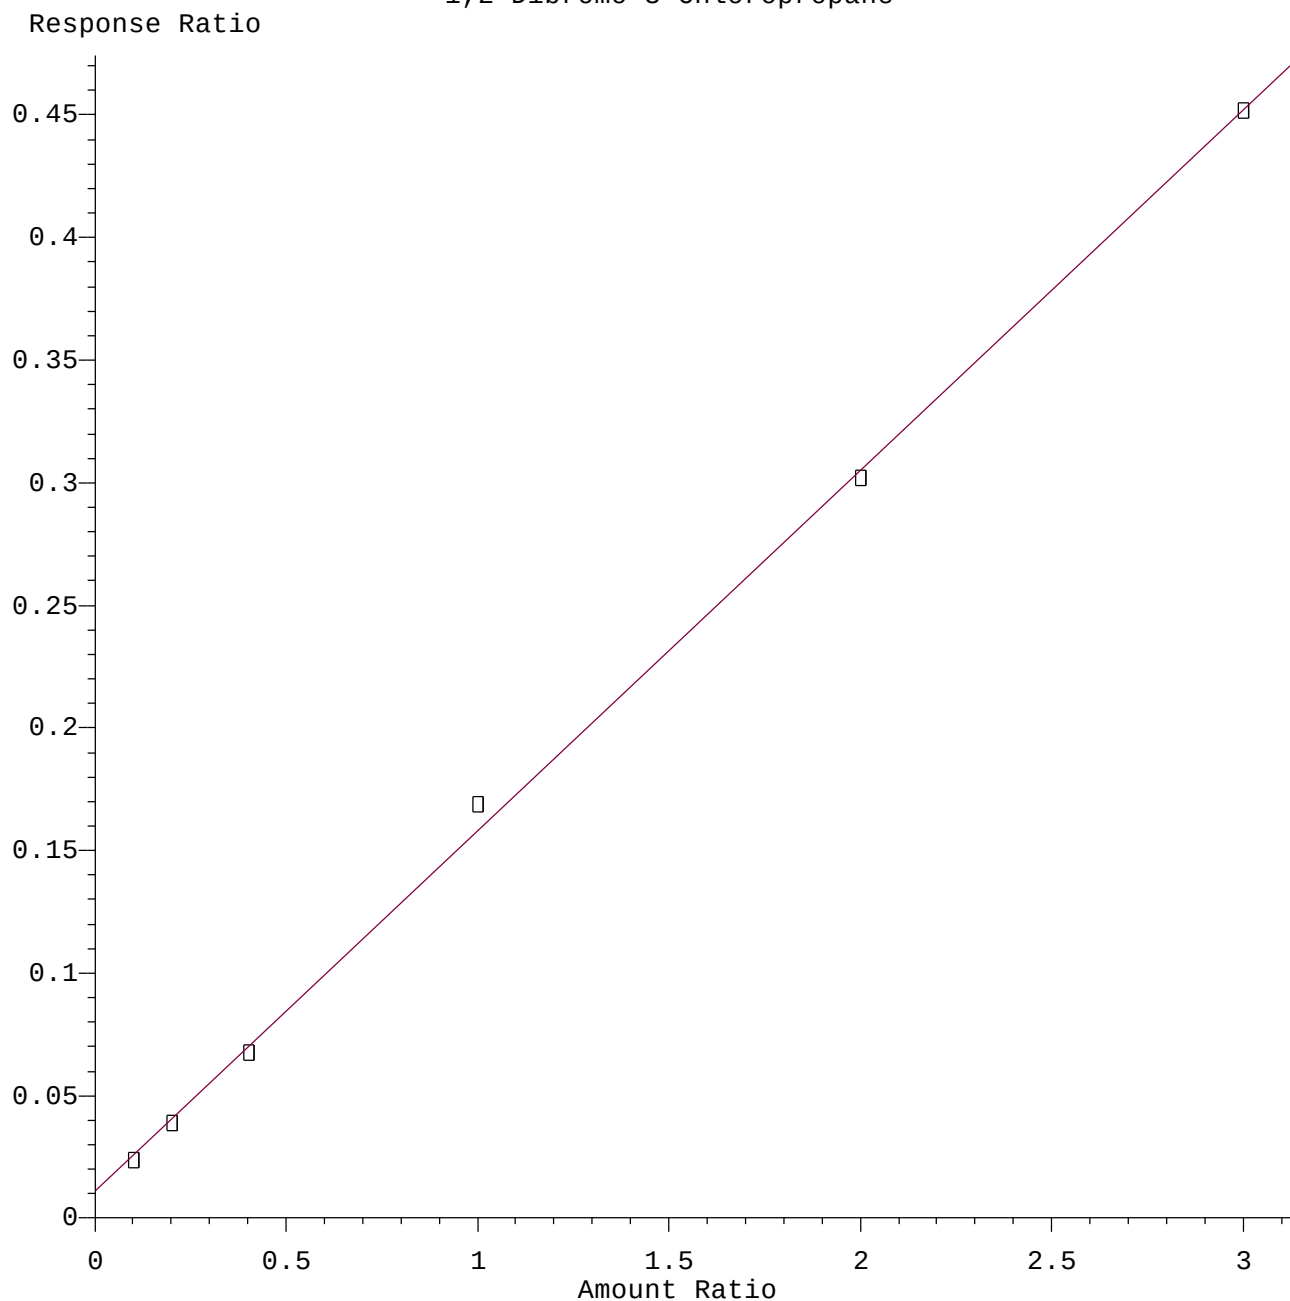

Resp Ratio = $1.47 \times 10^{-1} \times \text{Amt} + 1.10 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y091219S.M
Calibration Table Last Updated: Thu Sep 12 16:17:30 2019

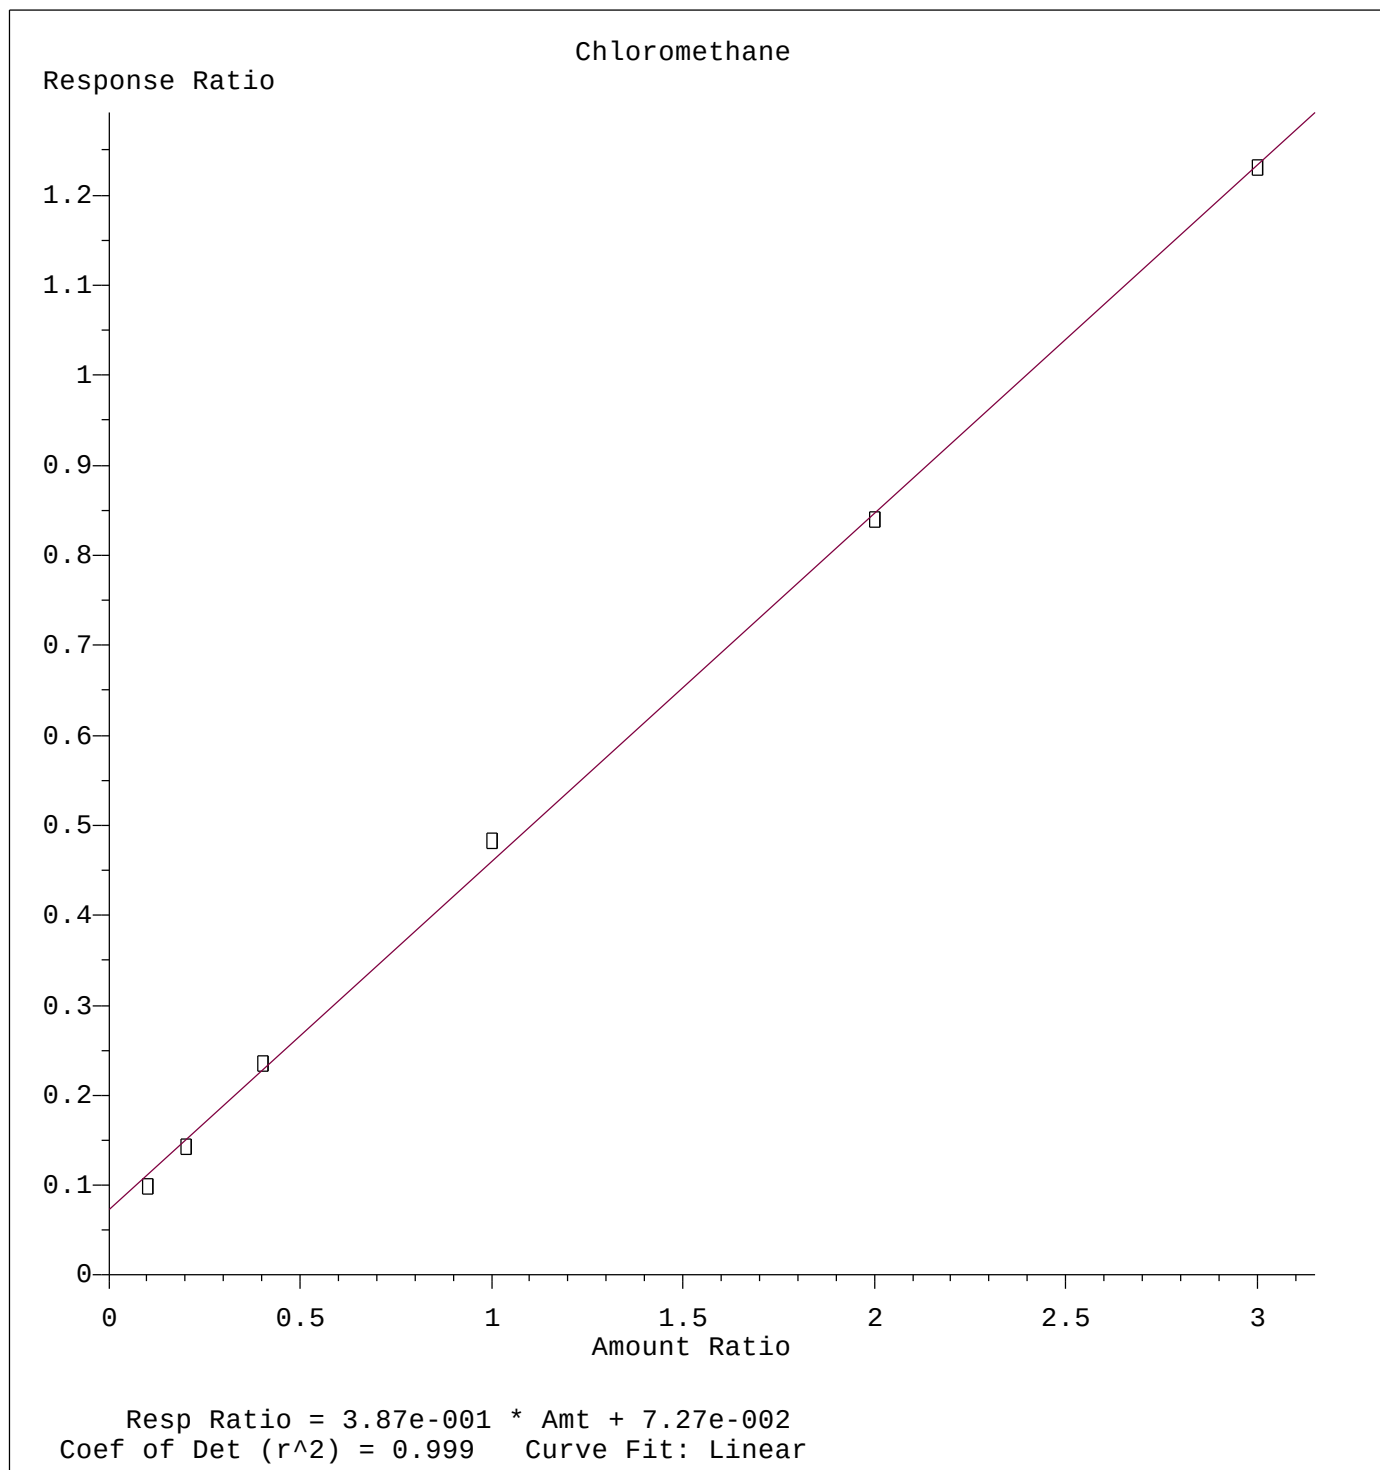

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y091219S.M
Calibration Table Last Updated: Thu Sep 12 16:17:30 2019