


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\vv091219\
Data File : VY000016.D
Acq On : 12 Sep 2019 09:18
Operator : SY/MD
Sample : BFB
Misc : 5.00µl/5.00ml
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y091219S.M
Title : SW846 8260
Last Update : Thu Sep 12 16:17:30 2019

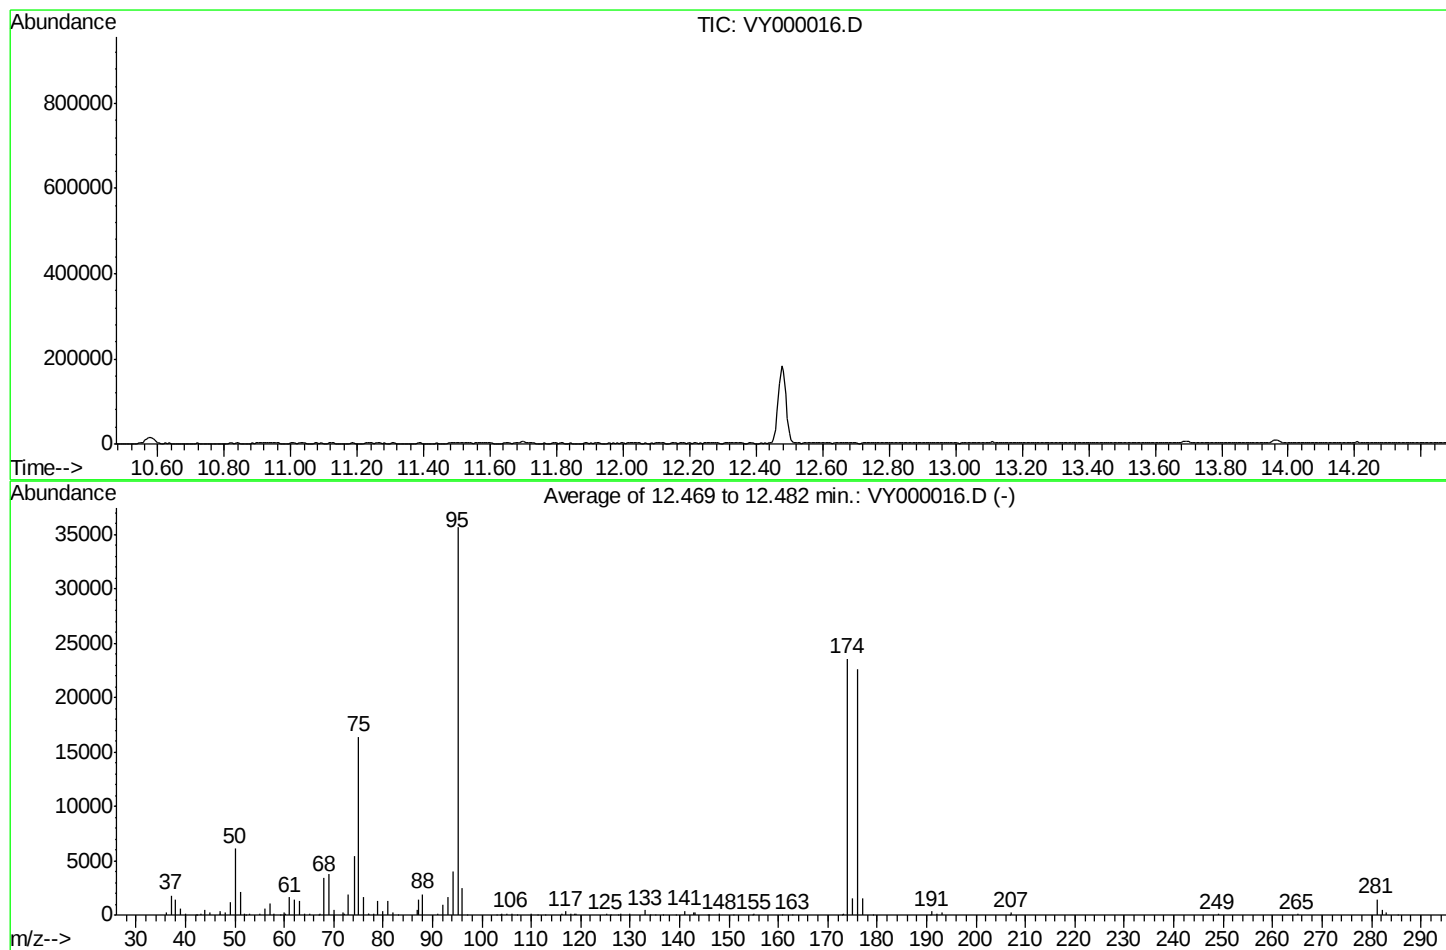

AutoFind: Scans 1785, 1786, 1787; Background Corrected with Scan 1778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	6117	PASS
75	95	30	60	46.0	16404	PASS
95	95	100	100	100.0	35669	PASS
96	95	5	9	7.1	2519	PASS
173	174	0.00	2	0.4	90	PASS
174	95	50	100	66.1	23570	PASS
175	174	5	9	6.7	1587	PASS
176	174	95	101	96.0	22618	PASS
177	176	5	9	6.8	1543	PASS