

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091223\
 Data File : VY015526.D
 Acq On : 12 Sep 2023 22:32
 Operator : SY/MD
 Sample : 04396-01
 Misc : 5.05g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 CHRT-24313

Quant Time: Sep 13 05:59:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y082923S.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 31 20:01:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	275561	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	445716	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	391173	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	174393	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.142	65	162693	55.076	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	110.160%
35) Dibromofluoromethane	7.716	113	139693	54.414	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	108.820%
50) Toluene-d8	10.179	98	524482	56.415	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	112.820%
62) 4-Bromofluorobenzene	12.483	95	164677	47.714	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	95.420%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091223\
Data File : VY015526.D
Acq On : 12 Sep 2023 22:32
Operator : SY/MD
Sample : 04396-01
Misc : 5.05g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
CHRT-24313

Quant Time: Sep 13 05:59:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y082923S.M
Quant Title : SW846 8260
QLast Update : Thu Aug 31 20:01:47 2023
Response via : Initial Calibration




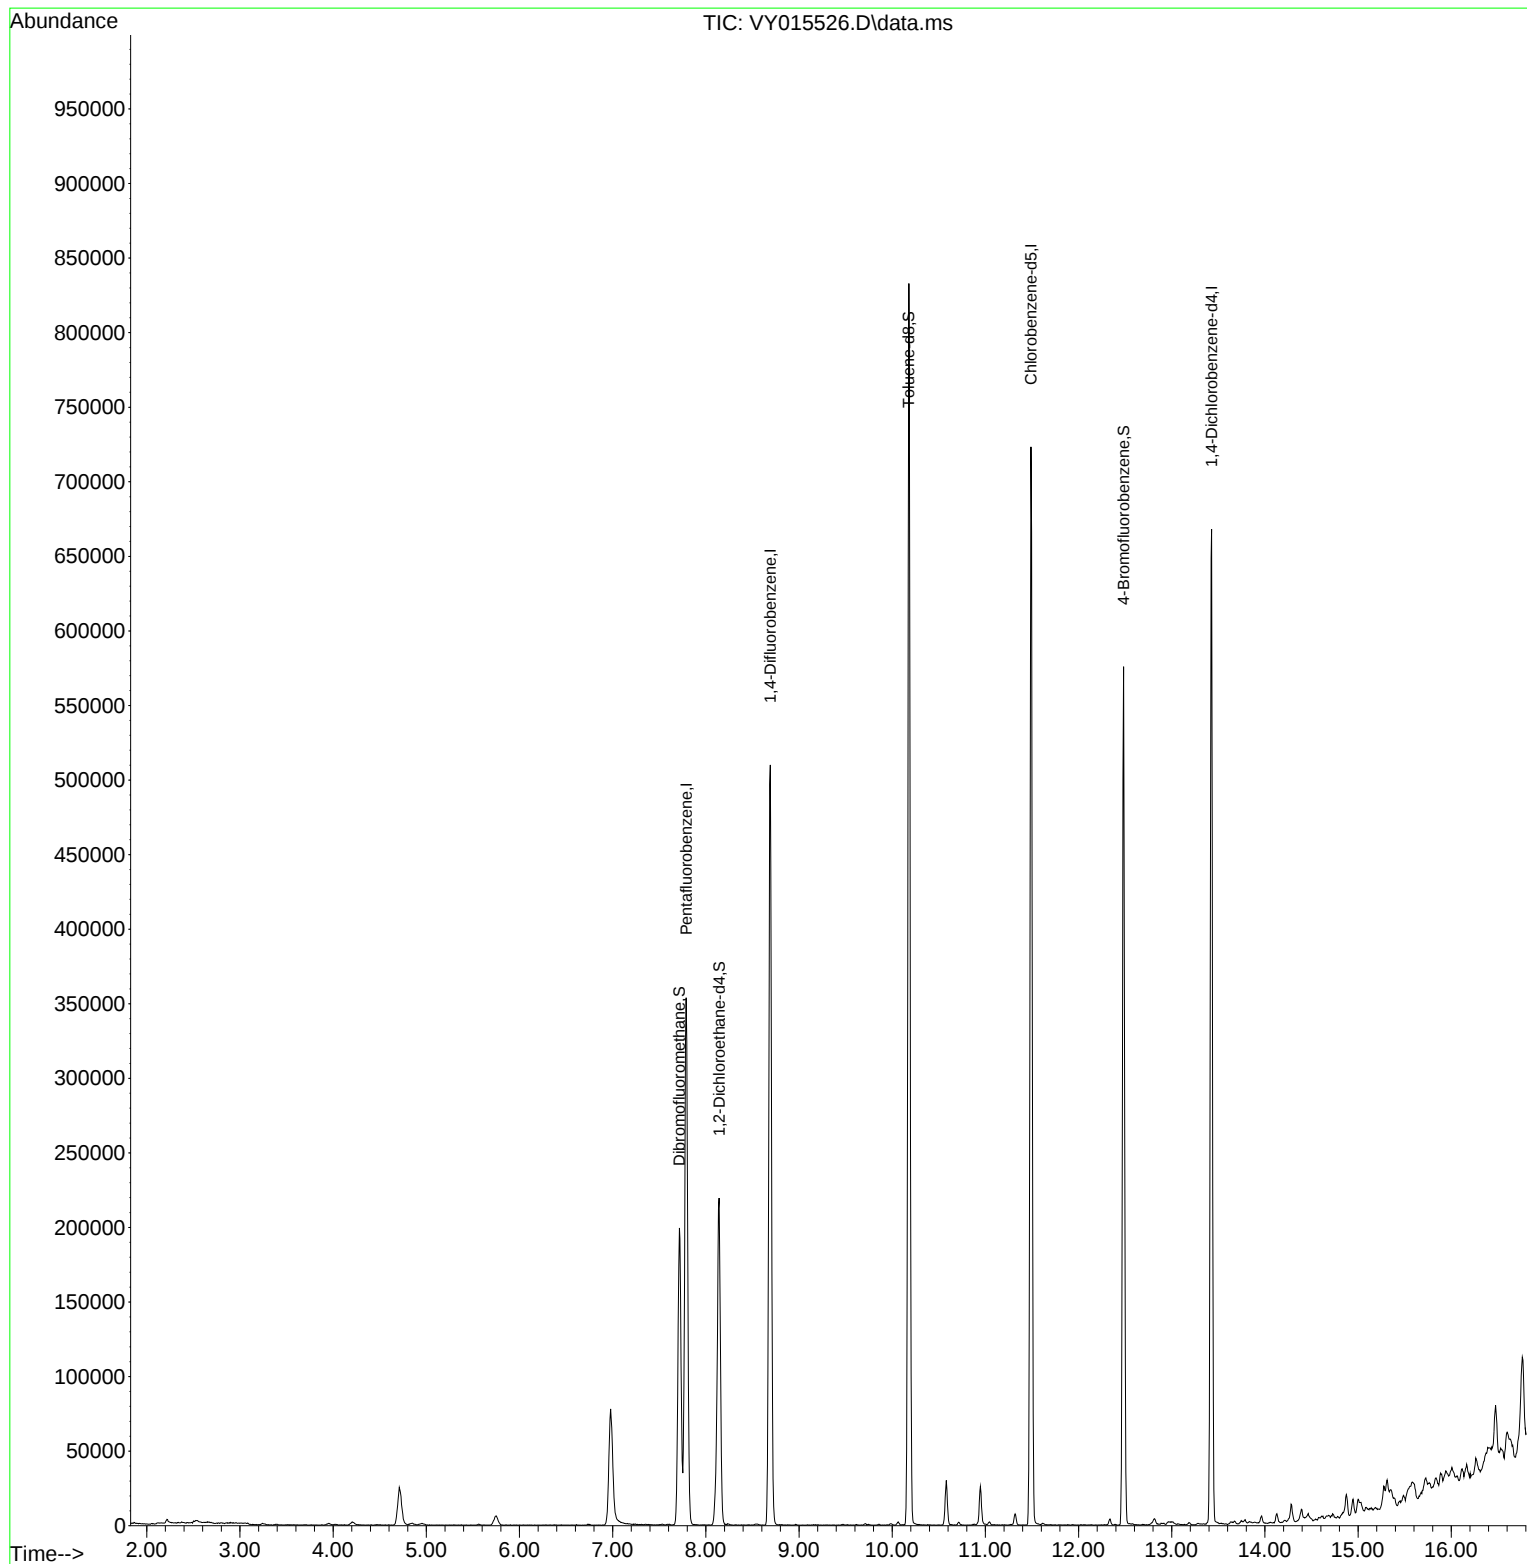


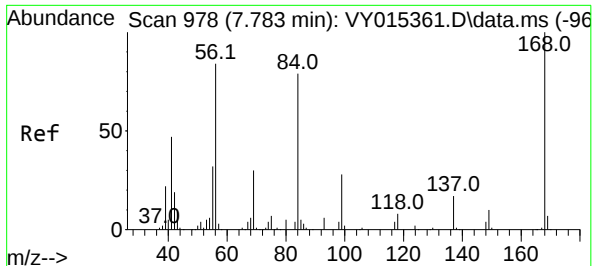

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY015526.D
Acq: 12 Sep 2023 22:32




Instrument :
MSVOA_Y
ClientSampleId :
CHRT-24313

Tgt Ion:168 Resp: 275561
Ion Ratio Lower Upper
168 100
99 55.2 43.4 65.0

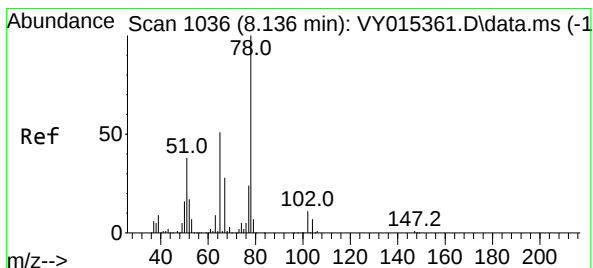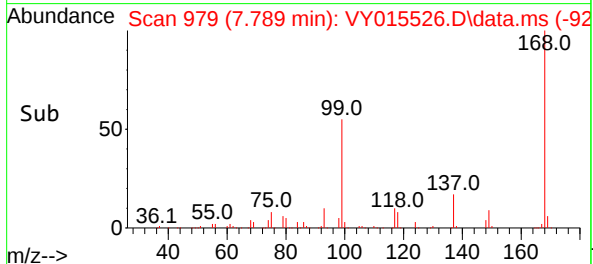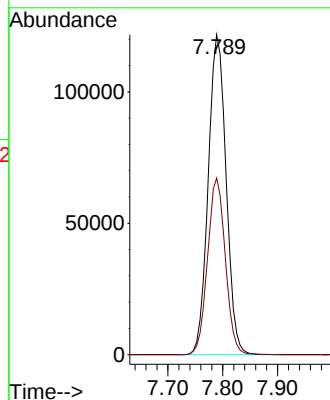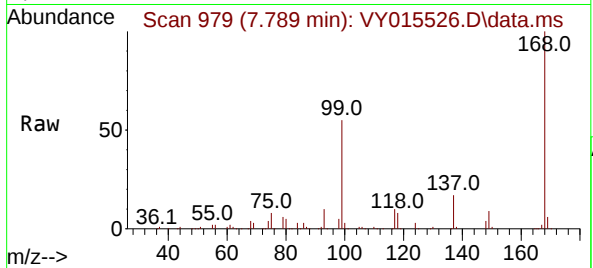

#33
1,2-Dichloroethane-d4
Concen: 55.076 ug/l
RT: 8.142 min Scan# 1037
Delta R.T. 0.006 min
Lab File: VY015526.D
Acq: 12 Sep 2023 22:32

Tgt Ion: 65 Resp: 162693
Ion Ratio Lower Upper
65 100
67 52.7 0.0 101.8

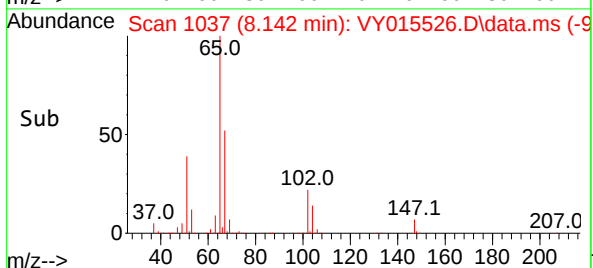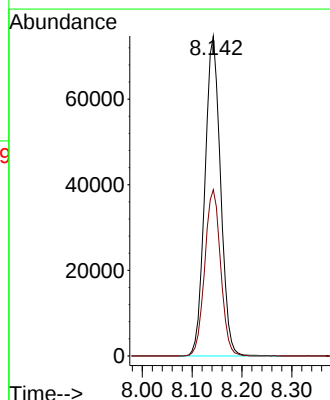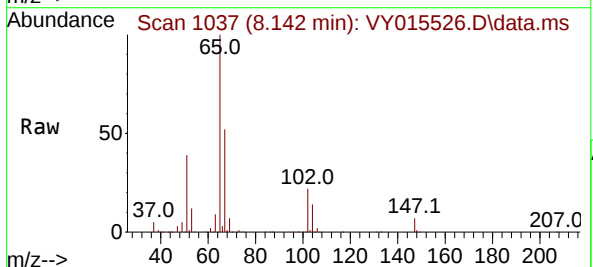



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VY015526.D

Acq: 12 Sep 2023 22:32

Instrument :

MSVOA_Y

ClientSampleId :

CHRT-24313





Tgt Ion:114 Resp: 445716

Ion Ratio Lower Upper

114 100

63 19.4 0.0 42.4

88 15.7 0.0 30.6

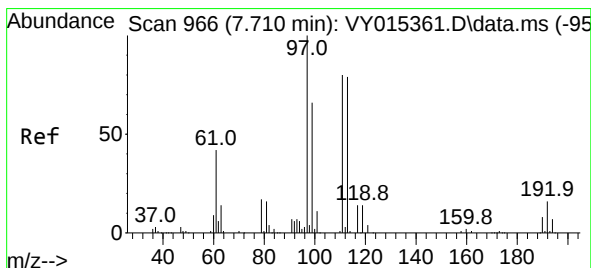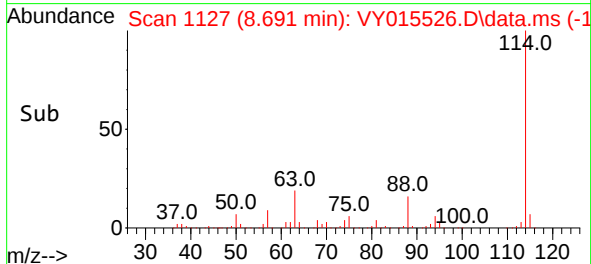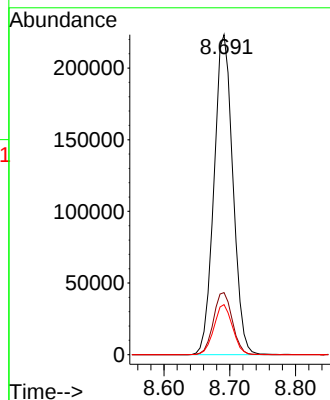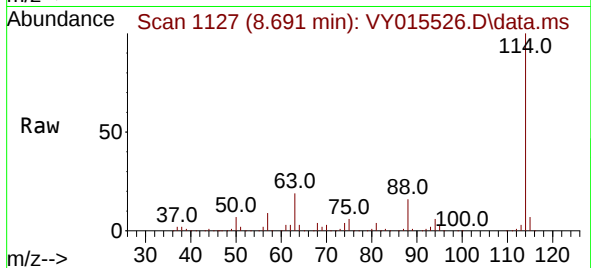

#35

Dibromofluoromethane

Concen: 54.414 ug/l

RT: 7.716 min Scan# 967

Delta R.T. 0.000 min

Lab File: VY015526.D

Acq: 12 Sep 2023 22:32




Tgt Ion:113 Resp: 139693

Ion Ratio Lower Upper

113 100

111 101.7 81.3 121.9

192 19.7 16.9 25.3

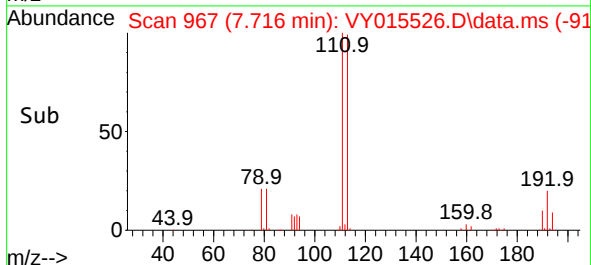
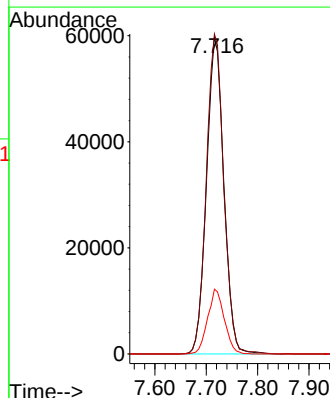
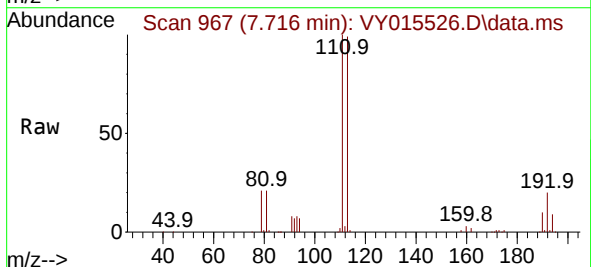




#50
Toluene-d8
Concen: 56.415 ug/l
RT: 10.179 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY015526.D
Acq: 12 Sep 2023 22:32




Instrument :
MSVOA_Y
ClientSampleId :
CHRT-24313


Tgt Ion: 98 Resp: 524482
Ion Ratio Lower Upper
98 100
100 64.9 50.1 75.1

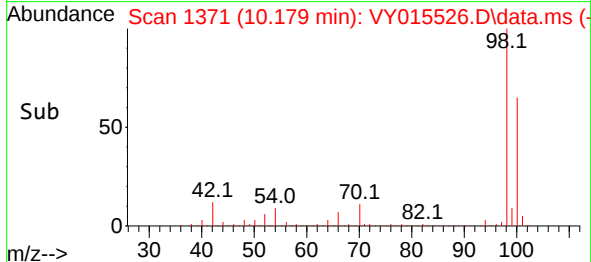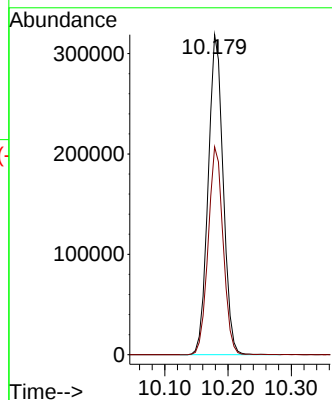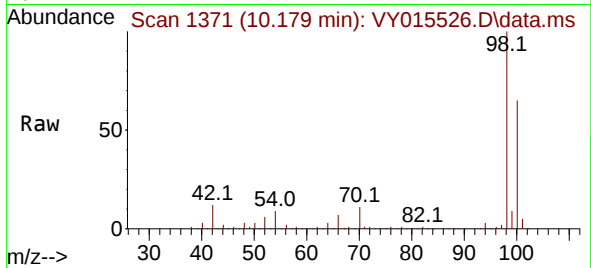

#62
4-Bromofluorobenzene
Concen: 47.714 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.006 min
Lab File: VY015526.D
Acq: 12 Sep 2023 22:32

Tgt Ion: 95 Resp: 164677
Ion Ratio Lower Upper
95 100
174 87.0 0.0 178.2
176 83.5 0.0 173.8

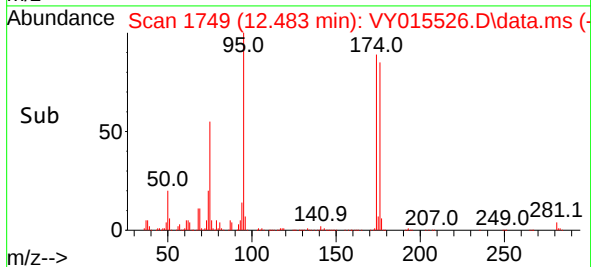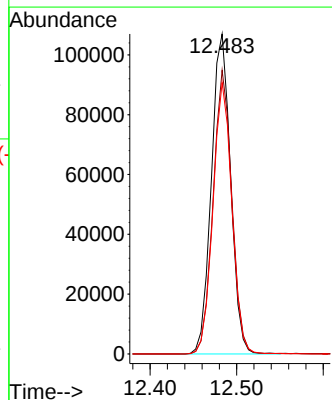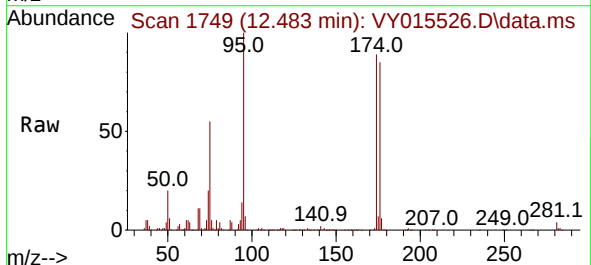

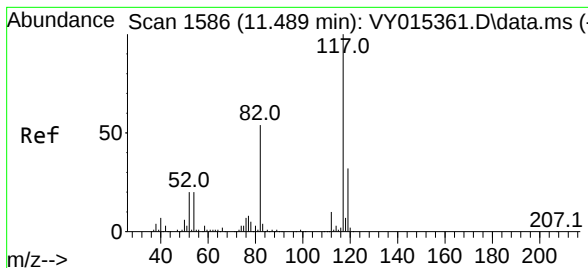

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.489 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY015526.D

Acq: 12 Sep 2023 22:32

Instrument :

MSVOA_Y

ClientSampleId :

CHRT-24313





Tgt Ion:117 Resp: 391173

Ion Ratio Lower Upper

117 100

82 55.4 43.4 65.0

119 32.5 26.3 39.5

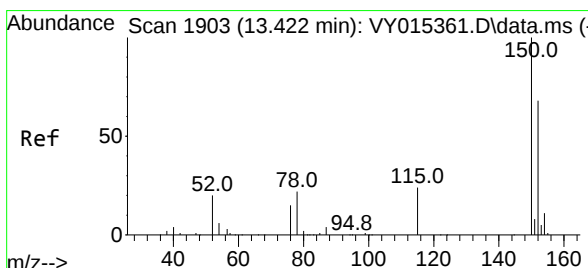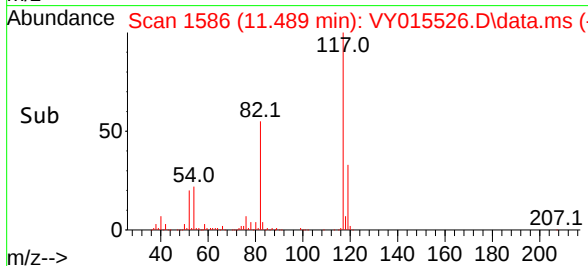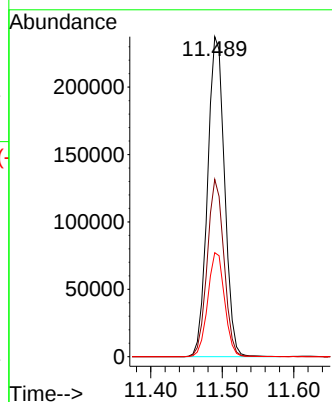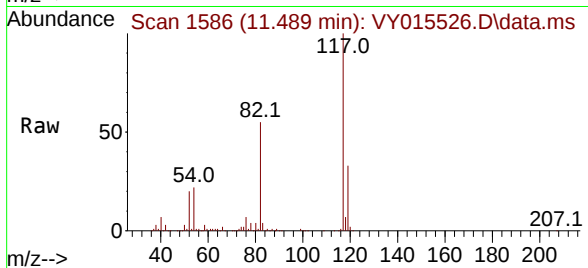

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.006 min

Lab File: VY015526.D

Acq: 12 Sep 2023 22:32

Tgt Ion:152 Resp: 174393

Ion Ratio Lower Upper

152 100

115 57.3 28.8 86.5

150 156.2 0.0 348.8

