
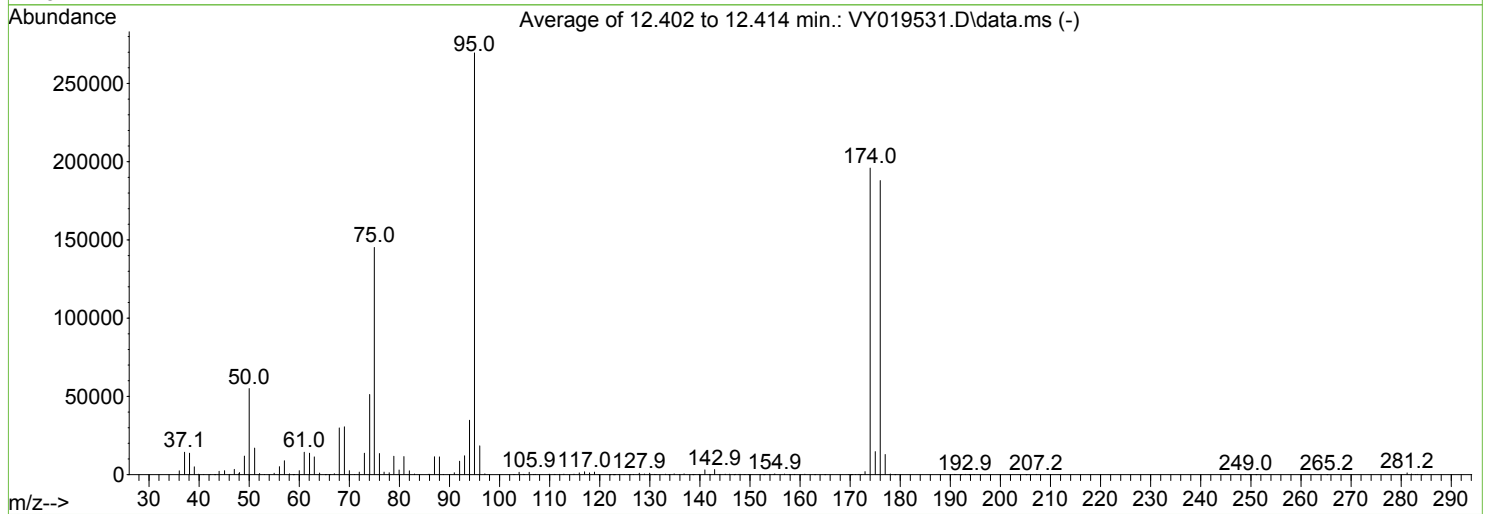


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091324\
Data File : VY019531.D
Acq On : 13 Sep 2024 08:49
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090924S.M
Title : SW846 8260
Last Update : Mon Sep 09 16:00:30 2024

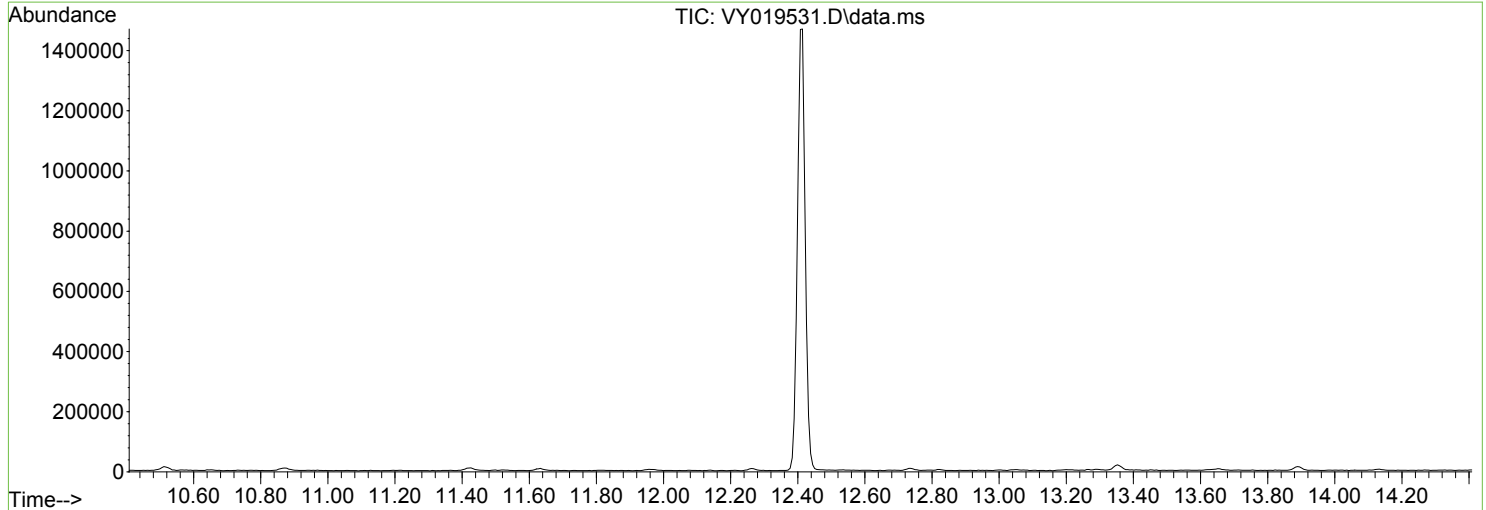

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1742

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	55041	PASS
75	95	30	60	53.9	145216	PASS
95	95	100	100	100.0	269568	PASS
96	95	5	9	6.8	18385	PASS
173	174	0.00	2	1.0	1935	PASS
174	95	50	100	72.7	195947	PASS
175	174	5	9	7.5	14724	PASS
176	174	95	101	95.9	187904	PASS
177	176	5	9	6.9	12897	PASS