

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091423\
 Data File : VY015549.D
 Acq On : 14 Sep 2023 21:24
 Operator : SY/MD
 Sample : 04409-06
 Misc : 3.53g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-2(0-2)GRAB

Quant Time: Sep 15 04:07:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y082923S.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 31 20:01:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	0.000	168	0	0.000	ug/l	-7.78
34) 1,4-Difluorobenzene	0.000	114	0	0.000	ug/l	-8.69
63) Chlorobenzene-d5	0.000	117	0	0.000	ug/l	-11.49
72) 1,4-Dichlorobenzene-d4	0.000	152	0	0.000	ug/l	-13.42
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	0.000	65	0	0.000	ug/l	
Spiked Amount	50.000	Range	50 - 163	Recovery	=	0.000%#
35) Dibromofluoromethane	0.000	113	0	0.000	ug/l	
Spiked Amount	50.000	Range	54 - 147	Recovery	=	0.000%#
50) Toluene-d8	0.000	98	0	0.000	ug/l	
Spiked Amount	50.000	Range	58 - 134	Recovery	=	0.000%#
62) 4-Bromofluorobenzene	12.282	95	23	0.000	ug/l	-0.20
Spiked Amount	50.000	Range	30 - 143	Recovery	=	0.000%#


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091423\
Data File : VY015549.D
Acq On : 14 Sep 2023 21:24
Operator : SY/MD
Sample : 04409-06
Misc : 3.53g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
WC-2(0-2)GRAB

Quant Time: Sep 15 04:07:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y082923S.M
Quant Title : SW846 8260
QLast Update : Thu Aug 31 20:01:47 2023
Response via : Initial Calibration

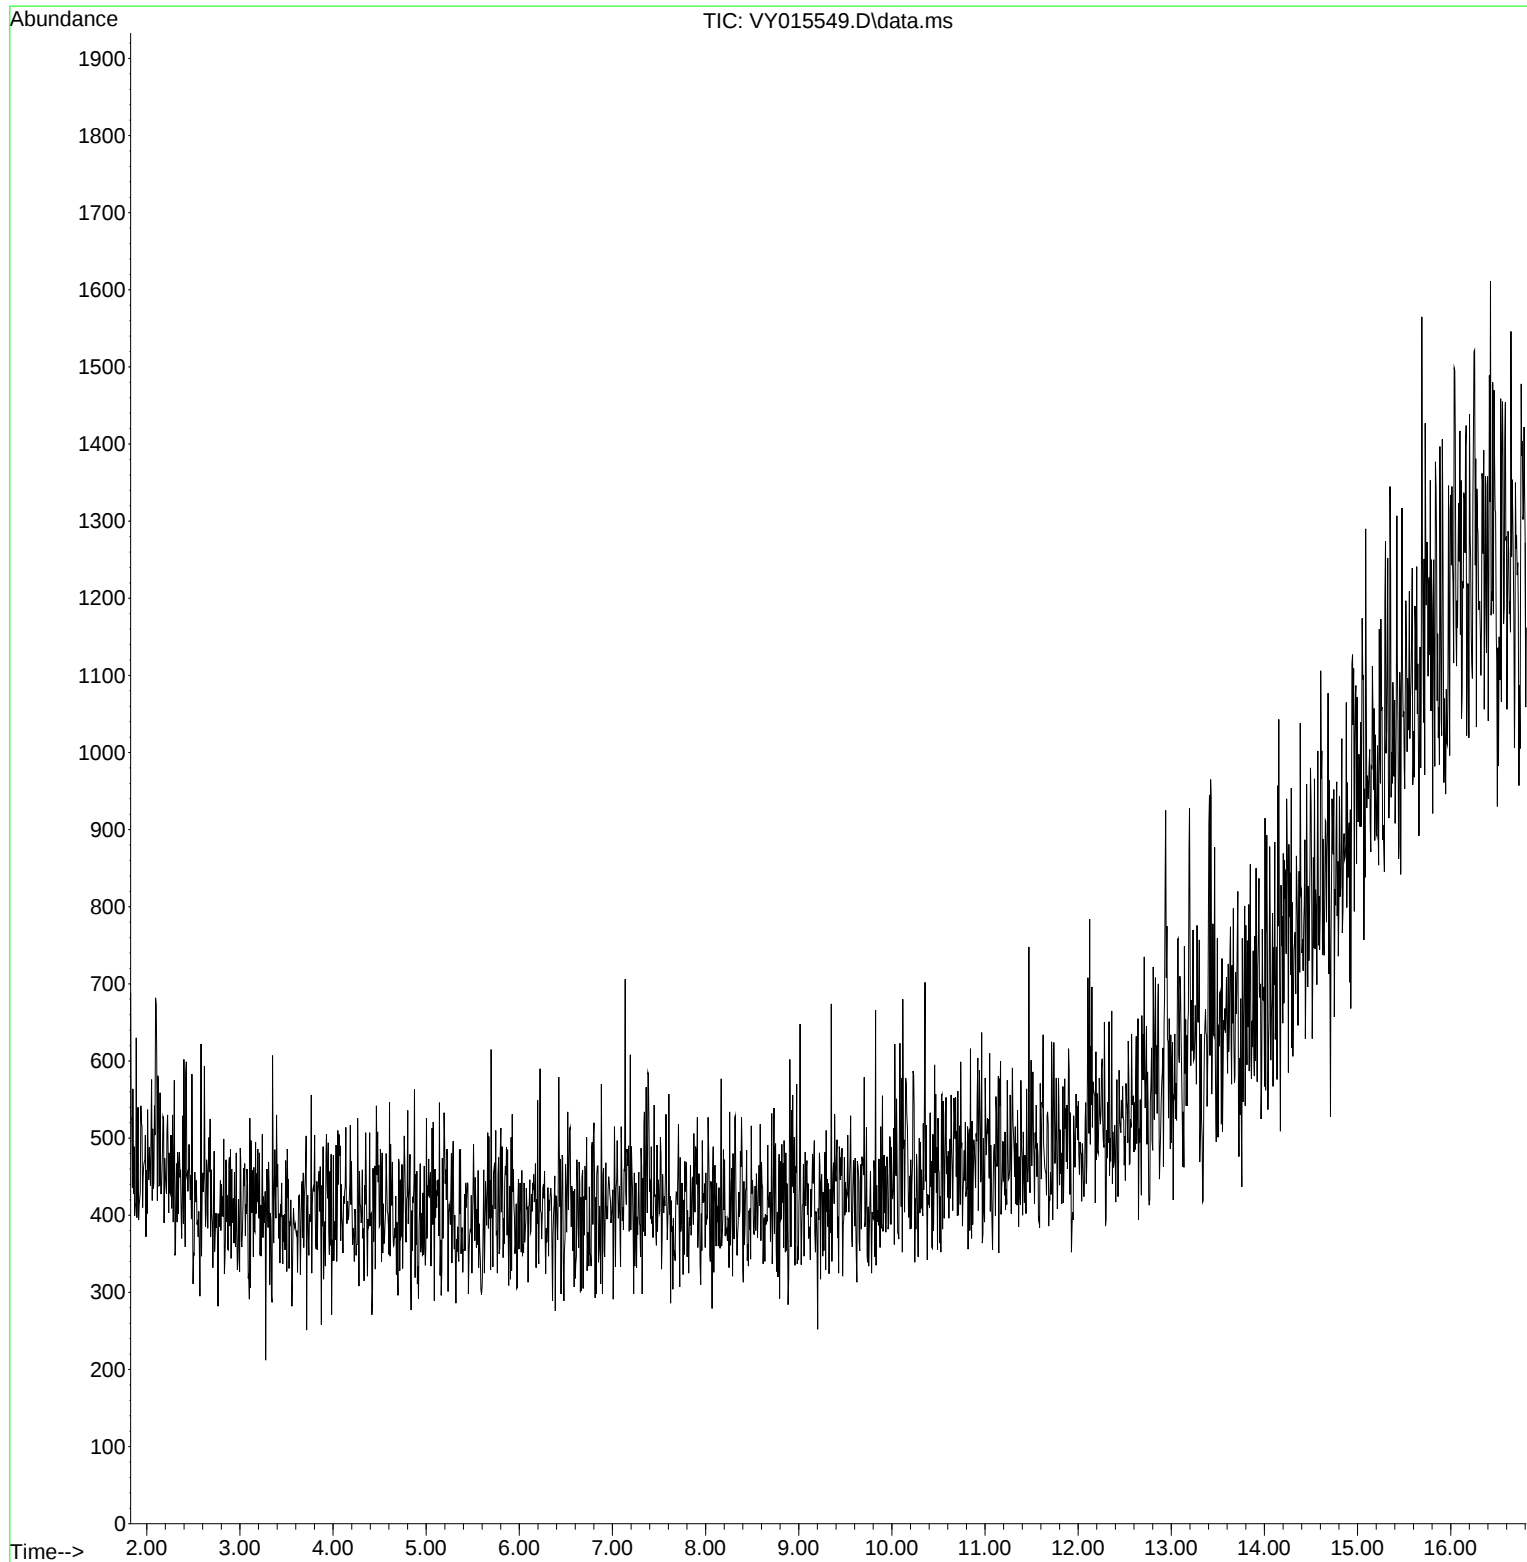


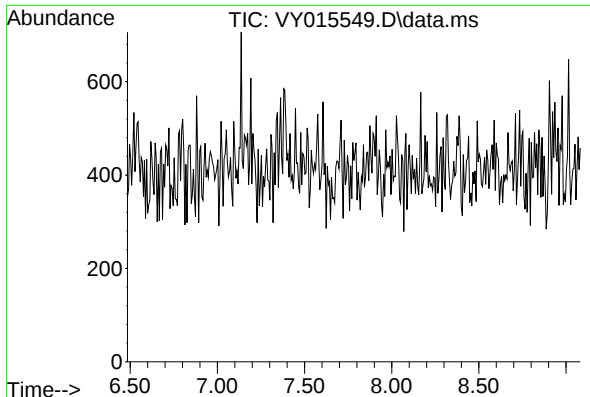


#1
Pentafluorobenzene
Concen: 0.000 ug/l
Expected RT: 7.78 min

Lab File: VY015549.D
Acq: 14 Sep 2023 21:24

Instrument :
MSVOA_Y
ClientSampleId :
WC-2(0-2)GRAB


Tgt Ion: 168
Sig Exp Ratio
168 100
99 54.2

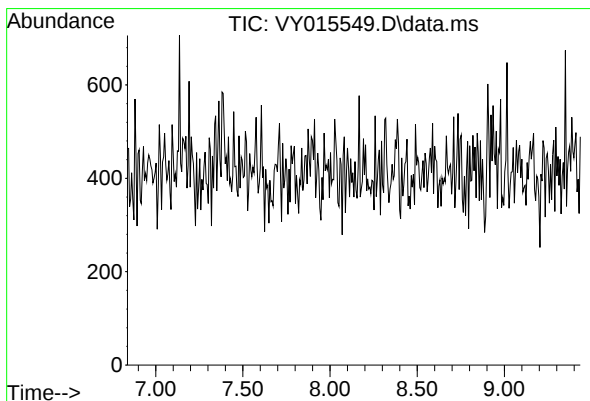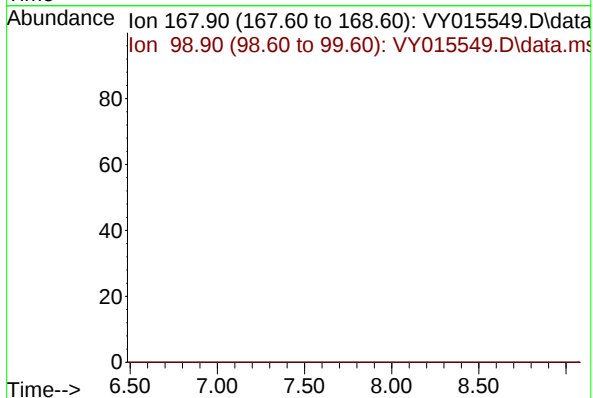


#33
1,2-Dichloroethane-d4
Concen: 0.000 ug/l
Expected RT: 8.14 min

Lab File: VY015549.D
Acq: 14 Sep 2023 21:24

Tgt Ion: 65
Sig Exp Ratio
65 100
67 50.9

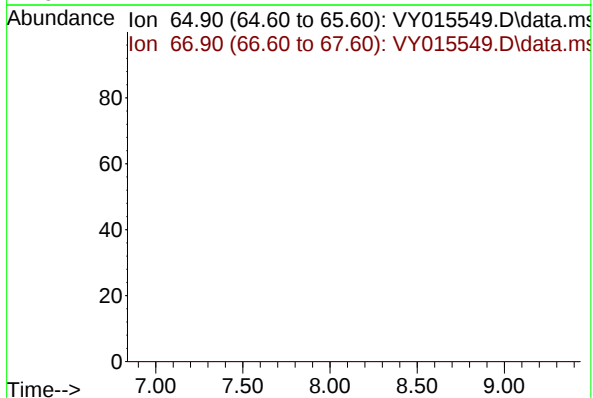


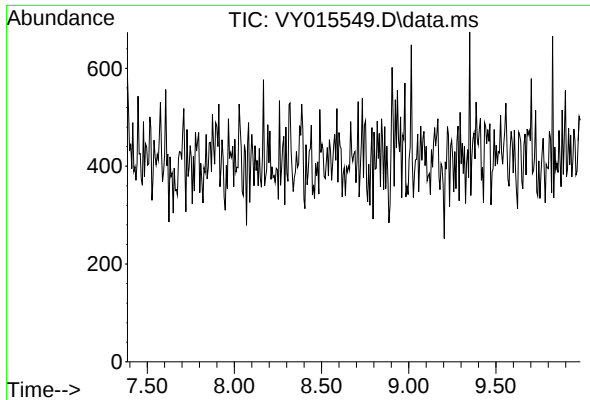


#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 8.69 min

Lab File: VY015549.D
 Acq: 14 Sep 2023 21:24

Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-2(0-2)GRAB


Tgt Ion: 114
 Sig Exp Ratio
 114 100
 63 21.2
 88 15.3

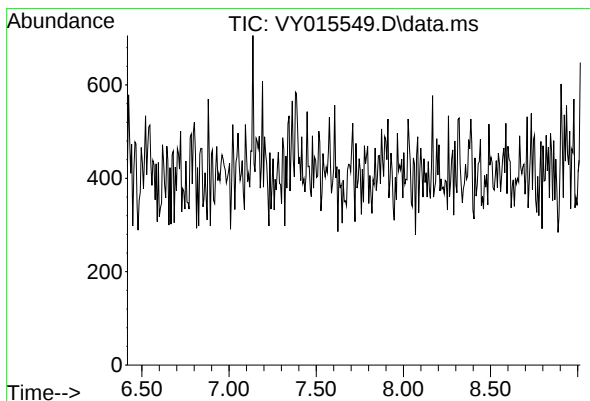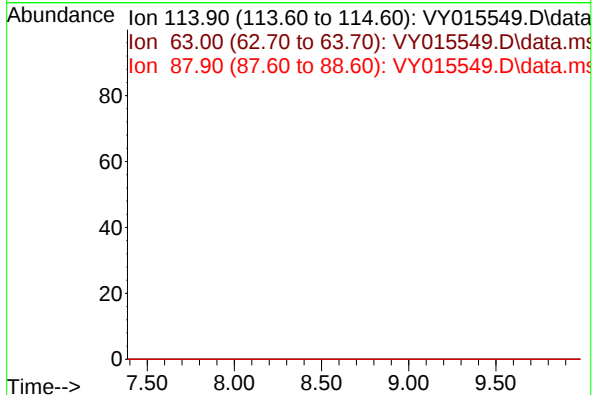


#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 7.72 min

Lab File: VY015549.D
 Acq: 14 Sep 2023 21:24

Tgt Ion: 113
 Sig Exp Ratio
 113 100
 111 101.6
 192 21.1


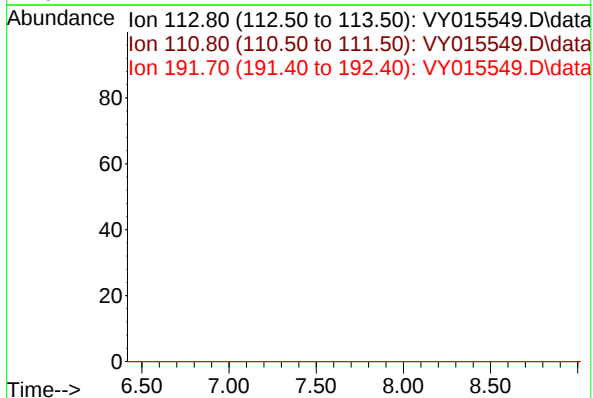


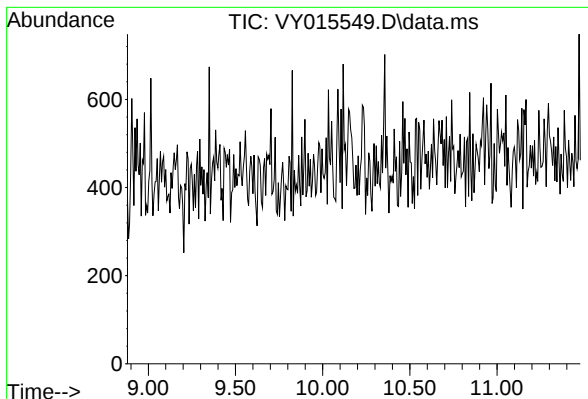

#50
 Toluene-d8
 Concen: 0.000 ug/l
 Expected RT: 10.18 min
 Lab File: VY015549.D
 Acq: 14 Sep 2023 21:24




Tgt Ion	Sig	Exp Ratio
98	98	100
100	100	62.6


Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-2(0-2)GRAB

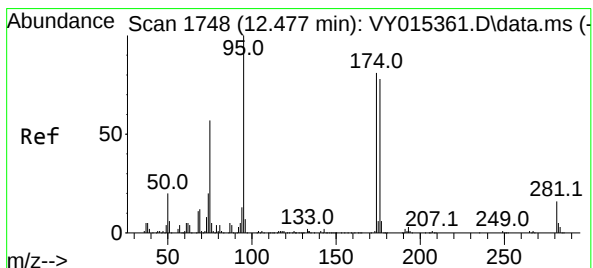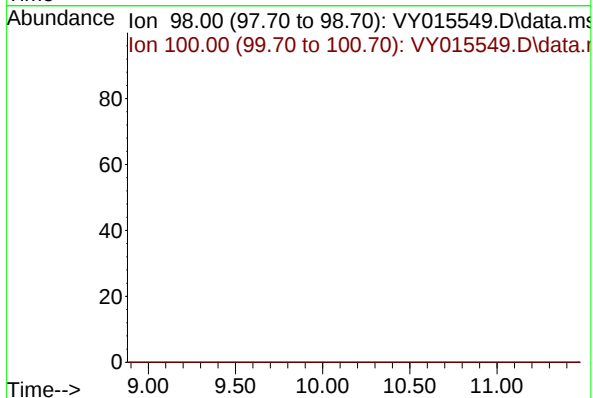

#62
 4-Bromofluorobenzene
 Concen: 0.000 ug/l
 RT: 12.282 min Scan# 1716
 Delta R.T. -0.195 min
 Lab File: VY015549.D
 Acq: 14 Sep 2023 21:24

Tgt Ion	Ratio	Lower	Upper
95	100		
174	0.0	0.0	178.2
176	0.0	0.0	173.8

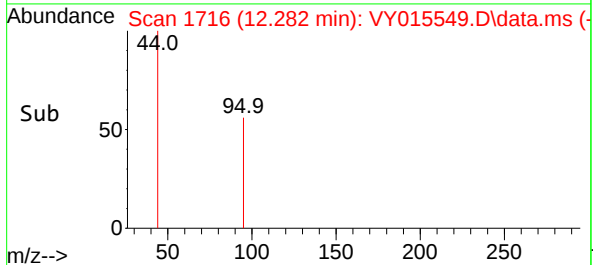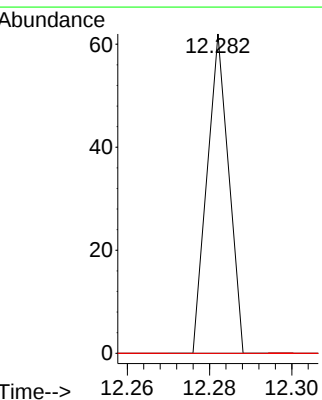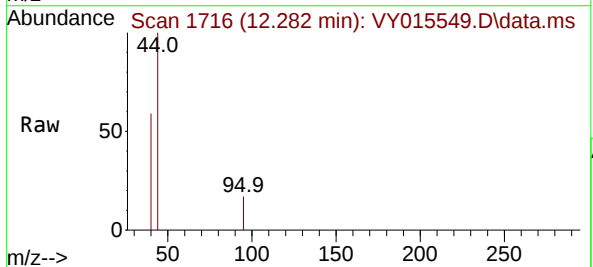


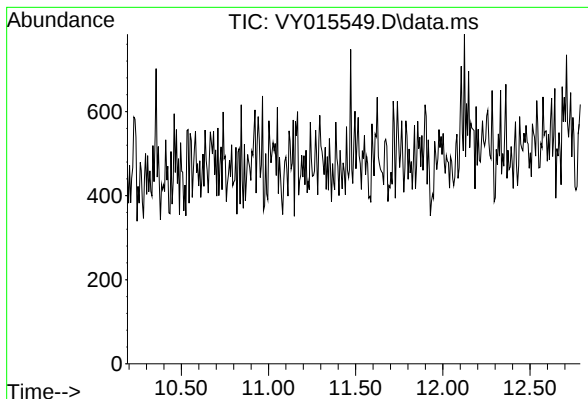


#63
Chlorobenzene-d5
Concen: 0.000 ug/l
Expected RT: 11.49 min

Lab File: VY015549.D
Acq: 14 Sep 2023 21:24

Instrument :
MSVOA_Y
ClientSampleId :
WC-2(0-2)GRAB

Tgt Ion: 117
Sig Exp Ratio
117 100
82 54.2
119 32.9

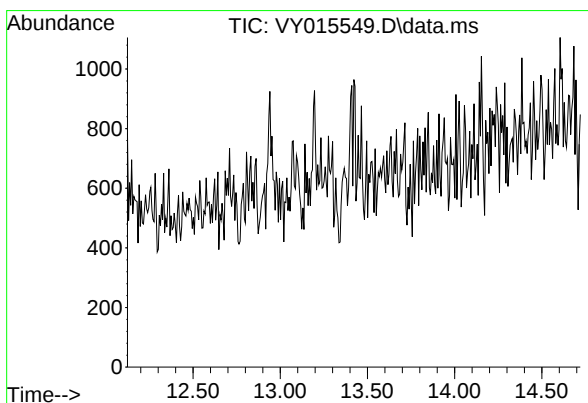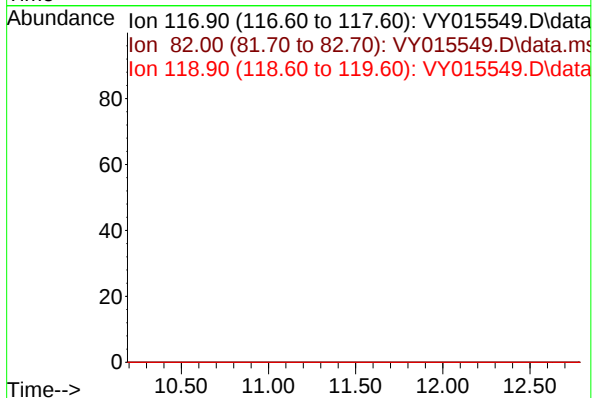

#72
1,4-Dichlorobenzene-d4
Concen: 0.000 ug/l
Expected RT: 13.42 min

Lab File: VY015549.D
Acq: 14 Sep 2023 21:24

Tgt Ion: 152
Sig Exp Ratio
152 100
115 57.7
150 174.4

