

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091523\
 Data File : VY015595.D
 Acq On : 16 Sep 2023 02:23
 Operator : SY/MD
 Sample : 04419-07
 Misc : 5.50g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :

Quant Time: Sep 16 05:28:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y082923S.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 31 20:01:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.801	168	249598	50.000	ug/l	0.02
34) 1,4-Difluorobenzene	8.703	114	424650	50.000	ug/l	0.02
63) Chlorobenzene-d5	11.502	117	395716	50.000	ug/l	0.01
72) 1,4-Dichlorobenzene-d4	13.434	152	186109	50.000	ug/l	0.01
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.155	65	167430	62.575	ug/l	0.02
Spiked Amount	50.000	Range	50 - 163	Recovery	= 125.160%	
35) Dibromofluoromethane	7.734	113	134492	54.987	ug/l	0.02
Spiked Amount	50.000	Range	54 - 147	Recovery	= 109.980%	
50) Toluene-d8	10.191	98	499390	56.381	ug/l	0.01
Spiked Amount	50.000	Range	58 - 134	Recovery	= 112.760%	
62) 4-Bromofluorobenzene	12.489	95	175956	53.511	ug/l	0.01
Spiked Amount	50.000	Range	30 - 143	Recovery	= 107.020%	
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	4.979	59	644	Below Cal	#	89
16) Acetone	3.966	43	3321	2.974	ug/l	90
20) Methylene Chloride	4.735	84	16847	Below Cal		93
31) Cyclohexane	7.801	56	5508	1.159	ug/l #	1
36) 1,1-Dichloropropene	7.801	75	19092	4.445	ug/l #	50
38) Carbon Tetrachloride	7.801	117	24582	5.542	ug/l #	17
76) 1,2,3-Trichloropropane	12.489	75	93600	37.925	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.489	75	93600	83.659	ug/l #	10


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091523\
Data File : VY015595.D
Acq On : 16 Sep 2023 02:23
Operator : SY/MD
Sample : 04419-07
Misc : 5.50g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :


Quant Time: Sep 16 05:28:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y082923S.M
Quant Title : SW846 8260
QLast Update : Thu Aug 31 20:01:47 2023
Response via : Initial Calibration

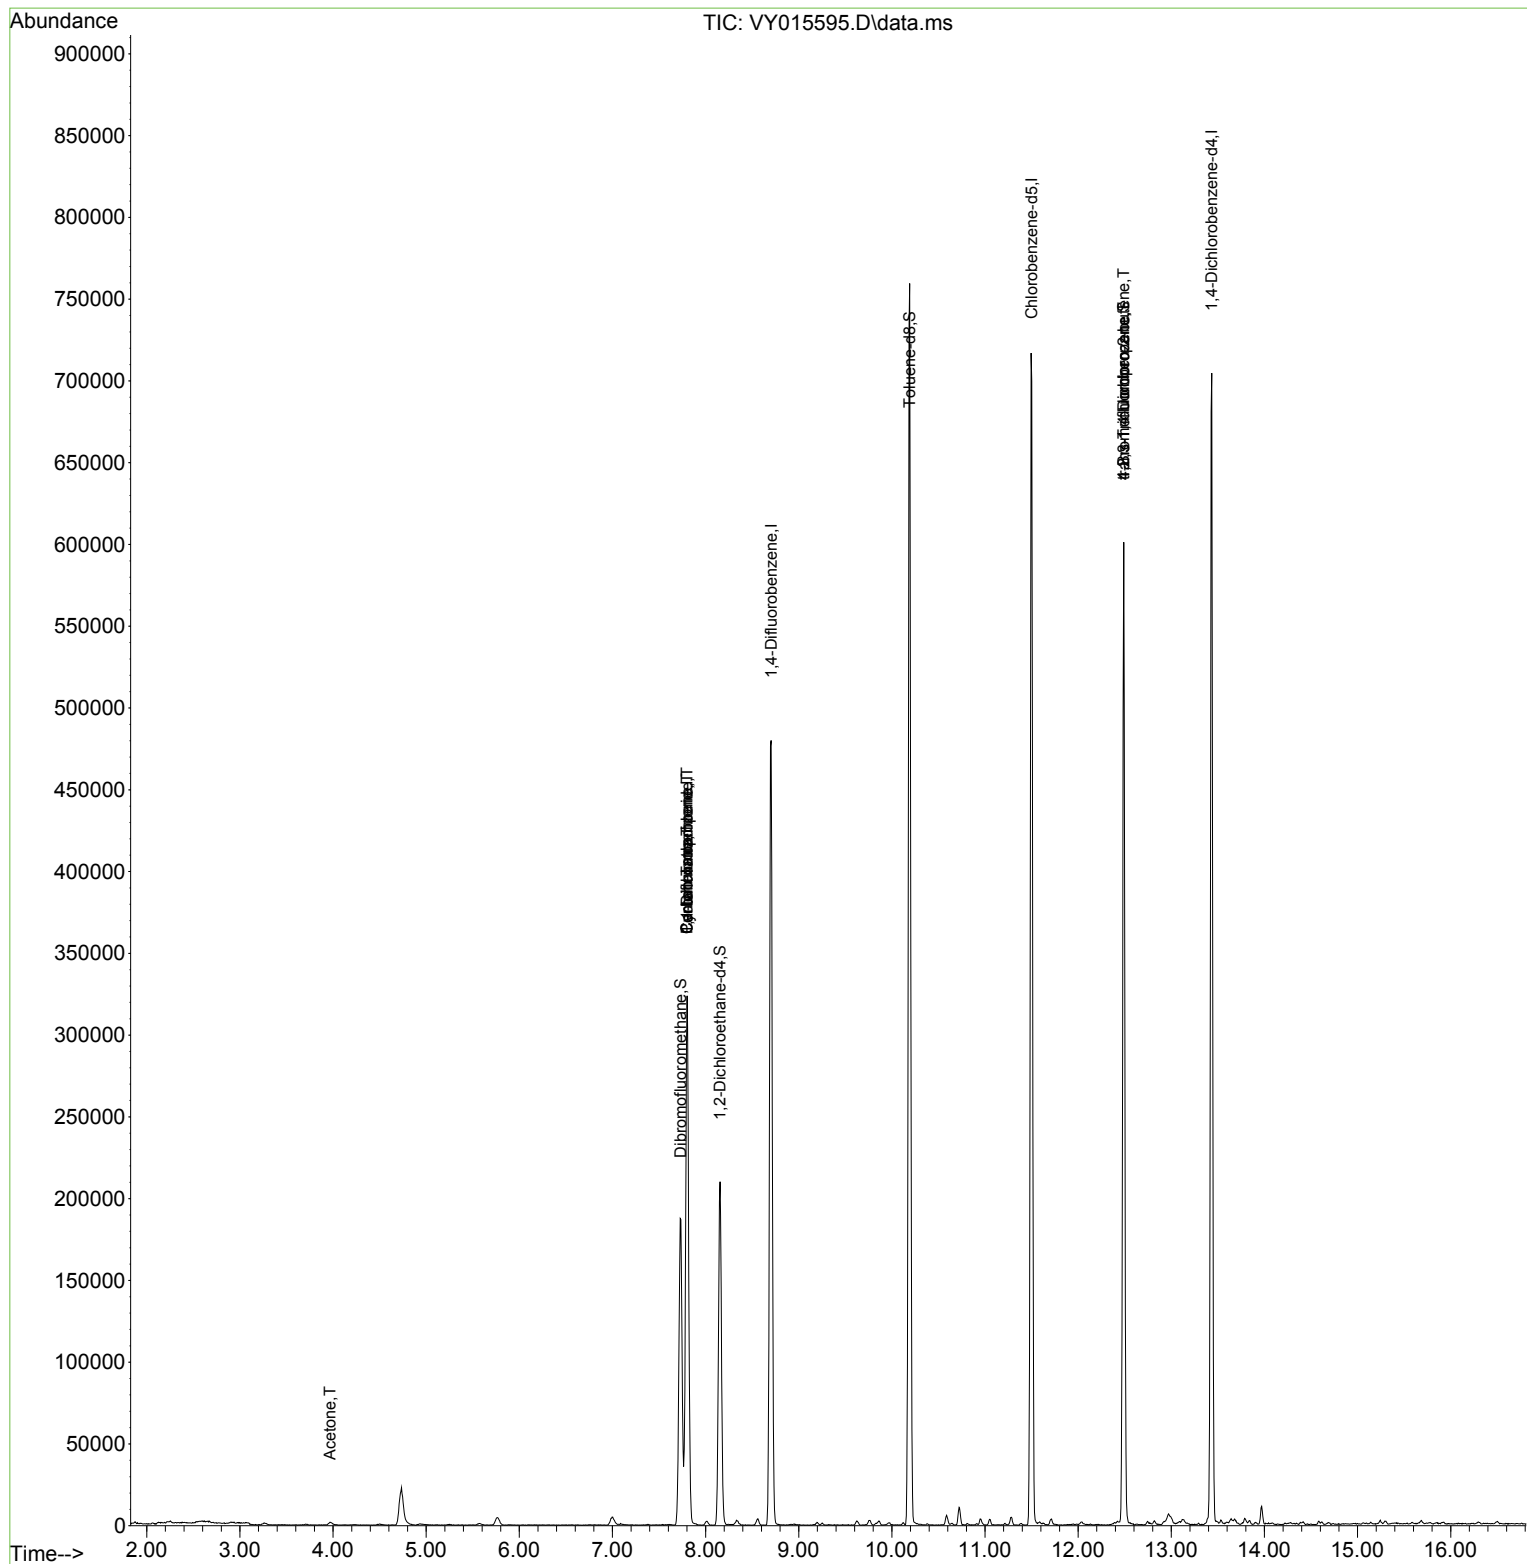



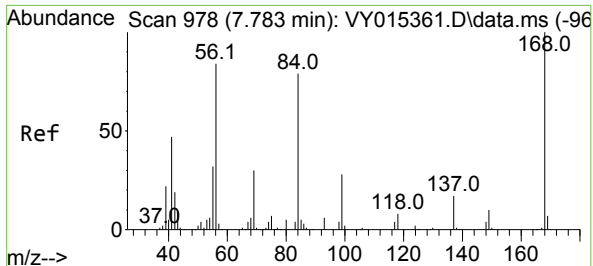


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.801 min Scan# 91
Delta R.T. 0.018 min
Lab File: VY015595.D
Acq: 16 Sep 2023 02:23

Instrument :
MSVOA_Y
ClientSampleId :



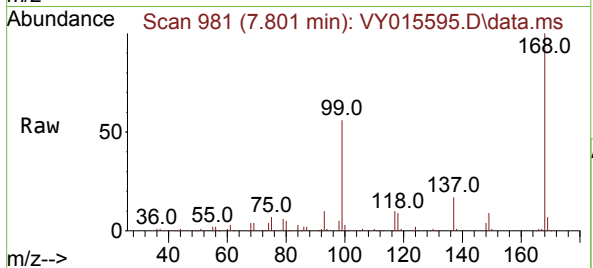



Tgt Ion:168 Resp: 249598
Ion Ratio Lower Upper
168 100
99 55.8 43.4 65.0

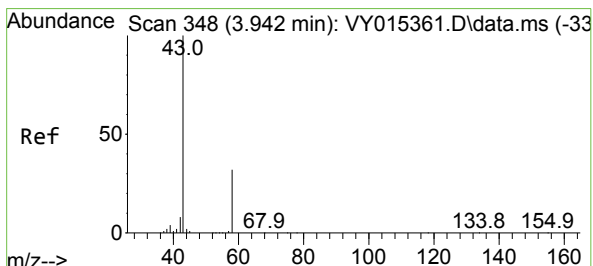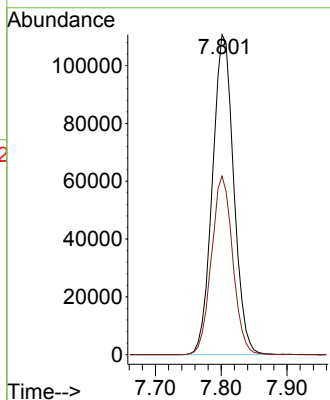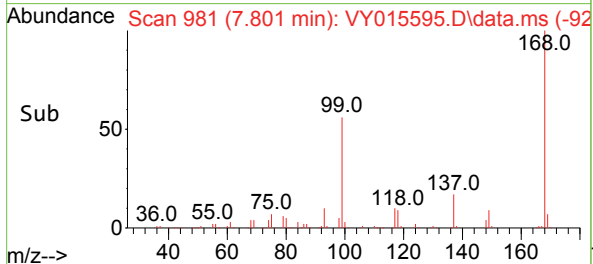

#16
Acetone
Concen: 2.974 ug/l
RT: 3.966 min Scan# 352
Delta R.T. 0.024 min
Lab File: VY015595.D
Acq: 16 Sep 2023 02:23


Tgt Ion: 43 Resp: 3321
Ion Ratio Lower Upper
43 100
58 33.5 22.7 34.1

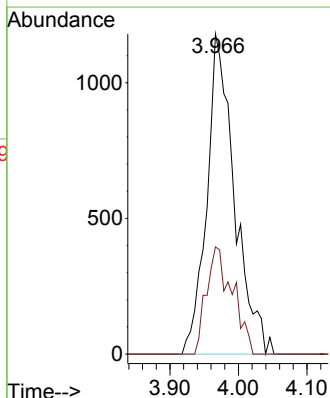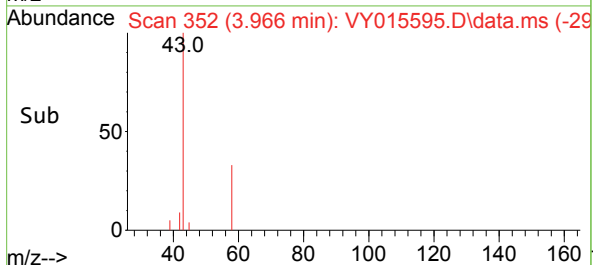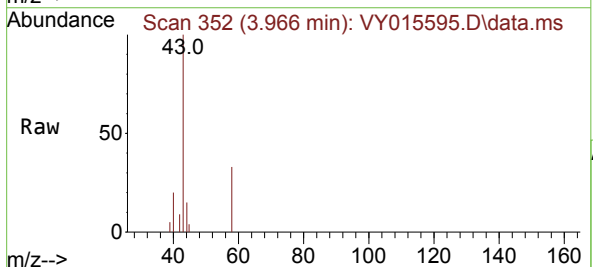



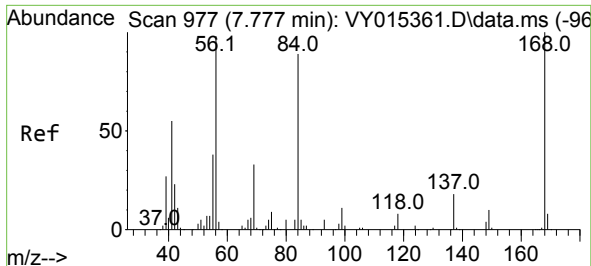


#31
Cyclohexane
Concen: 1.159 ug/l
RT: 7.801 min Scan# 91
Delta R.T. 0.018 min
Lab File: VY015595.D
Acq: 16 Sep 2023 02:23

Instrument :
MSVOA_Y
ClientSampleId :



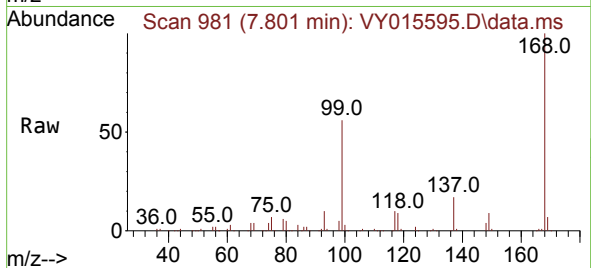



Tgt Ion: 56 Resp: 5508
Ion Ratio Lower Upper
56 100
69 170.9 27.8 41.6#
84 145.5 66.4 99.6#

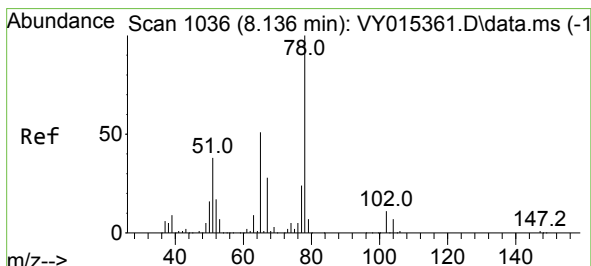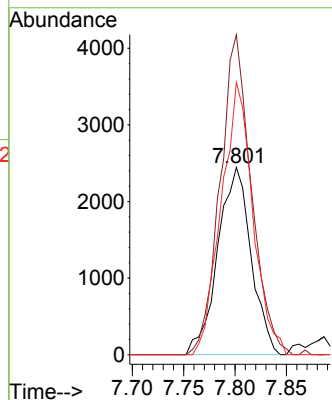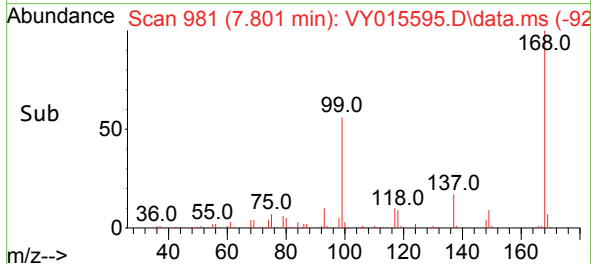

#33
1,2-Dichloroethane-d4
Concen: 62.575 ug/l
RT: 8.155 min Scan# 1039
Delta R.T. 0.018 min
Lab File: VY015595.D
Acq: 16 Sep 2023 02:23

Tgt Ion: 65 Resp: 167430
Ion Ratio Lower Upper
65 100
67 52.0 0.0 101.8

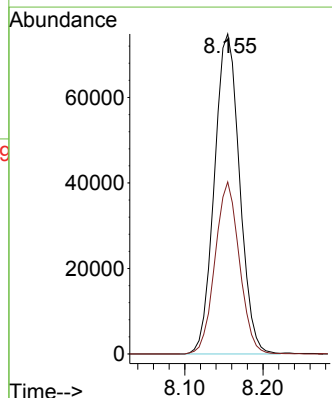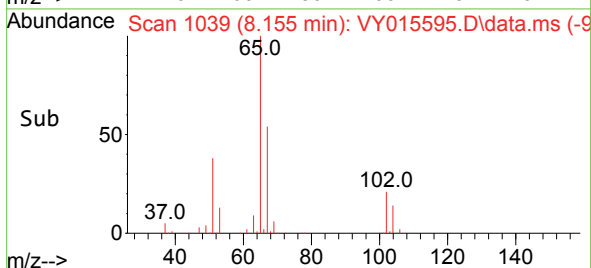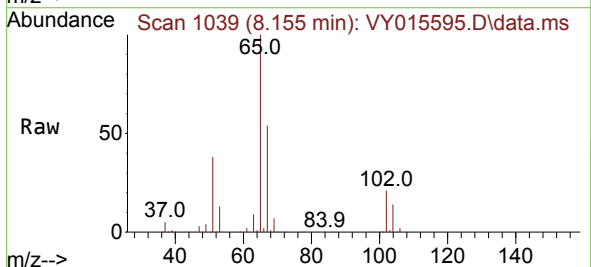

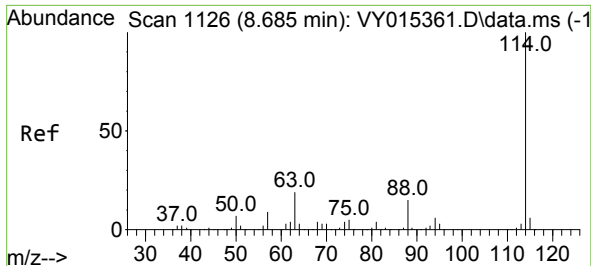

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.703 min Scan# 1126

Delta R.T. 0.018 min

Lab File: VY015595.D

Acq: 16 Sep 2023 02:23

Instrument :

MSVOA_Y

ClientSampleId :





Tgt Ion:114 Resp: 424650

Ion Ratio Lower Upper

114 100

63 19.4 0.0 42.4

88 15.1 0.0 30.6

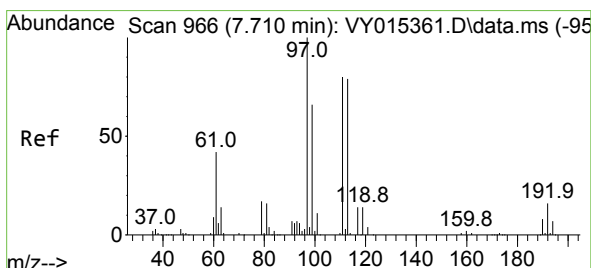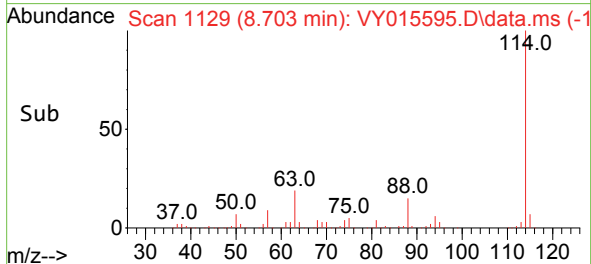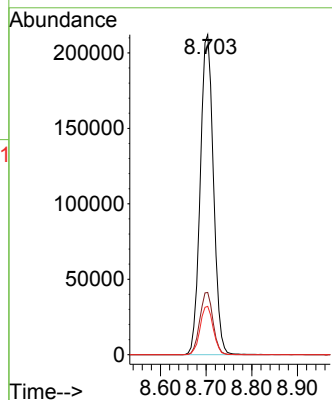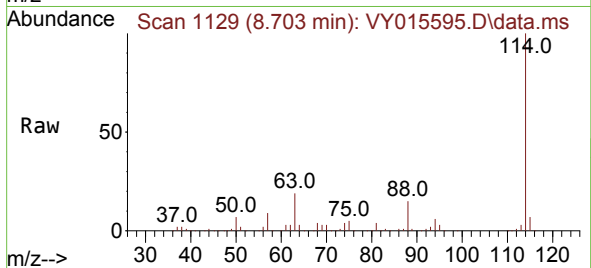

#35

Dibromofluoromethane

Concen: 54.987 ug/l

RT: 7.734 min Scan# 970

Delta R.T. 0.018 min

Lab File: VY015595.D

Acq: 16 Sep 2023 02:23




Tgt Ion:113 Resp: 134492


Ion Ratio Lower Upper

113 100

111 102.2 81.3 121.9


192 19.9 16.9 25.3

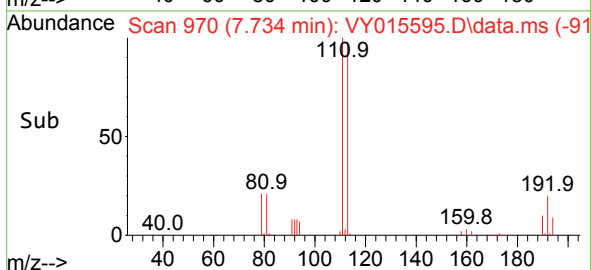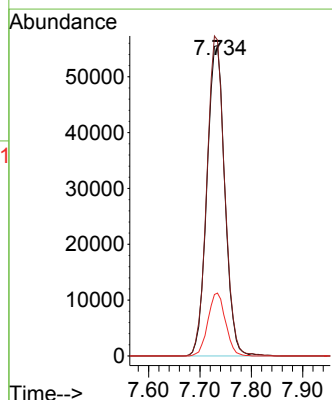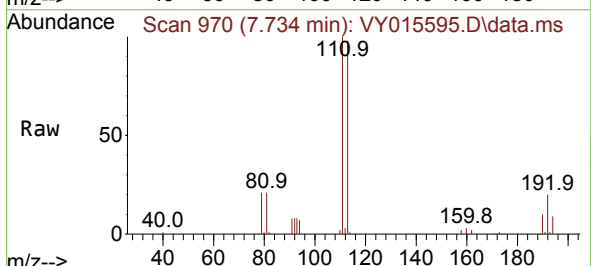



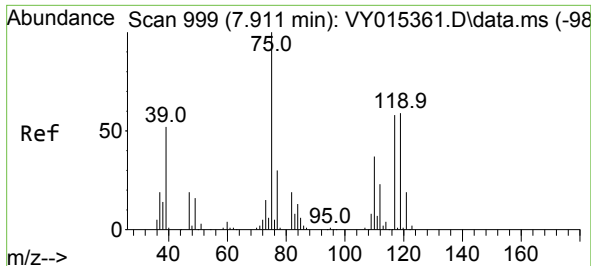


#36
 1,1-Dichloropropene
 Concen: 4.445 ug/l
 RT: 7.801 min Scan# 981
 Delta R.T. -0.110 min
 Lab File: VY015595.D
 Acq: 16 Sep 2023 02:23


Instrument :
 MSVOA_Y
 ClientSampleId :

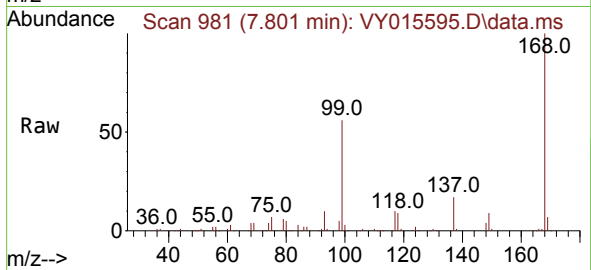



Tgt Ion: 75 Resp: 19092
 Ion Ratio Lower Upper
 75 100
 110 8.8 17.8 53.5#
 77 0.0 24.4 36.6#

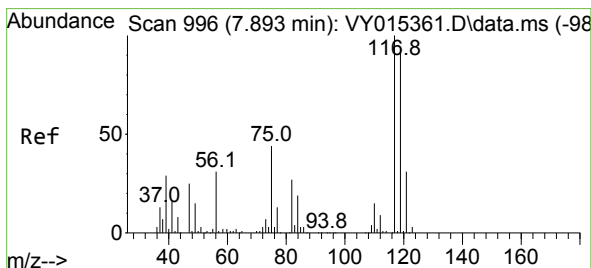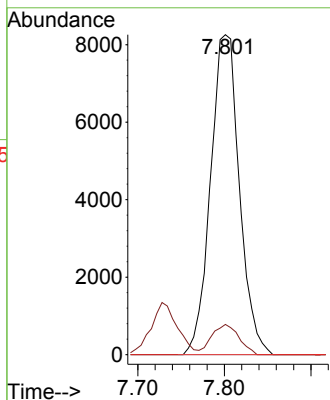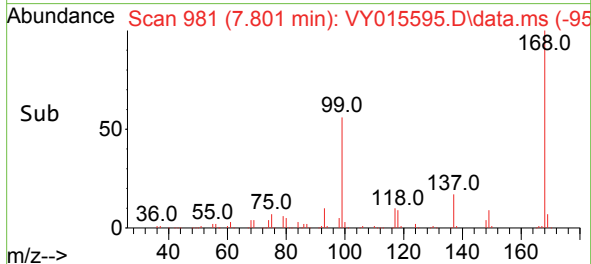


#38
 Carbon Tetrachloride
 Concen: 5.542 ug/l
 RT: 7.801 min Scan# 981
 Delta R.T. -0.091 min
 Lab File: VY015595.D
 Acq: 16 Sep 2023 02:23

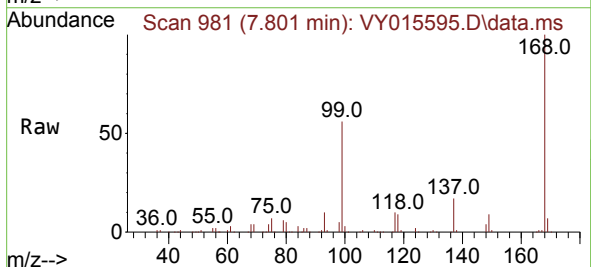

Tgt Ion: 117 Resp: 24582
 Ion Ratio Lower Upper
 117 100
 119 6.0 76.4 114.6#
 121 0.0 25.8 38.6#

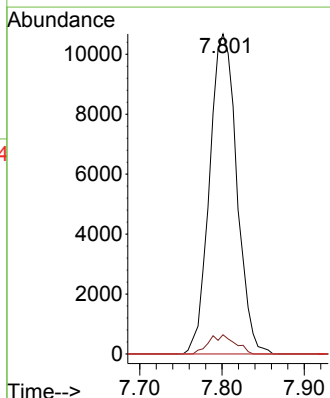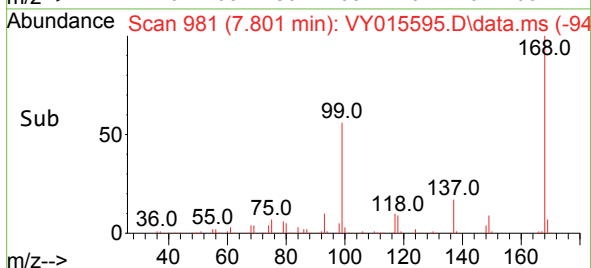

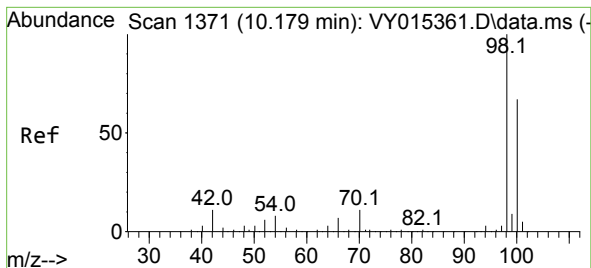

#50

Toluene-d8

Concen: 56.381 ug/l

RT: 10.191 min Scan# 11

Delta R.T. 0.012 min

Lab File: VY015595.D

Acq: 16 Sep 2023 02:23

Instrument :

MSVOA_Y





ClientSampleId :

Tgt Ion: 98 Resp: 499390

Ion Ratio Lower Upper

98 100

100 65.3 50.1 75.1

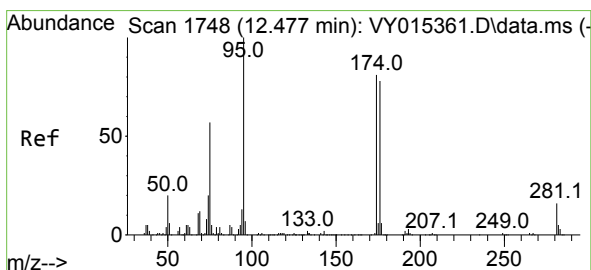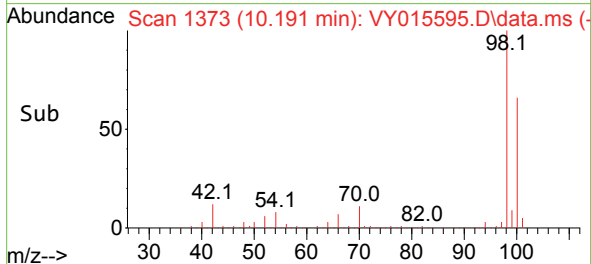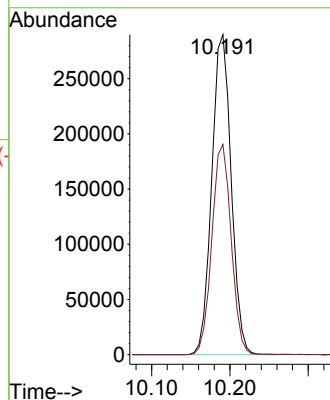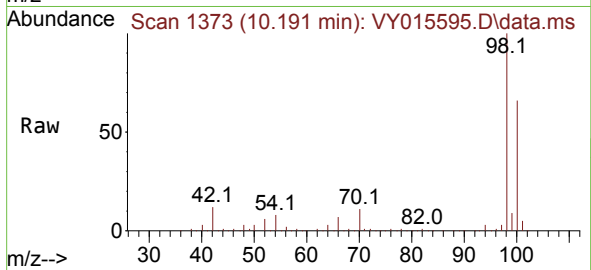

#62

4-Bromofluorobenzene

Concen: 53.511 ug/l

RT: 12.489 min Scan# 1750

Delta R.T. 0.012 min

Lab File: VY015595.D

Acq: 16 Sep 2023 02:23




Tgt Ion: 95 Resp: 175956


Ion Ratio Lower Upper

95 100

174 84.7 0.0 178.2

176 81.6 0.0 173.8

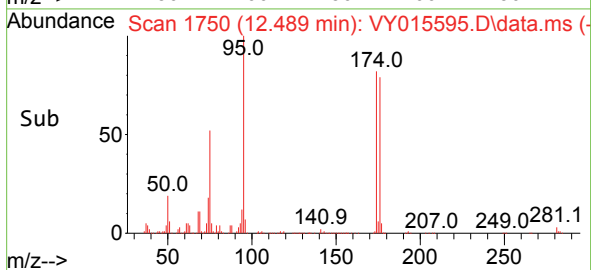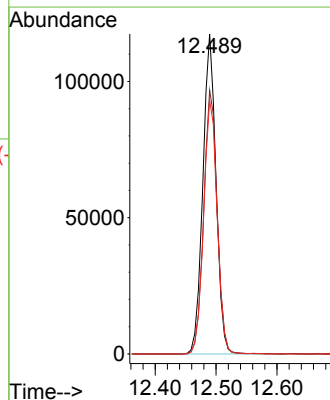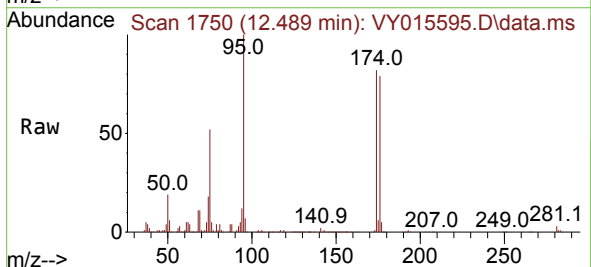

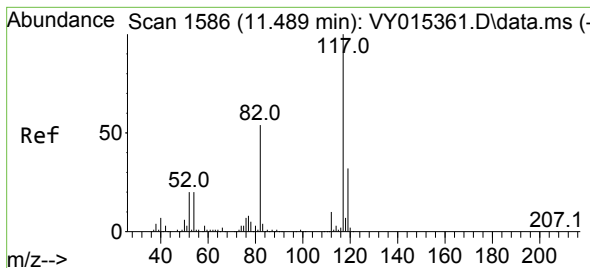

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.502 min Scan# 11

Delta R.T. 0.012 min


Lab File: VY015595.D

Acq: 16 Sep 2023 02:23

Instrument :

MSVOA_Y

ClientSampleId :

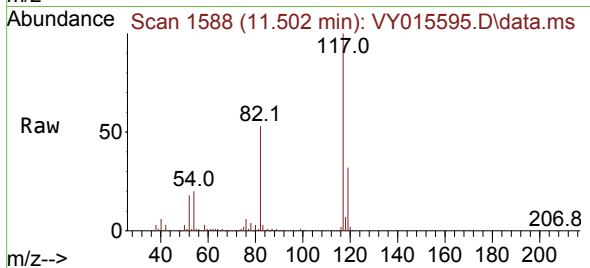




Tgt Ion:117 Resp: 395716

Ion Ratio Lower Upper

117 100

82 52.7 43.4 65.0

119 32.3 26.3 39.5

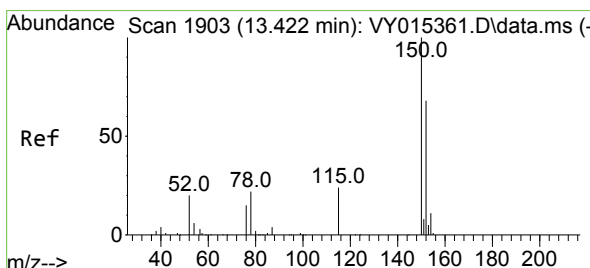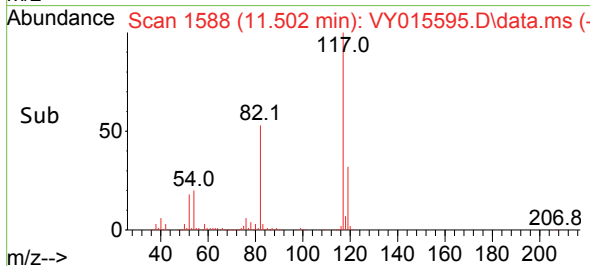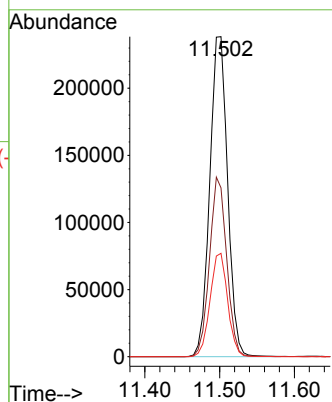

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.434 min Scan# 1905

Delta R.T. 0.012 min

Lab File: VY015595.D

Acq: 16 Sep 2023 02:23




Tgt Ion:152 Resp: 186109


Ion Ratio Lower Upper

152 100

115 58.2 28.8 86.5

150 156.5 0.0 348.8

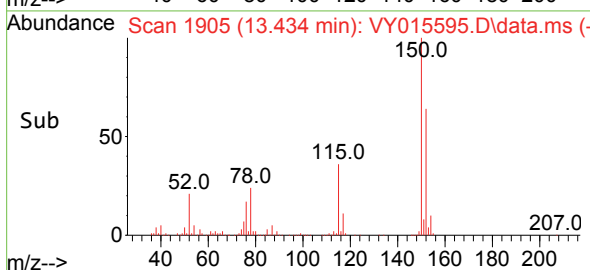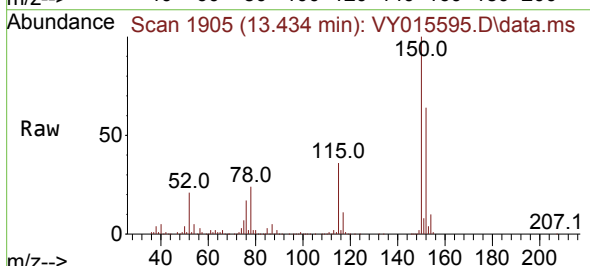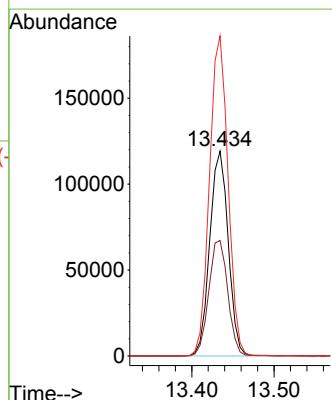

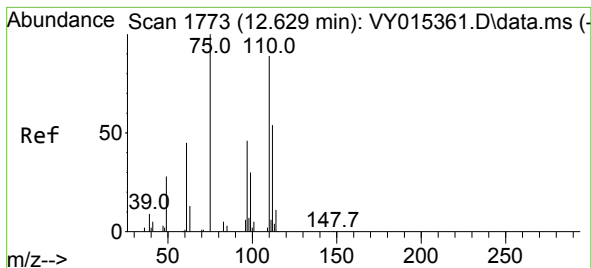

#76

1,2,3-Trichloropropane

Concen: 37.925 ug/l

RT: 12.489 min Scan# 1750

Delta R.T. -0.140 min

Lab File: VY015595.D

Acq: 16 Sep 2023 02:23

Instrument :

MSVOA_Y





ClientSampleId :

Tgt Ion: 75 Resp: 93600

Ion Ratio Lower Upper

75 100

77 1.5 0.0 0.0#

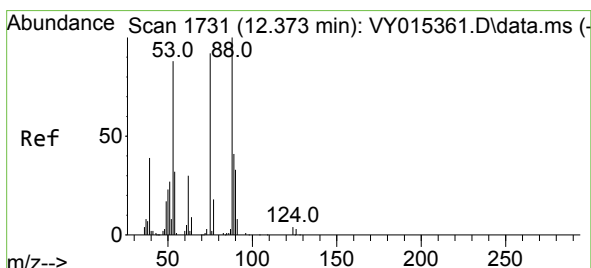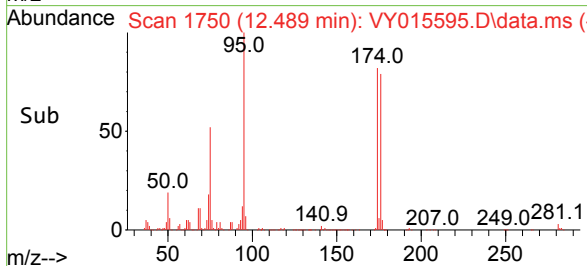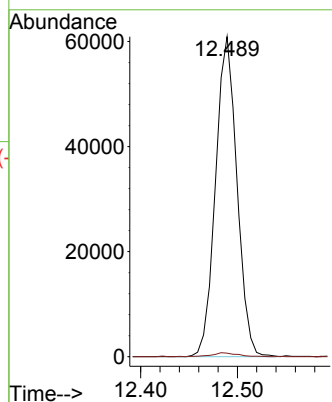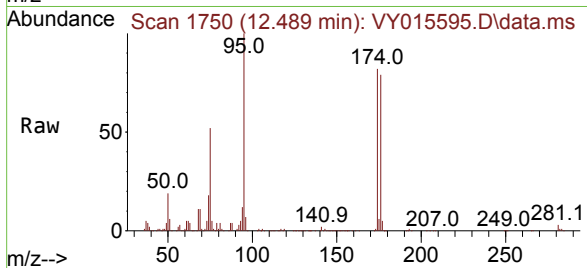

#81

trans-1,4-Dichloro-2-butene

Concen: 83.659 ug/l

RT: 12.489 min Scan# 1750

Delta R.T. 0.110 min

Lab File: VY015595.D

Acq: 16 Sep 2023 02:23

Tgt Ion: 75 Resp: 93600

Ion Ratio Lower Upper

75 100

53 0.0 77.8 116.8#

89 0.0 37.4 56.0#

