

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091523\
 Data File : VY015593.D
 Acq On : 16 Sep 2023 01:36
 Operator : SY/MD
 Sample : 04419-05
 Misc : 4.43g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 DB-07(25-27)

Quant Time: Sep 16 05:27:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y082923S.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 31 20:01:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.801	168	277661	50.000	ug/l	0.02
34) 1,4-Difluorobenzene	8.703	114	470368	50.000	ug/l	0.02
63) Chlorobenzene-d5	11.496	117	435130	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	203880	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.155	65	179234	60.217	ug/l	0.02
Spiked Amount	50.000	Range	50 - 163	Recovery	=	120.440%
35) Dibromofluoromethane	7.728	113	148057	54.649	ug/l	0.01
Spiked Amount	50.000	Range	54 - 147	Recovery	=	109.300%
50) Toluene-d8	10.185	98	553275	56.393	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	112.780%
62) 4-Bromofluorobenzene	12.489	95	194739	53.467	ug/l	0.01
Spiked Amount	50.000	Range	30 - 143	Recovery	=	106.940%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091523\
Data File : VY015593.D
Acq On : 16 Sep 2023 01:36
Operator : SY/MD
Sample : 04419-05
Misc : 4.43g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
DB-07(25-27)

Quant Time: Sep 16 05:27:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y082923S.M
Quant Title : SW846 8260
QLast Update : Thu Aug 31 20:01:47 2023
Response via : Initial Calibration




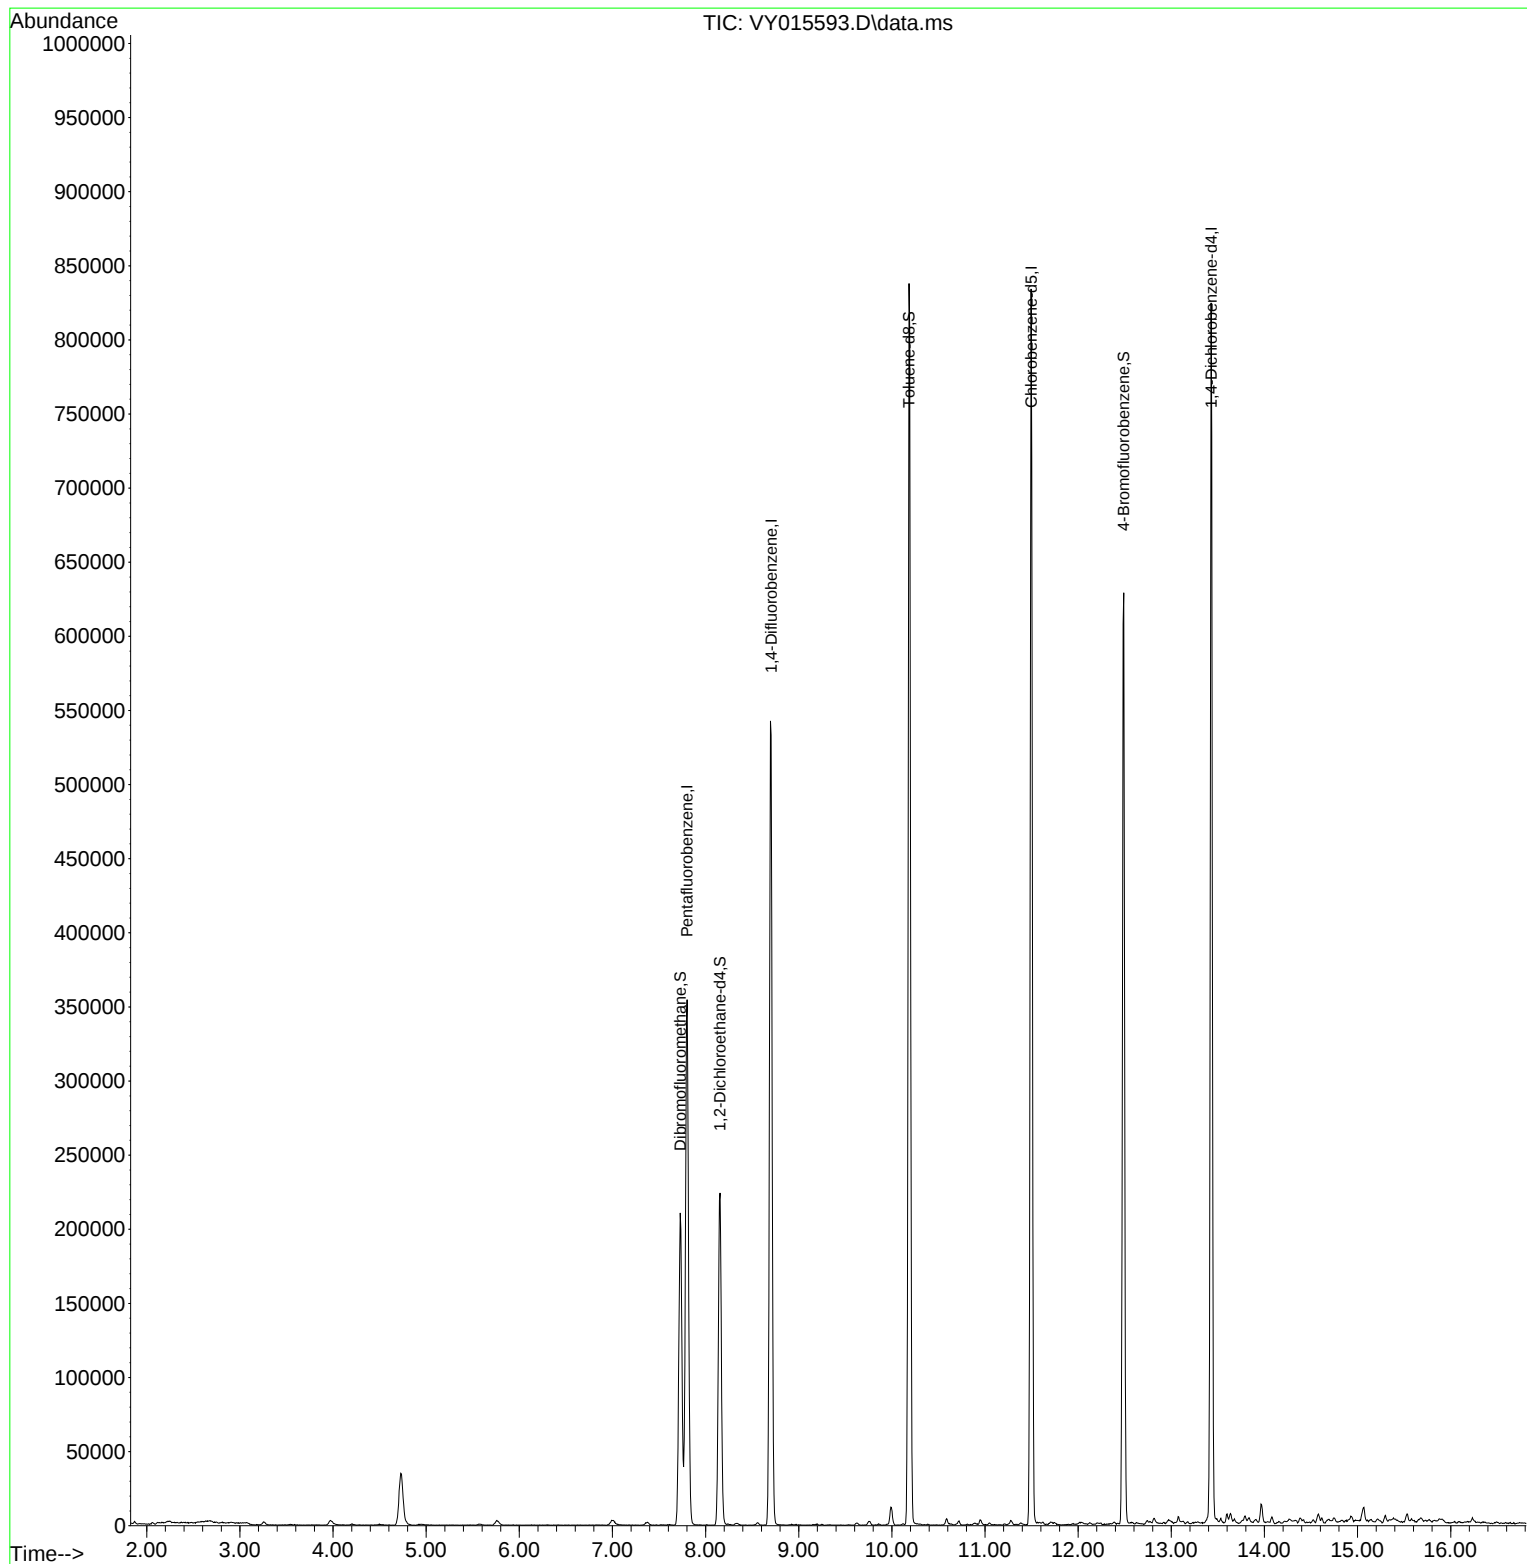


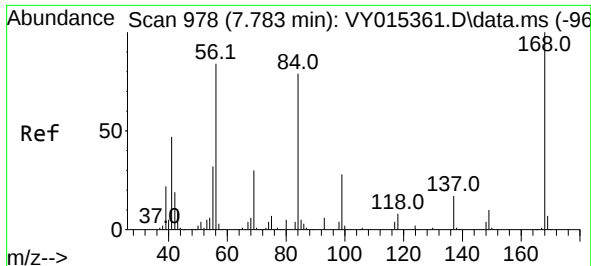

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.801 min Scan# 91
Delta R.T. 0.018 min
Lab File: VY015593.D
Acq: 16 Sep 2023 01:36




Instrument :
MSVOA_Y
ClientSampleId :
DB-07(25-27)


Tgt Ion:168 Resp: 277661
Ion Ratio Lower Upper
168 100
99 54.1 43.4 65.0

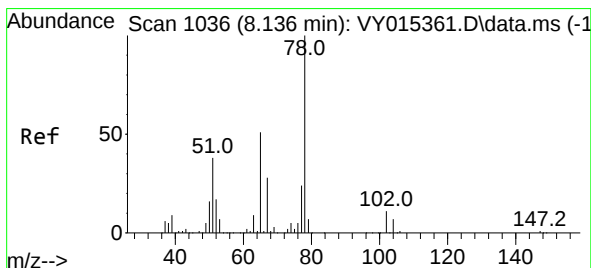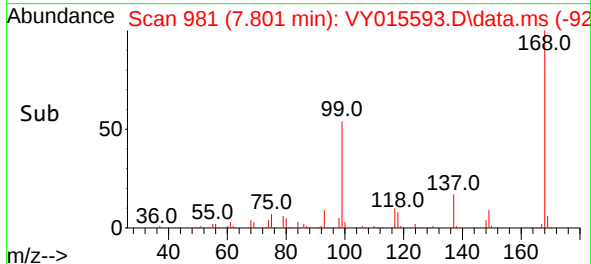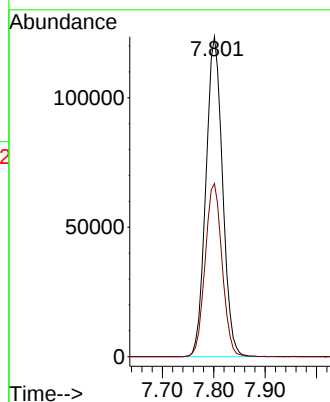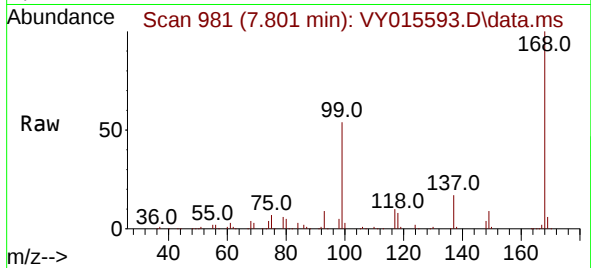

#33
1,2-Dichloroethane-d4
Concen: 60.217 ug/l
RT: 8.155 min Scan# 1039
Delta R.T. 0.018 min
Lab File: VY015593.D
Acq: 16 Sep 2023 01:36

Tgt Ion: 65 Resp: 179234
Ion Ratio Lower Upper
65 100
67 52.6 0.0 101.8

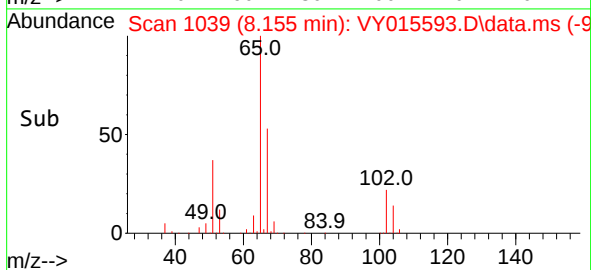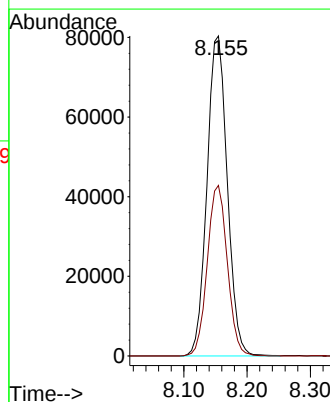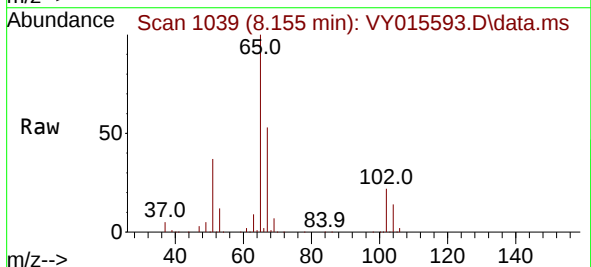

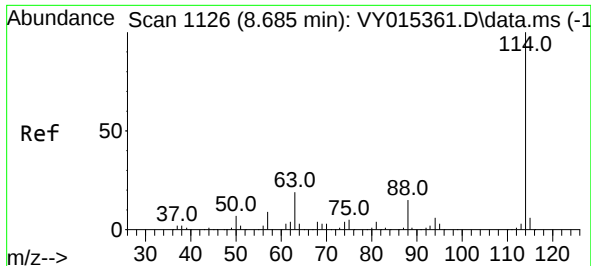

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.703 min Scan# 1126

Delta R.T. 0.018 min

Lab File: VY015593.D

Acq: 16 Sep 2023 01:36

Instrument :

MSVOA_Y

ClientSampleId :

DB-07(25-27)





Tgt Ion:114 Resp: 470368

Ion Ratio Lower Upper

114 100

63 19.0 0.0 42.4

88 14.3 0.0 30.6

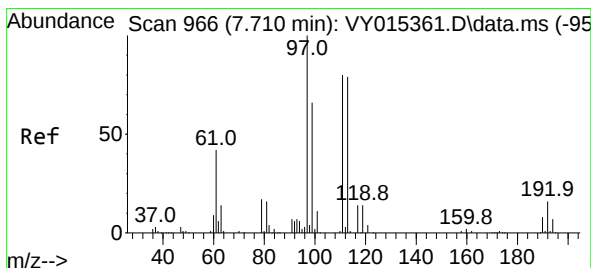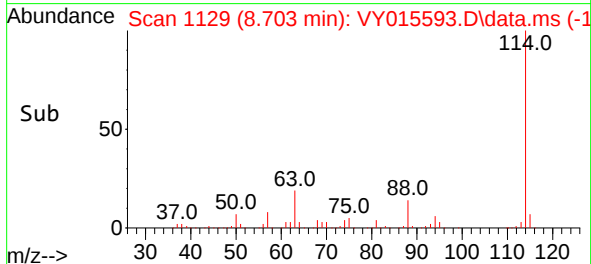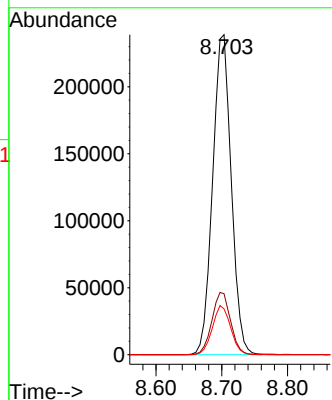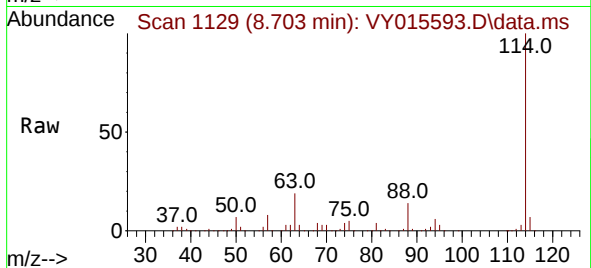

#35

Dibromofluoromethane

Concen: 54.649 ug/l

RT: 7.728 min Scan# 969

Delta R.T. 0.012 min

Lab File: VY015593.D

Acq: 16 Sep 2023 01:36




Tgt Ion:113 Resp: 148057


Ion Ratio Lower Upper

113 100

111 101.8 81.3 121.9

192 19.8 16.9 25.3


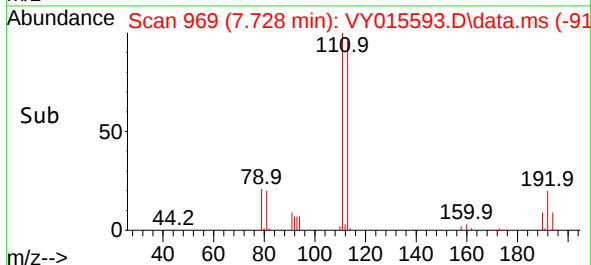
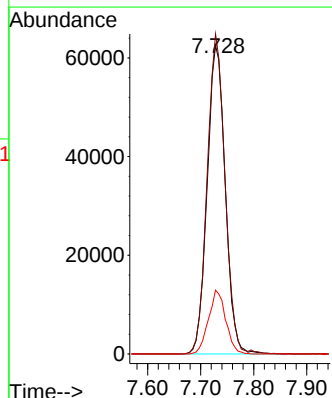
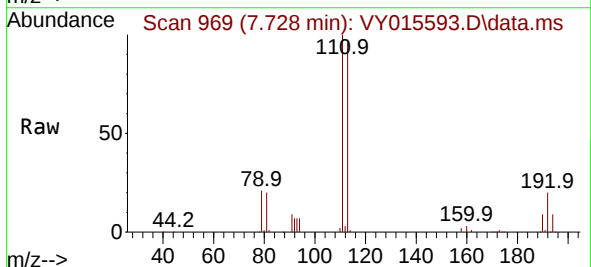


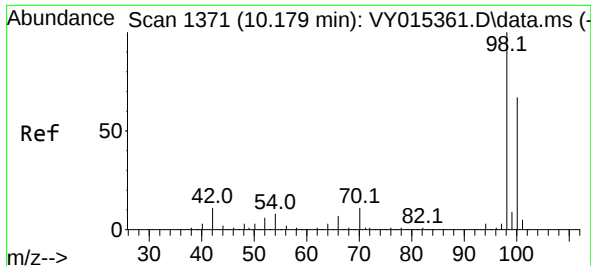

#50
Toluene-d8
Concen: 56.393 ug/l
RT: 10.185 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY015593.D
Acq: 16 Sep 2023 01:36




Instrument :
MSVOA_Y
ClientSampleId :
DB-07(25-27)


Tgt Ion: 98 Resp: 553275
Ion Ratio Lower Upper
98 100
100 65.3 50.1 75.1

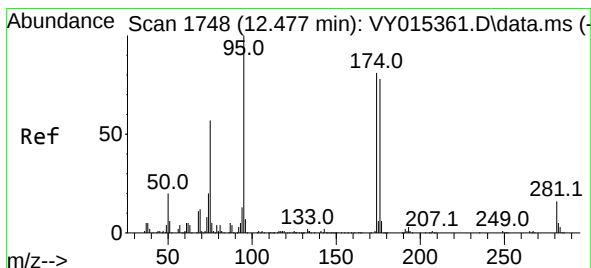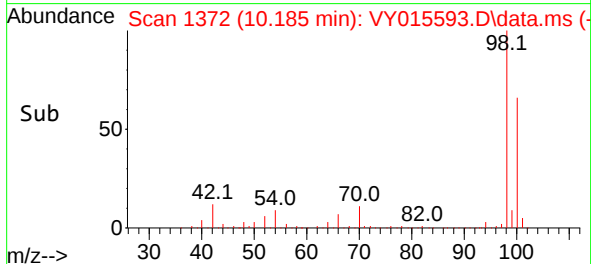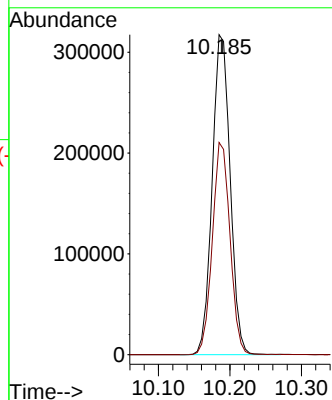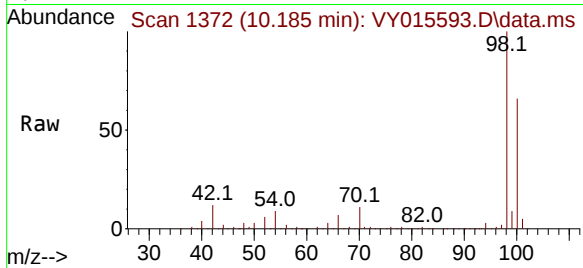

#62
4-Bromofluorobenzene
Concen: 53.467 ug/l
RT: 12.489 min Scan# 1750
Delta R.T. 0.012 min
Lab File: VY015593.D
Acq: 16 Sep 2023 01:36

Tgt Ion: 95 Resp: 194739
Ion Ratio Lower Upper
95 100
174 84.2 0.0 178.2
176 81.1 0.0 173.8

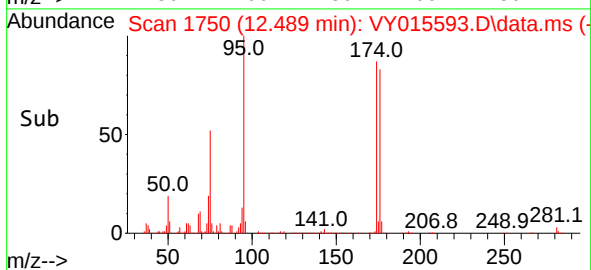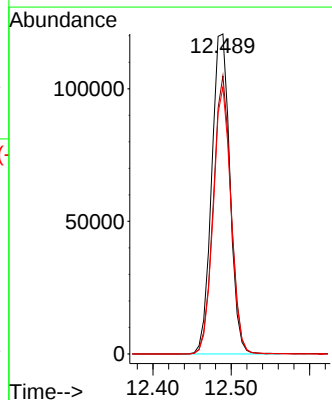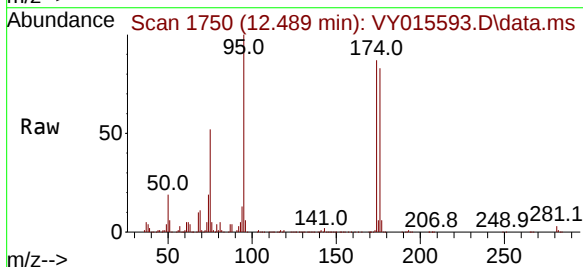

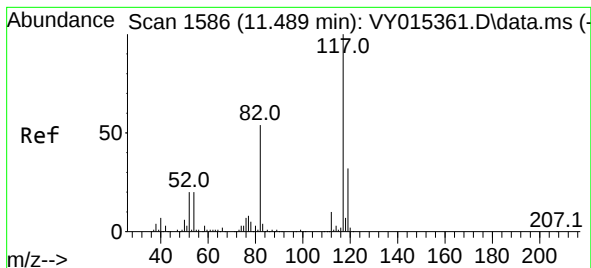

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.496 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY015593.D

Acq: 16 Sep 2023 01:36

Instrument :

MSVOA_Y

ClientSampleId :

DB-07(25-27)





Tgt Ion:117 Resp: 435130

Ion Ratio Lower Upper

117 100

82 54.6 43.4 65.0

119 32.1 26.3 39.5

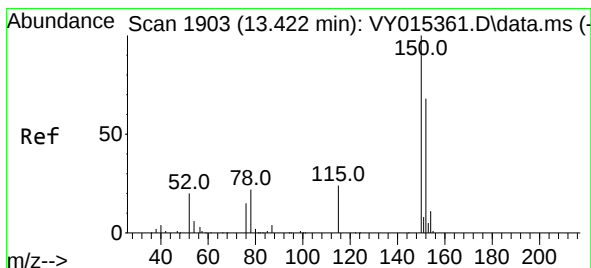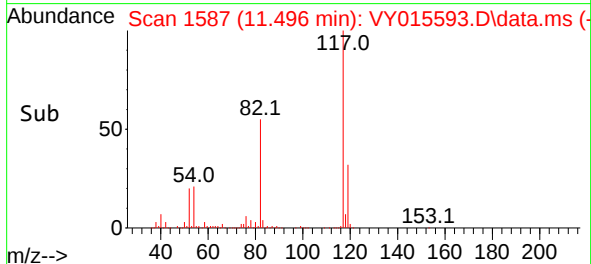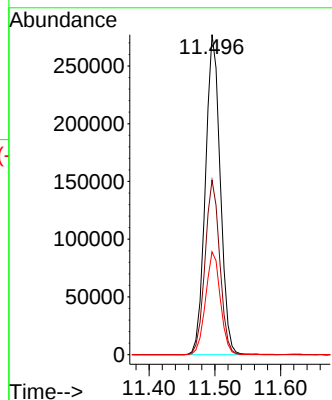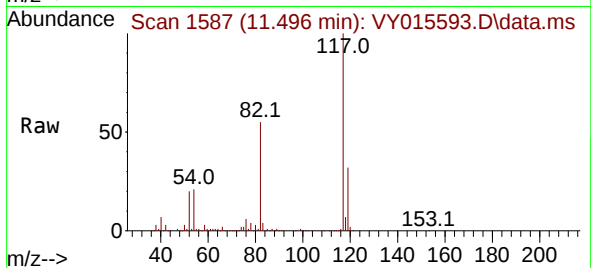

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.006 min

Lab File: VY015593.D

Acq: 16 Sep 2023 01:36

Tgt Ion:152 Resp: 203880

Ion Ratio Lower Upper

152 100

115 58.7 28.8 86.5

150 158.1 0.0 348.8

