
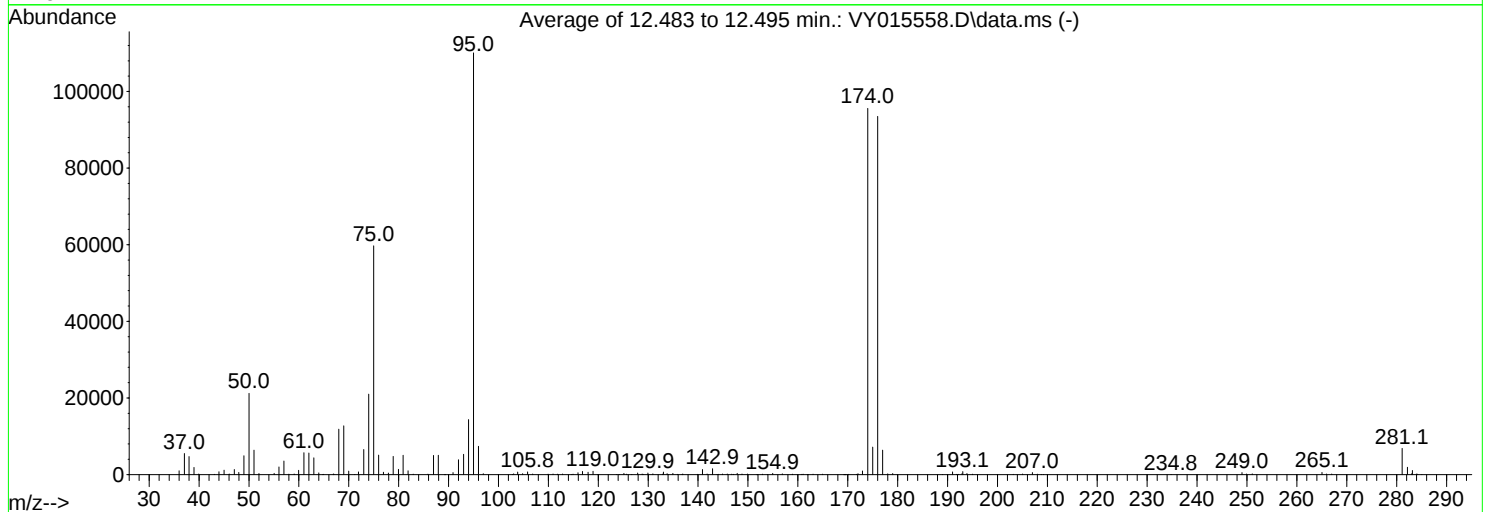


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091523\
Data File : VY015558.D
Acq On : 15 Sep 2023 08:55
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y082923S.M
Title : SW846 8260
Last Update : Thu Aug 31 20:01:47 2023

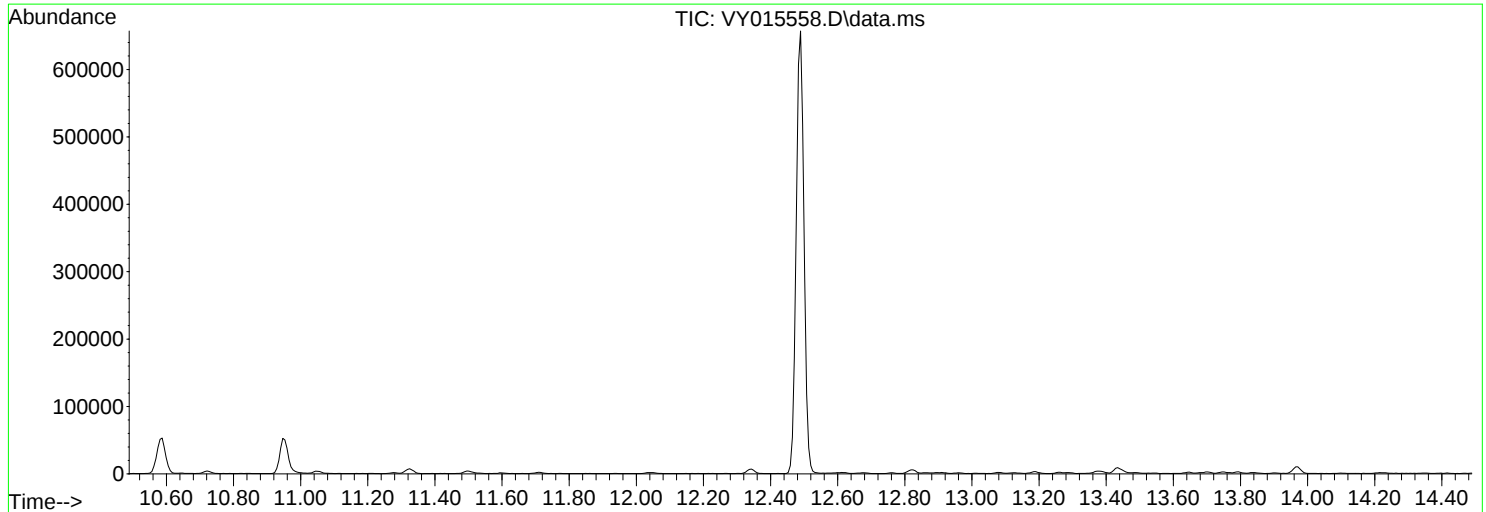

AutoFind: Scans 1749, 1750, 1751; Background Corrected with Scan 1741

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.3	21216	PASS
75	95	30	60	54.3	59725	PASS
95	95	100	100	100.0	110077	PASS
96	95	5	9	6.7	7413	PASS
173	174	0.00	2	1.0	982	PASS
174	95	50	100	86.8	95595	PASS
175	174	5	9	7.5	7174	PASS
176	174	95	101	97.8	93485	PASS
177	176	5	9	6.9	6407	PASS