


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv091619\
Data File : VY000041.D
Acq On : 16 Sep 2019 11:17
Operator : SY/MD
Sample : BFB
Misc : 5.00µl/5.00ml/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y091219S.M
Title : SW846 8260
Last Update : Tue Sep 17 07:02:53 2019

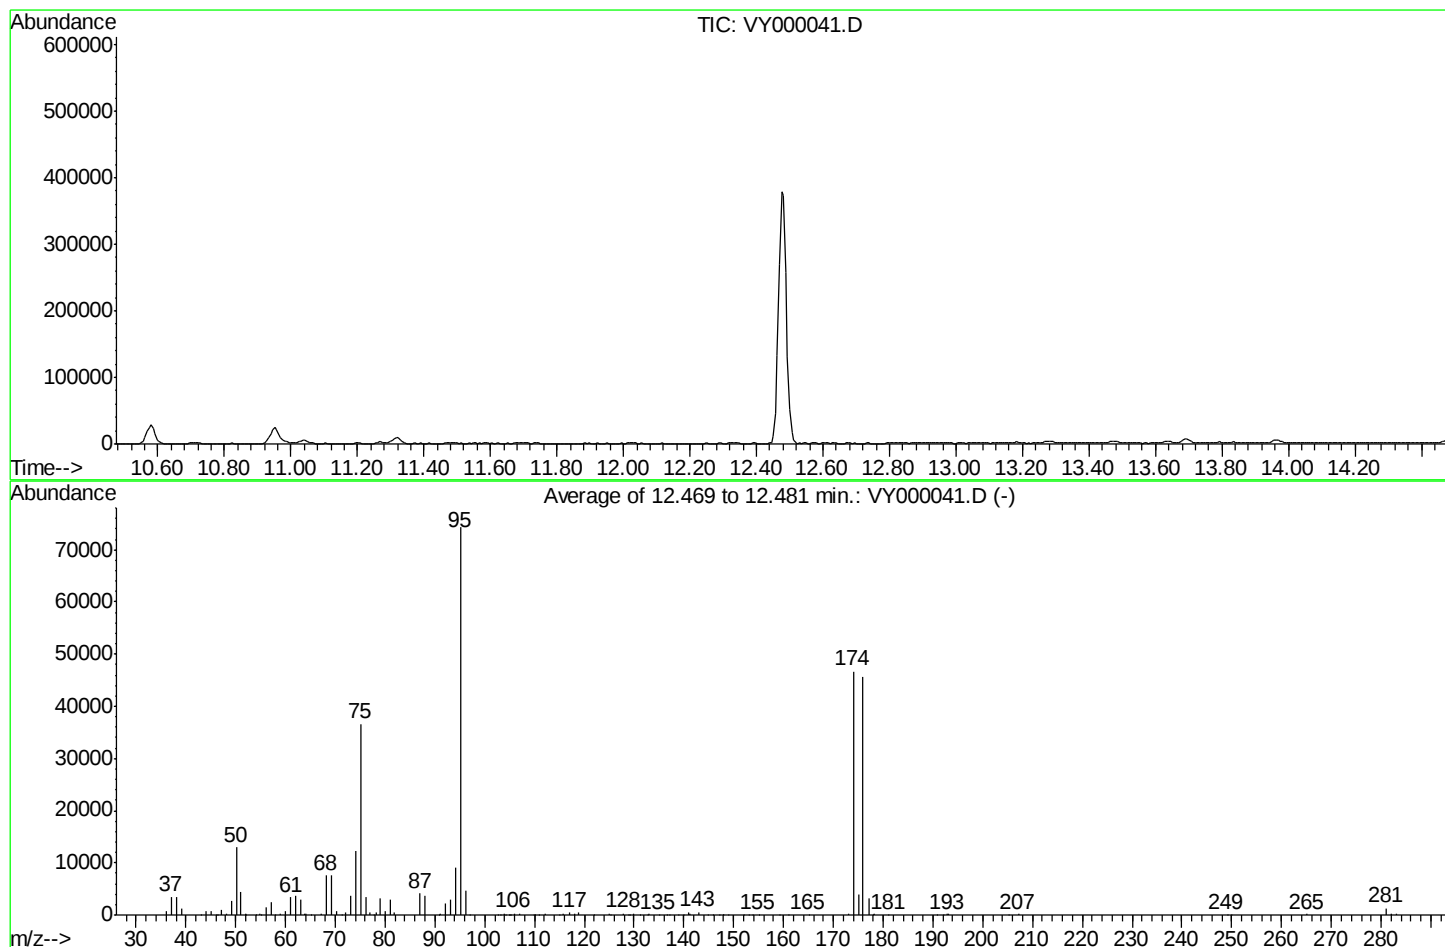

AutoFind: Scans 1785, 1786, 1787; Background Corrected with Scan 1778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	12966	PASS
75	95	30	60	49.3	36613	PASS
95	95	100	100	100.0	74298	PASS
96	95	5	9	6.2	4588	PASS
173	174	0.00	2	0.3	163	PASS
174	95	50	100	62.8	46669	PASS
175	174	5	9	8.3	3858	PASS
176	174	95	101	98.0	45752	PASS
177	176	5	9	7.0	3188	PASS