
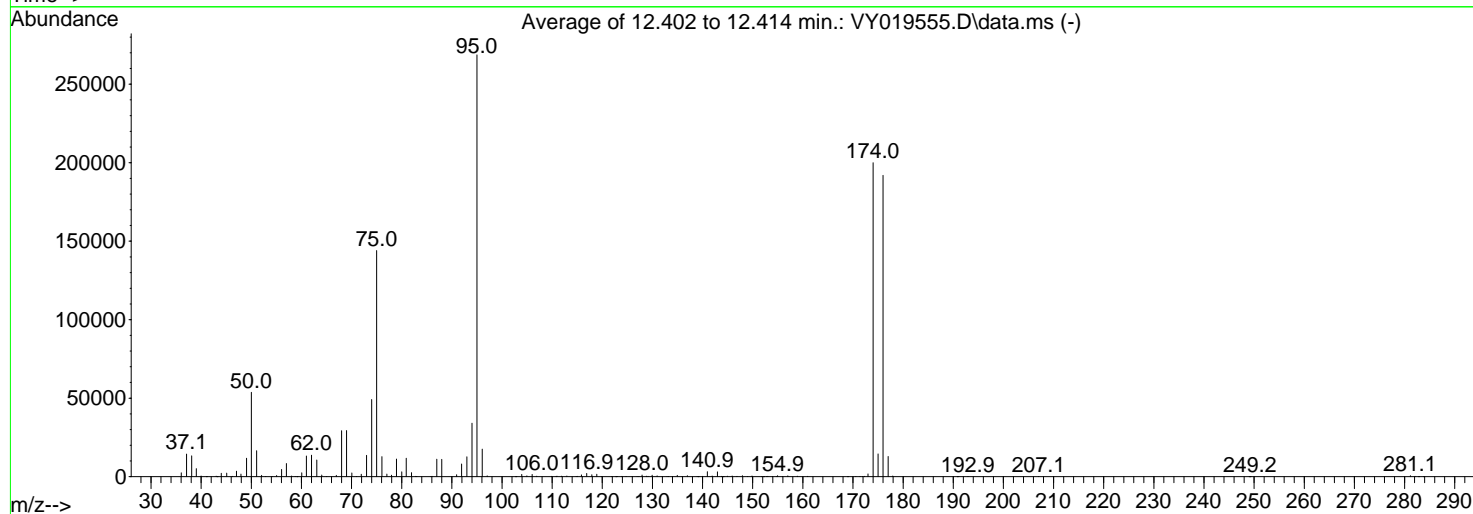


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY091624\  
 Data File : VY019555.D  
 Acq On : 16 Sep 2024 08:42  
 Operator : SY/MD  
 Sample : BFB  
 Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y090924S.M  
 Title : SW846 8260  
 Last Update : Mon Sep 09 16:00:30 2024

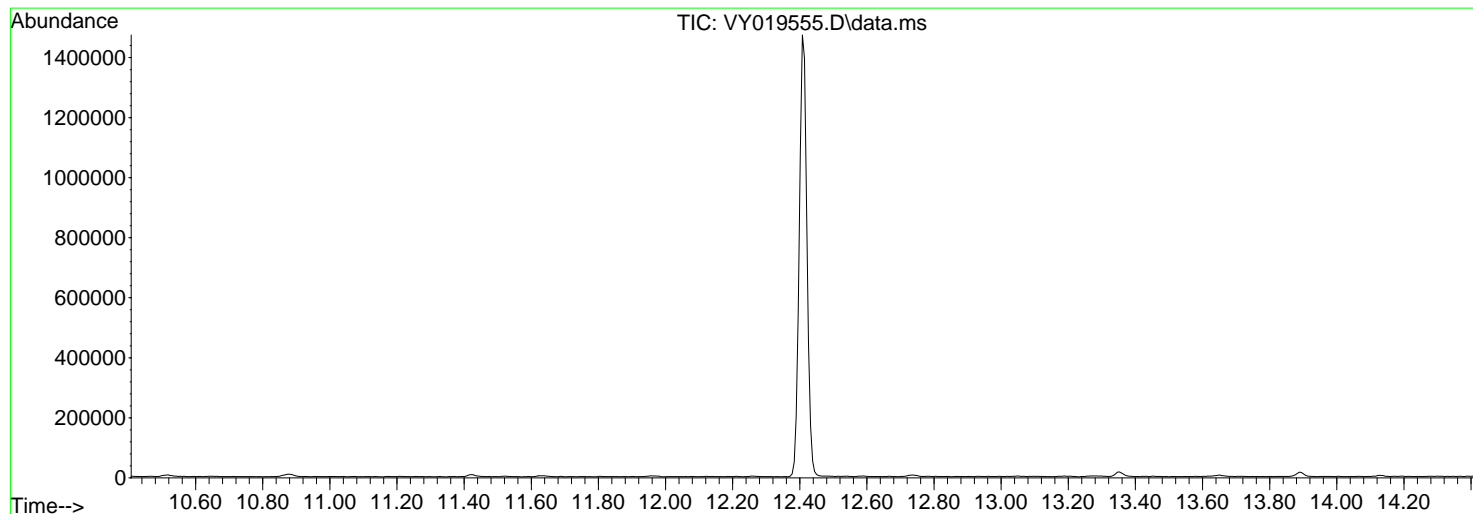

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result
50	95	15	40	20.0	53707	PASS
75	95	30	60	53.6	144000	PASS
95	95	100	100	100.0	268715	PASS
96	95	5	9	6.5	17582	PASS
173	174	0.00	2	0.9	1750	PASS
174	95	50	100	74.4	200021	PASS
175	174	5	9	7.2	14444	PASS
176	174	95	101	95.9	191893	PASS
177	176	5	9	6.7	12836	PASS