

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091721\
 Data File : VY006064.D
 Acq On : 17 Sep 2021 12:32
 Operator : SY/MD
 Sample : M3750-02RE
 Misc : 6.80G/5ML/MSVOA_Y/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 NAPL-AREA-03-(25-27)RE

Quant Time: Sep 20 01:39:18 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091421S.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 15 05:01:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.795	168	6844	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	11017	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	10861	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	4597	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.148	65	4904	51.585	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 103.160%			
35) Dibromofluoromethane	7.728	113	3542	51.762	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 103.520%			
50) Toluene-d8	10.185	98	13822	47.393	ug/l	0.00
Spiked Amount 50.000	Range 49 - 140		Recovery = 94.780%			
62) 4-Bromofluorobenzene	12.483	95	4435	44.790	ug/l	0.00
Spiked Amount 50.000	Range 25 - 144		Recovery = 89.580%			
Target Compounds						Qvalue
4) Vinyl Chloride	2.259	62	867	8.541	ug/l #	74
10) Methyl Iodide	4.112	142	164	2.345	ug/l #	35
16) Acetone	3.948	43	736	28.226	ug/l #	76
20) Methylene Chloride	4.740	84	324	Below Cal	#	78
25) 2-Butanone	6.990	43	89	2.476	ug/l #	54
27) cis-1,2-Dichloroethene	6.996	96	1910	22.342	ug/l	87
31) Cyclohexane	7.789	56	161	1.057	ug/l #	70
36) 1,1-Dichloropropene	7.789	75	535	4.499	ug/l #	42
37) Ethyl Acetate	6.990	43	89	1.083	ug/l #	1
38) Carbon Tetrachloride	7.789	117	648	5.006	ug/l #	11
44) Trichloroethene	8.947	130	472	5.555	ug/l	98
55) 1,1,2-Trichloroethane	10.617	97	103	1.642	ug/l #	15
59) 2-Hexanone	10.843	43	66	1.172	ug/l #	28
60) Dibromochloromethane	10.715	129	635	8.209	ug/l #	11
64) Tetrachloroethene	10.727	164	648	7.295	ug/l #	76
75) 1,1,2,2-Tetrachloroethane	12.641	83	155	2.314	ug/l #	26
76) 1,2,3-Trichloropropane	12.483	75	2685	54.782	ug/l #	100
79) 2-Chlorotoluene	12.763	91	247	1.020	ug/l	74
81) trans-1,4-Dichloro-2-b...	12.483	75	2685	100.717	ug/l #	7
84) 1,2,4-Trimethylbenzene	13.123	105	368	1.242	ug/l	73
87) 1,3-Dichlorobenzene	13.452	146	233	1.438	ug/l	83
88) 1,4-Dichlorobenzene	13.452	146	233	1.434	ug/l	81
89) n-Butylbenzene	13.696	91	445	1.458	ug/l #	74
91) 1,2-Dichlorobenzene	13.733	146	250	1.758	ug/l	77
93) 1,2,4-Trichlorobenzene	15.001	180	306	3.314	ug/l	90
94) Hexachlorobutadiene	15.110	225	122	2.042	ug/l #	36
95) Naphthalene	15.239	128	652	3.550	ug/l #	69
96) 1,2,3-Trichlorobenzene	15.421	180	361	4.511	ug/l #	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091721\
Data File : VY006064.D
Acq On : 17 Sep 2021 12:32
Operator : SY/MD
Sample : M3750-02RE
Misc : 6.80G/5ML/MSVOA_Y/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
NAPL-AREA-03-(25-27)RE

Quant Time: Sep 20 01:39:18 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091421S.M
Quant Title : SW846 8260
QLast Update : Wed Sep 15 05:01:47 2021
Response via : Initial Calibration




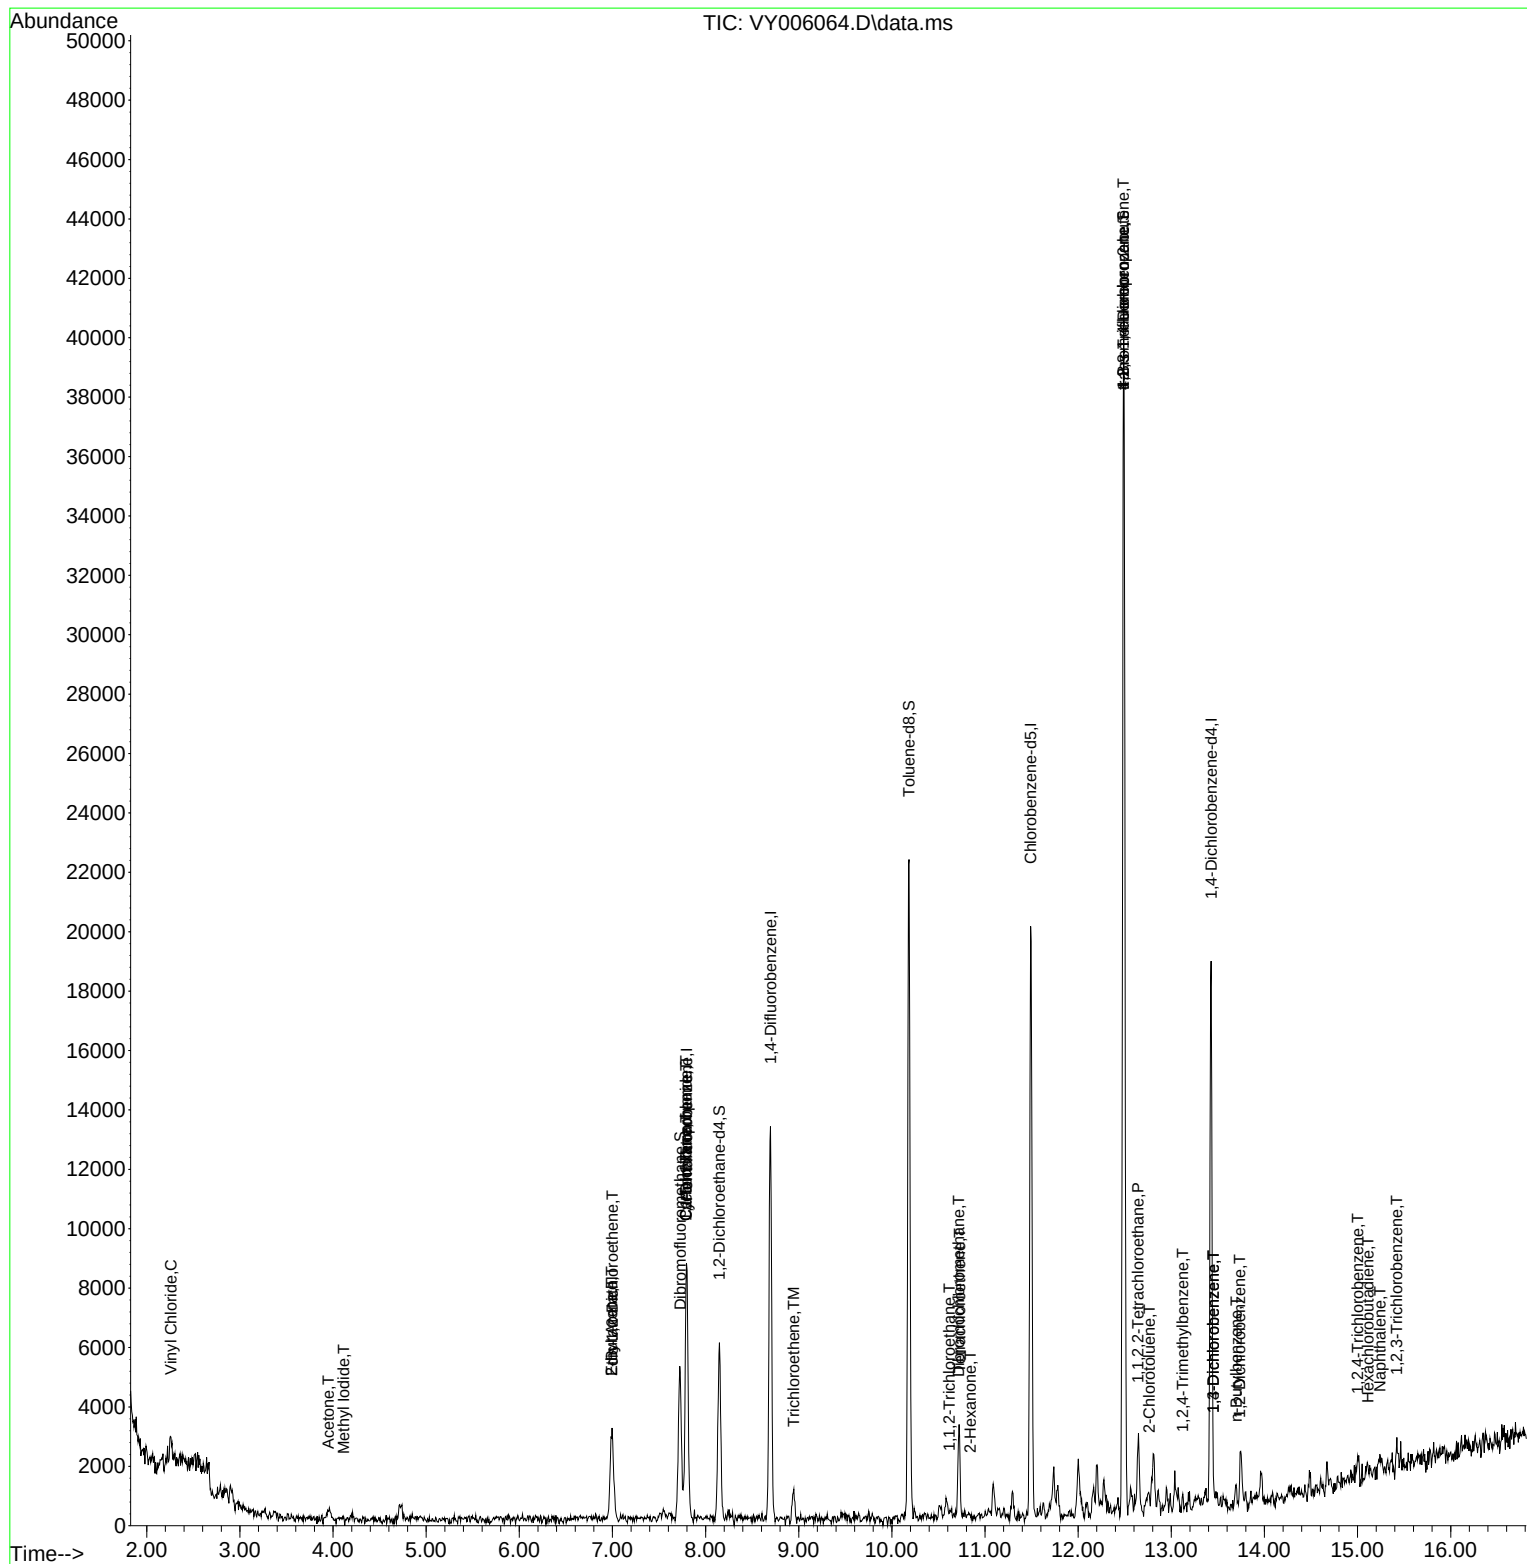




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.795 min Scan# 980
Delta R.T. -0.000 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32




Instrument :
MSVOA_Y
ClientSampleId :
NAPL-AREA-03-(25-27)RE


Tgt Ion:168 Resp: 6844
Ion Ratio Lower Upper
168 100
99 52.1 46.9 70.3

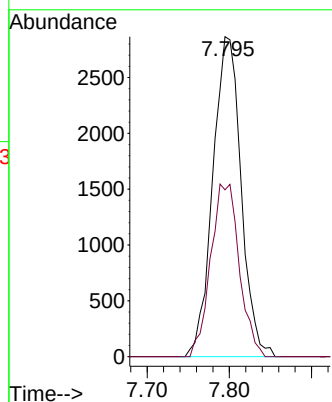

#4
Vinyl Chloride
Concen: 8.541 ug/l
RT: 2.259 min Scan# 72
Delta R.T. 0.006 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32


Tgt Ion: 62 Resp: 867
Ion Ratio Lower Upper
62 100
64 45.8 25.0 37.6#

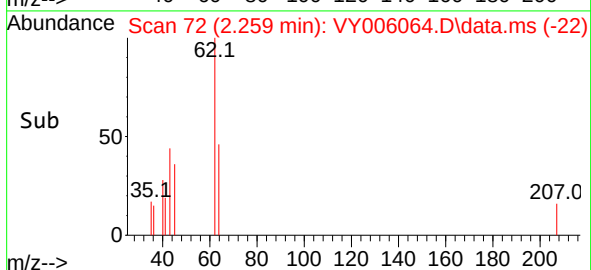



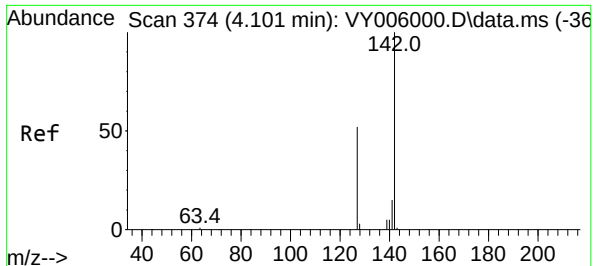


#10
Methyl Iodide
Concen: 2.345 ug/l
RT: 4.112 min Scan# 376
Delta R.T. 0.012 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32

Instrument :
MSVOA_Y
ClientSampleId :
NAPL-AREA-03-(25-27)RE



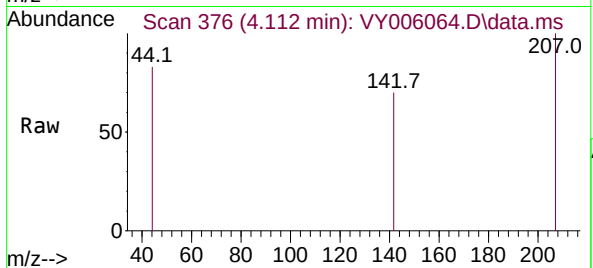



Tgt Ion:142 Resp: 164
Ion Ratio Lower Upper
142 100
127 0.0 41.5 62.3#
141 0.0 11.9 17.9#

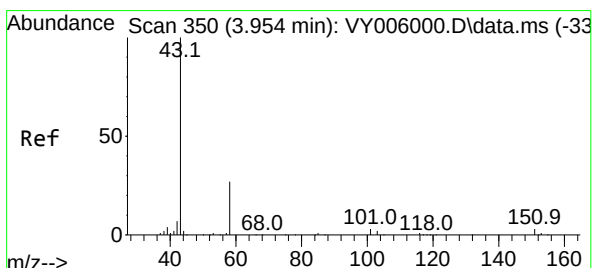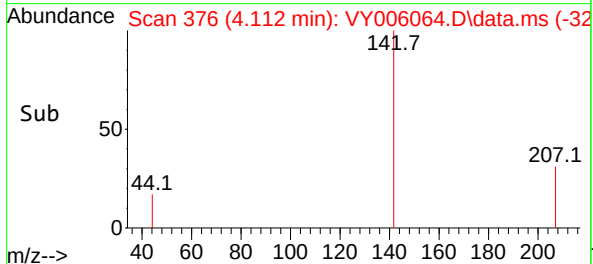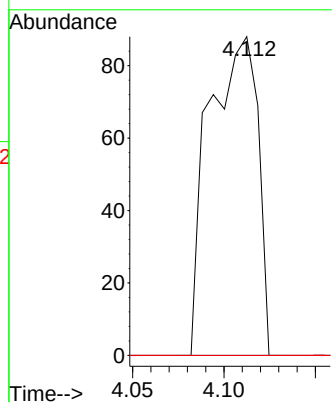

#16
Acetone
Concen: 28.226 ug/l
RT: 3.948 min Scan# 349
Delta R.T. -0.006 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32

Tgt Ion: 43 Resp: 736
Ion Ratio Lower Upper
43 100
58 40.0 22.0 33.0#

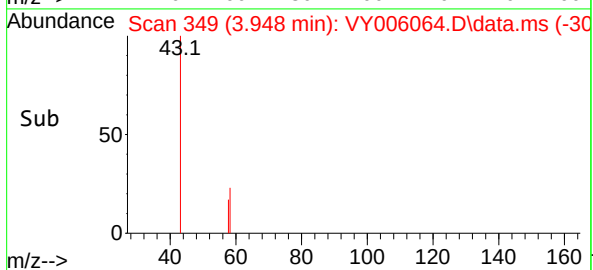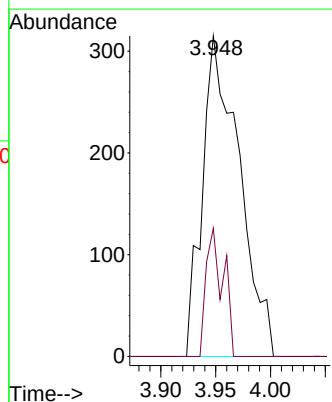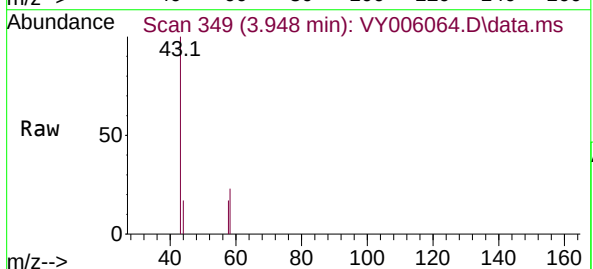



#25

2-Butanone

Concen: 2.476 ug/l

RT: 6.990 min Scan# 848

Delta R.T. -0.006 min

Lab File: VY006064.D

Acq: 17 Sep 2021 12:32

Instrument :

MSVOA_Y

ClientSampleId :





NAPL-AREA-03-(25-27)RE

Tgt Ion: 43 Resp: 89

Ion Ratio Lower Upper

43 100

72 0.0 17.7 26.5#

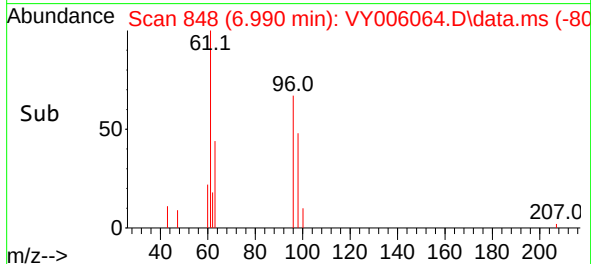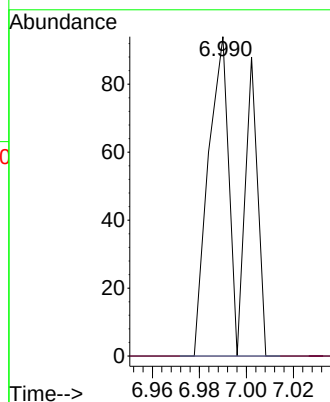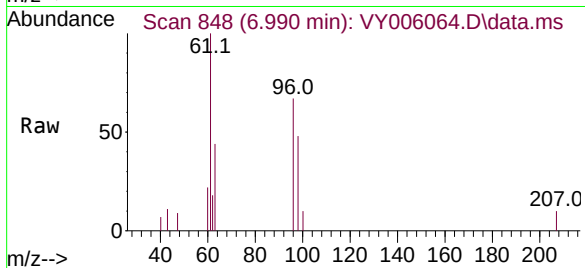

#27

cis-1,2-Dichloroethene

Concen: 22.342 ug/l

RT: 6.996 min Scan# 849

Delta R.T. -0.000 min

Lab File: VY006064.D

Acq: 17 Sep 2021 12:32




Tgt Ion: 96 Resp: 1910


Ion Ratio Lower Upper

96 100

61 135.7 0.0 319.8


98 64.0 0.0 127.0

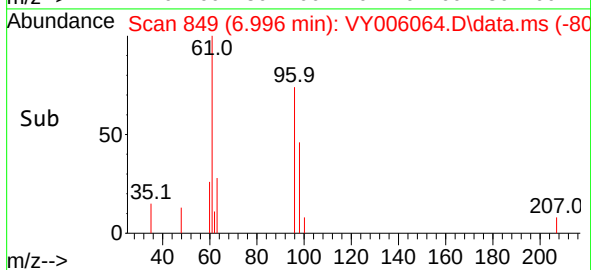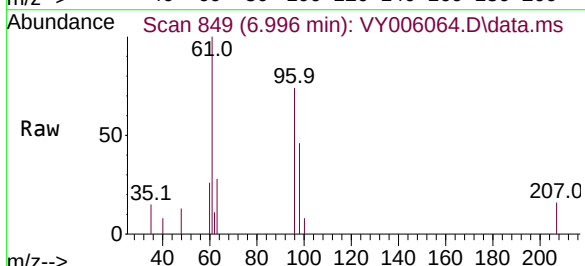






#31
Cyclohexane
Concen: 1.057 ug/l
RT: 7.789 min Scan# 979
Delta R.T. -0.000 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32


Instrument :
MSVOA_Y
ClientSampleId :
NAPL-AREA-03-(25-27)RE

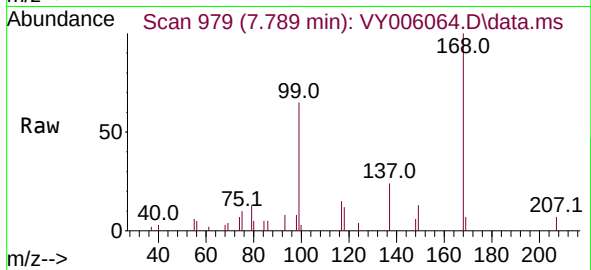



Tgt Ion: 56 Resp: 161
Ion Ratio Lower Upper
56 100
69 76.3 26.7 40.1#
84 94.7 67.2 100.8

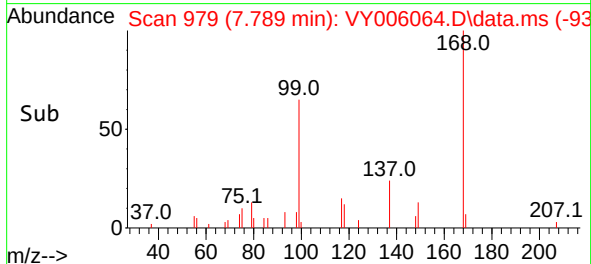


#33
1,2-Dichloroethane-d4
Concen: 51.585 ug/l
RT: 8.148 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32




Tgt Ion: 65 Resp: 4904
Ion Ratio Lower Upper
65 100
67 51.4 0.0 99.4








#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32


Instrument :
MSVOA_Y
ClientSampleId :
NAPL-AREA-03-(25-27)RE





Tgt Ion:	114	Resp:	11017
Ion Ratio	Lower	Upper	
114	100		
63	22.1	0.0	43.2
88	15.0	0.0	31.8

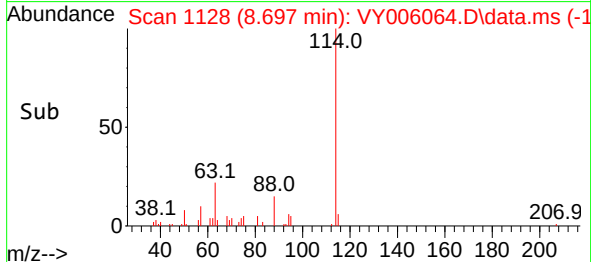


#35
Dibromofluoromethane
Concen: 51.762 ug/l
RT: 7.728 min Scan# 969
Delta R.T. -0.000 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32

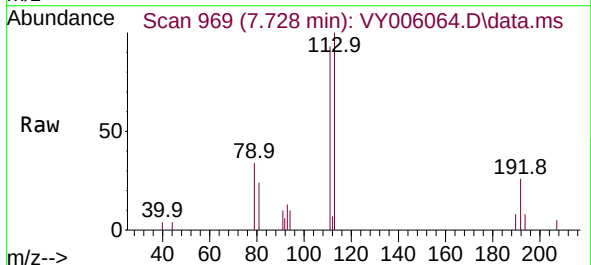

Tgt Ion:	113	Resp:	3542
Ion Ratio	Lower	Upper	
113	100		
111	94.3	82.6	124.0
192	22.6	17.6	26.4

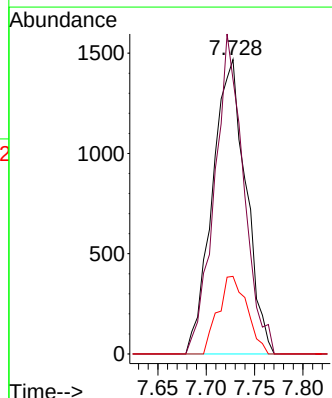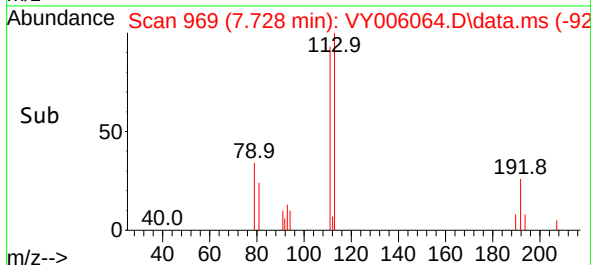



#36

1,1-Dichloropropene

Concen: 4.499 ug/l

RT: 7.789 min Scan# 979

Delta R.T. -0.134 min

Lab File: VY006064.D


Acq: 17 Sep 2021 12:32

Instrument :




MSVOA_Y

ClientSampleId :

NAPL-AREA-03-(25-27)RE



Tgt Ion: 75	Resp: 535
Ion Ratio	Lower Upper
75	100
110	0.0 17.1 51.2#
77	0.0 24.4 36.6#

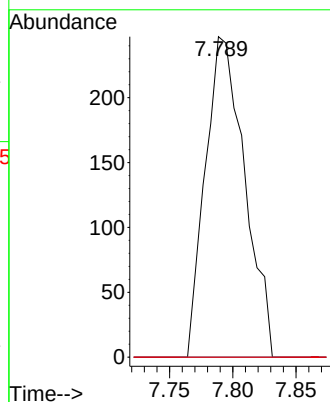

#37

Ethyl Acetate

Concen: 1.083 ug/l




RT: 6.990 min Scan# 848


Delta R.T. -0.092 min

Lab File: VY006064.D

Acq: 17 Sep 2021 12:32


Tgt Ion: 43	Resp: 89
Ion Ratio	Lower Upper
43	100
61	2912.4 9.7 14.5#
70	0.0 7.1 10.7#

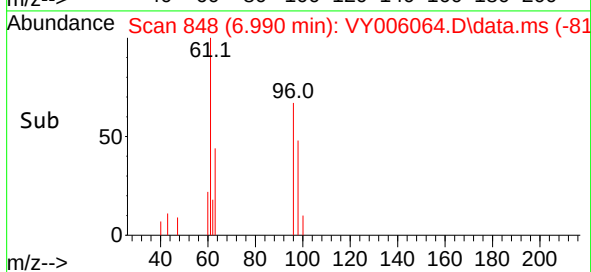






#38
Carbon Tetrachloride
Concen: 5.006 ug/l
RT: 7.789 min Scan# 979
Delta R.T. -0.116 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32

Instrument :
MSVOA_Y
ClientSampleId :
NAPL-AREA-03-(25-27)RE



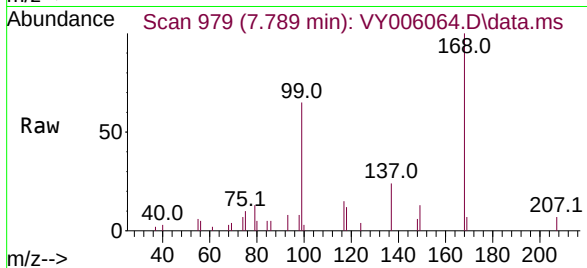



Tgt Ion:117 Resp: 648
Ion Ratio Lower Upper
117 100
119 0.0 77.9 116.9#
121 0.0 24.8 37.2#

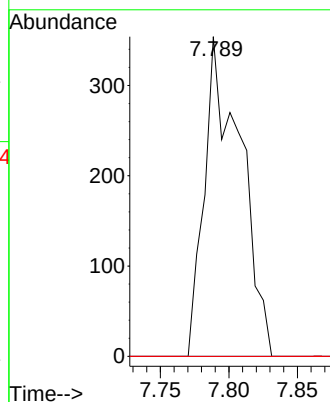

#44
Trichloroethene
Concen: 5.555 ug/l
RT: 8.947 min Scan# 1169
Delta R.T. -0.000 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32

Tgt Ion:130 Resp: 472
Ion Ratio Lower Upper
130 100
95 96.1 0.0 188.2



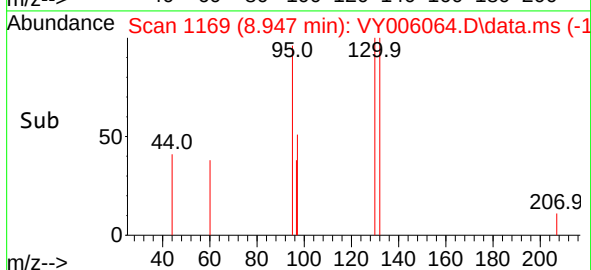
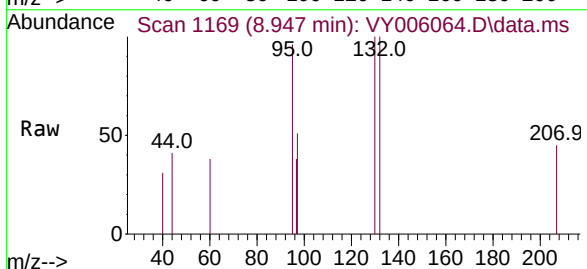


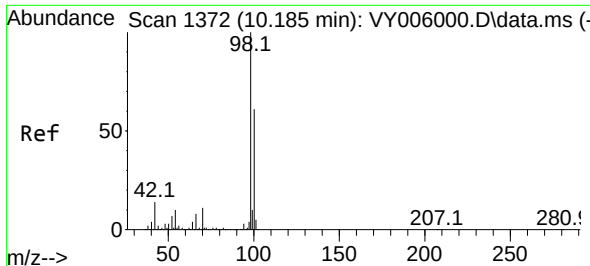

#50
Toluene-d8
Concen: 47.393 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32




Instrument :
MSVOA_Y
ClientSampleId :
NAPL-AREA-03-(25-27)RE


Tgt Ion: 98 Resp: 13822
Ion Ratio Lower Upper
98 100
100 66.1 50.2 75.2

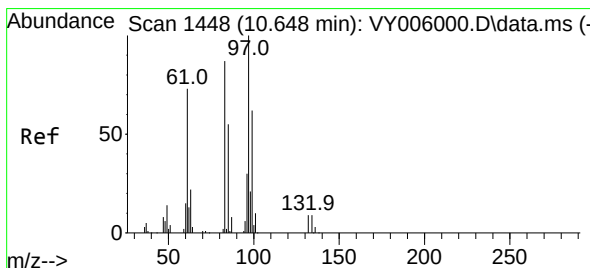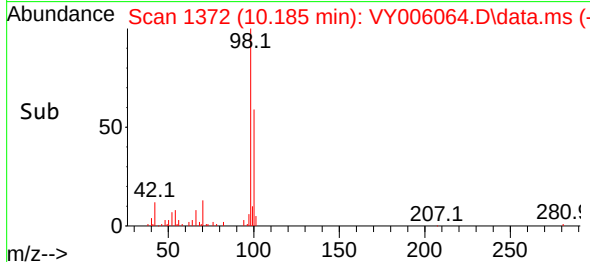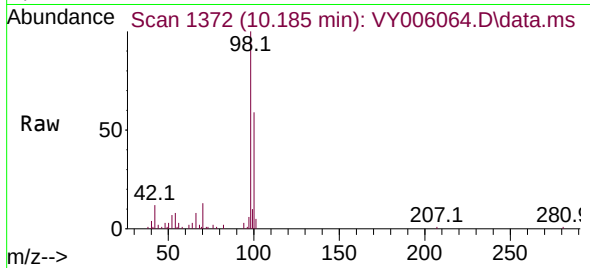

#55
1,1,2-Trichloroethane
Concen: 1.642 ug/l
RT: 10.617 min Scan# 1443
Delta R.T. -0.031 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32

Tgt Ion: 97 Resp: 103
Ion Ratio Lower Upper
97 100
83 0.0 69.8 104.8#
85 0.0 44.3 66.5#
99 0.0 49.8 74.6#


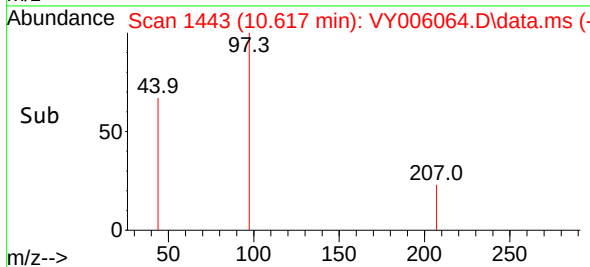

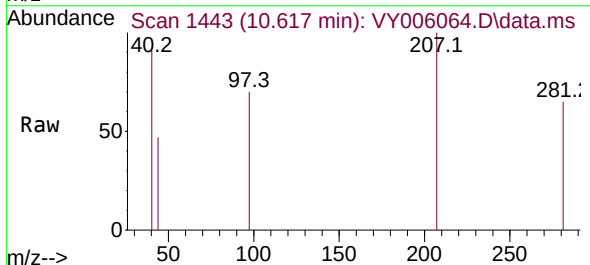




#59
2-Hexanone
Concen: 1.172 ug/l
RT: 10.843 min Scan# 1480
Delta R.T. 0.006 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32




Instrument :
MSVOA_Y
ClientSampleId :
NAPL-AREA-03-(25-27)RE


Tgt Ion: 43 Resp: 66
Ion Ratio Lower Upper
43 100
58 0.0 24.4 73.4#

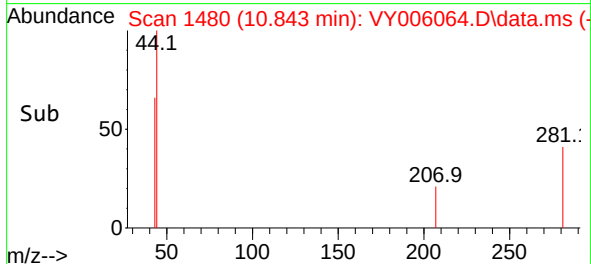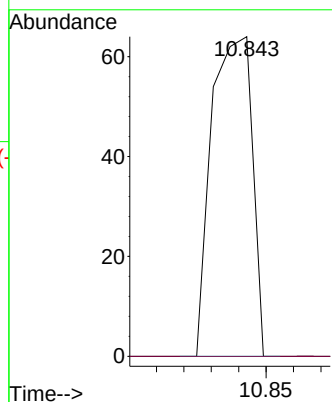

#60
Dibromochloromethane
Concen: 8.209 ug/l
RT: 10.715 min Scan# 1459
Delta R.T. -0.269 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32

Tgt Ion: 129 Resp: 635
Ion Ratio Lower Upper
129 100
127 0.0 38.7 116.1#



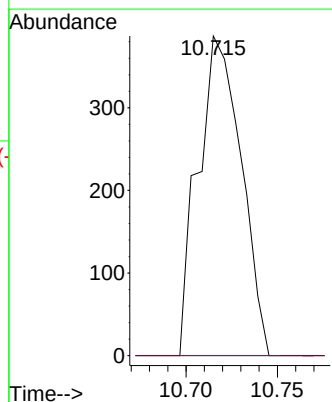





#62
4-Bromofluorobenzene
Concen: 44.790 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32




Instrument :
MSVOA_Y
ClientSampleId :
NAPL-AREA-03-(25-27)RE


Tgt Ion:	95	Resp:	4435
Ion Ratio	Lower	Upper	
95	100		
174	90.4	0.0	177.0
176	83.3	0.0	175.8

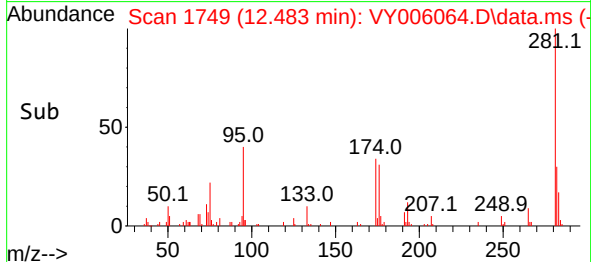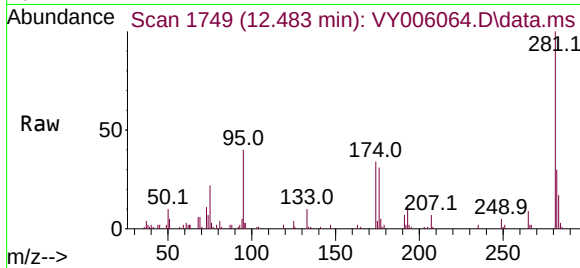

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. -0.006 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32

Tgt Ion:	117	Resp:	10861
Ion Ratio	Lower	Upper	
117	100		
82	56.8	43.0	64.4
119	36.6	25.4	38.0




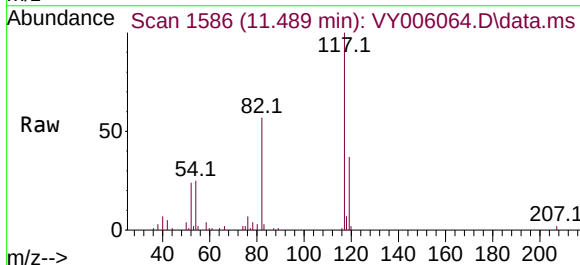




#64
Tetrachloroethene
Concen: 7.295 ug/l
RT: 10.727 min Scan# 1461
Delta R.T. 0.006 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32




Instrument :
MSVOA_Y
ClientSampleId :
NAPL-AREA-03-(25-27)RE


Tgt Ion:164	Resp:	648	
Ion	Ratio	Lower	Upper
164	100		
166	86.4	100.4	150.6#
129	75.5	71.4	107.0
131	69.9	70.8	106.2#

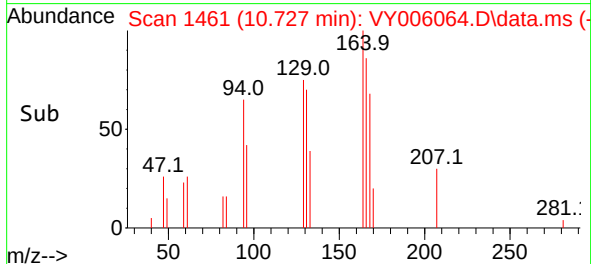

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32

Tgt Ion:152	Resp:	4597	
Ion	Ratio	Lower	Upper
152	100		
115	54.2	28.2	84.7
150	161.5	0.0	347.6









#75
1,1,2,2-Tetrachloroethane
Concen: 2.314 ug/l
RT: 12.641 min Scan# 1775
Delta R.T. 0.061 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32




Instrument :
MSVOA_Y
ClientSampleId :
NAPL-AREA-03-(25-27)RE


Tgt Ion: 83 Resp: 155
Ion Ratio Lower Upper
83 100
131 0.0 5.6 16.8#
85 0.0 32.3 96.8#

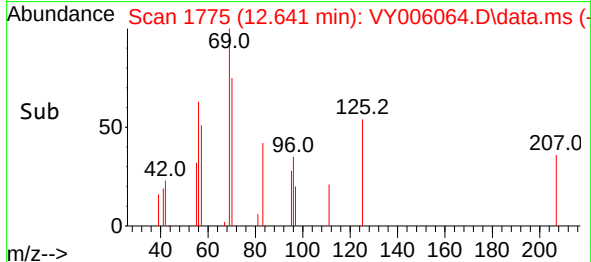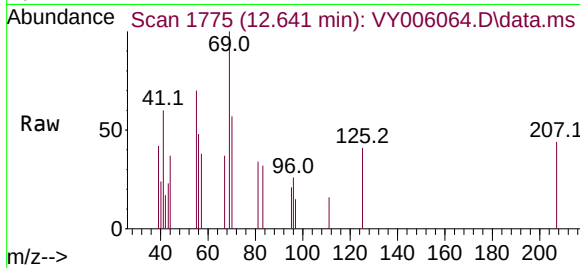

#76
1,2,3-Trichloropropane
Concen: 54.782 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.153 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32

Tgt Ion: 75 Resp: 2685
Ion Ratio Lower Upper
75 100
77 2.0 0.0 0.0#




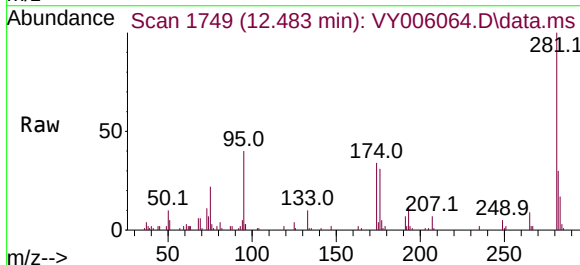




#79
2-Chlorotoluene
Concen: 1.020 ug/l
RT: 12.763 min Scan# 1795
Delta R.T. 0.006 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32




Instrument :
MSVOA_Y
ClientSampleId :
NAPL-AREA-03-(25-27)RE


Tgt Ion: 91 Resp: 247
Ion Ratio Lower Upper
91 100
126 18.6 16.9 50.6



#81
trans-1,4-Dichloro-2-butene
Concen: 100.717 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.103 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32

Tgt Ion: 75 Resp: 2685
Ion Ratio Lower Upper
75 100
53 0.0 85.3 127.9#
89 0.0 37.0 55.4#


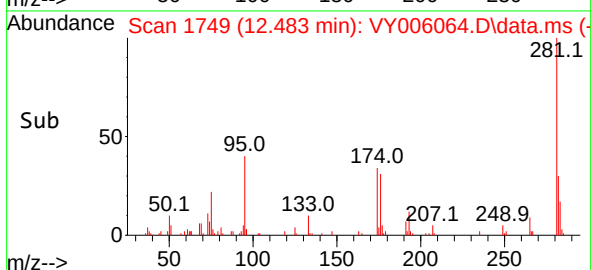






#84
1,2,4-Trimethylbenzene
Concen: 1.242 ug/l
RT: 13.123 min Scan# 1854
Delta R.T. -0.000 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32




Instrument :
MSVOA_Y
ClientSampleId :
NAPL-AREA-03-(25-27)RE


Tgt Ion:105 Resp: 368
Ion Ratio Lower Upper
105 100
120 26.9 22.3 66.9

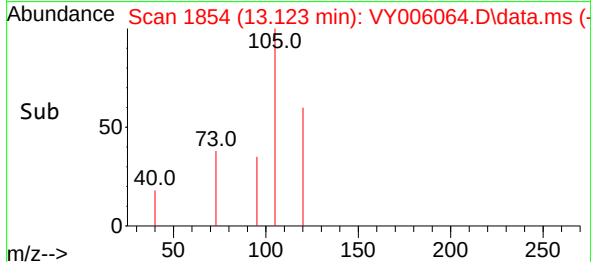

#87
1,3-Dichlorobenzene
Concen: 1.438 ug/l
RT: 13.452 min Scan# 1908
Delta R.T. 0.085 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32

Tgt Ion:146 Resp: 233
Ion Ratio Lower Upper
146 100
111 41.2 19.5 58.5
148 43.3 31.6 95.0




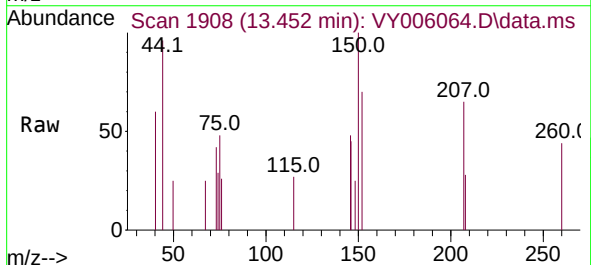




#88
1,4-Dichlorobenzene
Concen: 1.434 ug/l
RT: 13.452 min Scan# 1908
Delta R.T. 0.006 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32




Instrument :
MSVOA_Y
ClientSampleId :
NAPL-AREA-03-(25-27)RE


Tgt Ion:146 Resp: 233
Ion Ratio Lower Upper
146 100
111 41.2 19.3 57.8
148 43.3 32.6 97.8

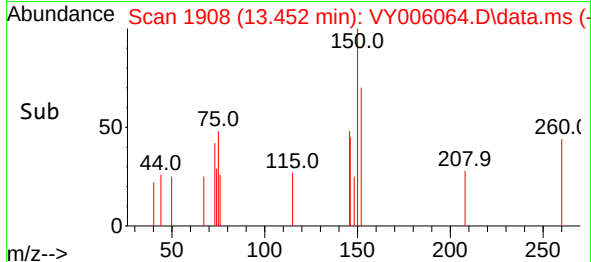

#89
n-Butylbenzene
Concen: 1.458 ug/l
RT: 13.696 min Scan# 1948
Delta R.T. -0.000 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32

Tgt Ion: 91 Resp: 445
Ion Ratio Lower Upper
91 100
92 39.1 26.3 78.9
134 5.6 13.0 38.9#


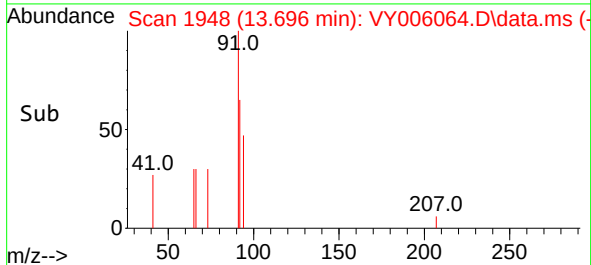






#91
1,2-Dichlorobenzene
Concen: 1.758 ug/l
RT: 13.733 min Scan# 1954
Delta R.T. -0.006 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32




Instrument :
MSVOA_Y
ClientSampleId :
NAPL-AREA-03-(25-27)RE


Tgt Ion:	146	Resp:	250
Ion	Ratio	Lower	Upper
146	100		
111	24.0	20.3	60.9
148	48.0	32.3	96.9

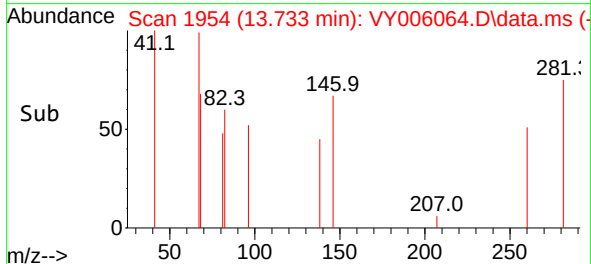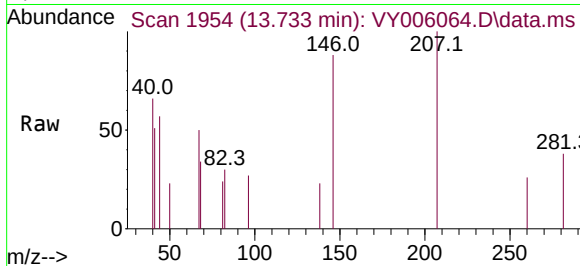

#93
1,2,4-Trichlorobenzene
Concen: 3.314 ug/l
RT: 15.001 min Scan# 2162
Delta R.T. -0.006 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32

Tgt Ion:	180	Resp:	306
Ion	Ratio	Lower	Upper
180	100		
182	85.6	47.3	141.9
145	21.6	14.6	43.8




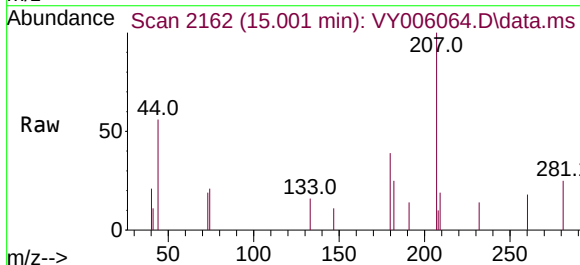




#94
Hexachlorobutadiene
Concen: 2.042 ug/l
RT: 15.110 min Scan# 2180
Delta R.T. -0.000 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32




Instrument :
MSVOA_Y
ClientSampleId :
NAPL-AREA-03-(25-27)RE


Tgt Ion:225 Resp: 122
Ion Ratio Lower Upper
225 100
223 26.2 30.8 92.3#
227 0.0 31.6 94.7#

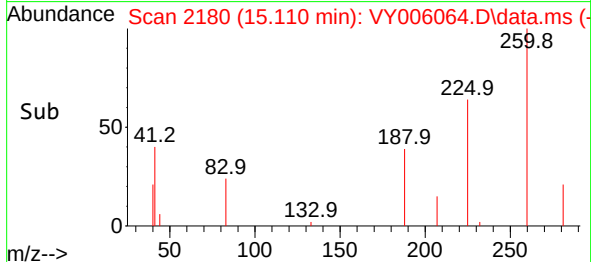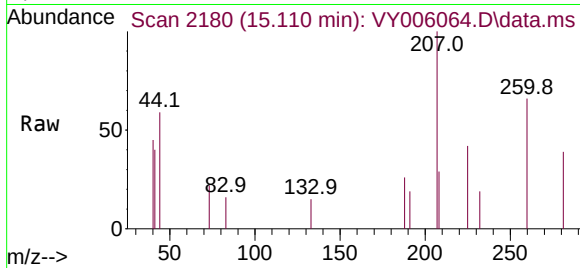

#95
Naphthalene
Concen: 3.550 ug/l
RT: 15.239 min Scan# 2201
Delta R.T. 0.006 min
Lab File: VY006064.D
Acq: 17 Sep 2021 12:32

Tgt Ion:128 Resp: 652
Ion Ratio Lower Upper
128 100
127 0.0 11.0 16.4#
129 0.0 8.4 12.6#

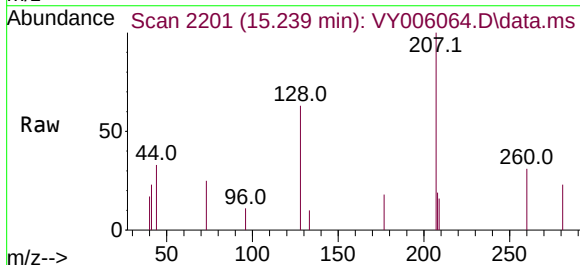



#96
 1,2,3-Trichlorobenzene
 Concen: 4.511 ug/l
 RT: 15.421 min Scan# 2231
 Delta R.T. -0.000 min
 Lab File: VY006064.D
 Acq: 17 Sep 2021 12:32

Instrument :
 MSVOA_Y
 ClientSampleId :
 NAPL-AREA-03-(25-27)RE

Tgt Ion:180 Resp: 361
 Ion Ratio Lower Upper
 180 100
 182 69.0 47.3 141.9
 145 0.0 15.3 45.9#

