

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091721\
 Data File : VY006061.D
 Acq On : 17 Sep 2021 11:14
 Operator : SY/MD
 Sample : VY0917SBL01
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0917SBL01

Quant Time: Sep 20 01:37:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091421S.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 15 05:01:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	102917	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	191700	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	212235	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	106231	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	78677	55.035	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	110.080%
35) Dibromofluoromethane	7.722	113	58733	49.327	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	98.660%
50) Toluene-d8	10.179	98	251868	49.632	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	99.260%
62) 4-Bromofluorobenzene	12.483	95	96019	55.729	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	111.460%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091721\
Data File : VY006061.D
Acq On : 17 Sep 2021 11:14
Operator : SY/MD
Sample : VY0917SBL01
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0917SBL01

Quant Time: Sep 20 01:37:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091421S.M
Quant Title : SW846 8260
QLast Update : Wed Sep 15 05:01:47 2021
Response via : Initial Calibration




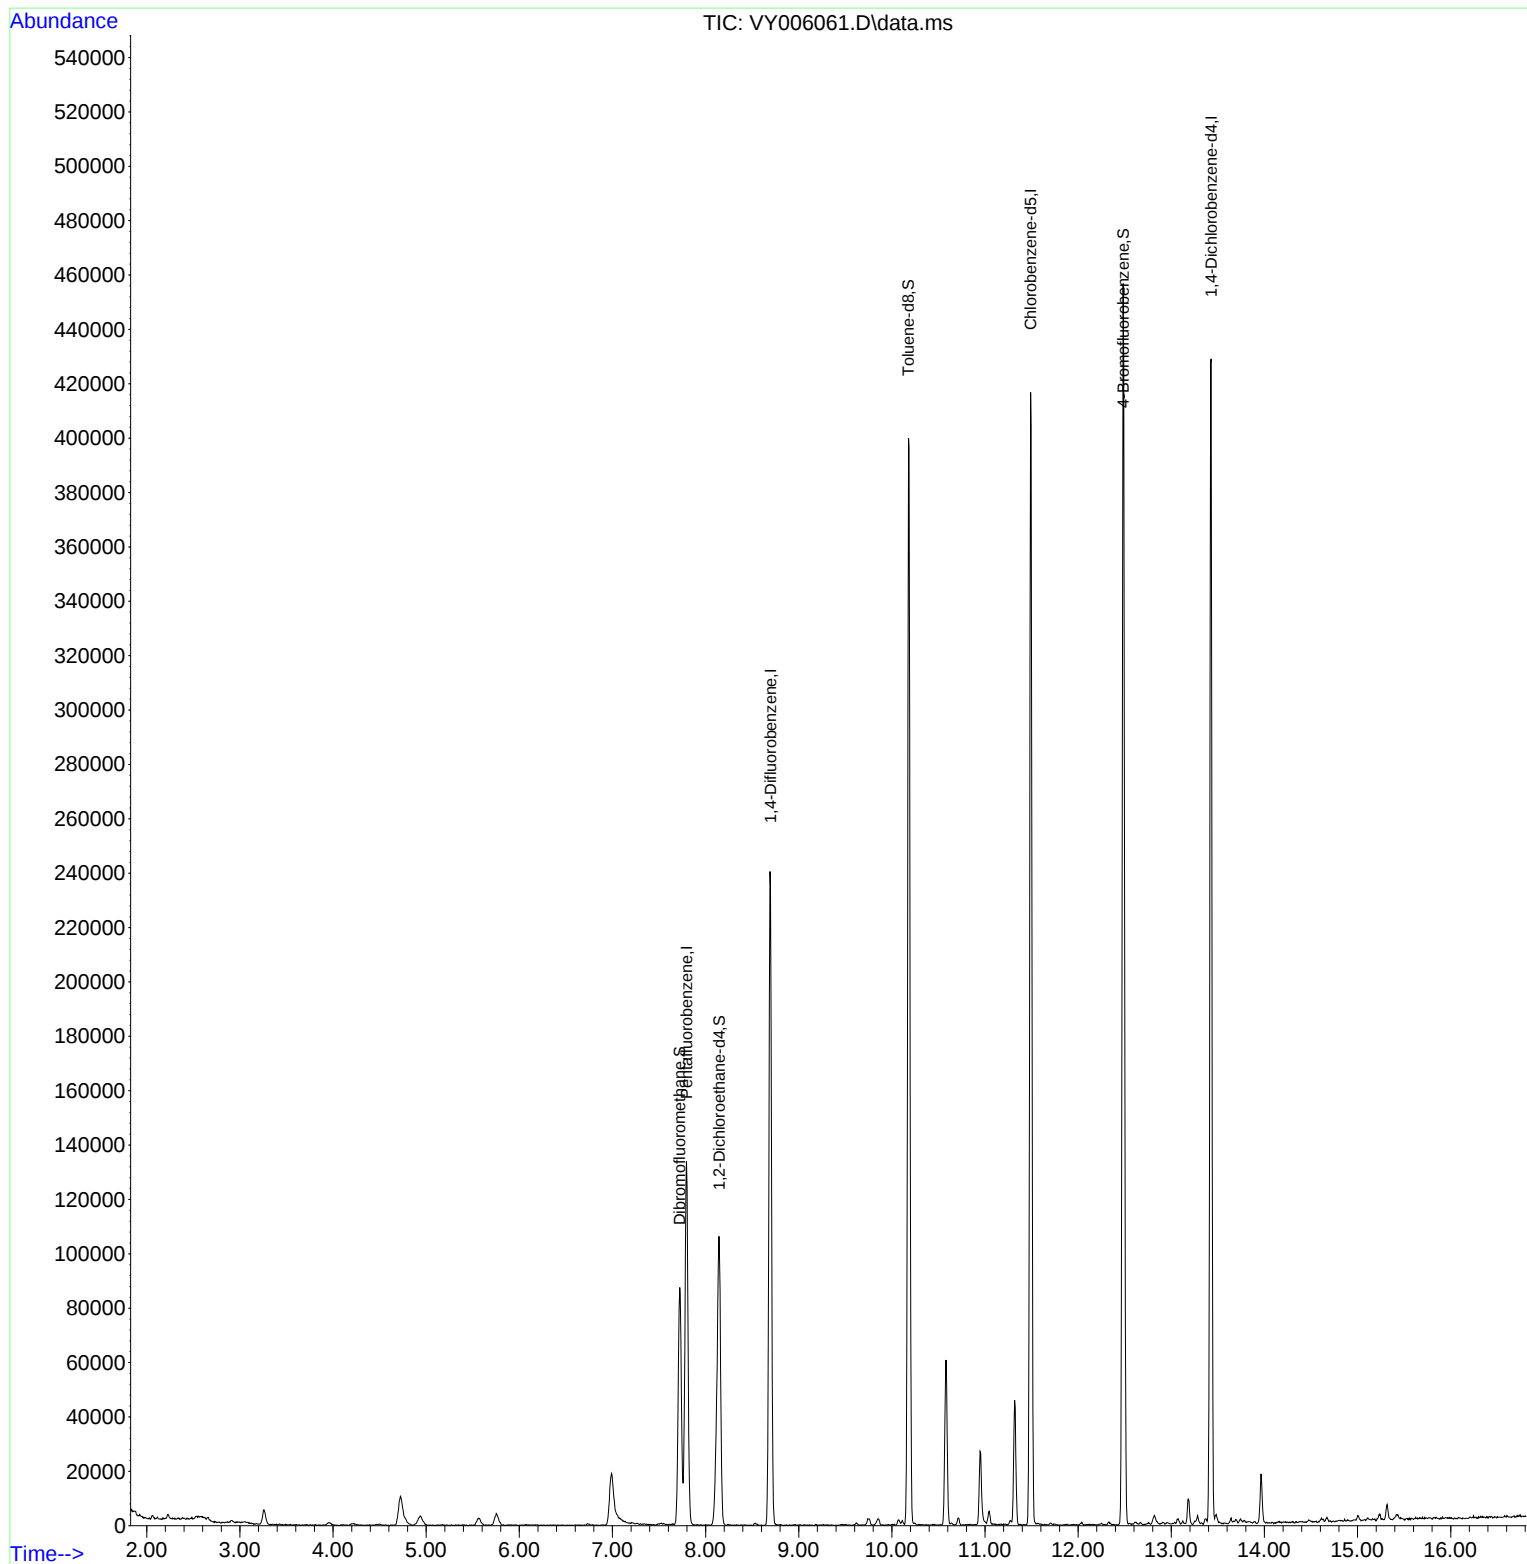


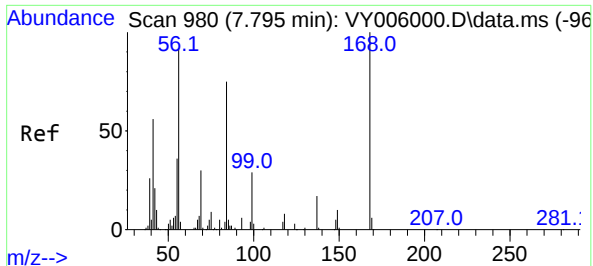

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.795 min Scan# 980
Delta R.T. -0.000 min
Lab File: VY006061.D
Acq: 17 Sep 2021 11:14




Instrument :
MSVOA_Y
ClientSampleId :
VY0917SBL01


Tgt Ion:168 Resp: 102917
Ion Ratio Lower Upper
168 100
99 54.9 46.9 70.3

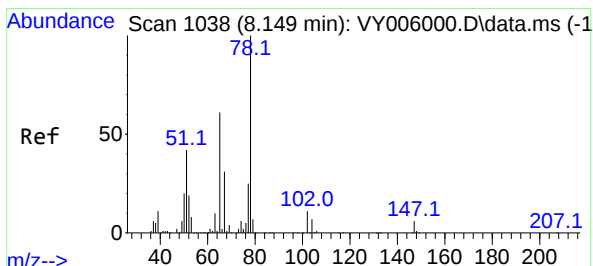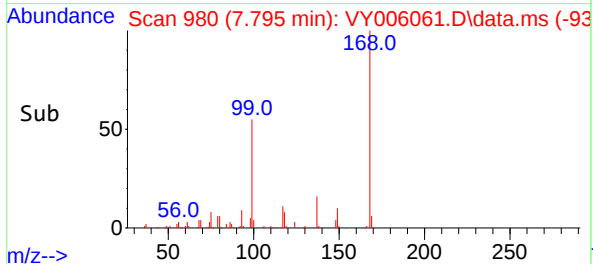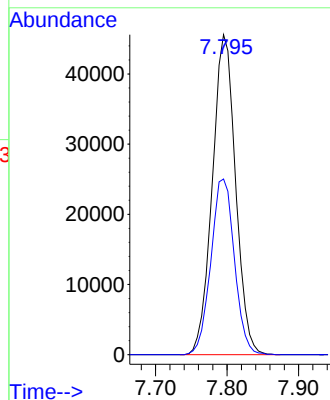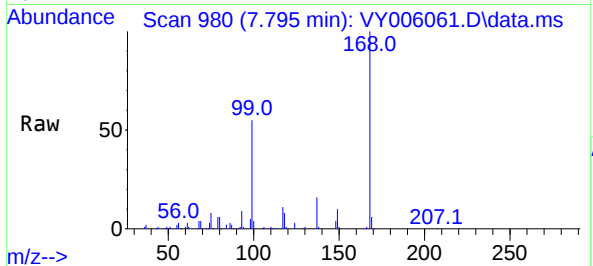

#33
1,2-Dichloroethane-d4
Concen: 55.035 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VY006061.D
Acq: 17 Sep 2021 11:14

Tgt Ion: 65 Resp: 78677
Ion Ratio Lower Upper
65 100
67 49.2 0.0 99.4


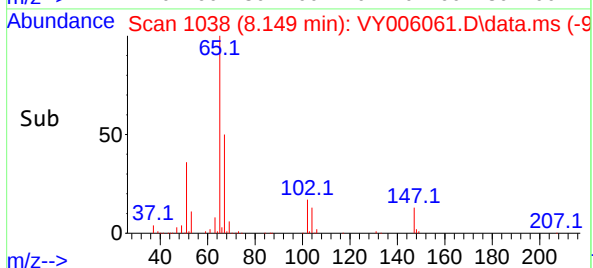
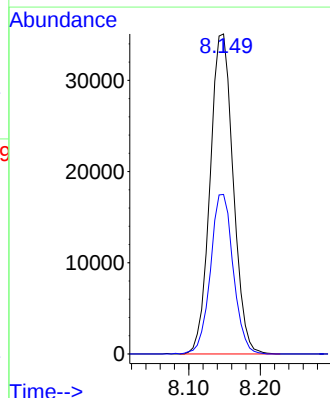
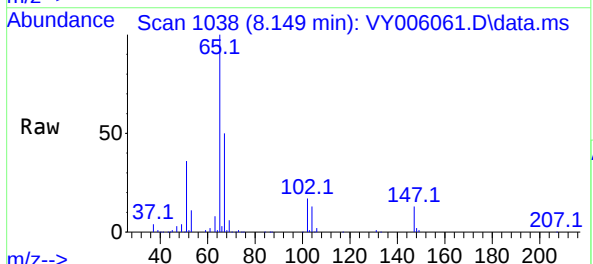


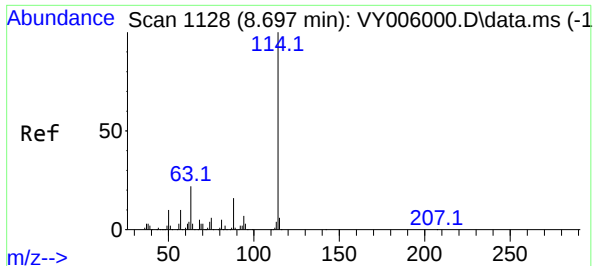

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VY006061.D
Acq: 17 Sep 2021 11:14




Instrument :
MSVOA_Y
ClientSampleId :
VY0917SBL01


Tgt Ion:	114	Resp:	191700
Ion	Ratio	Lower	Upper
114	100		
63	21.3	0.0	43.2
88	14.8	0.0	31.8

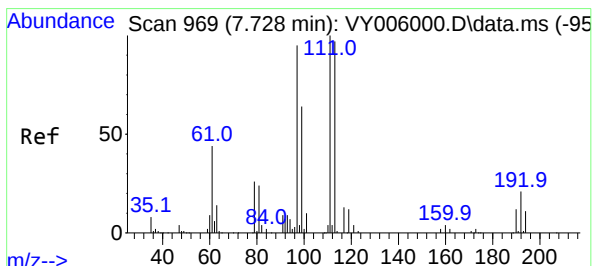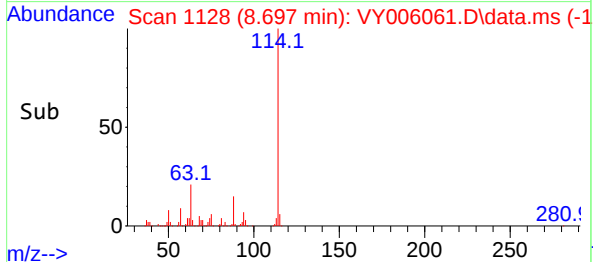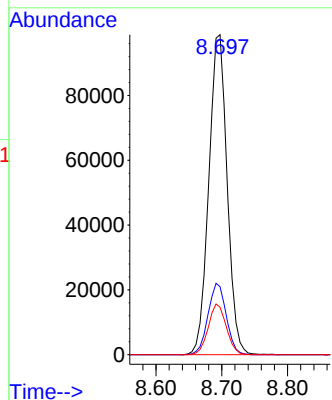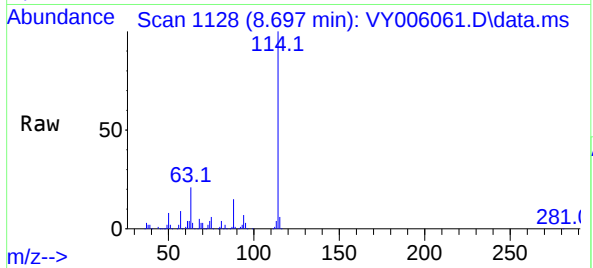

#35
Dibromofluoromethane
Concen: 49.327 ug/l
RT: 7.722 min Scan# 968
Delta R.T. -0.006 min
Lab File: VY006061.D
Acq: 17 Sep 2021 11:14

Tgt Ion:	113	Resp:	58733
Ion	Ratio	Lower	Upper
113	100		
111	103.0	82.6	124.0
192	21.9	17.6	26.4


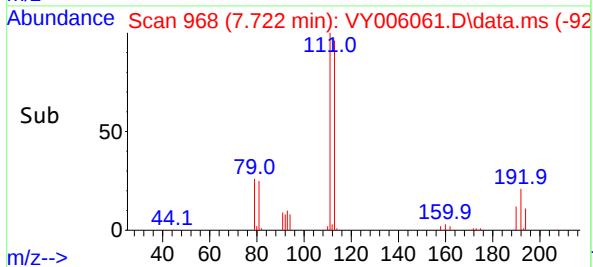
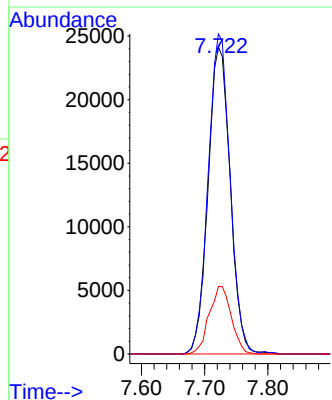
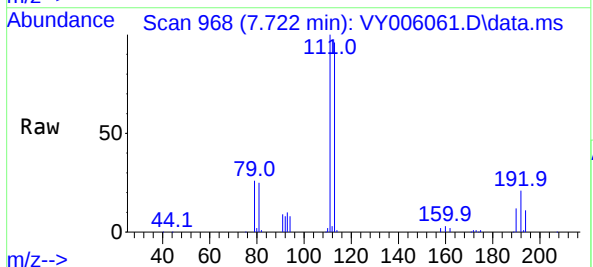


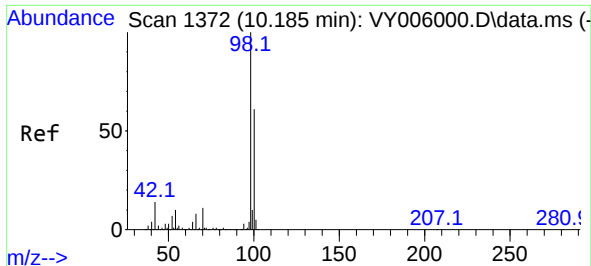

#50
Toluene-d8
Concen: 49.632 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.006 min
Lab File: VY006061.D
Acq: 17 Sep 2021 11:14




Instrument :
MSVOA_Y
ClientSampleId :
VY0917SBL01


Tgt Ion: 98 Resp: 251868
Ion Ratio Lower Upper
98 100
100 63.8 50.2 75.2

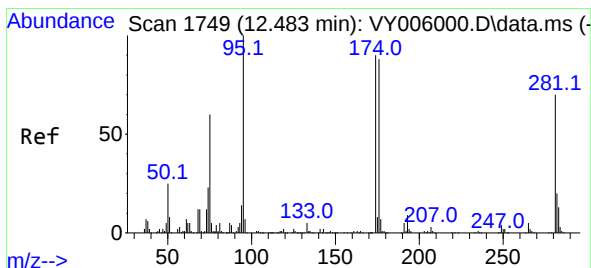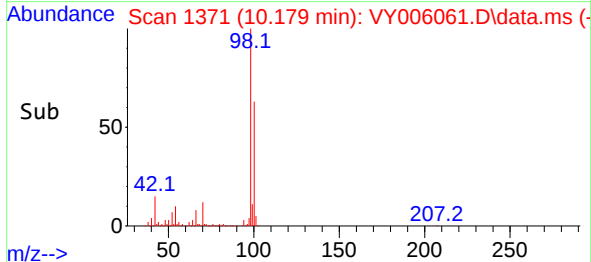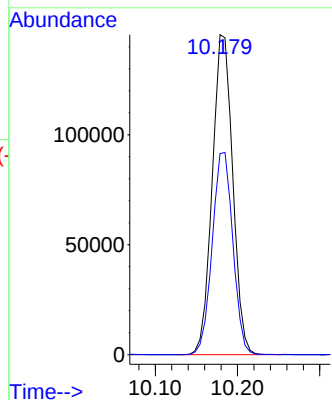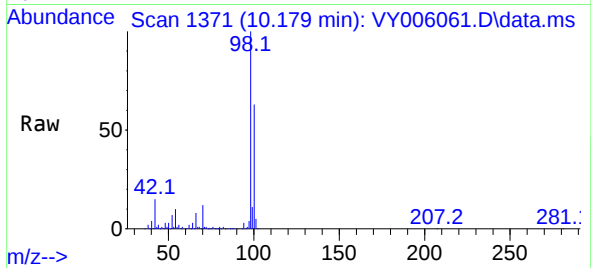

#62
4-Bromofluorobenzene
Concen: 55.729 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY006061.D
Acq: 17 Sep 2021 11:14

Tgt Ion: 95 Resp: 96019
Ion Ratio Lower Upper
95 100
174 90.4 0.0 177.0
176 87.6 0.0 175.8


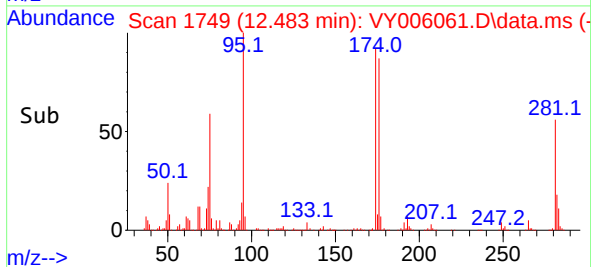
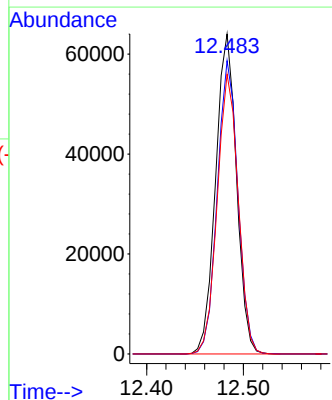
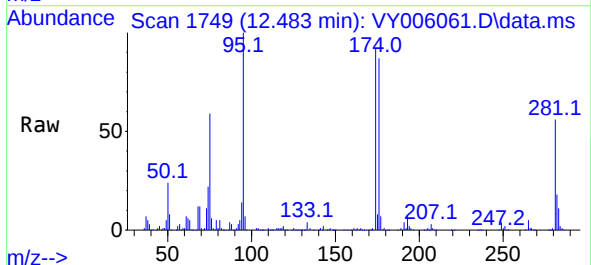


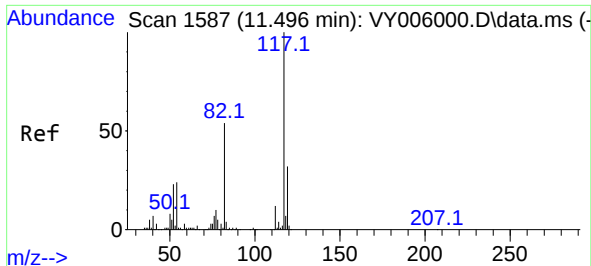

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. -0.006 min
Lab File: VY006061.D
Acq: 17 Sep 2021 11:14

Instrument :
MSVOA_Y
ClientSampleId :
VY0917SBL01

Tgt Ion:	117	Resp:	212235
Ion	Ratio	Lower	Upper
117	100		
82	56.8	43.0	64.4
119	32.3	25.4	38.0

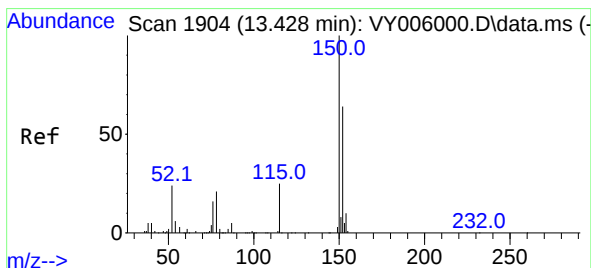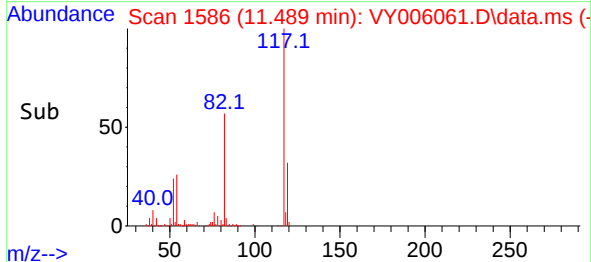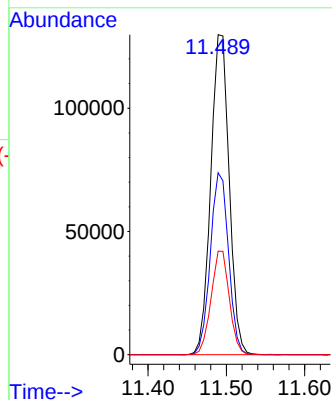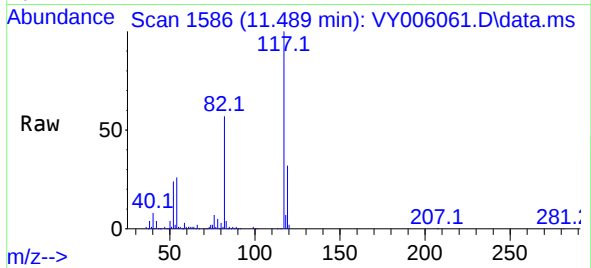

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY006061.D
Acq: 17 Sep 2021 11:14

Tgt Ion:	152	Resp:	106231
Ion	Ratio	Lower	Upper
152	100		
115	56.0	28.2	84.7
150	154.7	0.0	347.6

