


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv091819\
Data File : VY000058.D
Acq On : 18 Sep 2019 13:57
Operator : SY/MD
Sample : BFB
Misc : 5.00µl/5.00ml/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y091719S.M
Title : SW846 8260
Last Update : Thu Sep 19 05:38:39 2019

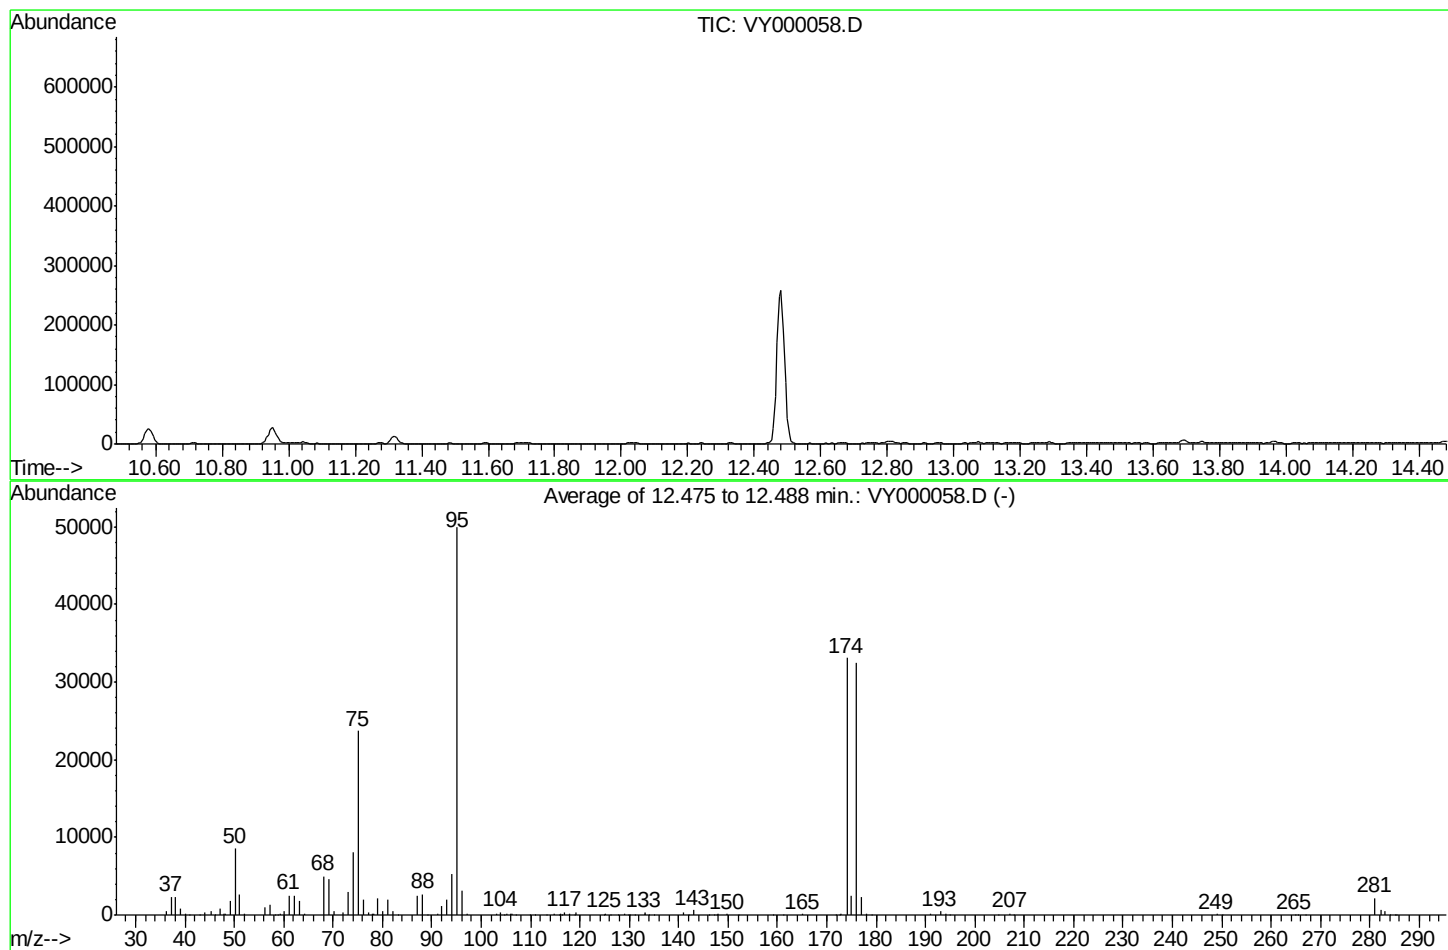

AutoFind: Scans 1786, 1787, 1788; Background Corrected with Scan 1777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	8506	PASS
75	95	30	60	47.4	23669	PASS
95	95	100	100	100.0	49933	PASS
96	95	5	9	6.4	3184	PASS
173	174	0.00	2	0.4	131	PASS
174	95	50	100	66.4	33133	PASS
175	174	5	9	7.5	2481	PASS
176	174	95	101	98.0	32456	PASS
177	176	5	9	7.2	2347	PASS