

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091824\
 Data File : VY019596.D
 Acq On : 18 Sep 2024 10:43
 Operator : SY/MD
 Sample : VY0918SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0918SBL01

Quant Time: Sep 19 01:23:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090924S.M
 Quant Title : SW846 8260
 QLast Update : Mon Sep 09 16:00:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.707	168	345018	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.615	114	661162	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	570722	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	202452	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.061	65	194630	60.921	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 121.840%	
35) Dibromofluoromethane	7.634	113	203149	54.192	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 108.380%	
50) Toluene-d8	10.109	98	775808	55.953	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 111.900%	
62) 4-Bromofluorobenzene	12.407	95	243380	45.651	ug/l	0.00
Spiked Amount	50.000	Range	29 - 146	Recovery	= 91.300%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY091824\
Data File : VY019596.D
Acq On : 18 Sep 2024 10:43
Operator : SY/MD
Sample : VY0918SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0918SBL01

Quant Time: Sep 19 01:23:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y090924S.M
Quant Title : SW846 8260
QLast Update : Mon Sep 09 16:00:30 2024
Response via : Initial Calibration




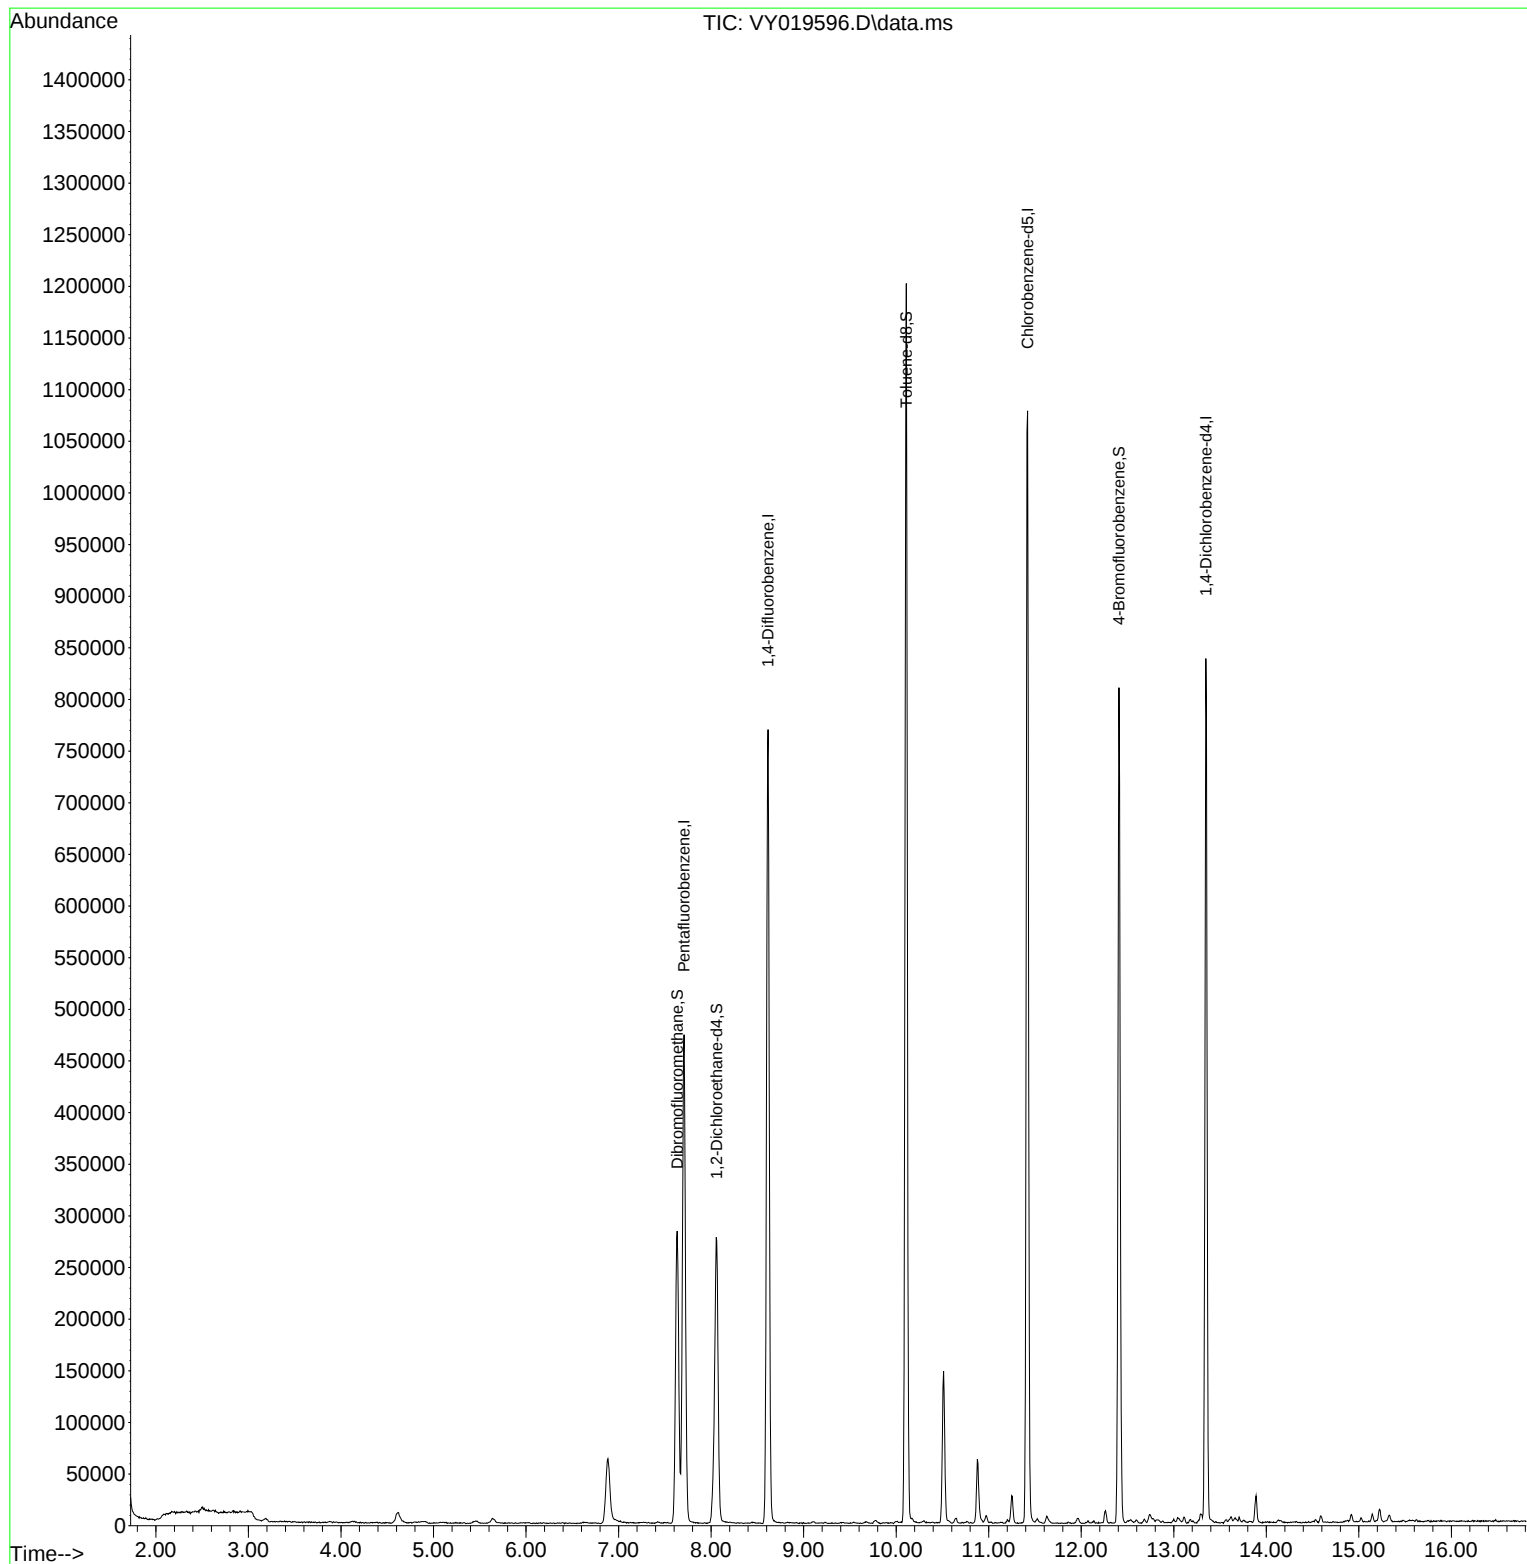


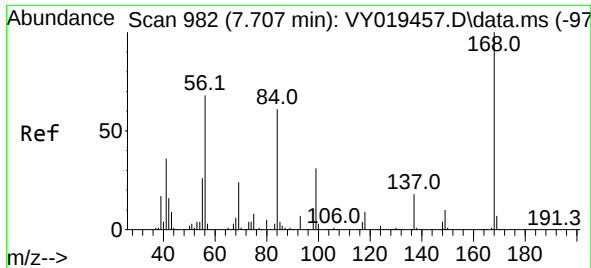

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.707 min Scan# 91
Delta R.T. 0.000 min
Lab File: VY019596.D
Acq: 18 Sep 2024 10:43




Instrument :
MSVOA_Y
ClientSampleId :
VY0918SBL01

Tgt Ion:168 Resp: 345018
Ion Ratio Lower Upper
168 100
99 61.9 39.1 58.7#

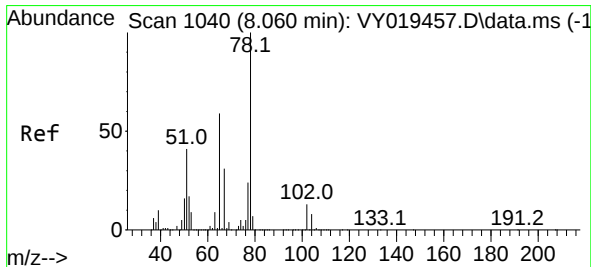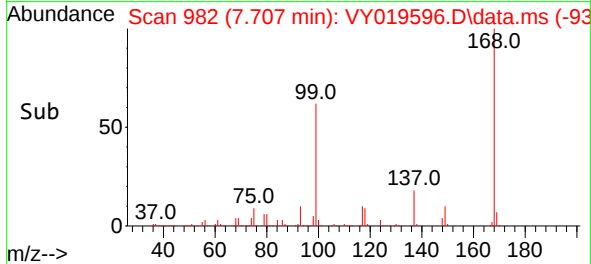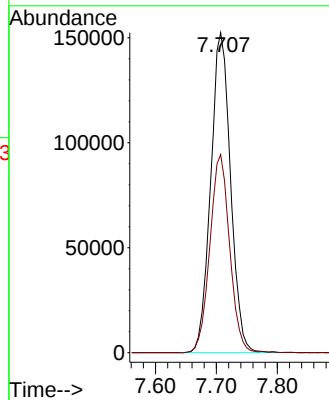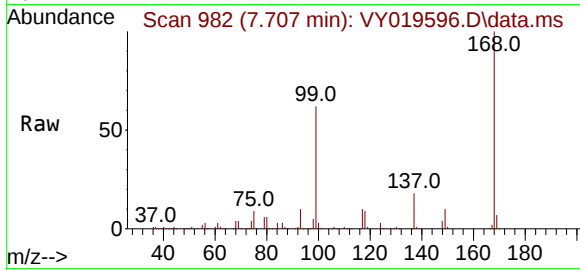

#33
1,2-Dichloroethane-d4
Concen: 60.921 ug/l
RT: 8.061 min Scan# 1040
Delta R.T. 0.000 min
Lab File: VY019596.D
Acq: 18 Sep 2024 10:43

Tgt Ion: 65 Resp: 194630
Ion Ratio Lower Upper
65 100
67 52.7 0.0 109.6

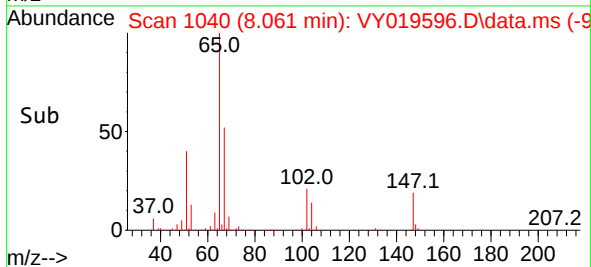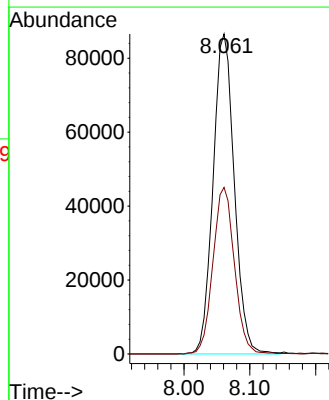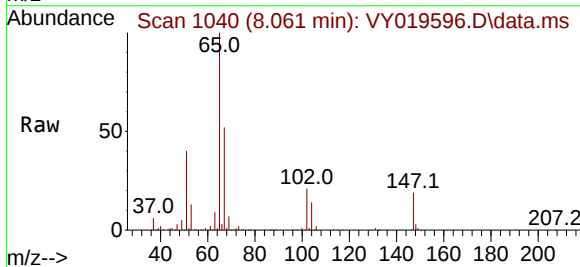



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.615 min Scan# 1131

Delta R.T. 0.000 min

Lab File: VY019596.D

Acq: 18 Sep 2024 10:43

Instrument :

MSVOA_Y

ClientSampleId :

VY0918SBL01





Tgt Ion:114 Resp: 661162

Ion Ratio Lower Upper

114 100

63 20.3 0.0 35.0

88 16.0 0.0 27.2

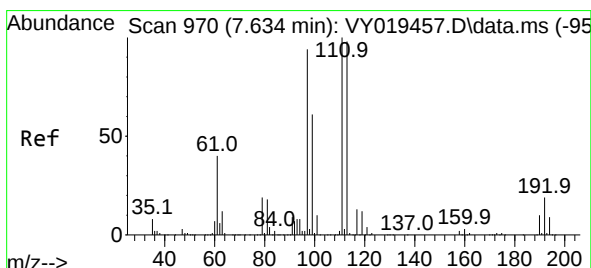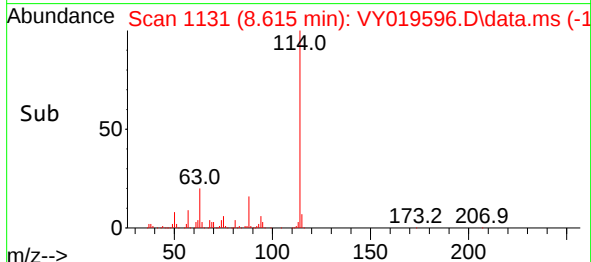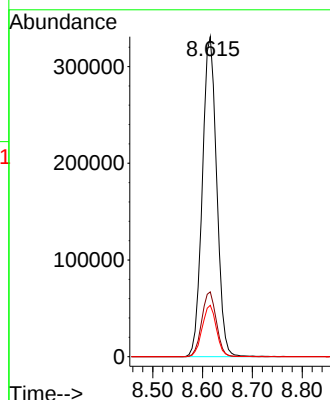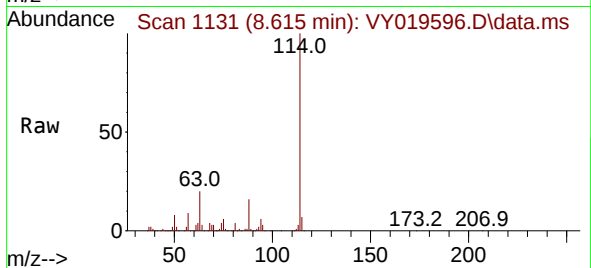

#35

Dibromofluoromethane

Concen: 54.192 ug/l

RT: 7.634 min Scan# 970

Delta R.T. 0.000 min

Lab File: VY019596.D

Acq: 18 Sep 2024 10:43




Tgt Ion:113 Resp: 203149

Ion Ratio Lower Upper

113 100

111 105.8 82.2 123.4

192 17.9 15.9 23.9


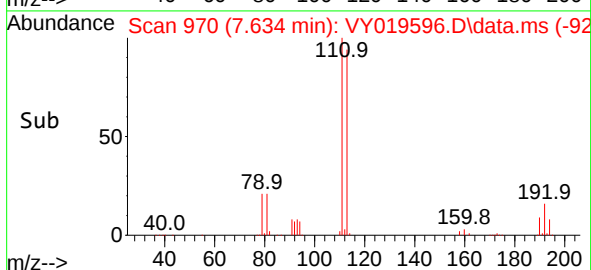
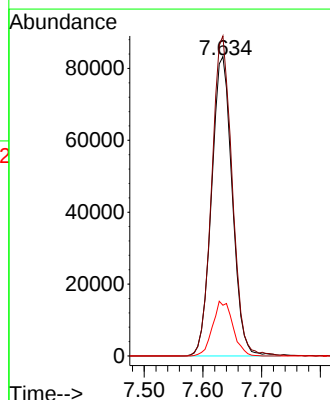
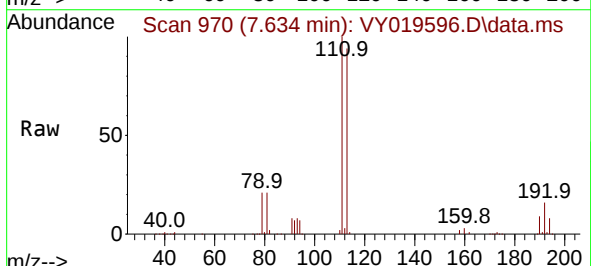




#50
Toluene-d8
Concen: 55.953 ug/l
RT: 10.109 min Scan# 1376
Delta R.T. 0.000 min
Lab File: VY019596.D
Acq: 18 Sep 2024 10:43




Instrument :
MSVOA_Y
ClientSampleId :
VY0918SBL01


Tgt Ion: 98 Resp: 775808
Ion Ratio Lower Upper
98 100
100 65.3 52.0 78.0

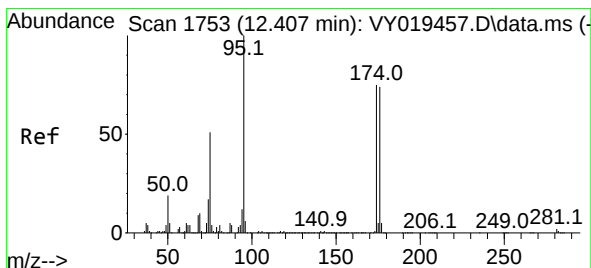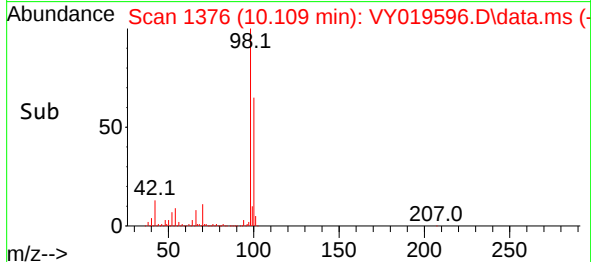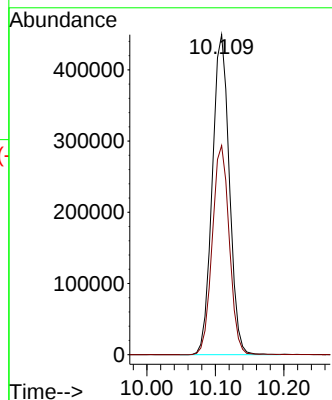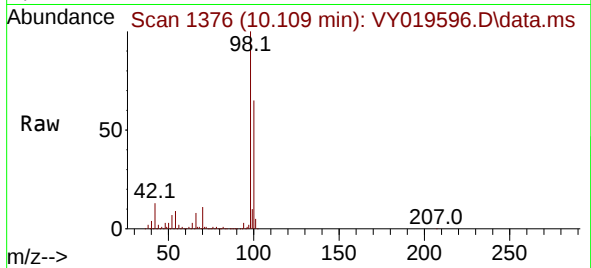

#62
4-Bromofluorobenzene
Concen: 45.651 ug/l
RT: 12.407 min Scan# 1753
Delta R.T. 0.000 min
Lab File: VY019596.D
Acq: 18 Sep 2024 10:43

Tgt Ion: 95 Resp: 243380
Ion Ratio Lower Upper
95 100
174 74.0 0.0 175.6
176 72.3 0.0 171.4

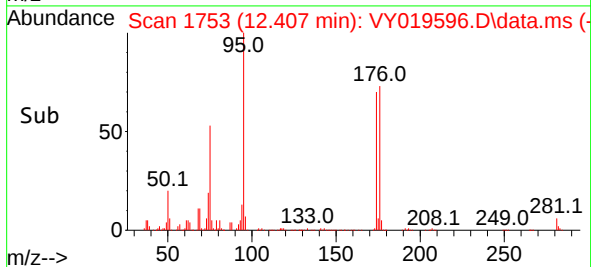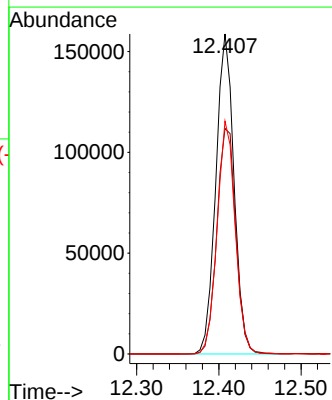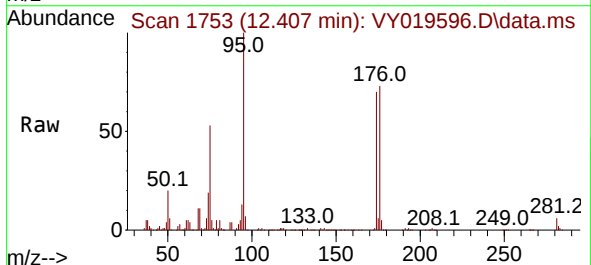

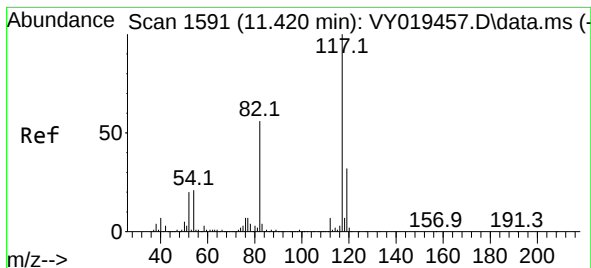

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.420 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY019596.D

Acq: 18 Sep 2024 10:43

Instrument :

MSVOA_Y

ClientSampleId :

VY0918SBL01




Tgt Ion:117 Resp: 570722

Ion Ratio Lower Upper

117 100

82 56.4 42.4 63.6

119 31.9 25.9 38.9

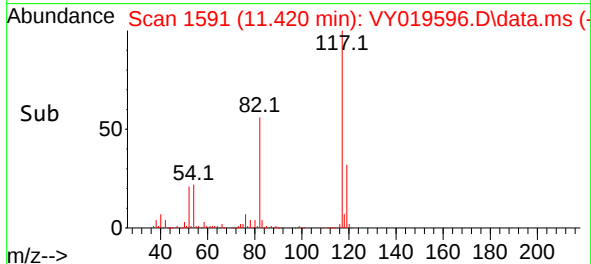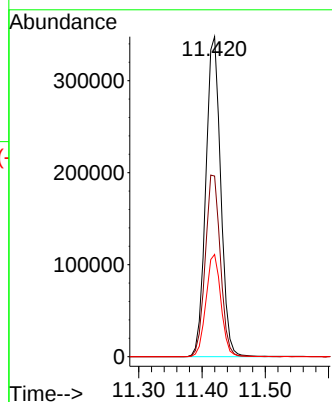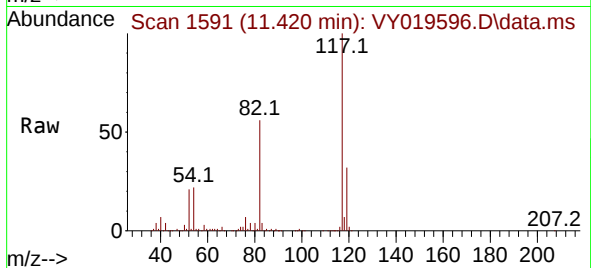

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.346 min Scan# 1907

Delta R.T. 0.000 min

Lab File: VY019596.D

Acq: 18 Sep 2024 10:43

Tgt Ion:152 Resp: 202452

Ion Ratio Lower Upper

152 100

115 61.9 28.2 84.7

150 158.4 0.0 345.6

