


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv091919\
Data File : VY000069.D
Acq On : 19 Sep 2019 11:25
Operator : SY/MD
Sample : BFB
Misc : 5.00µl/5.00ml/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y091719S.M
Title : SW846 8260
Last Update : Thu Sep 19 05:38:39 2019

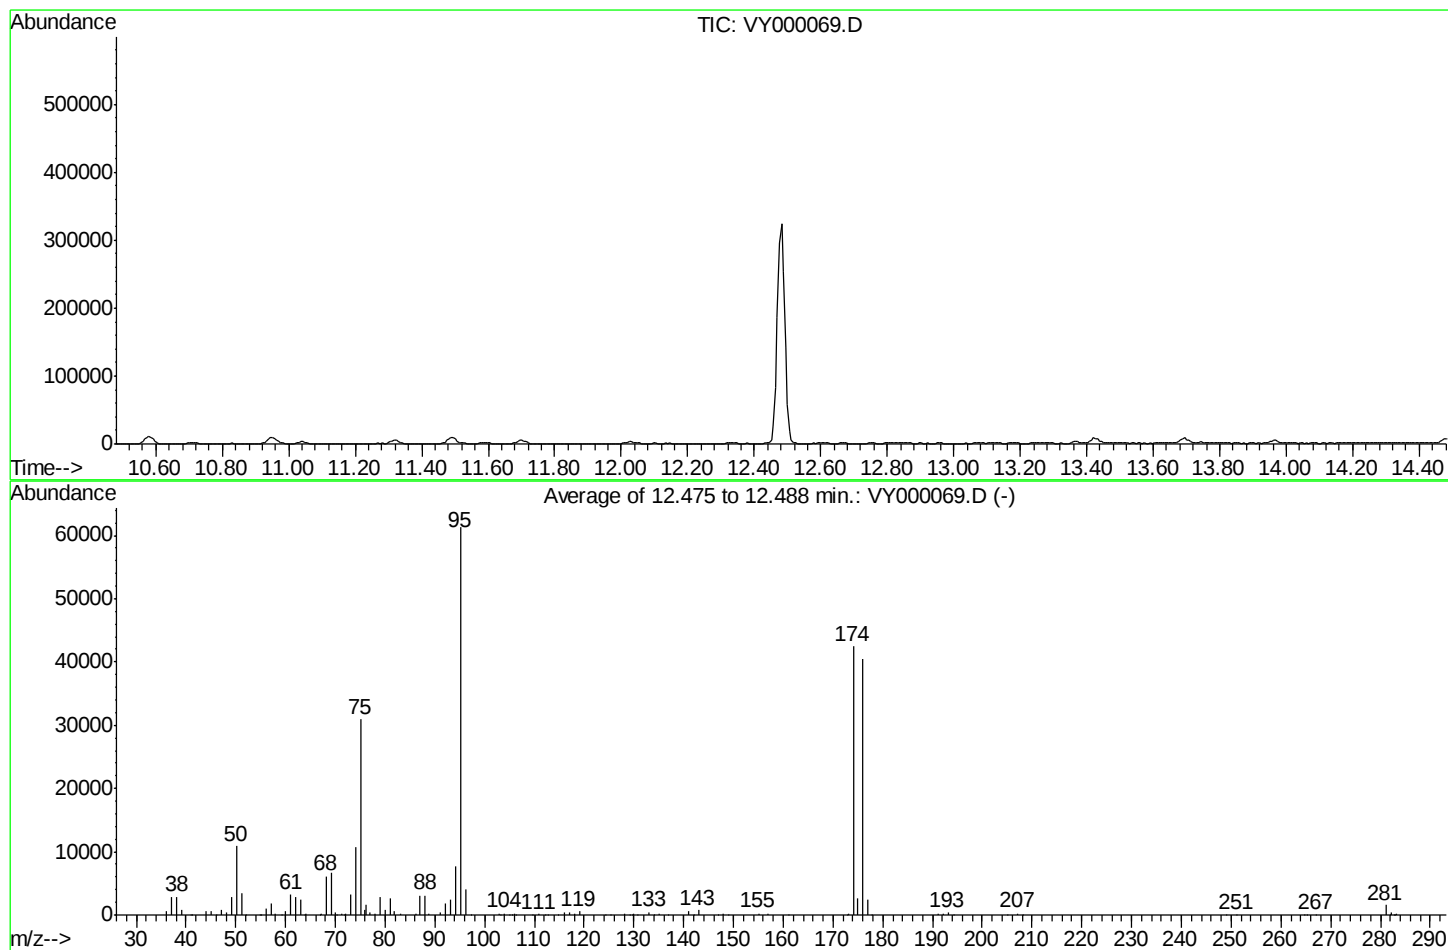

AutoFind: Scans 1786, 1787, 1788; Background Corrected with Scan 1778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	10912	PASS
75	95	30	60	50.5	30928	PASS
95	95	100	100	100.0	61280	PASS
96	95	5	9	6.8	4146	PASS
173	174	0.00	2	0.3	128	PASS
174	95	50	100	69.2	42421	PASS
175	174	5	9	6.3	2667	PASS
176	174	95	101	95.3	40413	PASS
177	176	5	9	6.1	2468	PASS