


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv092019\
Data File : VY000095.D
Acq On : 20 Sep 2019 09:32
Operator : SY/MD
Sample : BFB
Misc : 5.00µl/5.00ml/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y091719S.M
Title : SW846 8260
Last Update : Thu Sep 19 05:38:39 2019

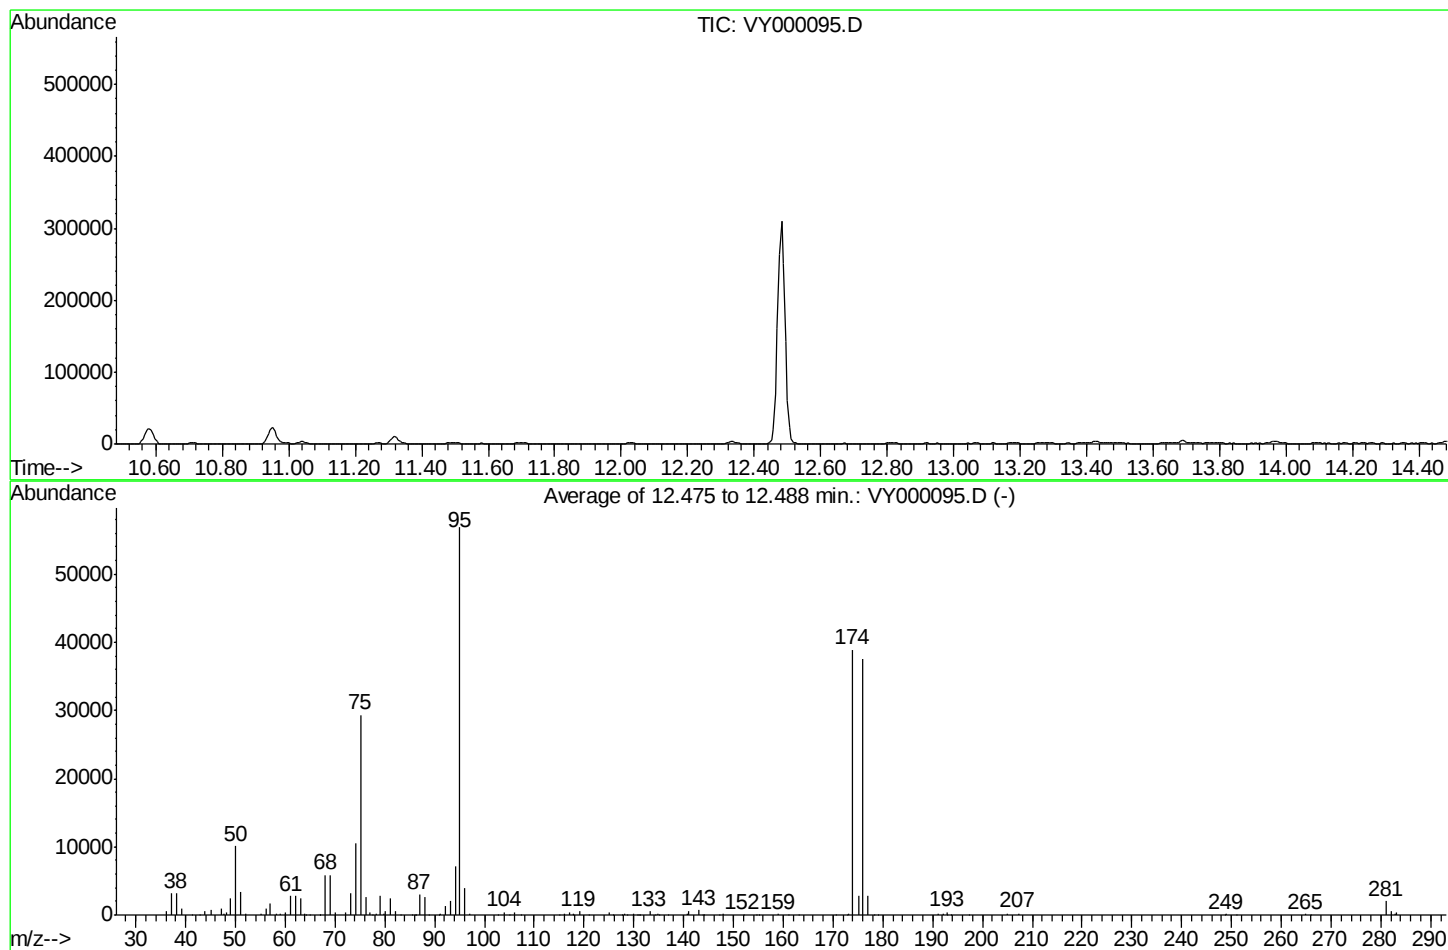

AutoFind: Scans 1786, 1787, 1788; Background Corrected with Scan 1778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	10100	PASS
75	95	30	60	51.7	29389	PASS
95	95	100	100	100.0	56861	PASS
96	95	5	9	7.0	3991	PASS
173	174	0.00	2	0.5	185	PASS
174	95	50	100	68.4	38920	PASS
175	174	5	9	7.3	2825	PASS
176	174	95	101	96.5	37560	PASS
177	176	5	9	7.4	2765	PASS