

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092123\
 Data File : VY015673.D
 Acq On : 21 Sep 2023 16:23
 Operator : SY/MD
 Sample : 04567-03
 Misc : 5.77g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 SE-SOIL-2

Quant Time: Sep 22 01:21:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091923S.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 20 01:39:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	137576	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	236541	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	217569	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	97949	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	89338	59.019	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 118.040%	
35) Dibromofluoromethane	7.716	113	75371	53.236	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 106.480%	
50) Toluene-d8	10.179	98	276704	57.642	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 115.280%	
62) 4-Bromofluorobenzene	12.483	95	93797	49.790	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 99.580%	
Target Compounds						
					Qvalue	
20) Methylene Chloride	4.710	84	30100	13.426	ug/l	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092123\
Data File : VY015673.D
Acq On : 21 Sep 2023 16:23
Operator : SY/MD
Sample : 04567-03
Misc : 5.77g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
SE-SOIL-2

Quant Time: Sep 22 01:21:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091923S.M
Quant Title : SW846 8260
QLast Update : Wed Sep 20 01:39:40 2023
Response via : Initial Calibration




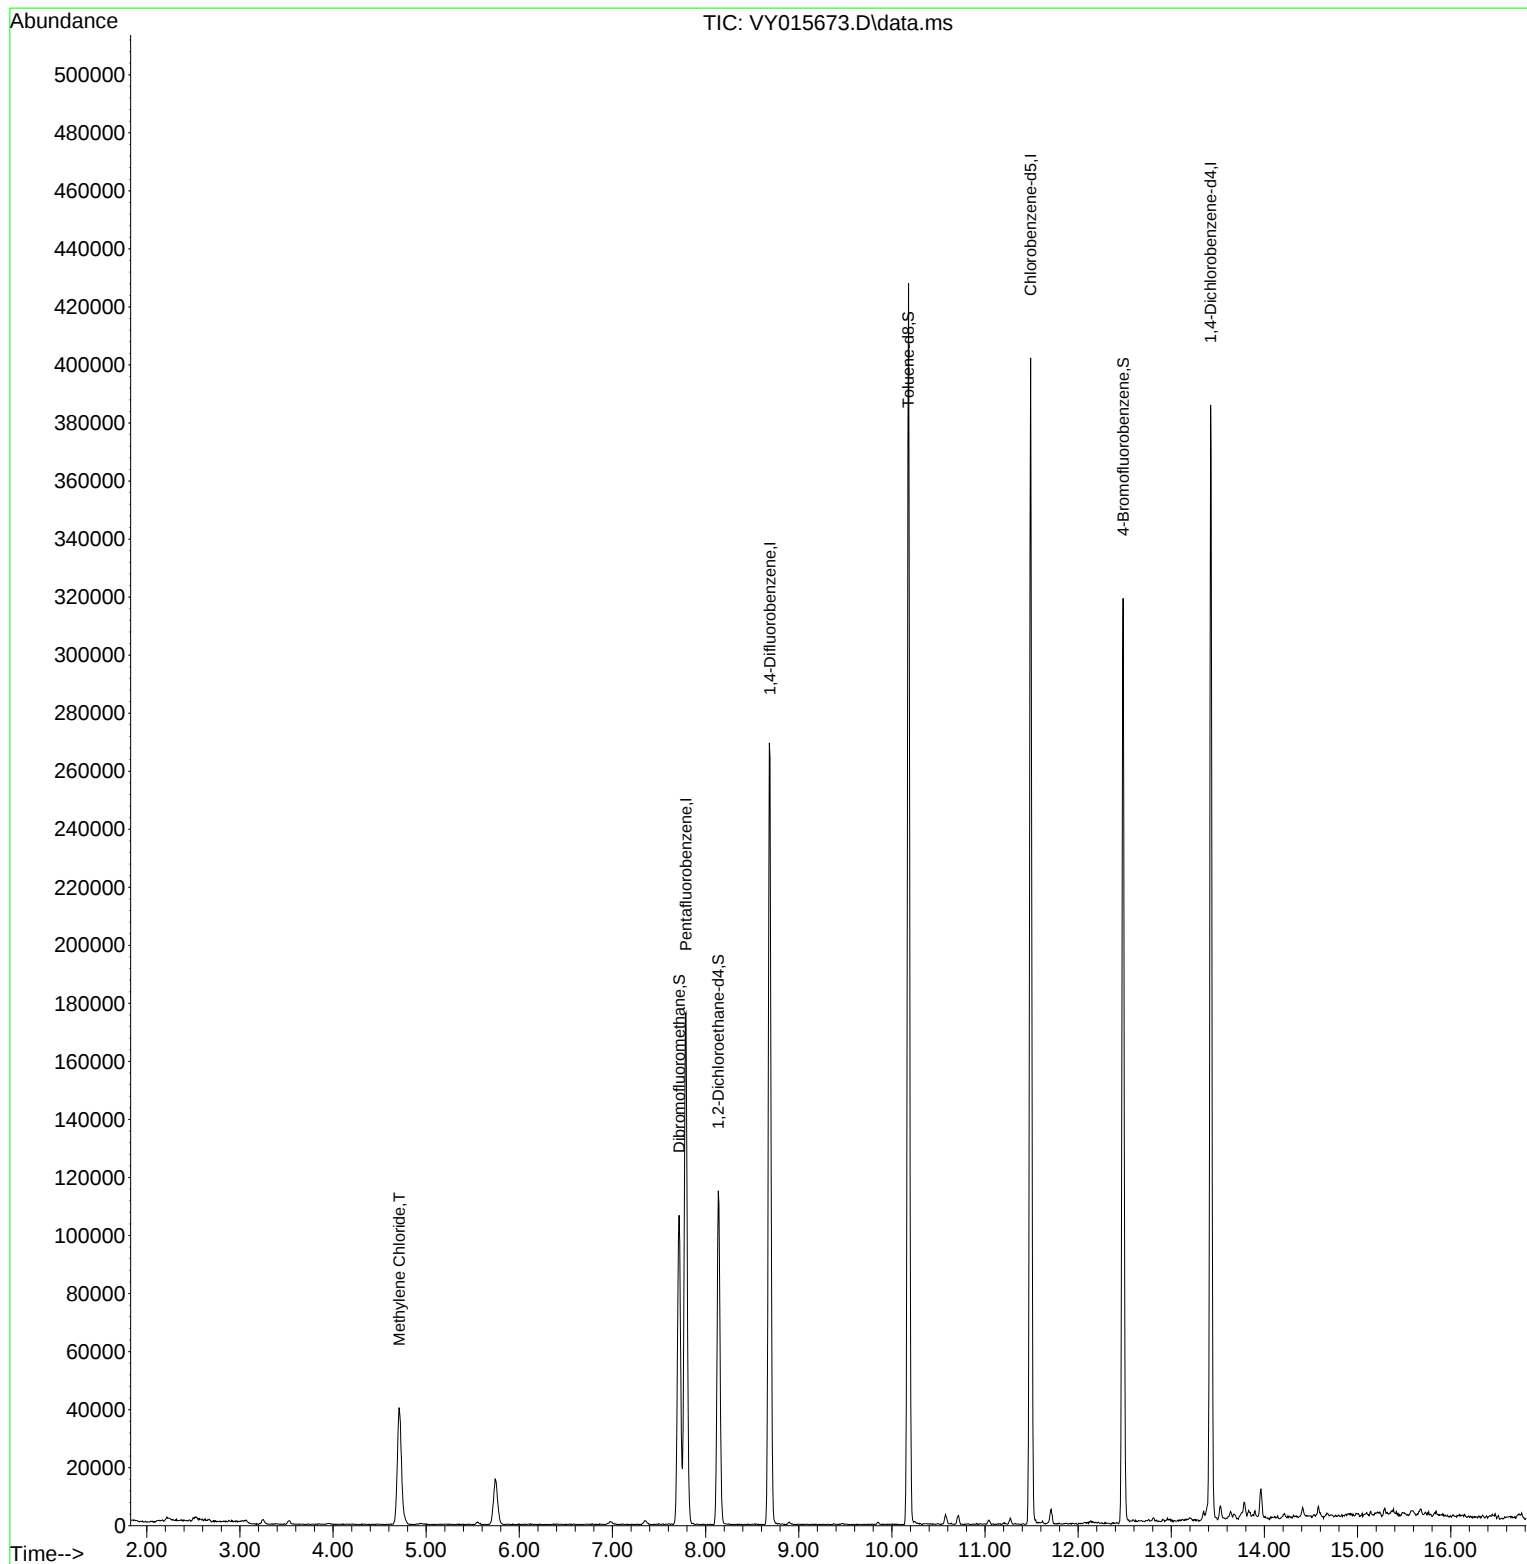




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY015673.D
Acq: 21 Sep 2023 16:23




Instrument :
MSVOA_Y
ClientSampleId :
SE-SOIL-2


Tgt Ion:168 Resp: 137576
Ion Ratio Lower Upper
168 100
99 54.0 43.4 65.0

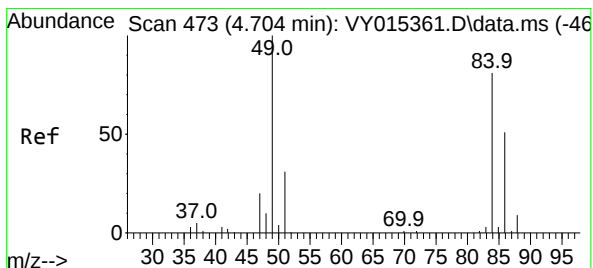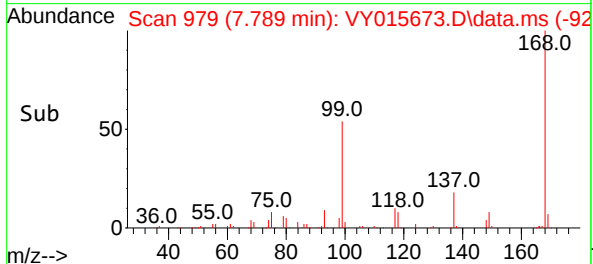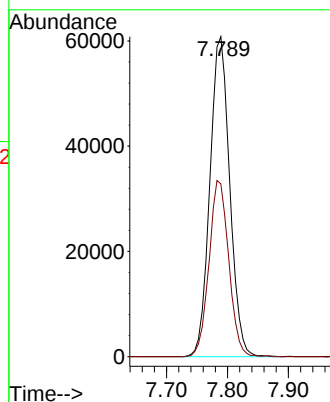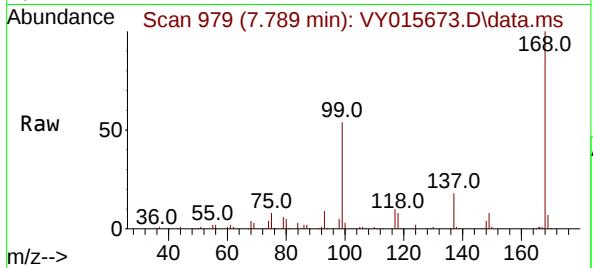

#20
Methylene Chloride
Concen: 13.426 ug/l
RT: 4.710 min Scan# 474
Delta R.T. 0.006 min
Lab File: VY015673.D
Acq: 21 Sep 2023 16:23

Tgt Ion: 84 Resp: 30100
Ion Ratio Lower Upper
84 100
49 123.6 106.9 160.3
51 35.0 33.2 49.8
86 67.1 51.0 76.6

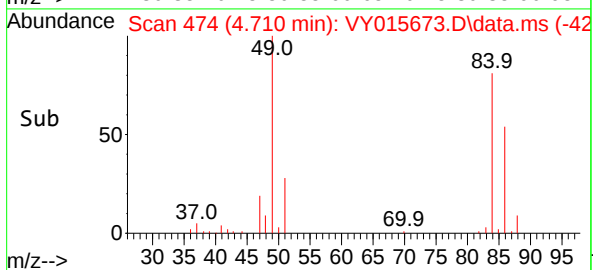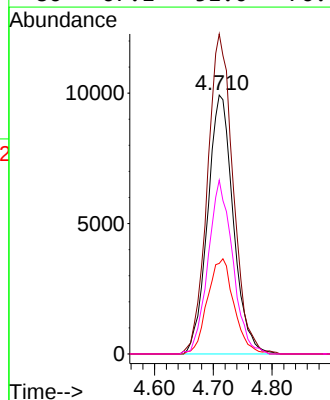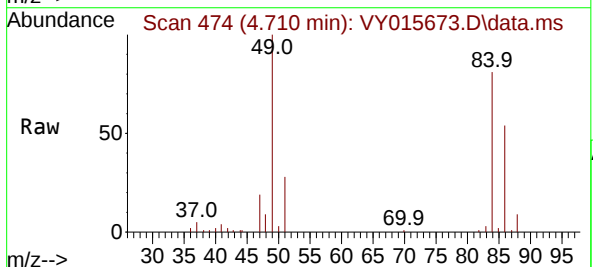

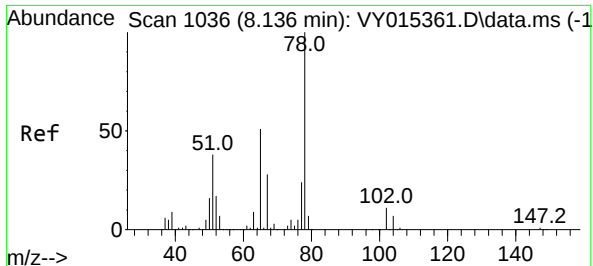

#33

1,2-Dichloroethane-d4

Concen: 59.019 ug/l

RT: 8.136 min Scan# 110

Delta R.T. 0.000 min

Lab File: VY015673.D

Acq: 21 Sep 2023 16:23

Instrument :

MSVOA_Y

ClientSampleId :





SE-SOIL-2

Tgt Ion: 65 Resp: 89338

Ion Ratio Lower Upper

65 100

67 52.0 0.0 101.8

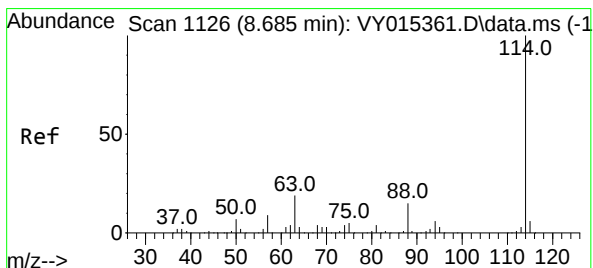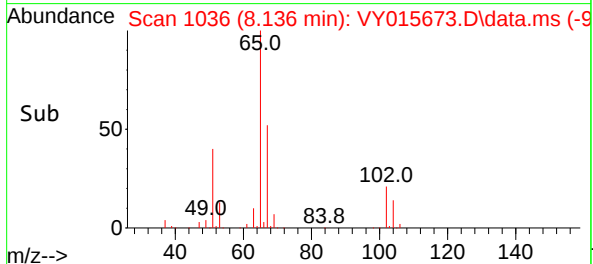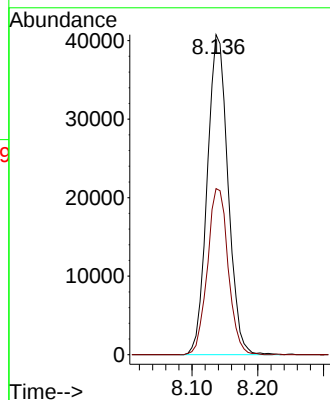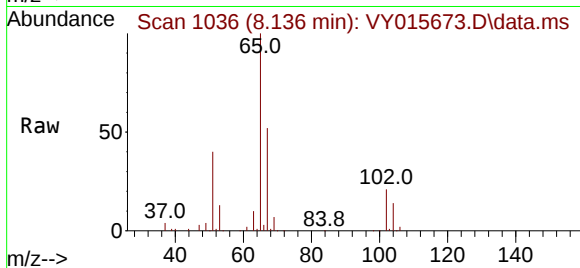

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VY015673.D

Acq: 21 Sep 2023 16:23




Tgt Ion: 114 Resp: 236541


Ion Ratio Lower Upper

114 100

63 18.9 0.0 42.4

88 14.7 0.0 30.6


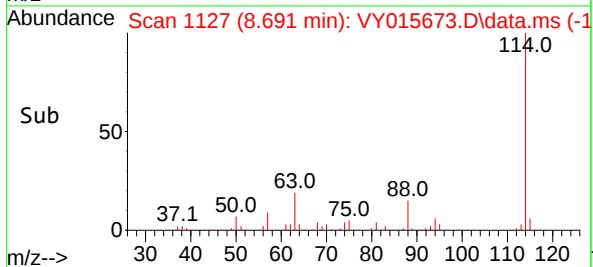
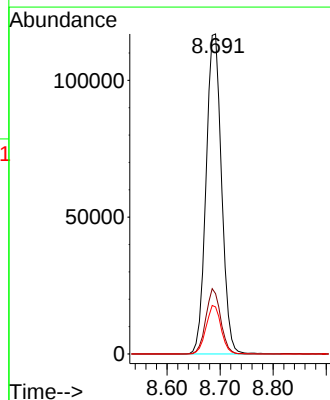
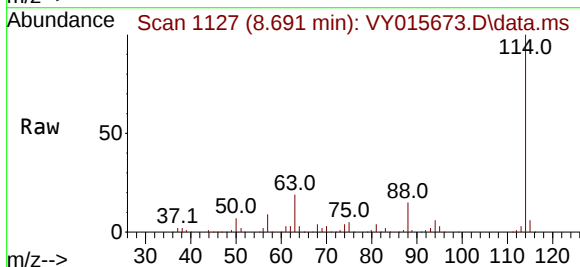


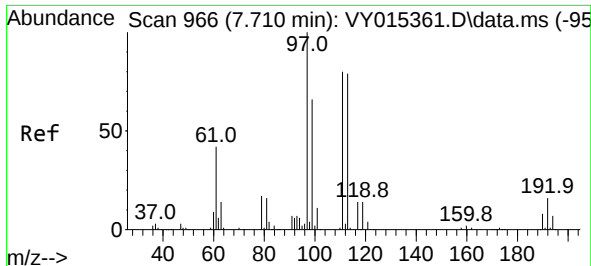

#35
Dibromofluoromethane
Concen: 53.236 ug/l
RT: 7.716 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY015673.D
Acq: 21 Sep 2023 16:23




Instrument :
MSVOA_Y
ClientSampleId :
SE-SOIL-2


Tgt Ion:113 Resp: 75371
Ion Ratio Lower Upper
113 100
111 102.5 81.3 121.9
192 18.9 16.9 25.3

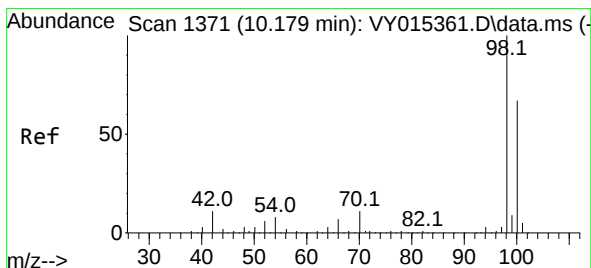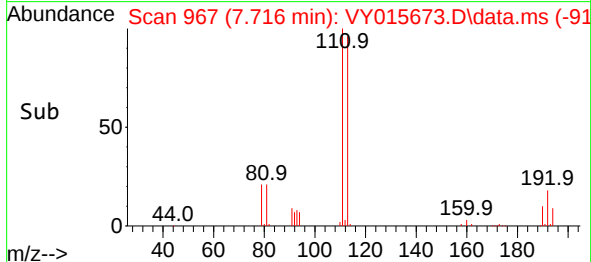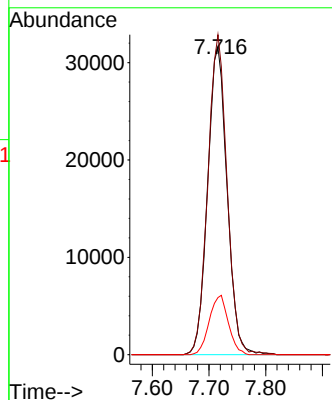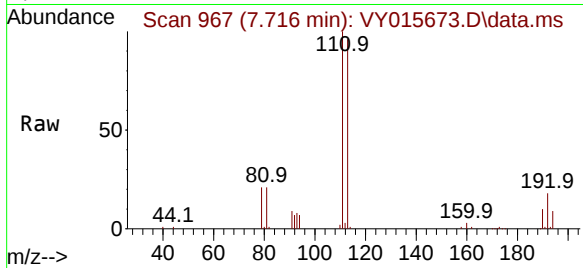

#50
Toluene-d8
Concen: 57.642 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY015673.D
Acq: 21 Sep 2023 16:23

Tgt Ion: 98 Resp: 276704
Ion Ratio Lower Upper
98 100
100 65.3 50.1 75.1


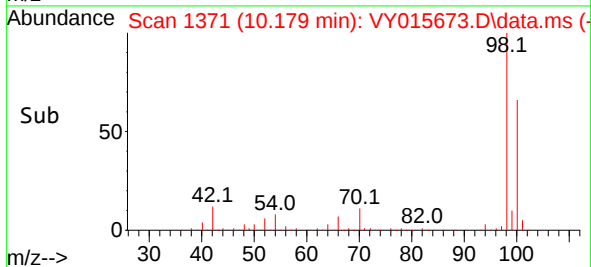
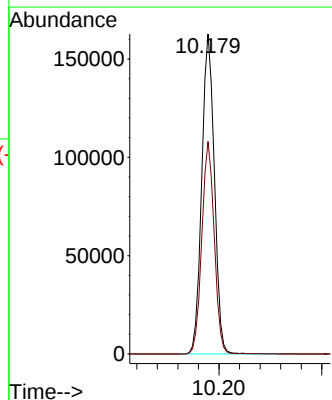
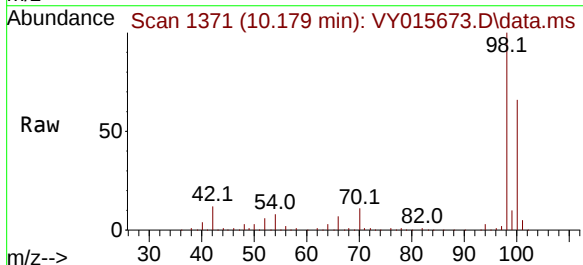


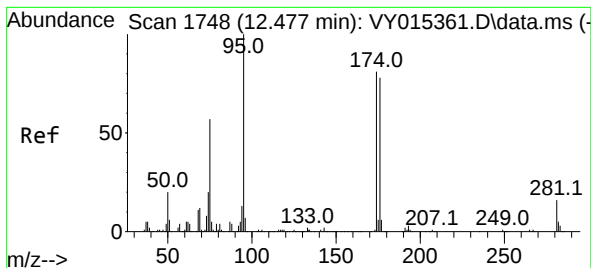

#62
4-Bromofluorobenzene
Concen: 49.790 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.006 min
Lab File: VY015673.D
Acq: 21 Sep 2023 16:23




Instrument :
MSVOA_Y
ClientSampleId :
SE-SOIL-2


Tgt Ion: 95 Resp: 93797
Ion Ratio Lower Upper
95 100
174 84.5 0.0 178.2
176 81.0 0.0 173.8

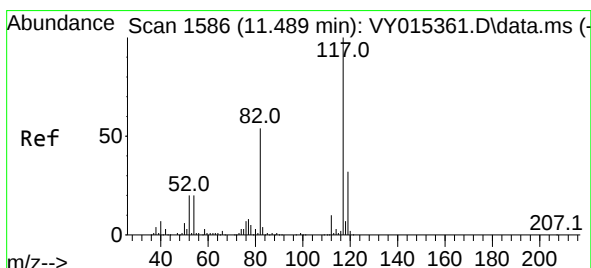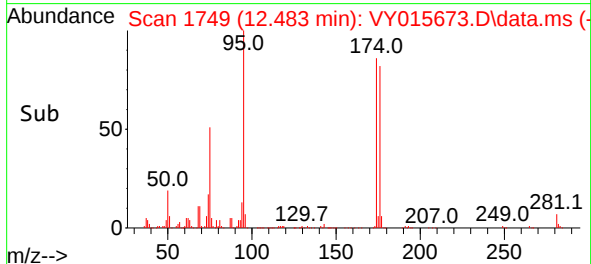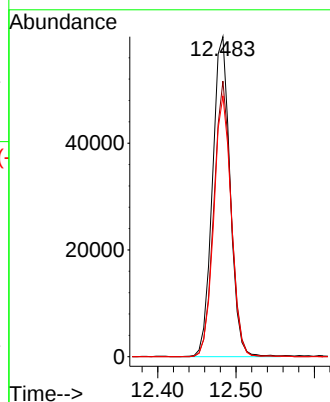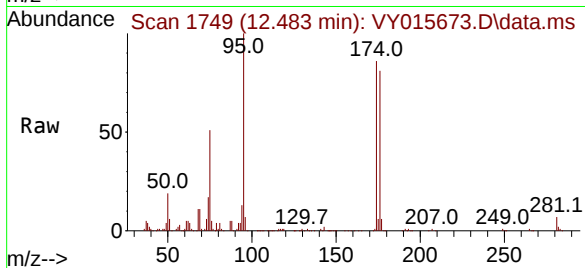

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. 0.000 min
Lab File: VY015673.D
Acq: 21 Sep 2023 16:23

Tgt Ion: 117 Resp: 217569
Ion Ratio Lower Upper
117 100
82 53.2 43.4 65.0
119 31.2 26.3 39.5

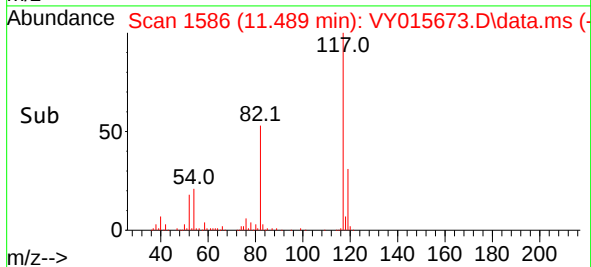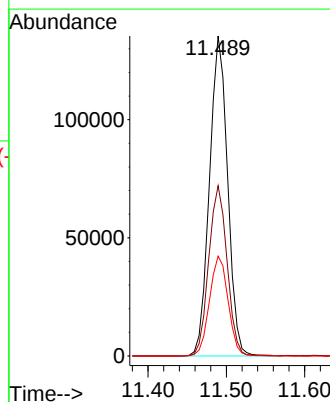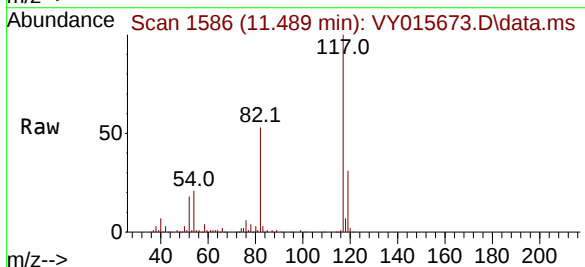

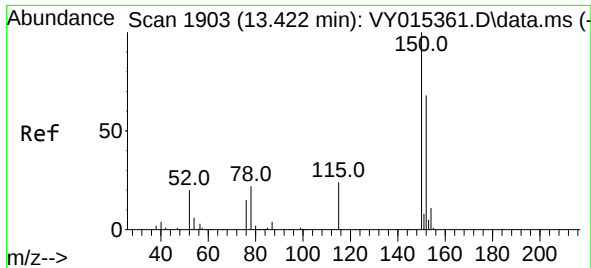

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. 0.000 min

Lab File: VY015673.D


Acq: 21 Sep 2023 16:23

Instrument :

MSVOA_Y

ClientSampleId :

SE-SOIL-2

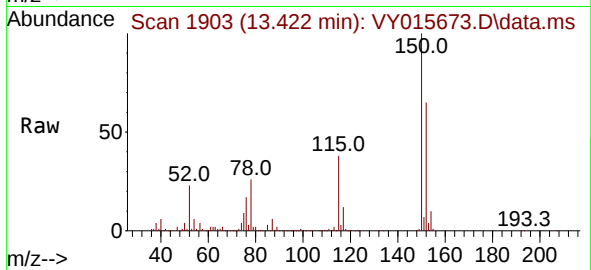

Tgt Ion:152 Resp: 97949

Ion Ratio Lower Upper

152 100

115 58.0 28.8 86.5

150 156.8 0.0 348.8

