


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY092221\
 Data File : VY006101.D
 Acq On : 22 Sep 2021 09:10
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y091421S.M
 Title : SW846 8260
 Last Update : Wed Sep 15 05:01:47 2021

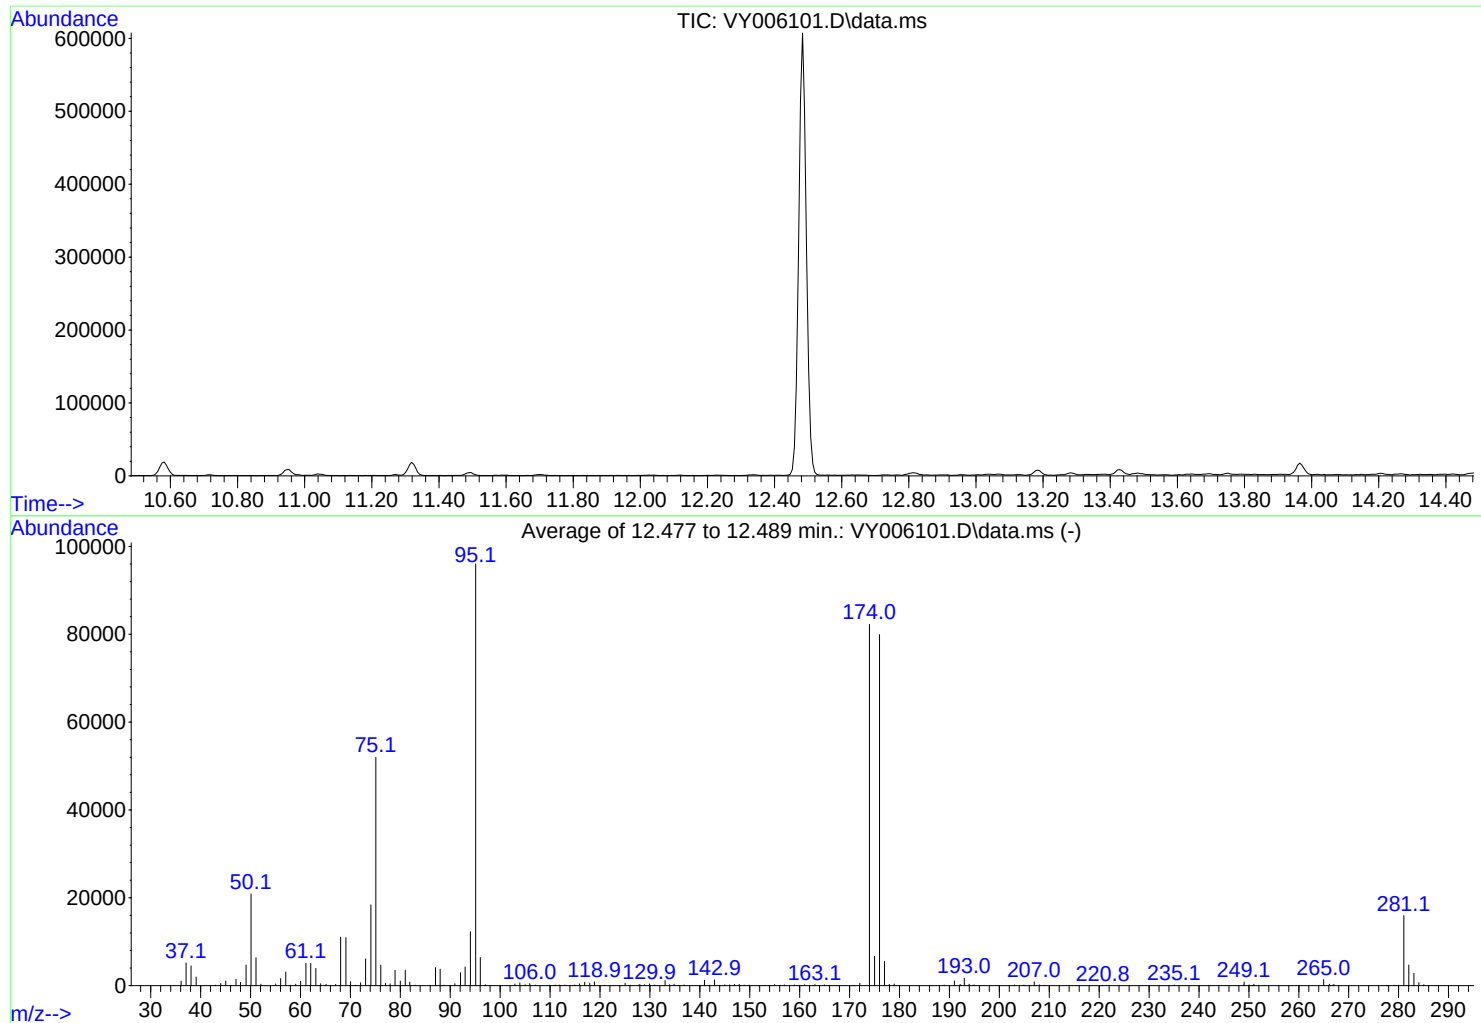

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	20904	PASS
75	95	30	60	54.1	51997	PASS
95	95	100	100	100.0	96040	PASS
96	95	5	9	6.7	6426	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	85.7	82275	PASS
175	174	5	9	8.1	6668	PASS
176	174	95	101	97.2	79933	PASS
177	176	5	9	6.9	5515	PASS